

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
 Data File : BM014073.D
 Acq On : 01 Feb 2018 14:58
 Operator : SJ/JU
 Sample : J1339-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 02 01:05:22 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 02 01:03:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	80260	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	311206	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	195705	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	461534	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	518089	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	530778	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	9334	5.34	ng/uL	0.00
5) Phenol-d5	6.75	99	39438	6.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	116262	31.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	127496	26.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	80657	15.97	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	86871	38.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	91219	36.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	146682	28.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	318	0.07	ng/ul	-0.15
43) Dimethylphthalate-d6	13.63	166	609636	37.54	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	746679	37.89	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	1176	0.53	ng/ul	0.03
57) Fluorene-d10	15.22	176	542079	37.29	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	77572	27.37	ng/ul	0.00
70) Anthracene-d10	17.07	188	834973	37.26	ng/ul	0.00
76) Pyrene-d10	19.37	212	989908	39.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.22	264	982570	37.72	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.64	165	3260	1.072	ng/ul#	21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
Data File : BM014073.D
Acq On : 01 Feb 2018 14:58
Operator : SJ/JU
Sample : J1339-19
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 02 01:05:22 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 02 01:03:24 2018
Response via : Initial Calibration

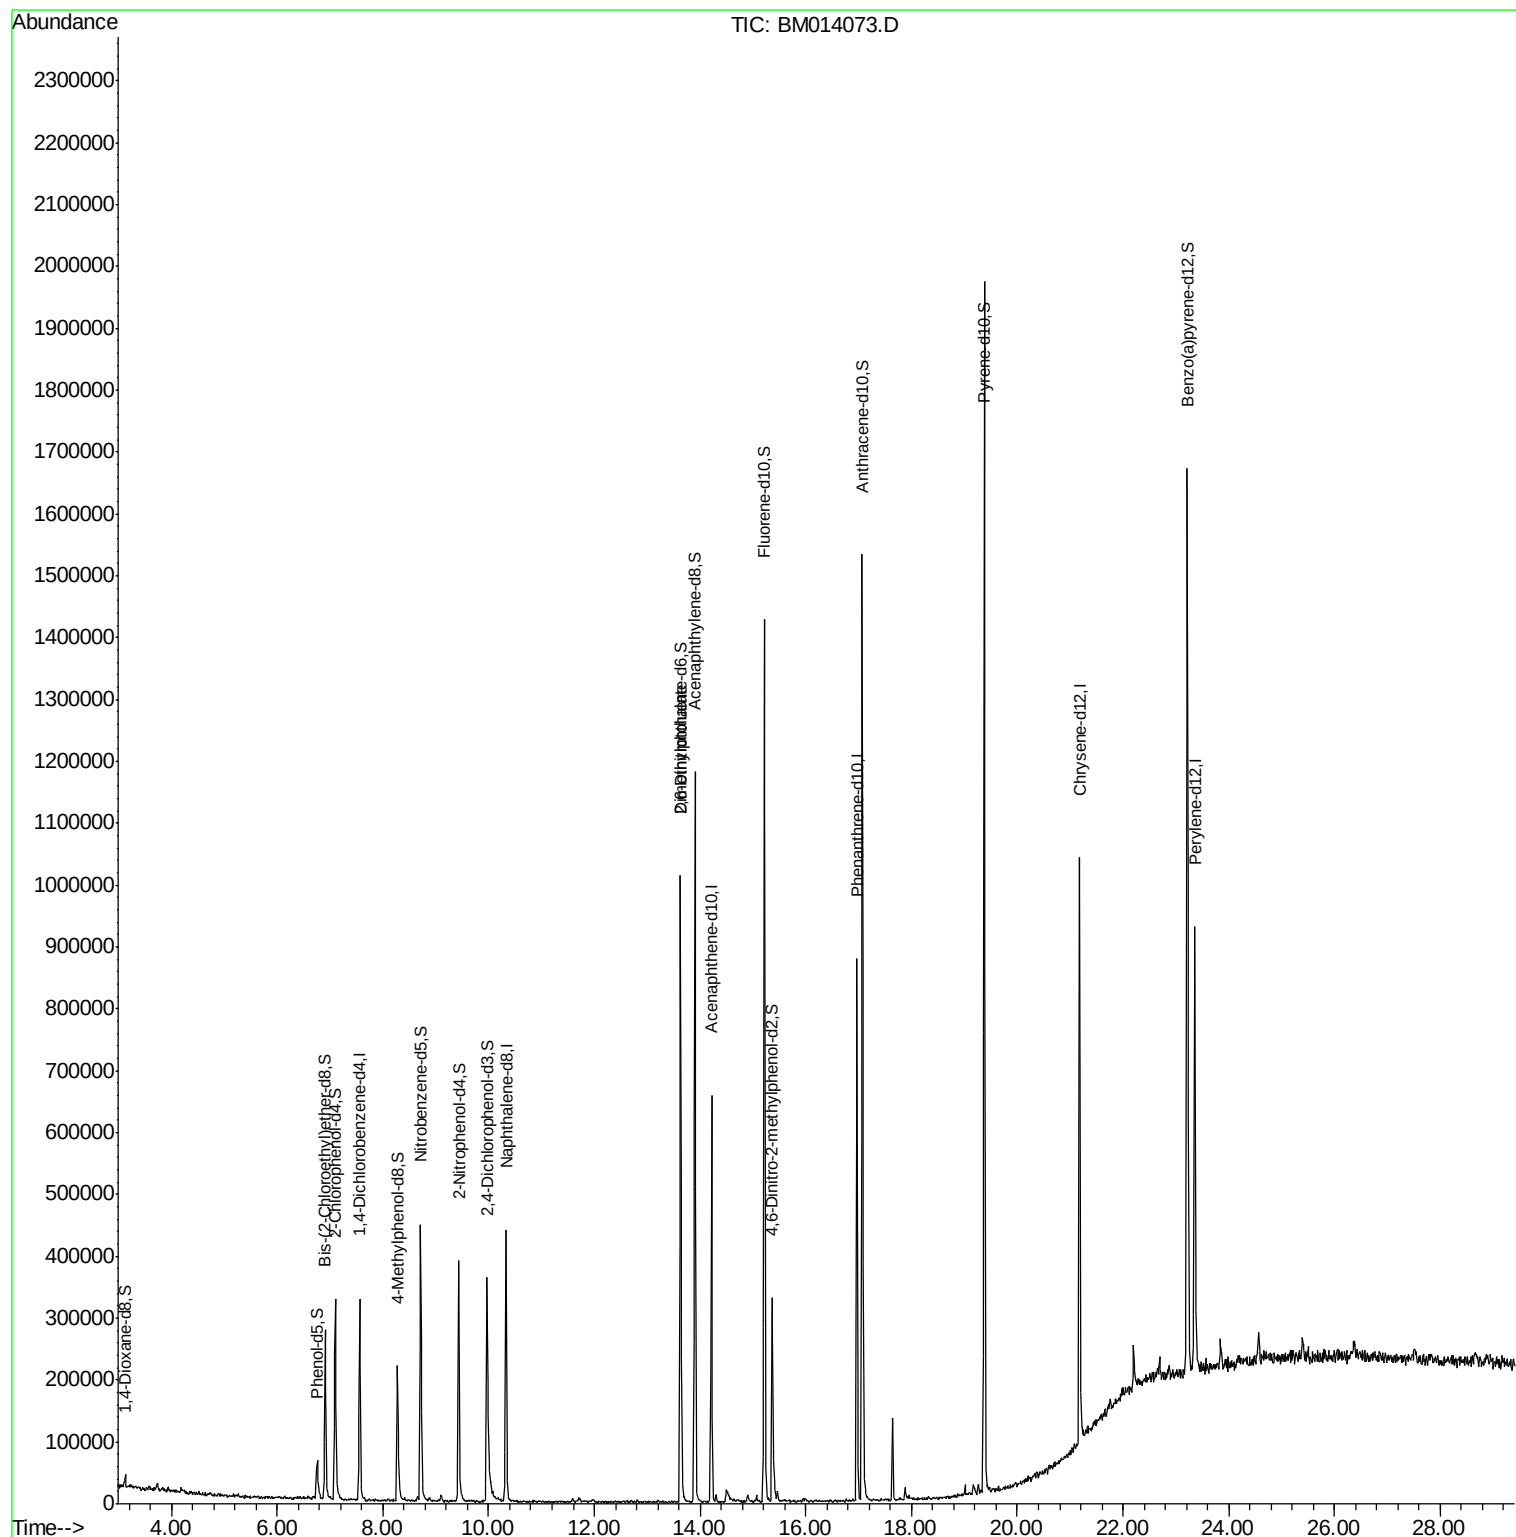

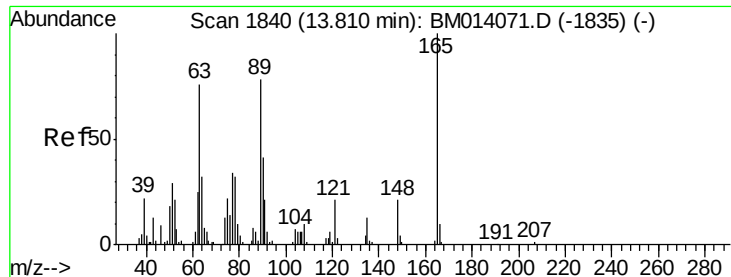

#45
 2,6-Dinitrotoluene
 Concen: 1.072 ng/ul
 RT: 13.64 min Scan# 1811
 Delta R.T. -0.17 min
 Lab File: BM014073.D
 Acq: 01 Feb 2018 14:58

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	52.6	79.0#
121	46.3	14.6	22.0#

