

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
 Data File : BM014075.D
 Acq On : 01 Feb 2018 16:10
 Operator : SJ/JU
 Sample : PB106227BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 02 01:05:41 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 02 01:03:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	87609	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	355729	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	227916	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	515094	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	552607	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	556234	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	11706	6.13	ng/uL	0.00
5) Phenol-d5	6.75	99	186857	28.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	119804	30.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	150736	28.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	161132	29.22	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	84751	33.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	95300	33.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	2105	0.35	ng/ul	0.08
29) 4-Chloroaniline-d4	10.49	131	209537	40.43	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	620861	32.82	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	757706	33.02	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	833	0.32	ng/ul	0.12
57) Fluorene-d10	15.22	176	552166	32.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	75047	23.73	ng/ul	0.00
70) Anthracene-d10	16.97	188	515094	20.60	ng/ul	-0.10
76) Pyrene-d10	19.37	212	938911	35.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.22	264	899994	32.97	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.27	70	5436	1.142	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
Data File : BM014075.D
Acq On : 01 Feb 2018 16:10
Operator : SJ/JU
Sample : PB106227BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 02 01:05:41 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 02 01:03:24 2018
Response via : Initial Calibration

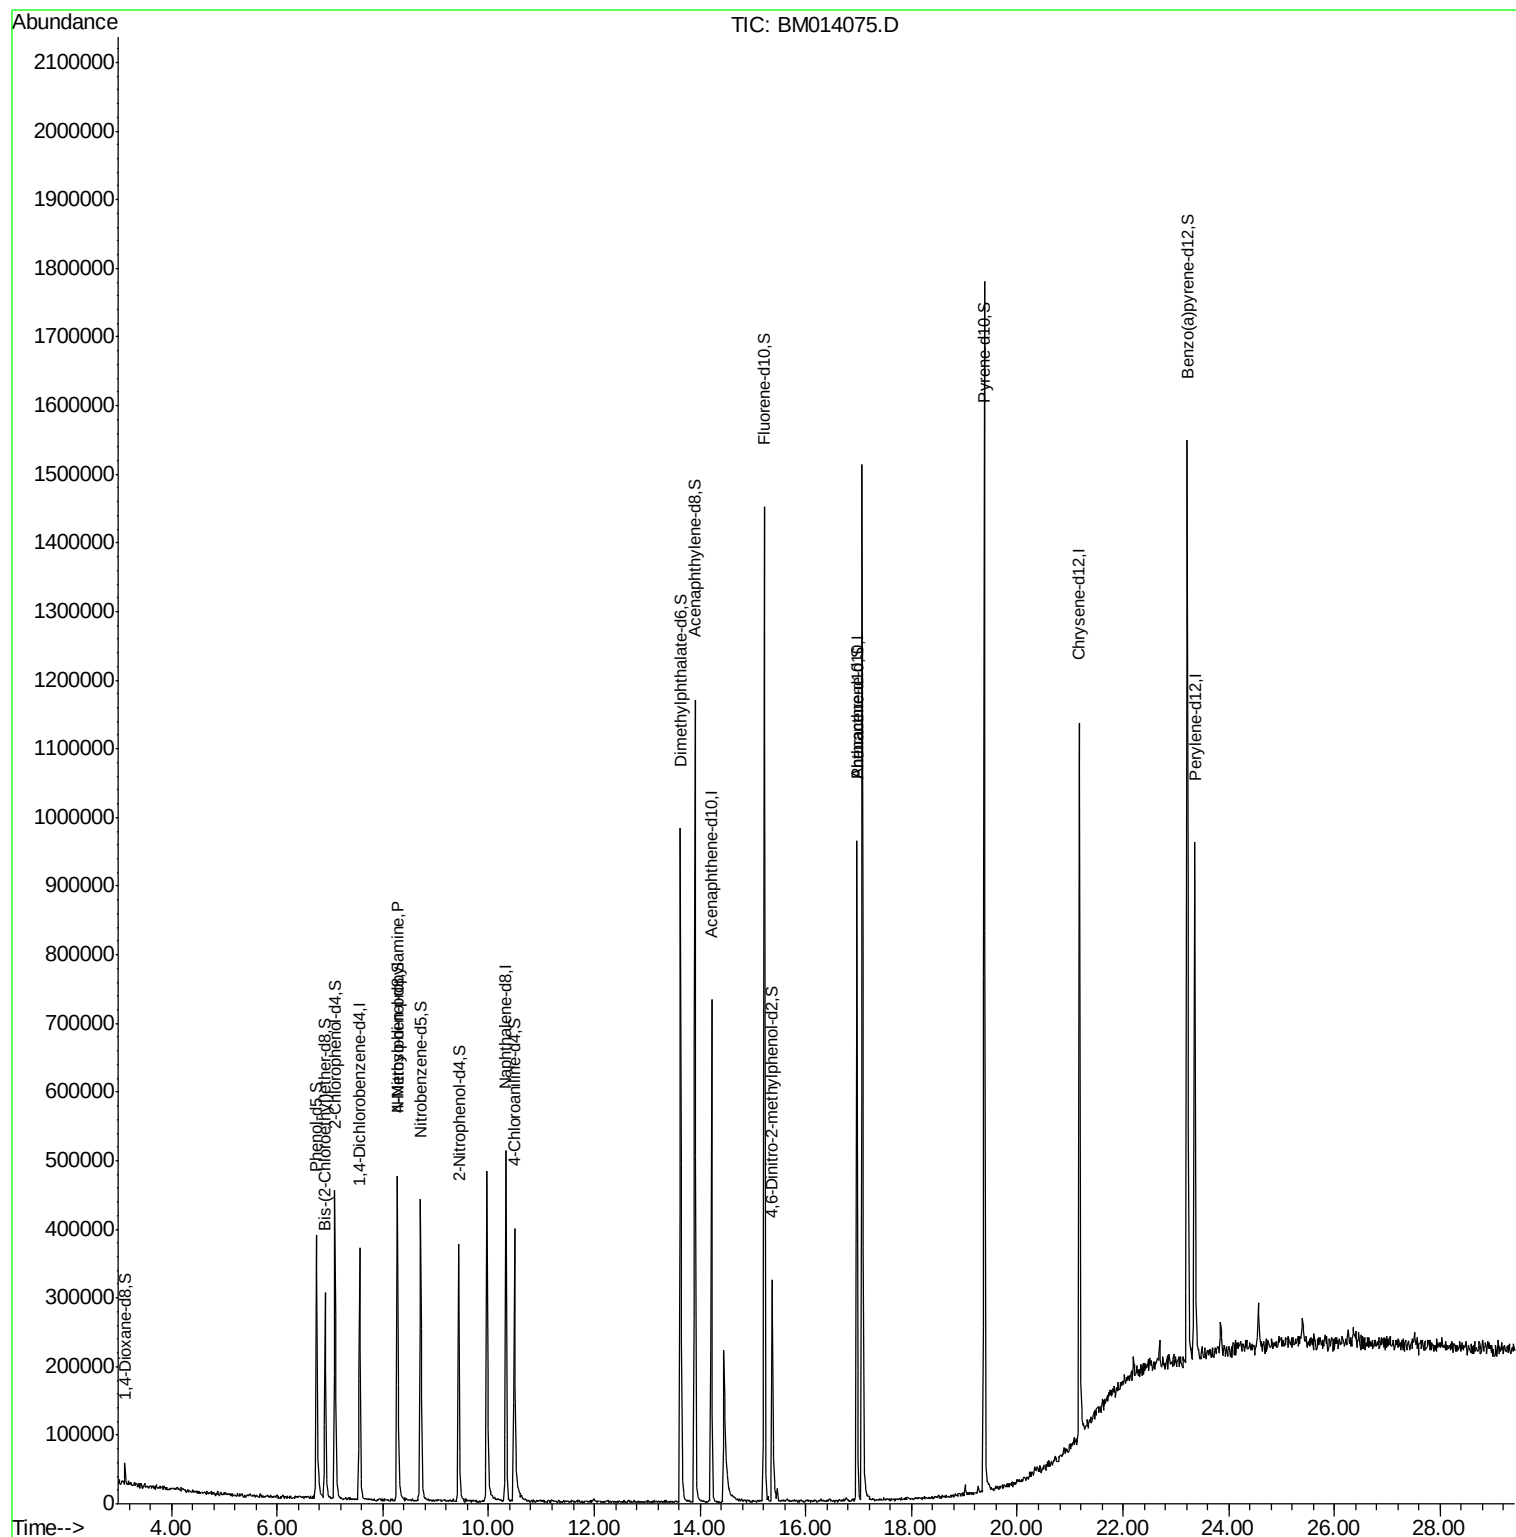

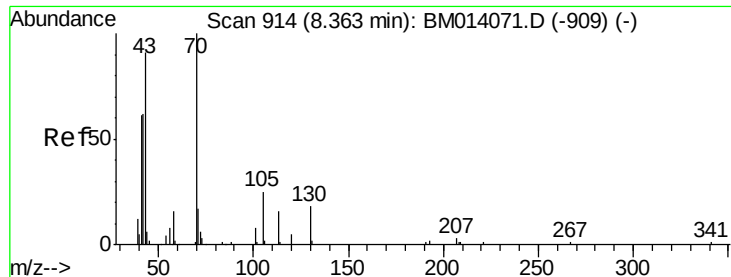

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.142 ng/ul
 RT: 8.27 min Scan# 899
 Delta R.T. -0.09 min
 Lab File: BM014075.D
 Acq: 01 Feb 2018 16:10

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 5436
 Ion Ratio Lower Upper
 70 100
 42 490.2 76.0 114.0#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

