

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
 Data File : BM014074.D
 Acq On : 01 Feb 2018 15:34
 Operator : SJ/JU
 Sample : J1316-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6D38

Manual Integrations
 APPROVED

Sohil
 2/2/2018 4:39:01 PM

Quant Time: Feb 02 01:24:23 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 02 01:03:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	77813	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	329571	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	211664	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	499966m	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	551047	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	554567	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	9008	5.31	ng/uL	0.00
5) Phenol-d5	6.75	99	160445	27.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	104705	29.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	136314	29.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	146622	29.94	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	70759	29.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	79916	30.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	141993	25.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	180870m	37.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	532542	30.32	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	641952	30.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	49691m	20.53	ng/ul	0.01
57) Fluorene-d10	15.22	176	478227	30.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	58345	19.00	ng/ul	0.00
70) Anthracene-d10	17.07	188	746437	30.75	ng/ul	0.00
76) Pyrene-d10	19.37	212	859057	32.37	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.21	264	833261	30.61	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.68	163	82662	4.881	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
Data File : BM014074.D
Acq On : 01 Feb 2018 15:34
Operator : SJ/JU
Sample : J1316-15
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6D38

Quant Time: Feb 02 01:24:23 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 02 01:03:24 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
2/2/2018 4:39:01 PM

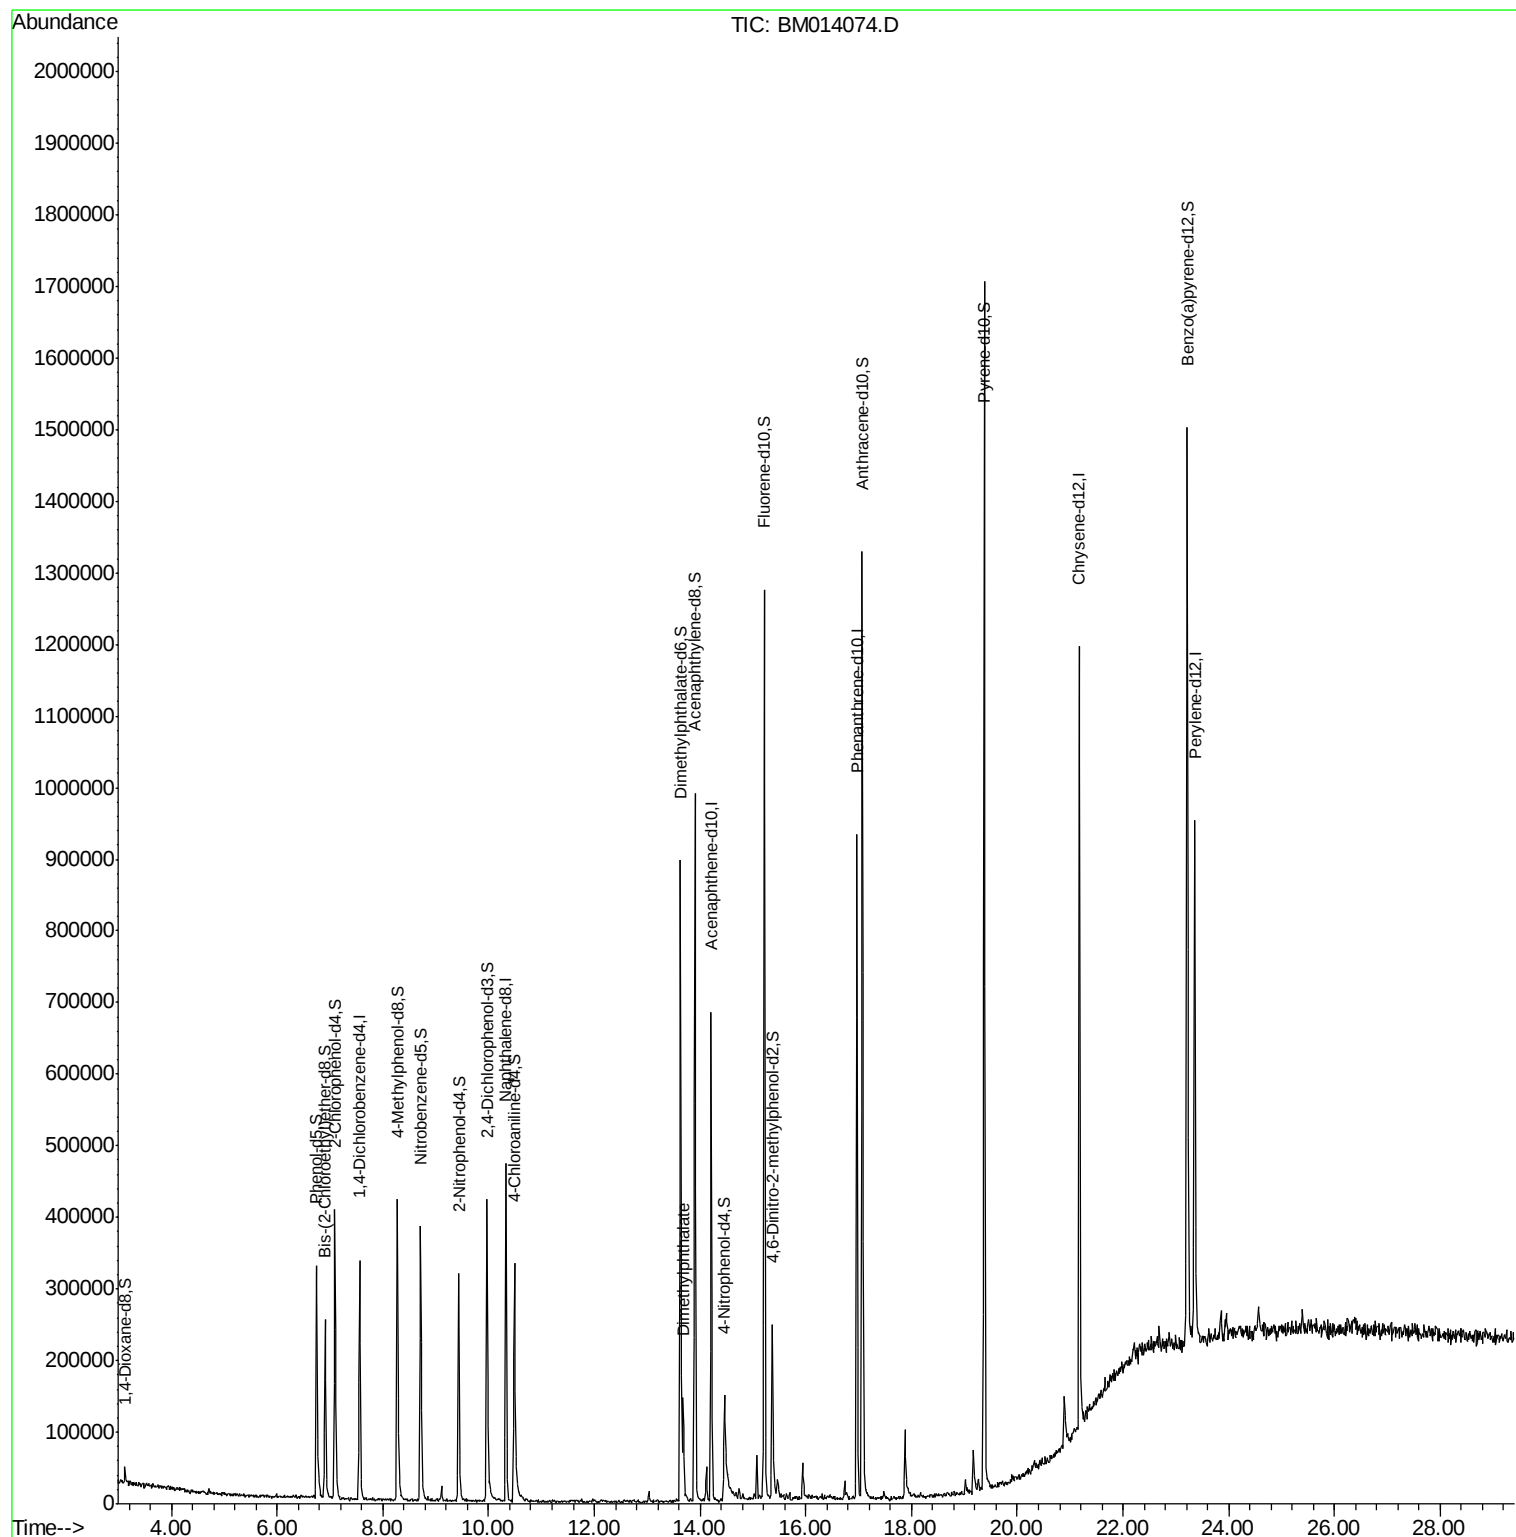

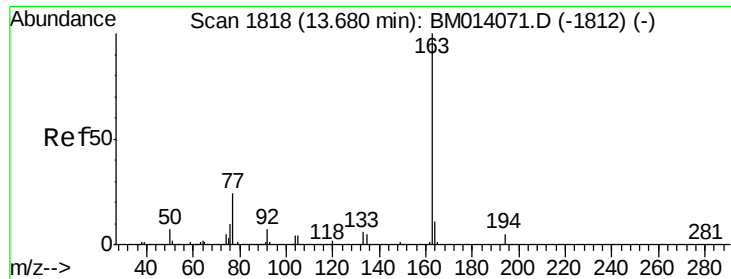

#44
 Dimethylphthalate
 Concen: 4.881 ng/ul
 RT: 13.68 min Scan# 1818
 Delta R.T. 0.00 min
 Lab File: BM014074.D
 Acq: 01 Feb 2018 15:34

Instrument :
 BNA_M
 ClientSampleId :
 F6D38

Tot Ion:	163	Resp:	82662
Ion Ratio	Lower	Upper	
163	100		
194	4.9	3.5	5.3
164	9.6	8.2	12.4

Manual Integrations
 APPROVED

Sohil
 2/2/2018 4:39:01 PM

