

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
 Data File : BM014079.D
 Acq On : 01 Feb 2018 18:34
 Operator : SJ/JU
 Sample : J1316-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6C99

Manual Integrations
 APPROVED

Sohil
 2/2/2018 4:39:13 PM

Quant Time: Feb 02 01:58:40 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 02 01:03:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	87175	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	350034	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	213188	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	516797	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	574882	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	597838	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	9640	5.07	ng/uL	0.00
5) Phenol-d5	6.75	99	161441	24.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	103576	26.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	143635	27.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	140358	25.58	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	71712	28.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	80537	28.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	138485	23.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	159331	31.25	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	505996	28.60	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	624501	29.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	42816m	17.56	ng/ul	0.01
57) Fluorene-d10	15.22	176	449310	28.38	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	56792	17.90	ng/ul	0.00
70) Anthracene-d10	17.07	188	691383	27.55	ng/ul	0.00
76) Pyrene-d10	19.37	212	795027	28.72	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.21	264	807490	27.52	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.68	163	96727	5.671	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
Data File : BM014079.D
Acq On : 01 Feb 2018 18:34
Operator : SJ/JU
Sample : J1316-19
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6C99

Manual Integrations
APPROVED

Sohil
2/2/2018 4:39:13 PM

Quant Time: Feb 02 01:58:40 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 02 01:03:24 2018
Response via : Initial Calibration

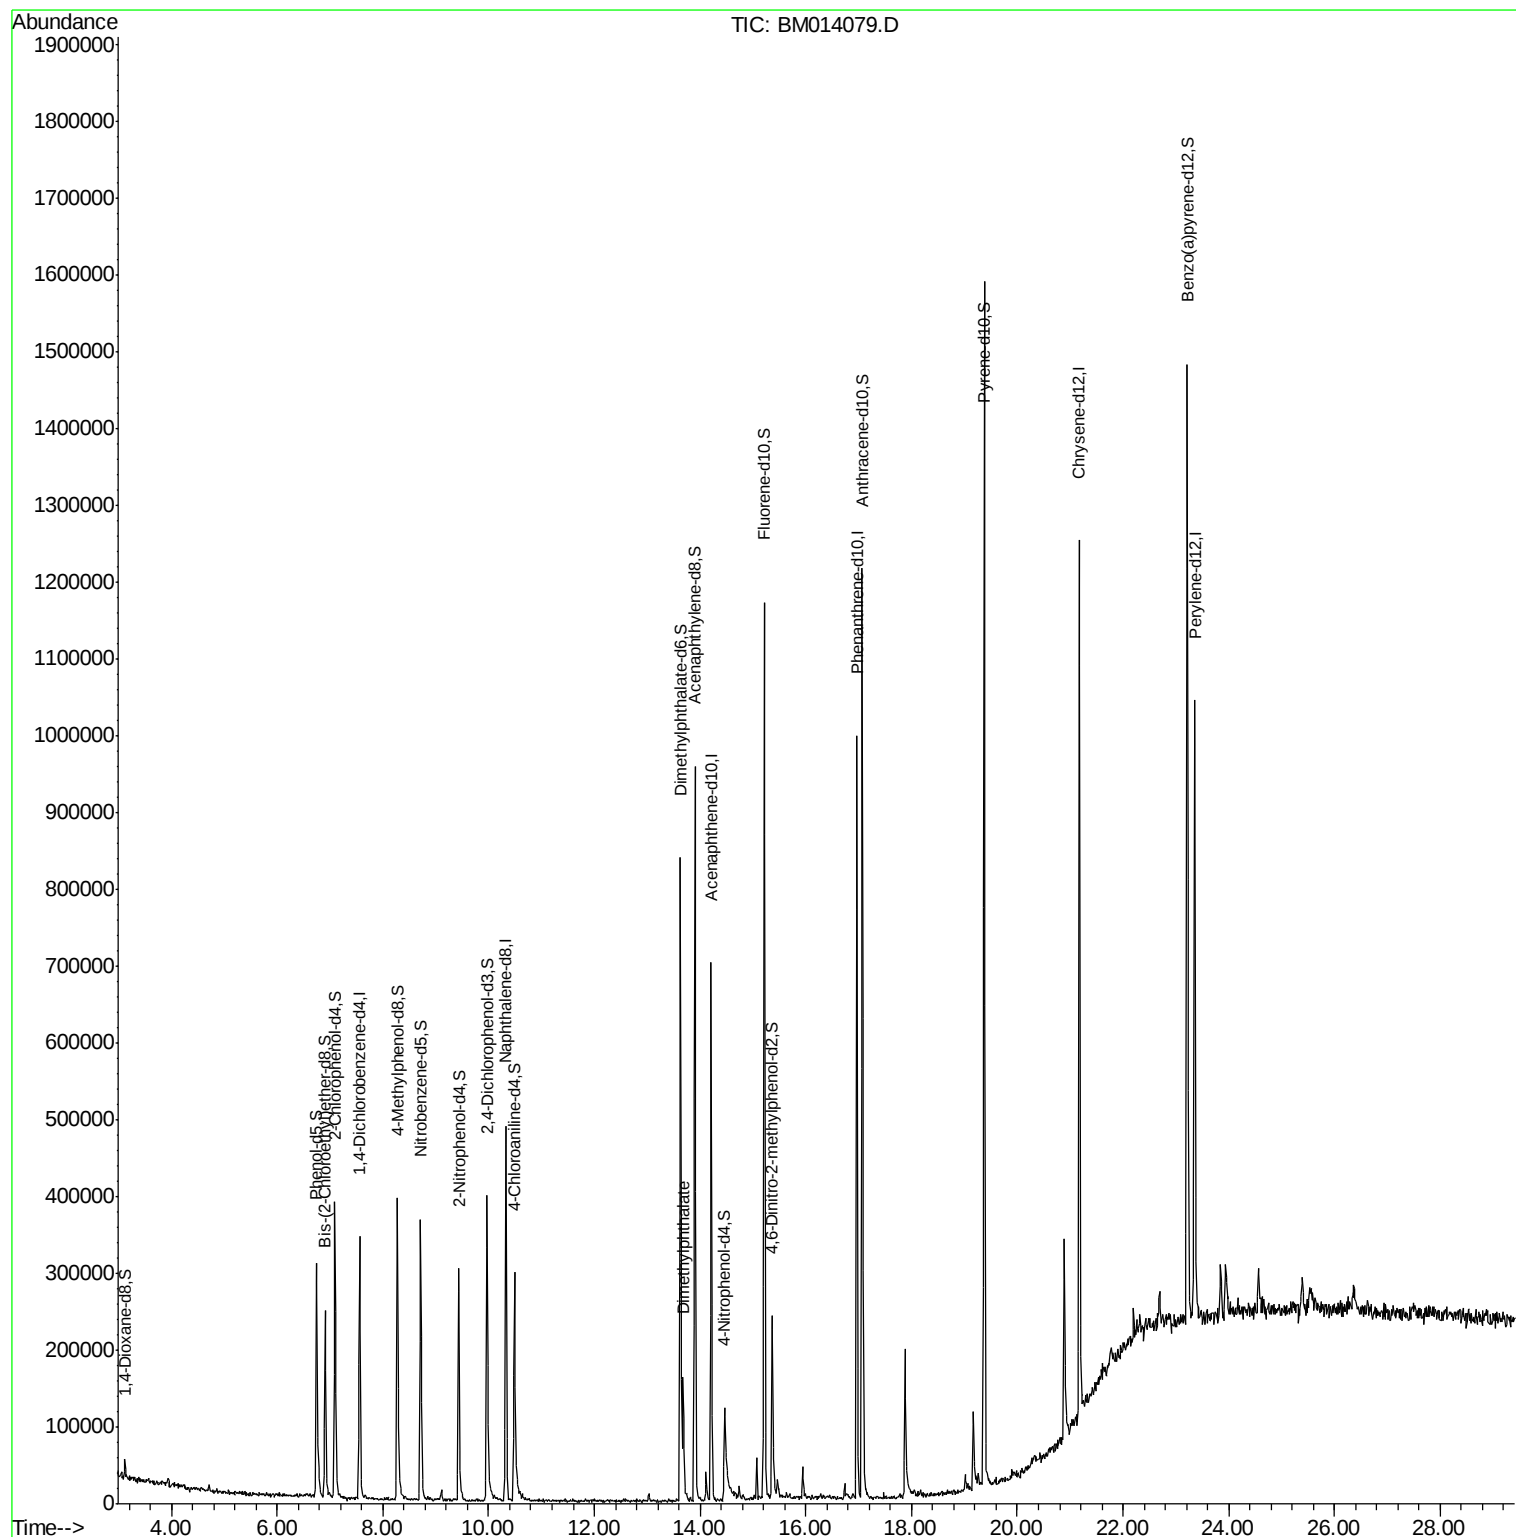

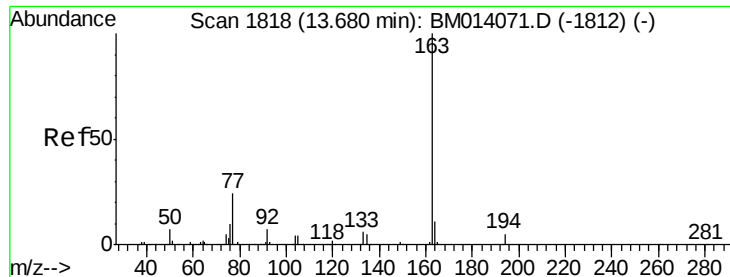

#44
 Dimethylphthalate
 Concen: 5.671 ng/ul
 RT: 13.68 min Scan# 1818
 Delta R.T. 0.00 min
 Lab File: BM014079.D
 Acq: 01 Feb 2018 18:34

Instrument :
 BNA_M
 ClientSampleId :
 F6C99

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	3.9	3.5	5.3
164	13.1	8.2	12.4

Manual Integrations
 APPROVED

Sohil
 2/2/2018 4:39:13 PM

