

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
 Data File : BM014083.D
 Acq On : 01 Feb 2018 20:58
 Operator : SJ/JU
 Sample : J1316-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6D36

Manual Integrations
 APPROVED

Sohil
 2/2/2018 4:39:20 PM

Quant Time: Feb 02 02:43:28 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 02 01:03:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	88166	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	355579	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	230421	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	530220	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	581976	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	610915	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	9092	4.73	ng/uL	0.00
5) Phenol-d5	6.75	99	150328	22.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	98411	24.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	129925	24.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	133538	24.07	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	68067	26.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	74581	26.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	138228	23.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	161712	31.22	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	516249	27.00	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	620629	26.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	47052m	17.85	ng/ul	0.01
57) Fluorene-d10	15.22	176	452053	26.41	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	59065m	18.14	ng/ul	0.00
70) Anthracene-d10	17.07	188	705422	27.40	ng/ul	0.00
76) Pyrene-d10	19.37	212	813499	29.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.21	264	810971	27.05	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.68	163	83626	4.536	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020118\
Data File : BM014083.D
Acq On : 01 Feb 2018 20:58
Operator : SJ/JU
Sample : J1316-13
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6D36

Quant Time: Feb 02 02:43:28 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 02 01:03:24 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
2/2/2018 4:39:20 PM

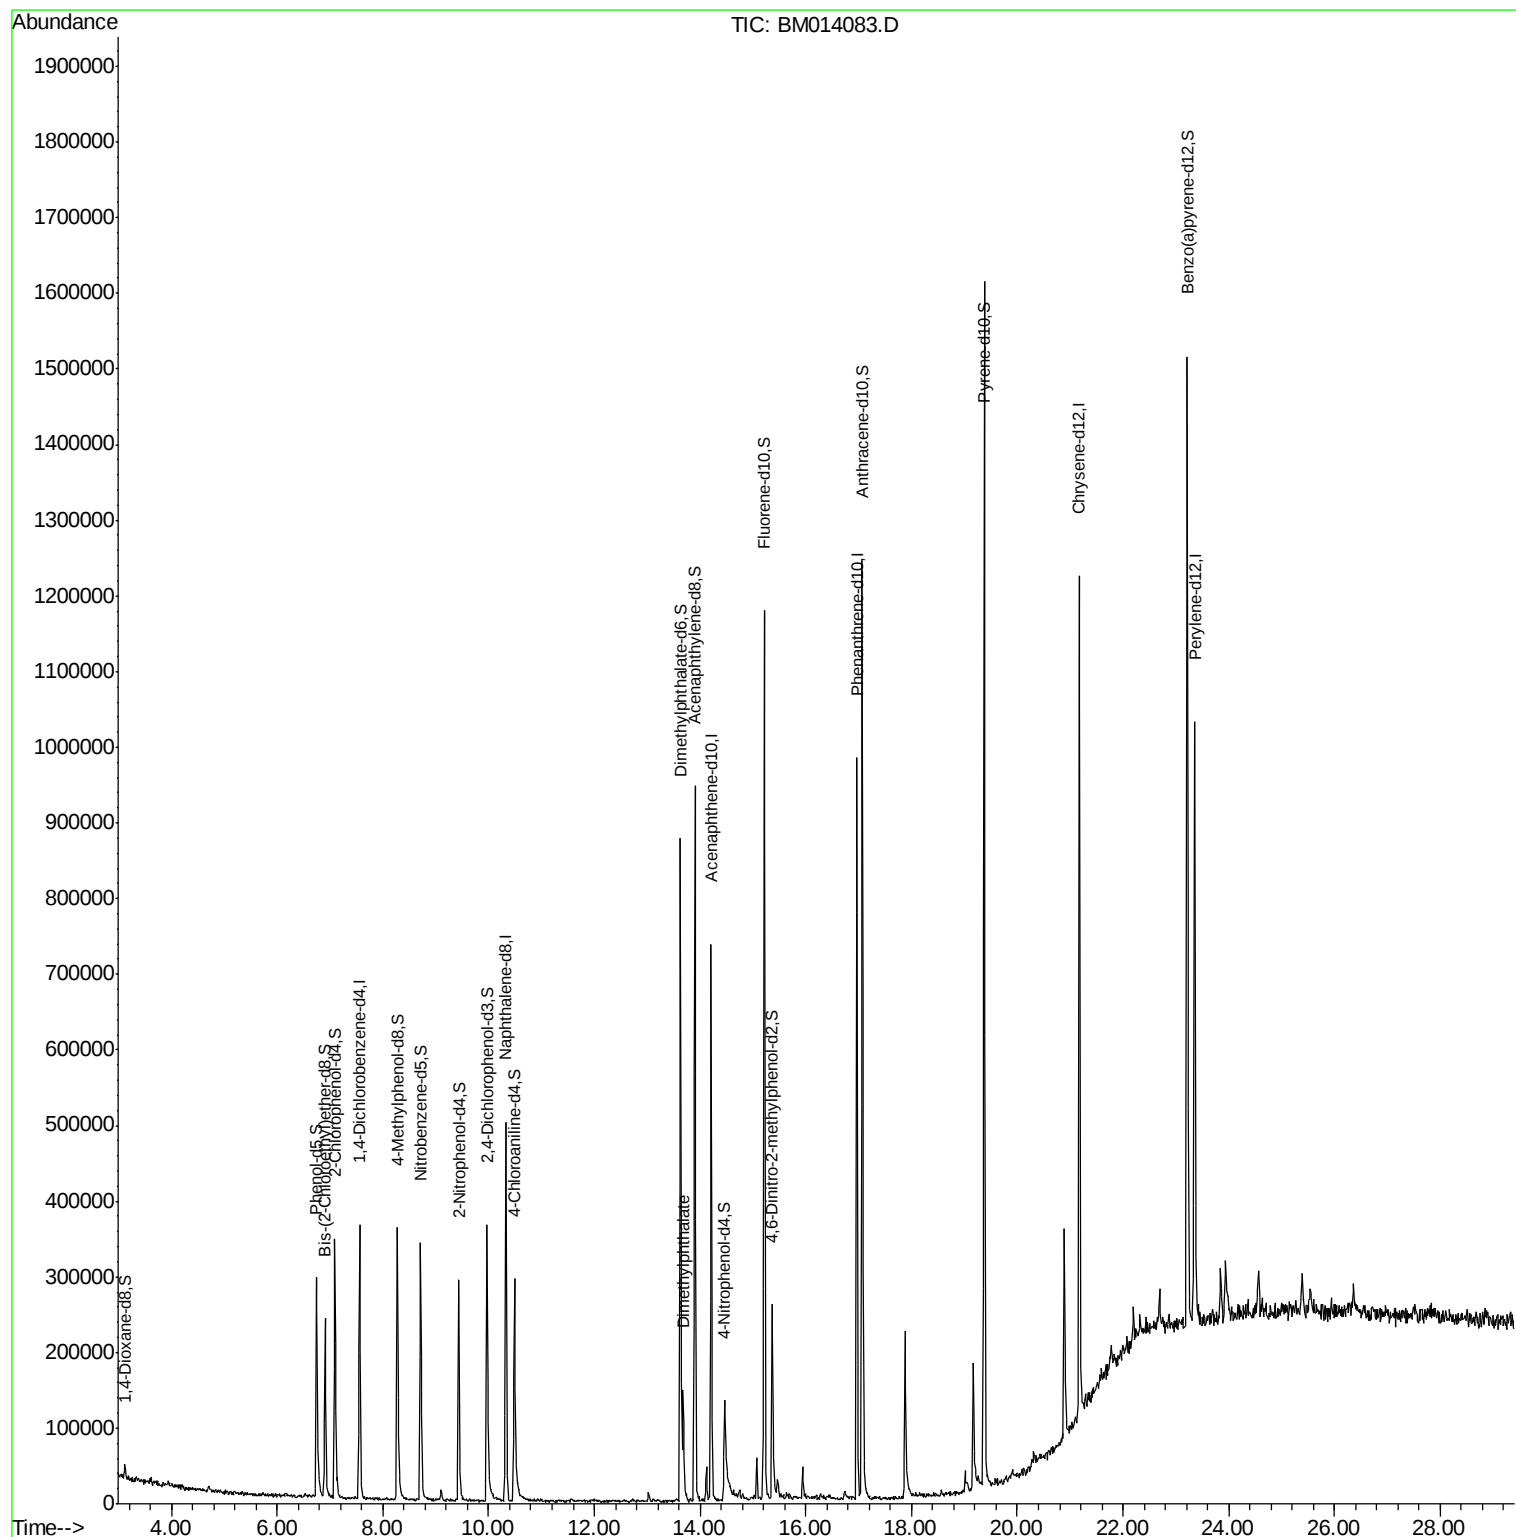

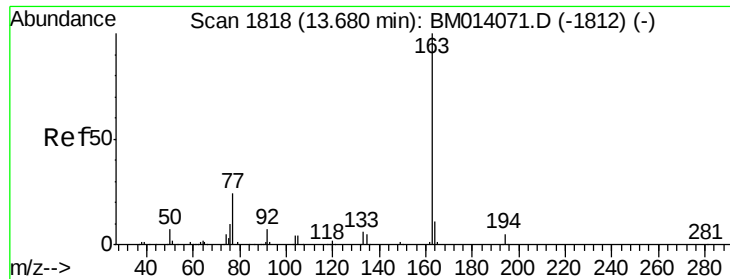

#44
 Dimethylphthalate
 Concen: 4.536 ng/ul
 RT: 13.68 min Scan# 1818
 Delta R.T. 0.00 min
 Lab File: BM014083.D
 Acq: 01 Feb 2018 20:58

Instrument :
 BNA_M
 ClientSampleId :
 F6D36

Tot Ion	Ratio	Resp	Lower	Upper
163	100	83626		
194	4.2		3.5	5.3
164	12.1		8.2	12.4

Manual Integrations
 APPROVED

Sohil
 2/2/2018 4:39:20 PM

