

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043956.D
 Acq On : 01 Feb 2024 21:16
 Operator : MA/JU
 Sample : PB158662BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK662

Quant Time: Feb 01 23:55:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	9350	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	27770	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.567	164	14178	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.415	188	2055447	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.52
23) Perylene-d12	23.922	264	30864	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.365	96	72566	6.032	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	11787	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	21706	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.561	166	3937	0.067	ng/ul#	14
26) Benzo(a)pyrene	23.773	252	7370	0.069	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043956.D
Acq On : 01 Feb 2024 21:16
Operator : MA/JU
Sample : PB158662BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK662

Quant Time: Feb 01 23:55:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration




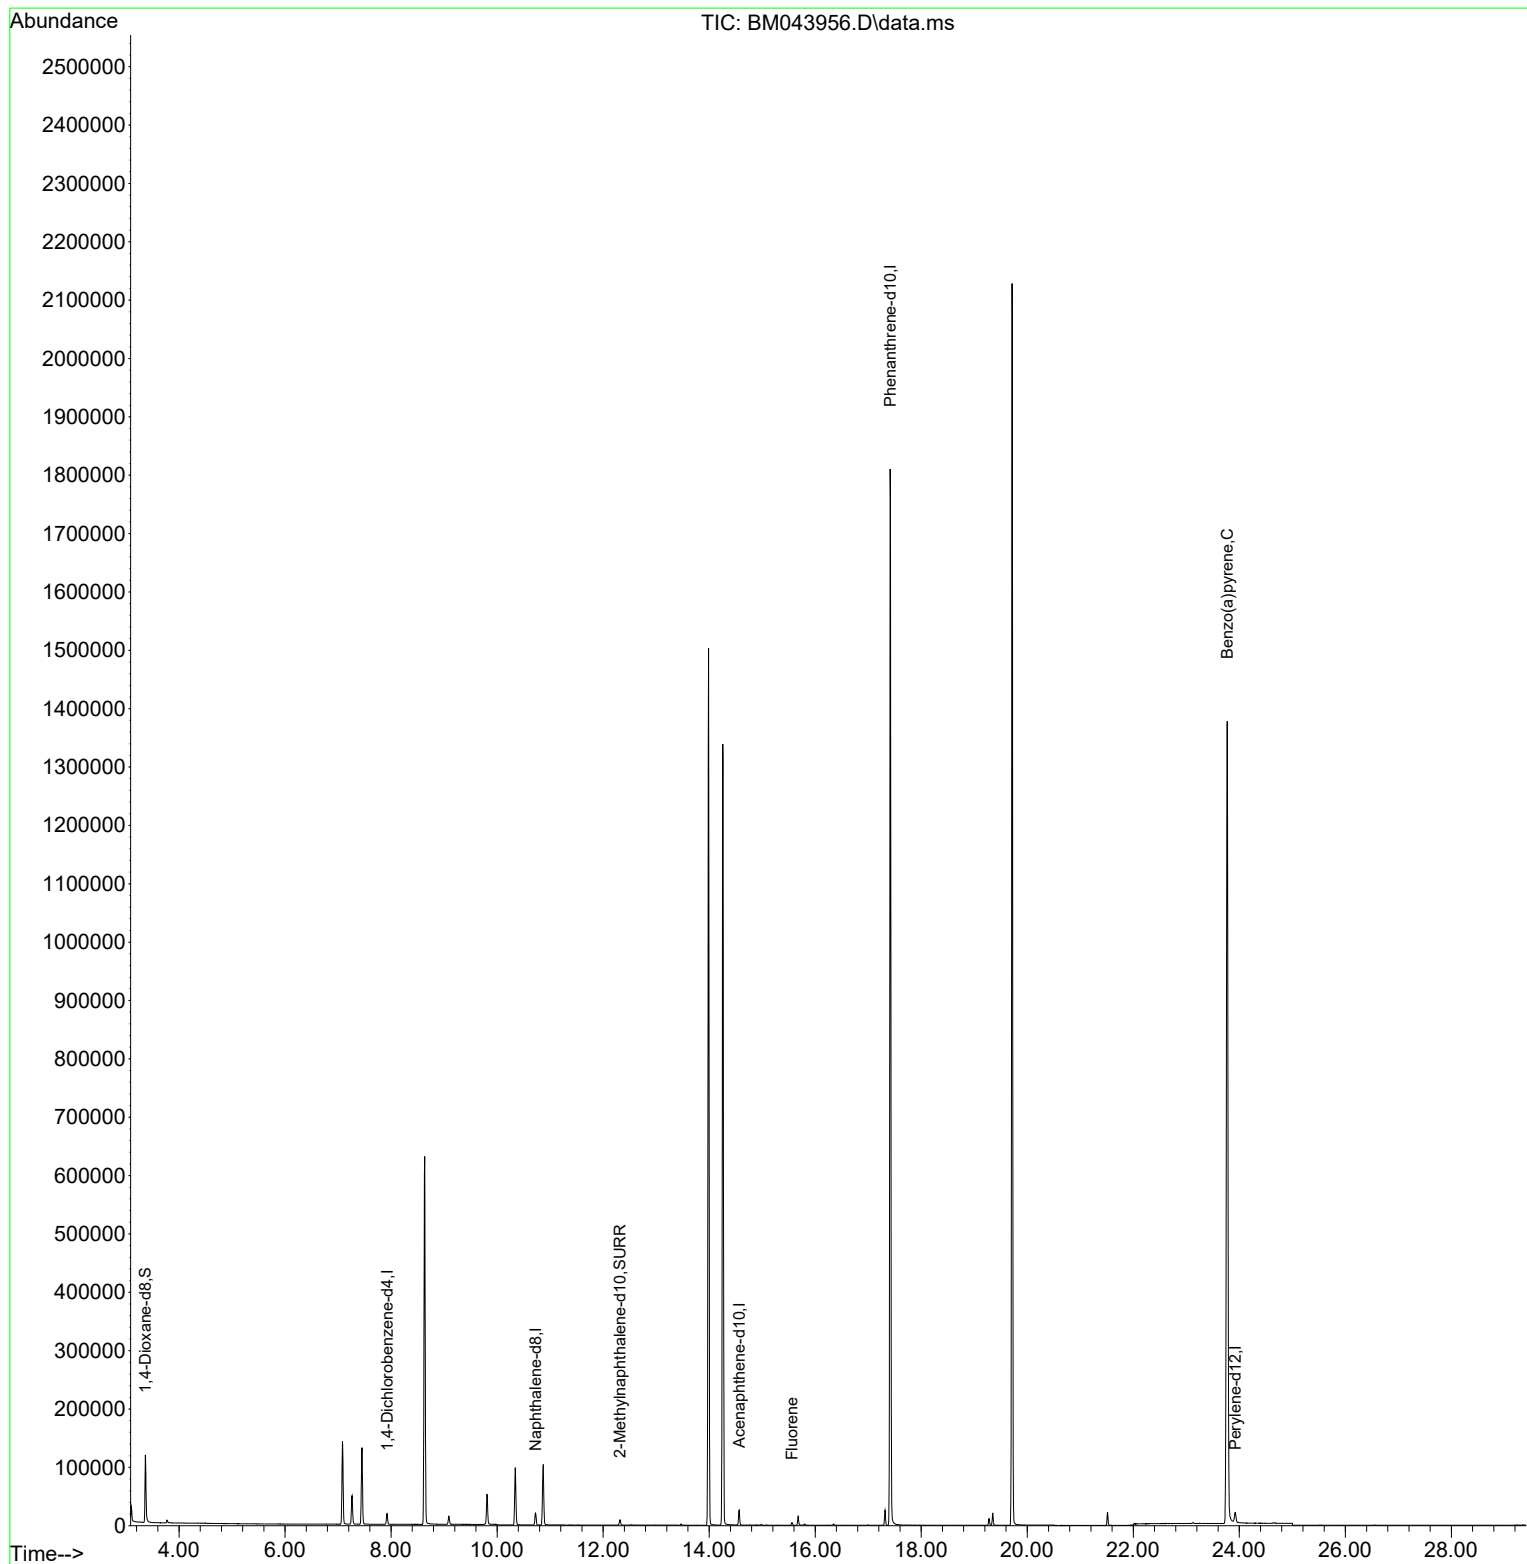


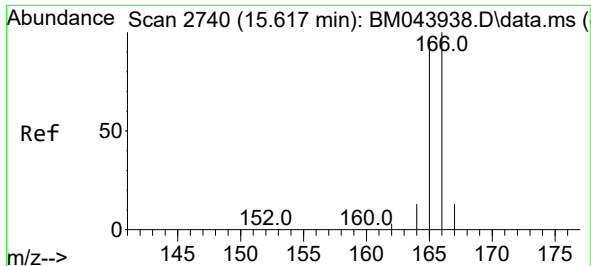

#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.561 min Scan# 21
Delta R.T. -0.055 min
Lab File: BM043956.D
Acq: 01 Feb 2024 21:16

Instrument :
BNA_M
ClientSampleId :
SBLK662

Tgt Ion:166 Resp: 3937
Ion Ratio Lower Upper
166 100
165 8.2 79.5 119.3#
167 31.5 10.9 16.3#

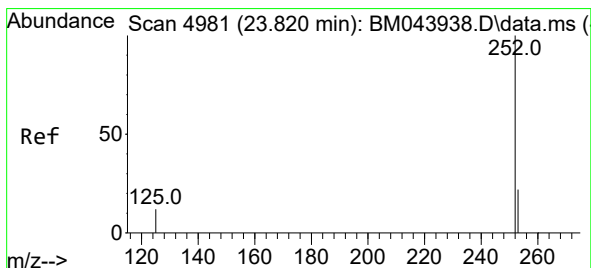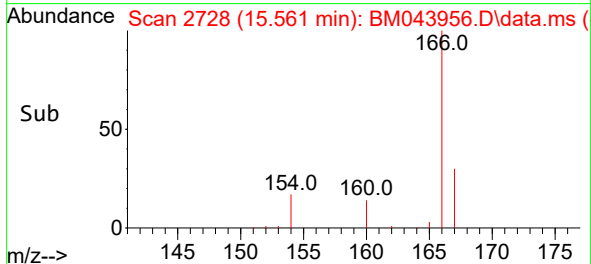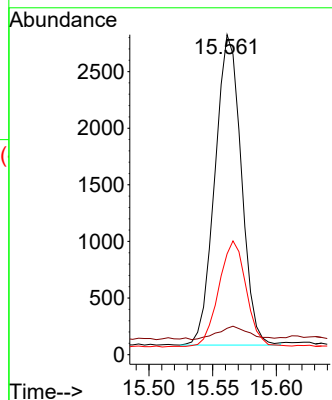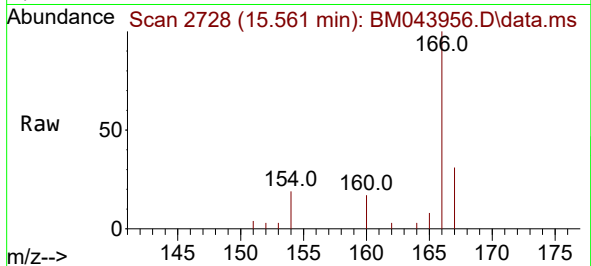

#26
Benzo(a)pyrene
Concen: 0.069 ng/ul
RT: 23.773 min Scan# 4965
Delta R.T. -0.048 min
Lab File: BM043956.D
Acq: 01 Feb 2024 21:16

Tgt Ion:252 Resp: 7370
Ion Ratio Lower Upper
252 100
253 43.0 20.6 31.0#
125 32.0 12.6 18.8#

