

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043957.D
 Acq On : 01 Feb 2024 21:52
 Operator : MA/JU
 Sample : PB158664BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK664

Quant Time: Feb 01 23:55:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	8827	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	25756	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.566	164	12867	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.415	188	1964212	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.52
23) Perylene-d12	23.925	264	27615	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.365	96	73022	6.429	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	11379	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	20399	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.561	166	3744	0.071	ng/ul#	14
26) Benzo(a)pyrene	23.773	252	6984	0.073	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043957.D
Acq On : 01 Feb 2024 21:52
Operator : MA/JU
Sample : PB158664BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK664

Quant Time: Feb 01 23:55:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration




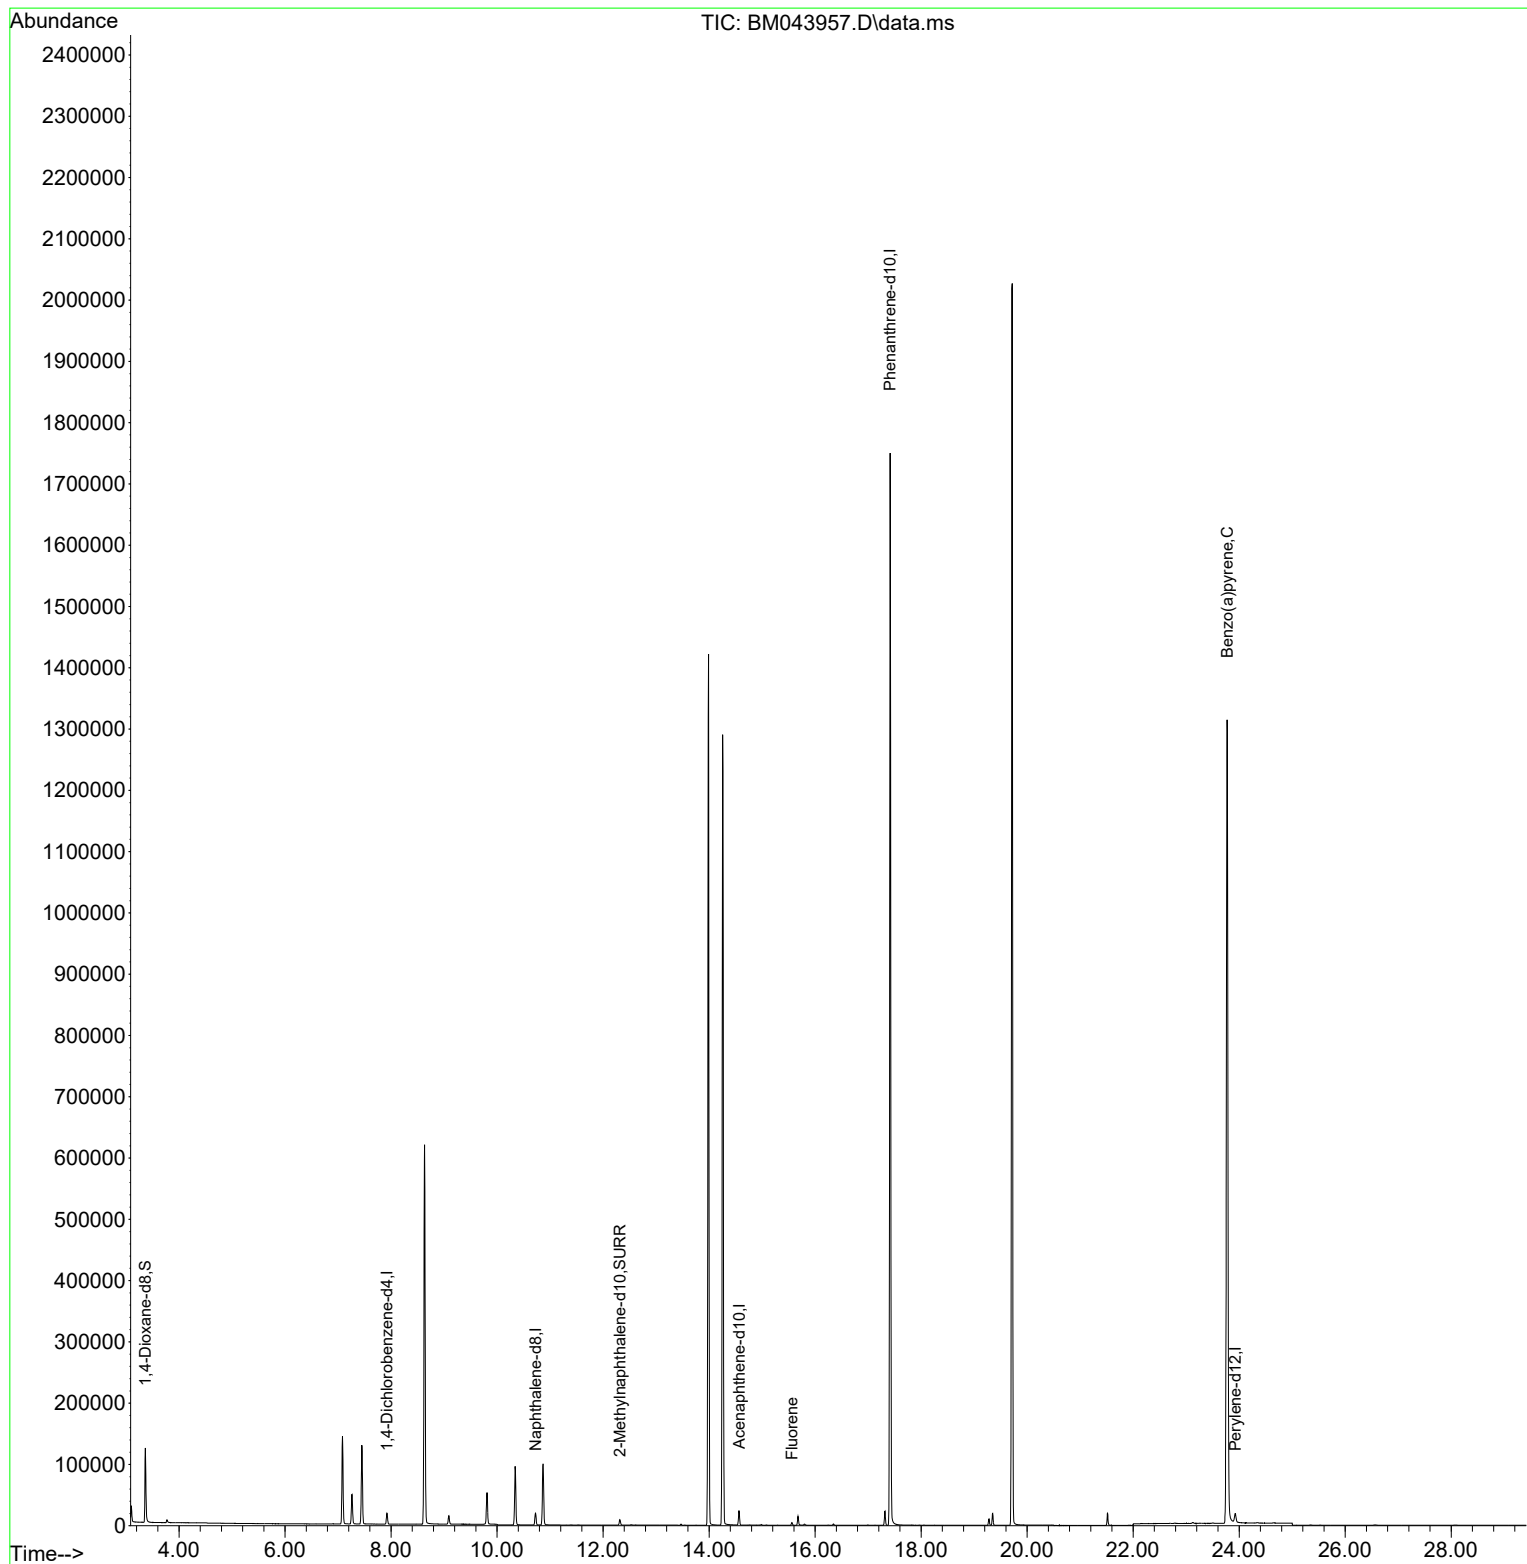


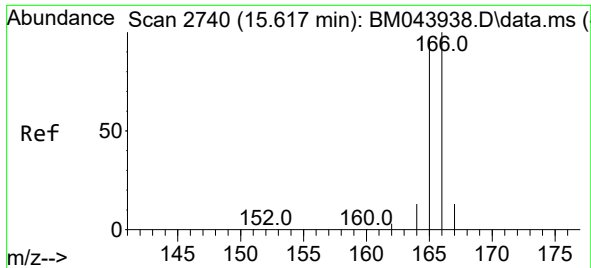

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.561 min Scan# 21
Delta R.T. -0.055 min
Lab File: BM043957.D
Acq: 01 Feb 2024 21:52

Instrument :
BNA_M
ClientSampleId :
SBLK664

Tgt Ion:166 Resp: 3744
Ion Ratio Lower Upper
166 100
165 8.6 79.5 119.3#
167 34.2 10.9 16.3#

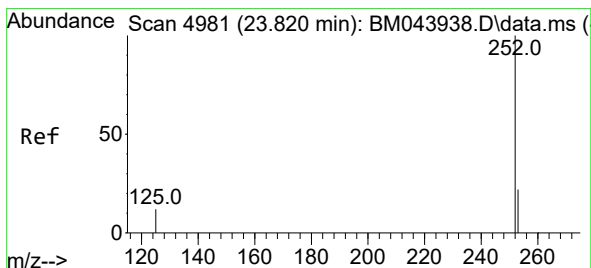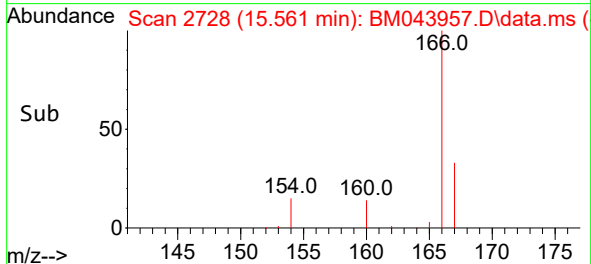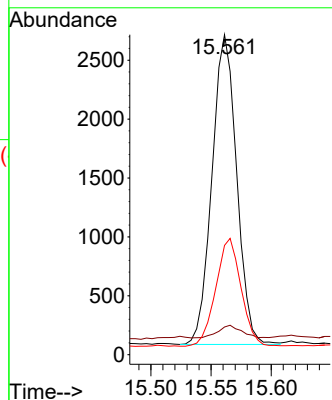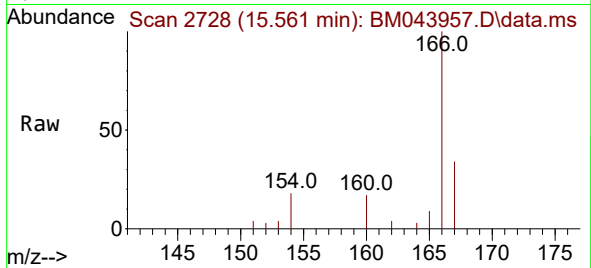

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.773 min Scan# 4965
Delta R.T. -0.048 min
Lab File: BM043957.D
Acq: 01 Feb 2024 21:52

Tgt Ion:252 Resp: 6984
Ion Ratio Lower Upper
252 100
253 43.4 20.6 31.0#
125 33.5 12.6 18.8#

