




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043939.D
Acq On : 01 Feb 2024 10:21
Operator : MA/JU
Sample : PB158633BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK633

Manual IntegrationsAPPROVED

Quant Time: Feb 01 10:50:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

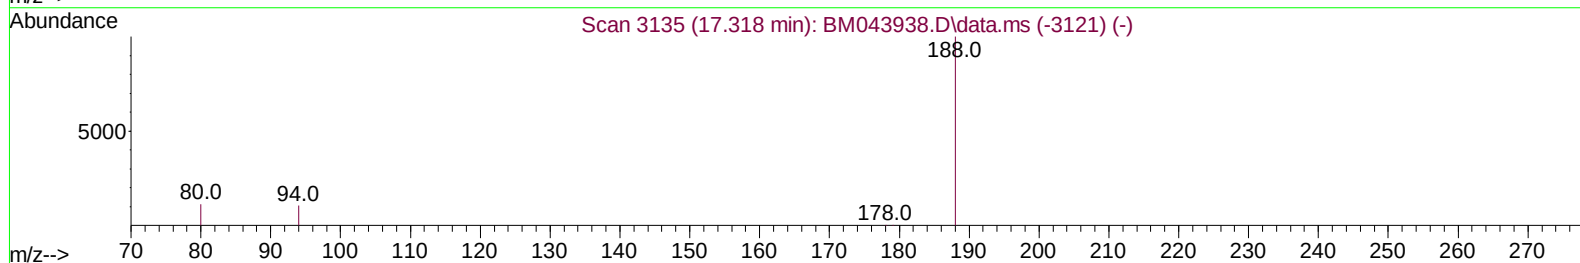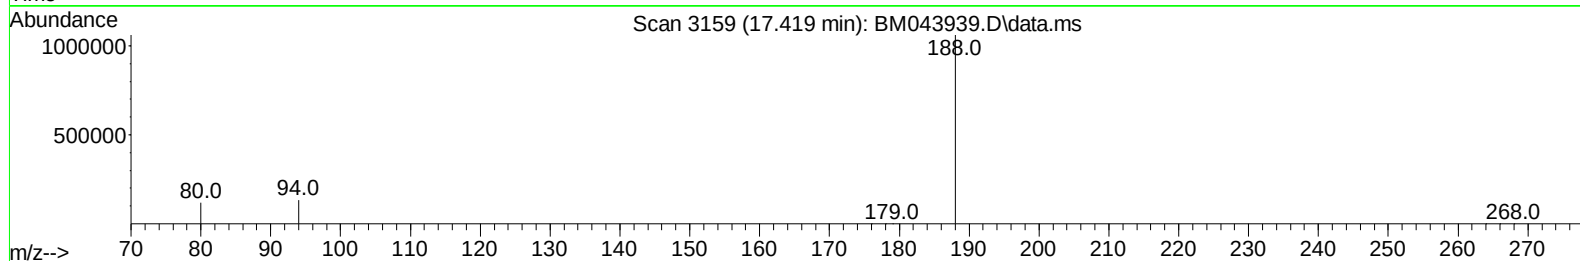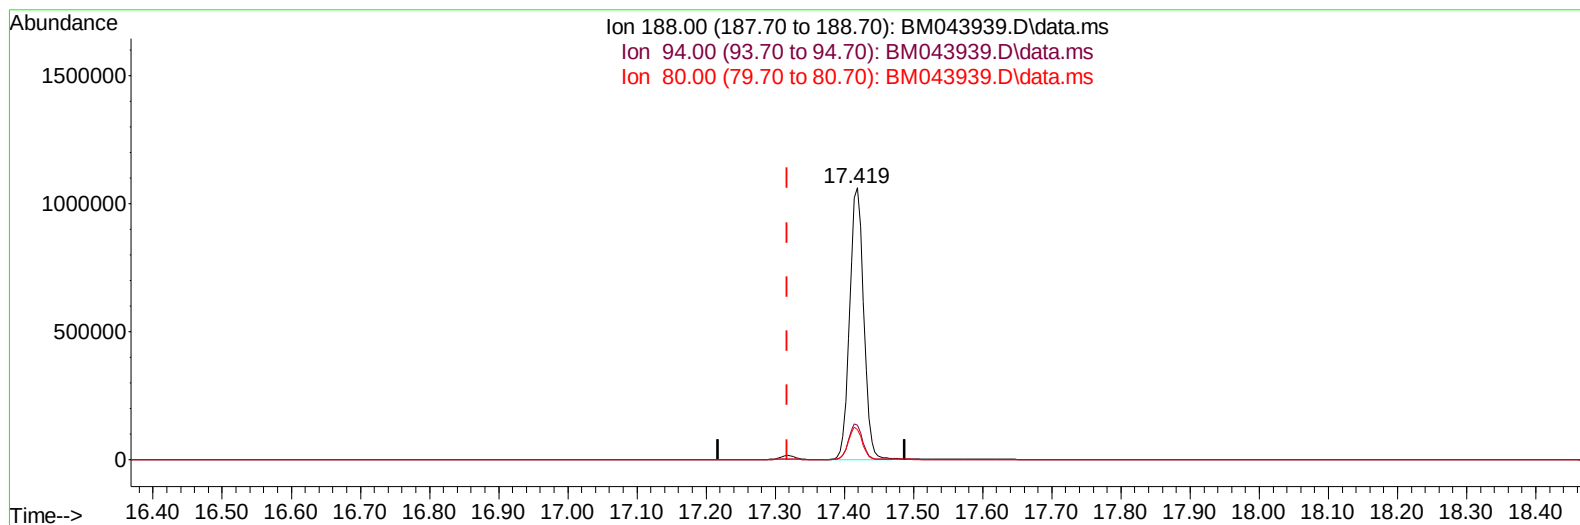

TIC: BM043939.D\data.ms

(13) Phenanthrene-d10 (I)

17.419min (+ 0.101) 0.40 ng/u1

response 1483500

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	12.61
80.00	12.90	11.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043939.D
Acq On : 01 Feb 2024 10:21
Operator : MA/JU
Sample : PB158633BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK633

Manual IntegrationsAPPROVED

Quant Time: Feb 01 10:50:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

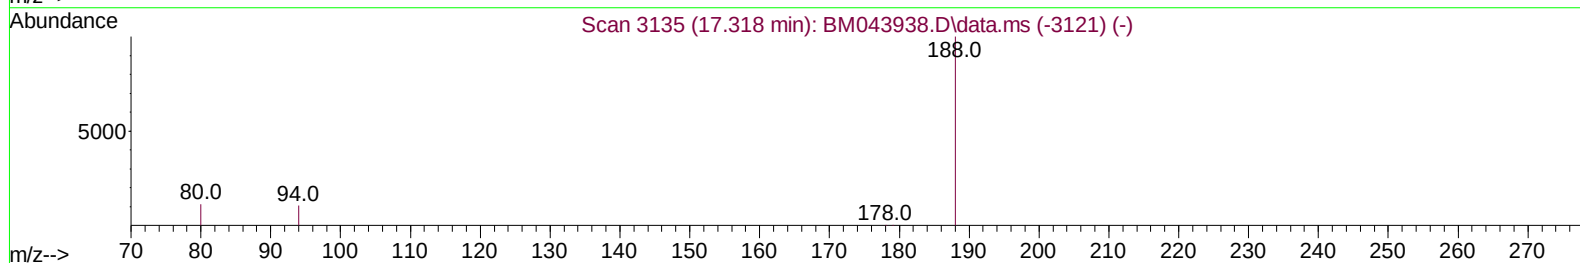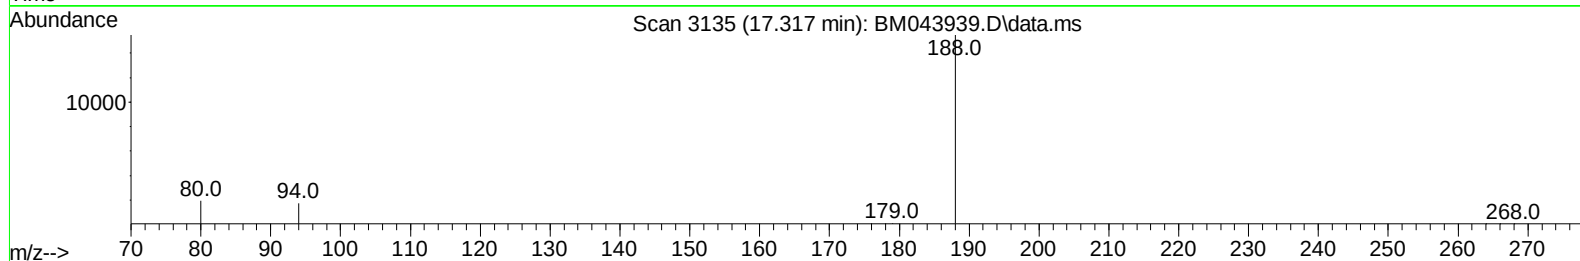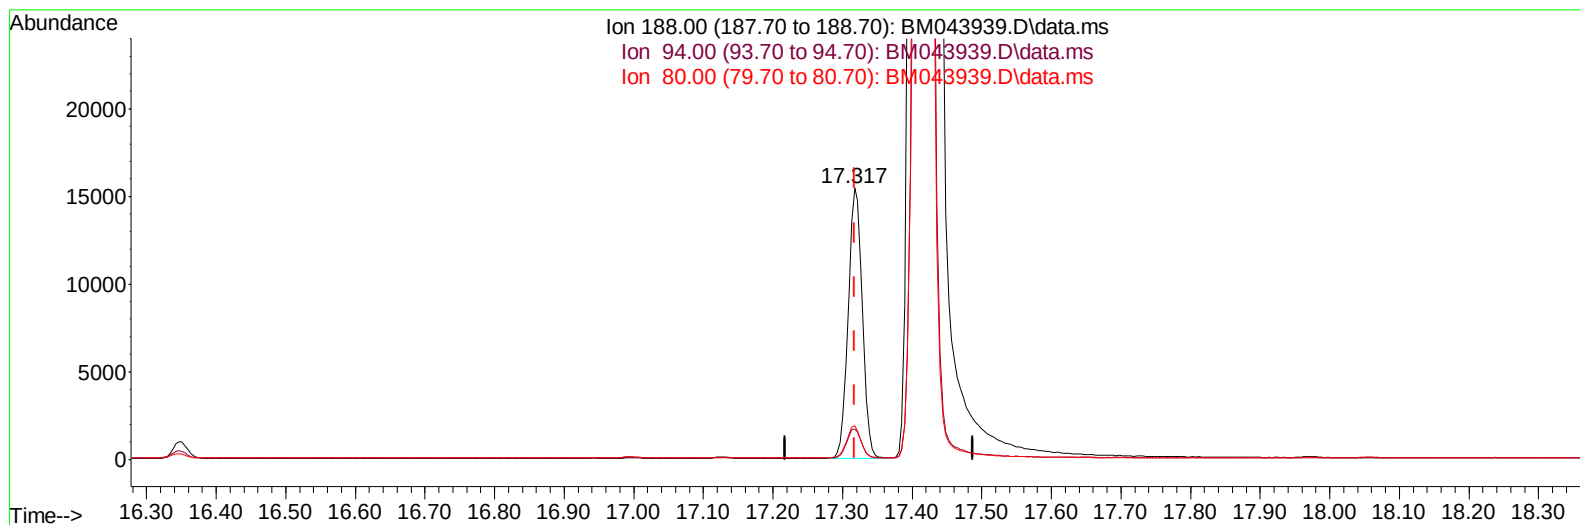

TIC: BM043939.D\data.ms

(13) Phenanthrene-d10 (I)

17.317min (-0.000) 0.40 ng/ul m

response 21663

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	11.27
80.00	12.90	12.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043939.D
Acq On : 01 Feb 2024 10:21
Operator : MA/JU
Sample : PB158633BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK633

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 10:50:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

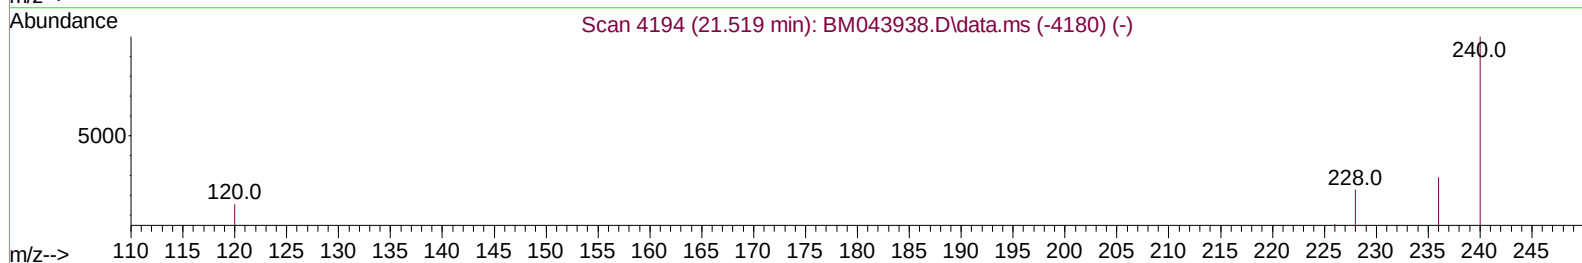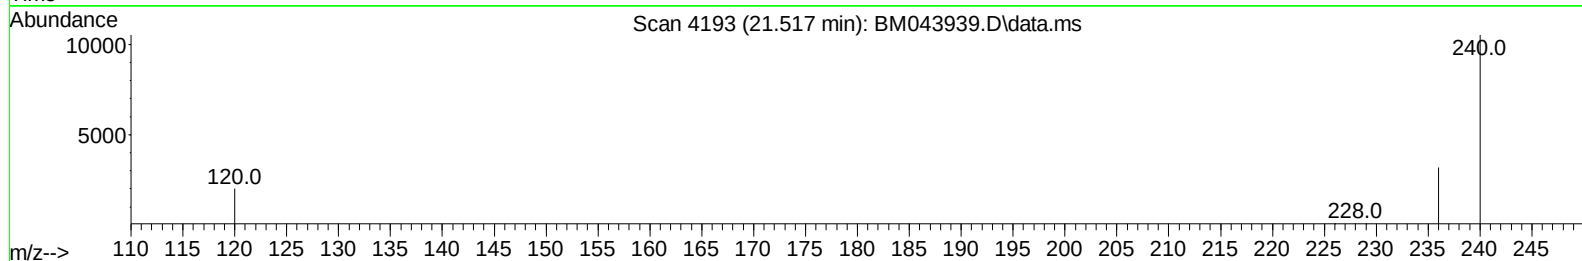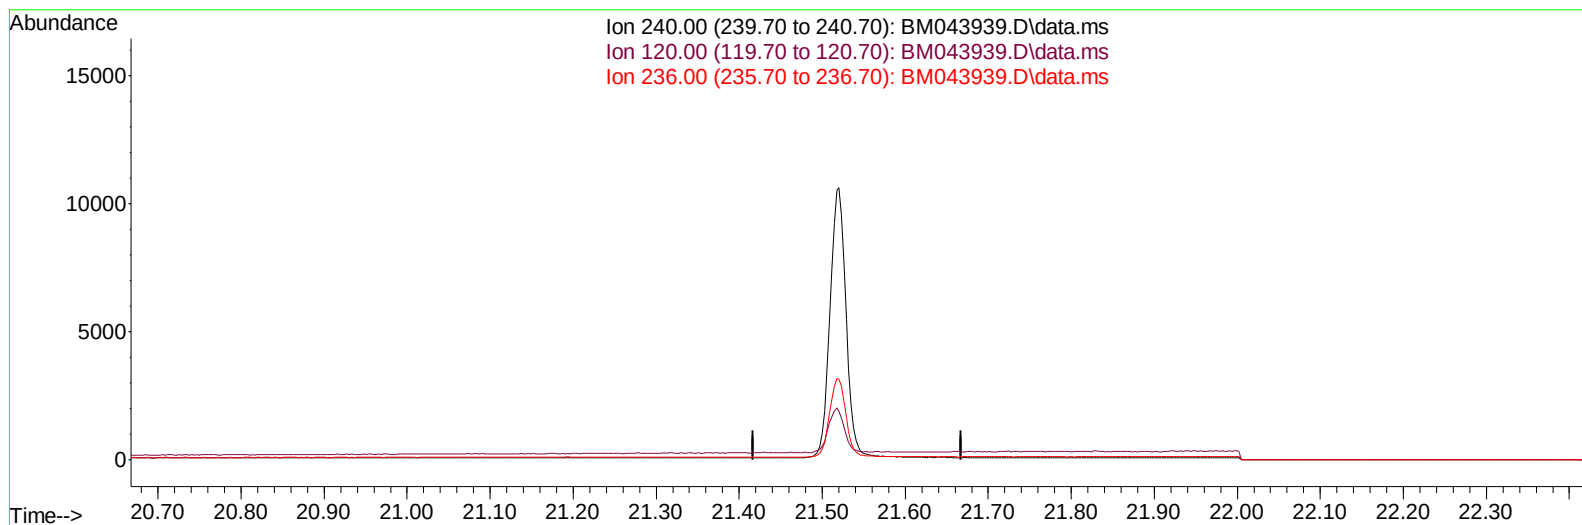

TIC: BM043939.D\data.ms

(17) Chrysene-d12

21.517min (-21.517) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	17.60	0.00#
236.00	29.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043939.D
Acq On : 01 Feb 2024 10:21
Operator : MA/JU
Sample : PB158633BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK633

Manual IntegrationsAPPROVED

Quant Time: Feb 01 10:50:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

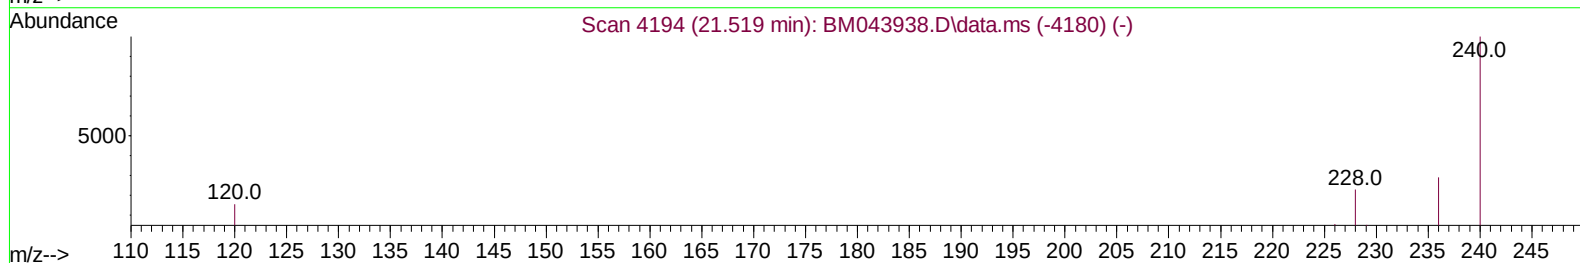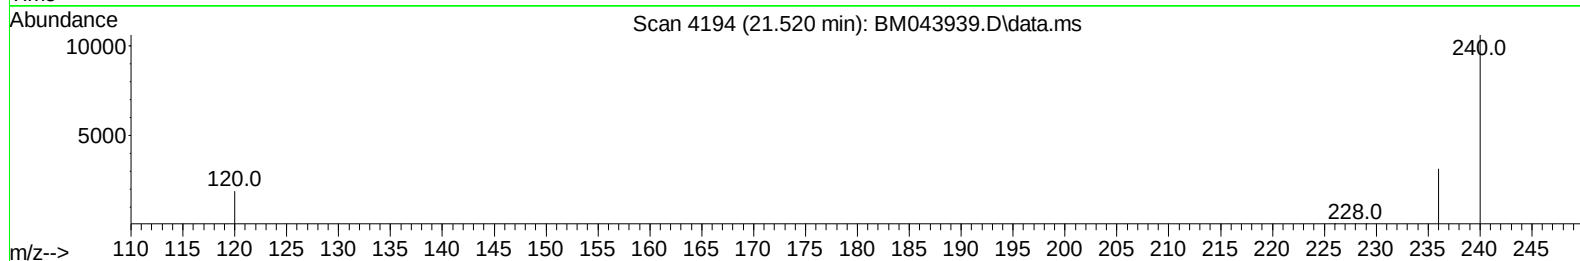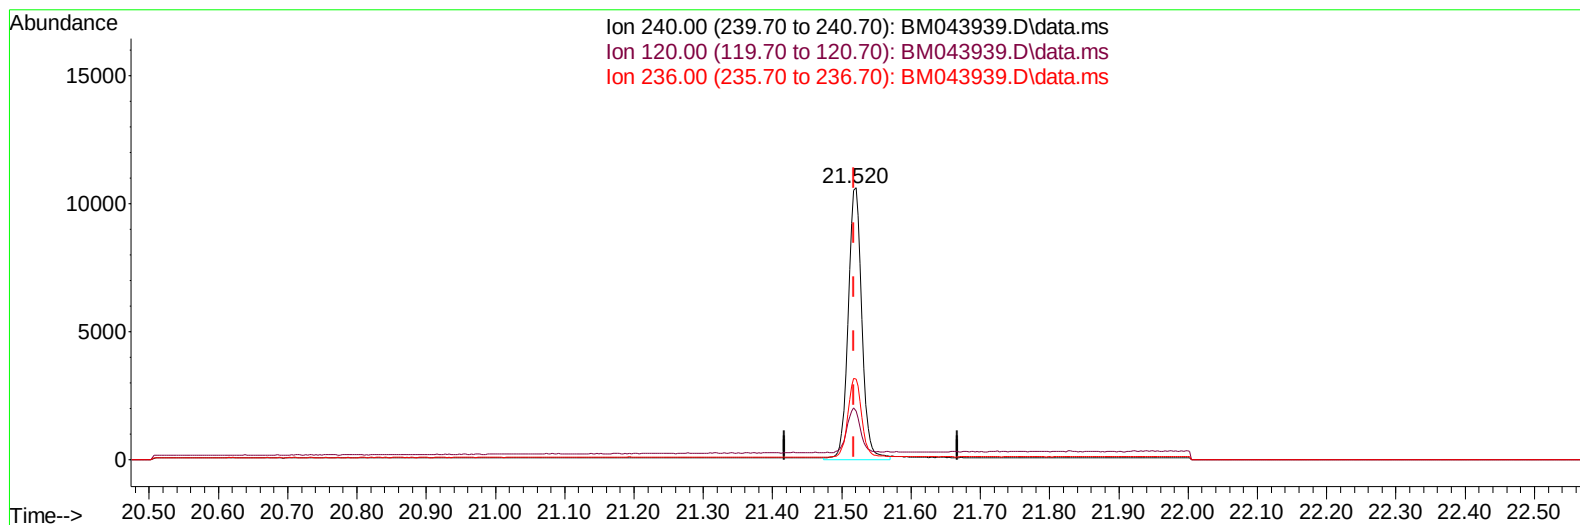

TIC: BM043939.D\data.ms

(17) Chrysene-d12

21.520min (+ 0.003) 0.40 ng/ul m

response 14565

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	17.60	17.88
236.00	29.90	29.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043939.D
Acq On : 01 Feb 2024 10:21
Operator : MA/JU
Sample : PB158633BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK633

Manual IntegrationsAPPROVED

Quant Time: Feb 01 10:50:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

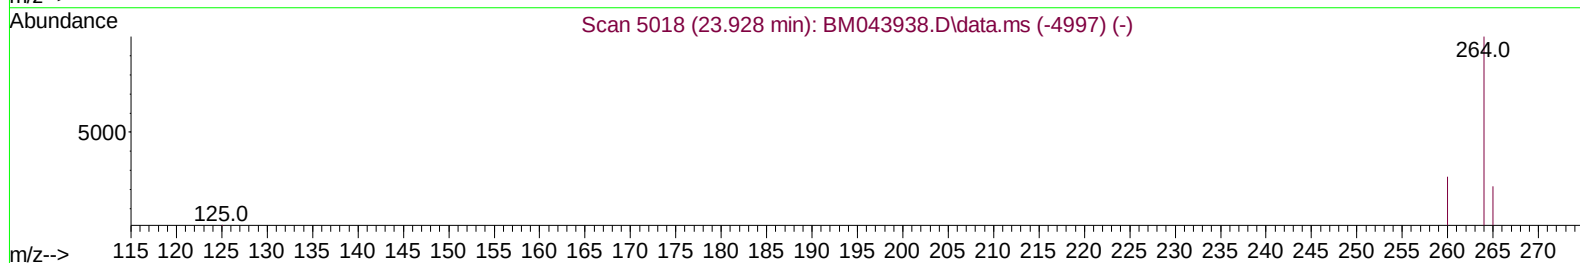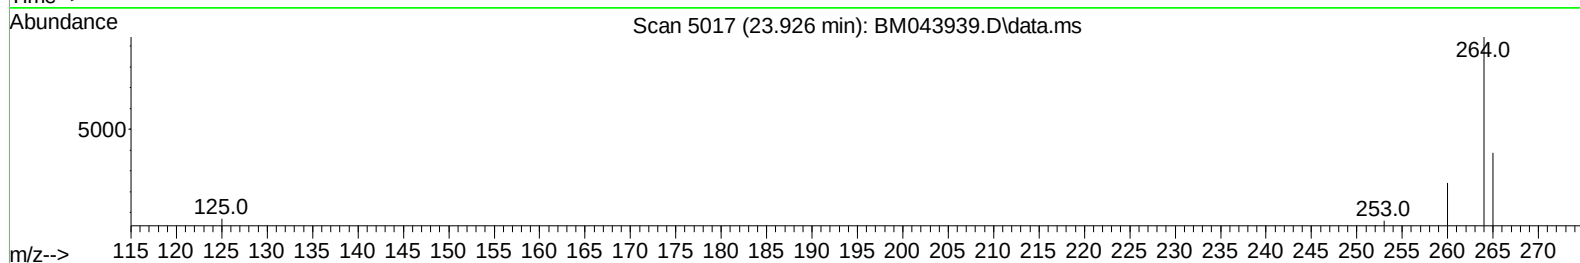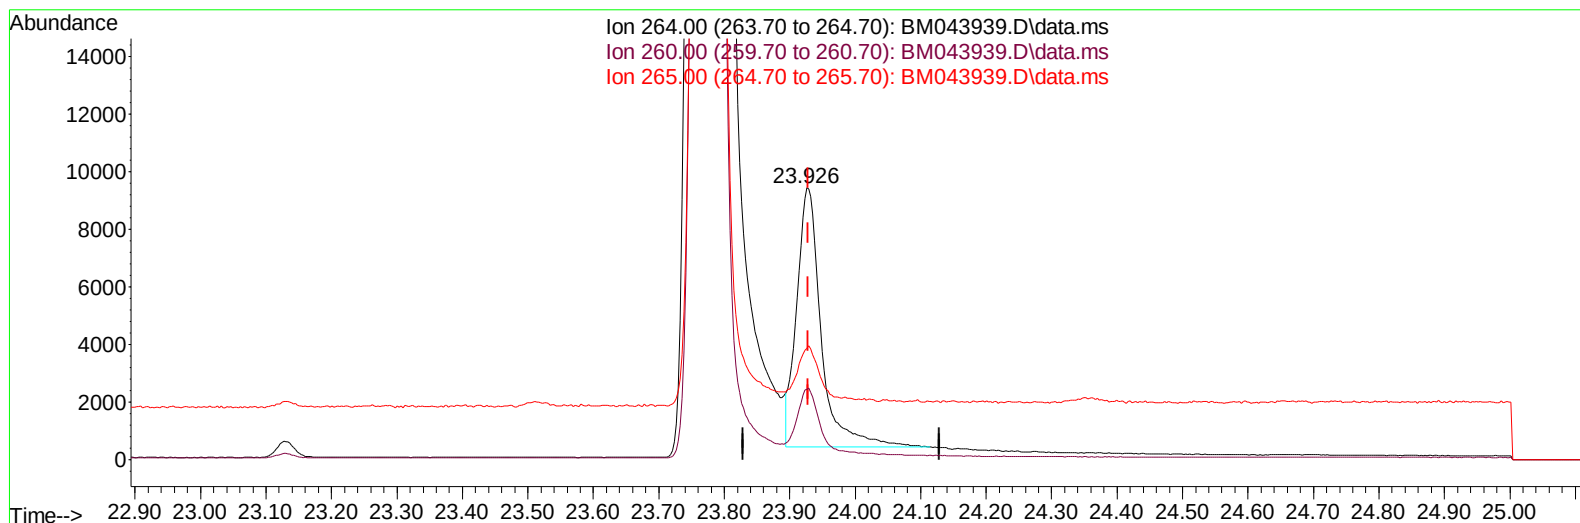

TIC: BM043939.D\data.ms

(23) Perylene-d12 (I)

23.926min (-0.003) 0.40 ng/u1

response 23615

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	25.74
265.00	42.60	40.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043939.D
Acq On : 01 Feb 2024 10:21
Operator : MA/JU
Sample : PB158633BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK633

Manual IntegrationsAPPROVED

Quant Time: Feb 01 10:50:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

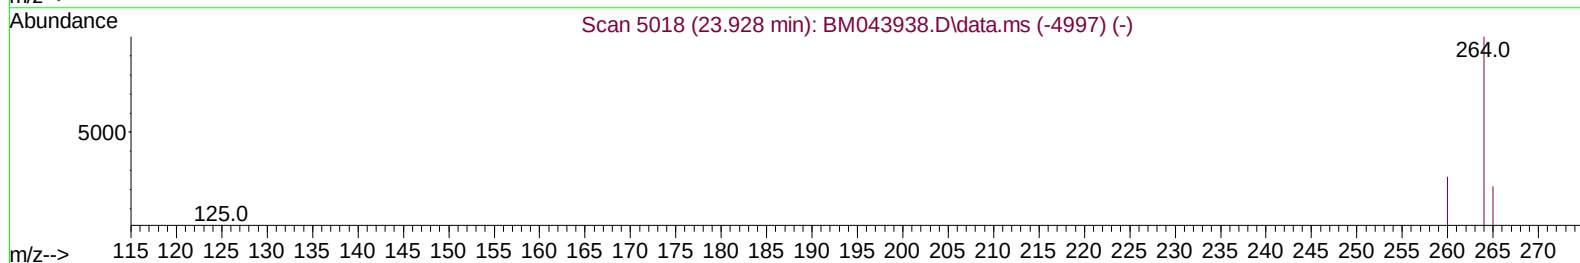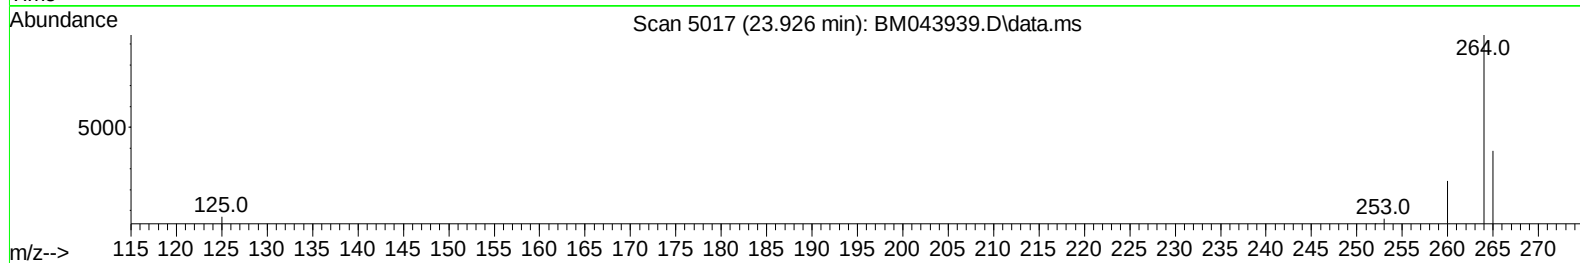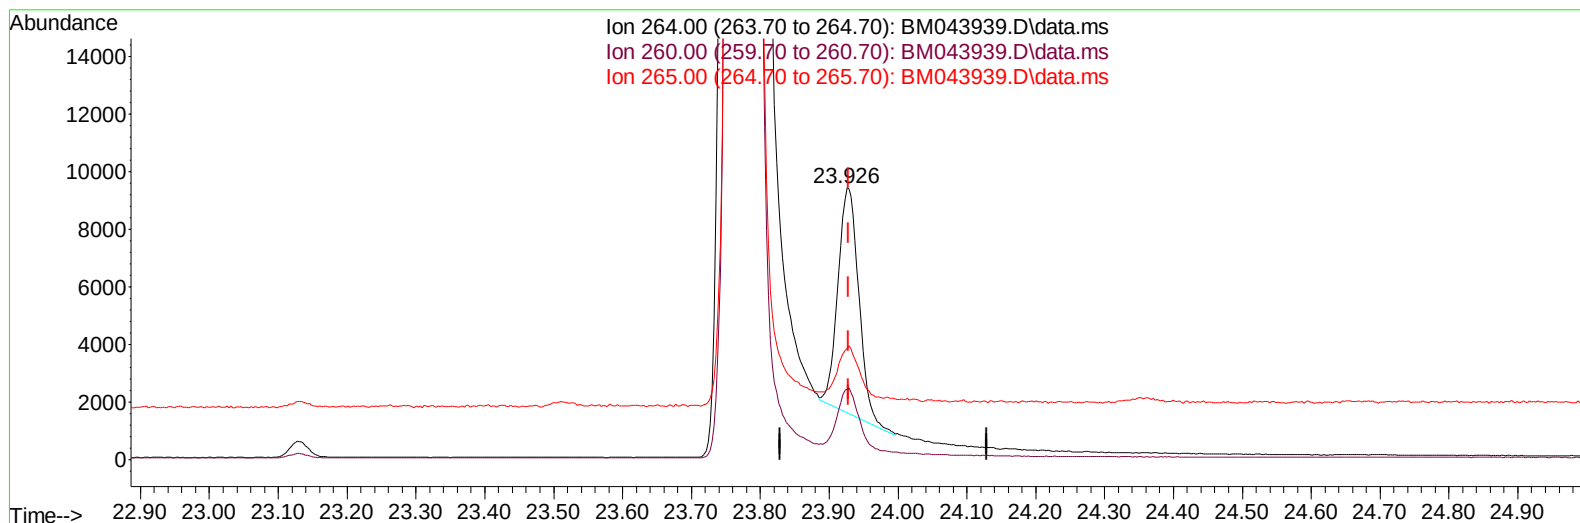

TIC: BM043939.D\data.ms

(23) Perylene-d12 (I)

23.926min (-0.003) 0.40 ng/ul m

response 16465

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	25.74
265.00	42.60	40.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043939.D
 Acq On : 01 Feb 2024 10:21
 Operator : MA/JU
 Sample : PB158633BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK633

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 10:50:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.921	152	8113	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	22791	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.566	164	10709	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.317	188	21663m	0.400	ng/ul	0.00
17) Chrysene-d12	21.520	240	14565m	0.400	ng/ul	0.00
23) Perylene-d12	23.926	264	16465m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.365	96	63065	6.041	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	9097	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	14991	0.328	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043939.D
Acq On : 01 Feb 2024 10:21
Operator : MA/JU
Sample : PB158633BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK633

Manual IntegrationsAPPROVED

Quant Time: Feb 01 10:50:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

