




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043940.D
Acq On : 01 Feb 2024 10:57
Operator : MA/JU
Sample : PB158635BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Manual IntegrationsAPPROVED

Quant Time: Feb 01 11:26:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

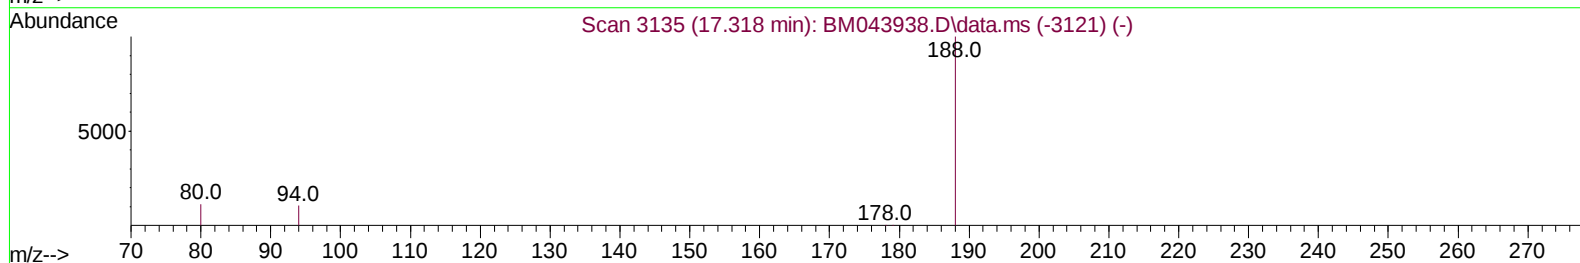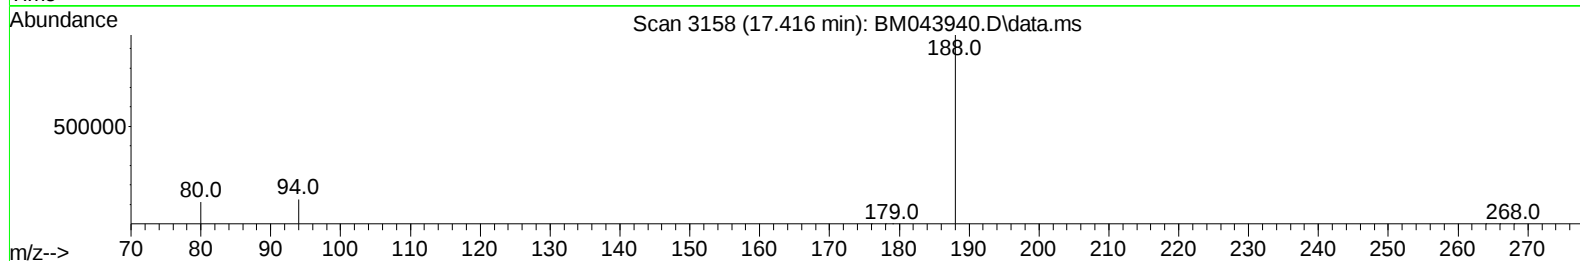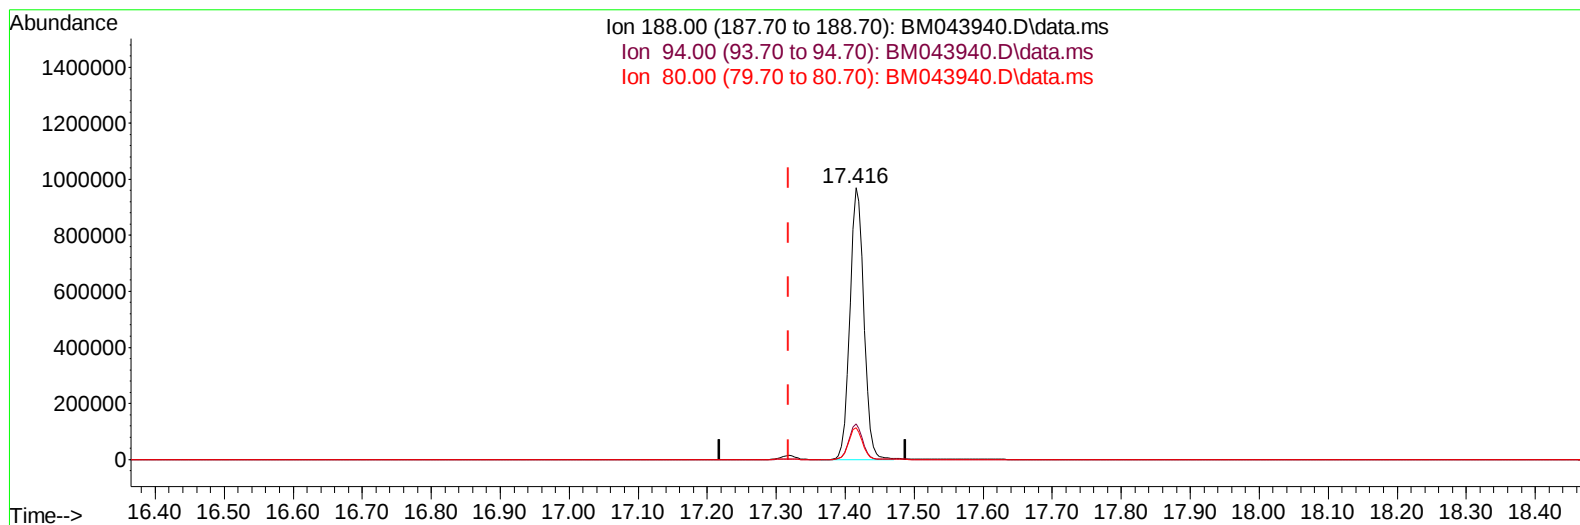

TIC: BM043940.D\data.ms

(13) Phenanthrene-d10 (I)

17.416min (+ 0.098) 0.40 ng/u1

response 1368382

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	13.07
80.00	12.90	11.61
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043940.D
Acq On : 01 Feb 2024 10:57
Operator : MA/JU
Sample : PB158635BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Manual IntegrationsAPPROVED

Quant Time: Feb 01 11:26:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

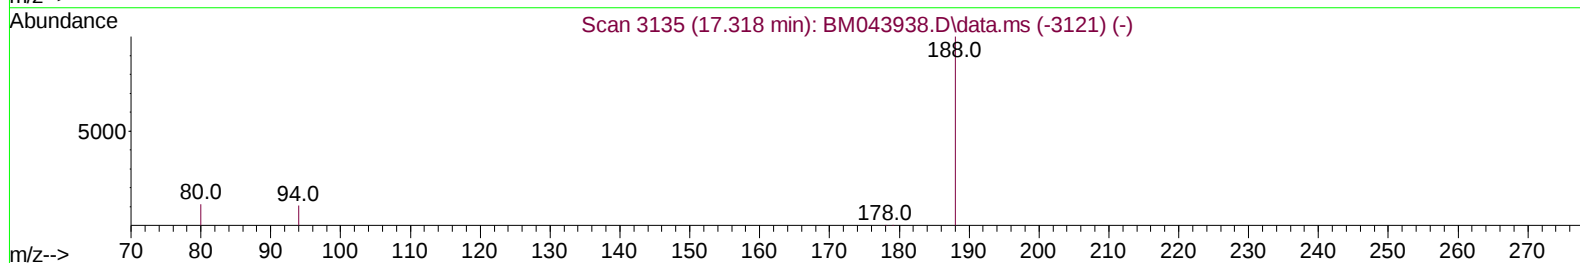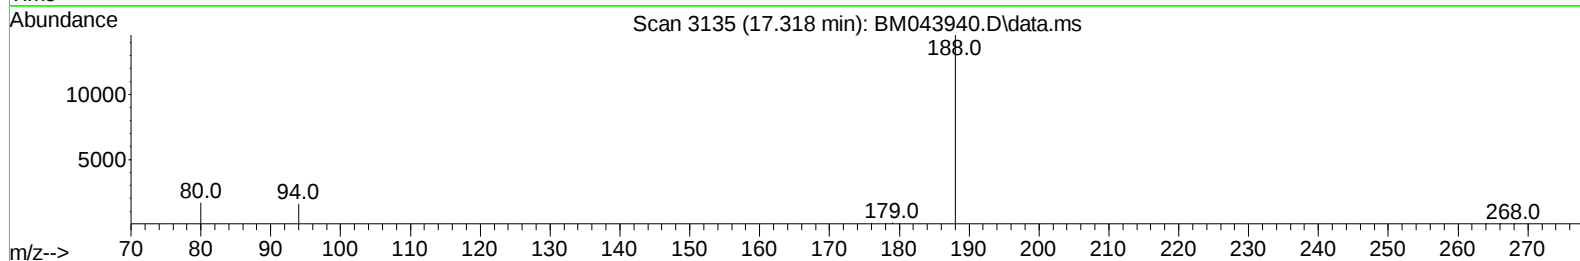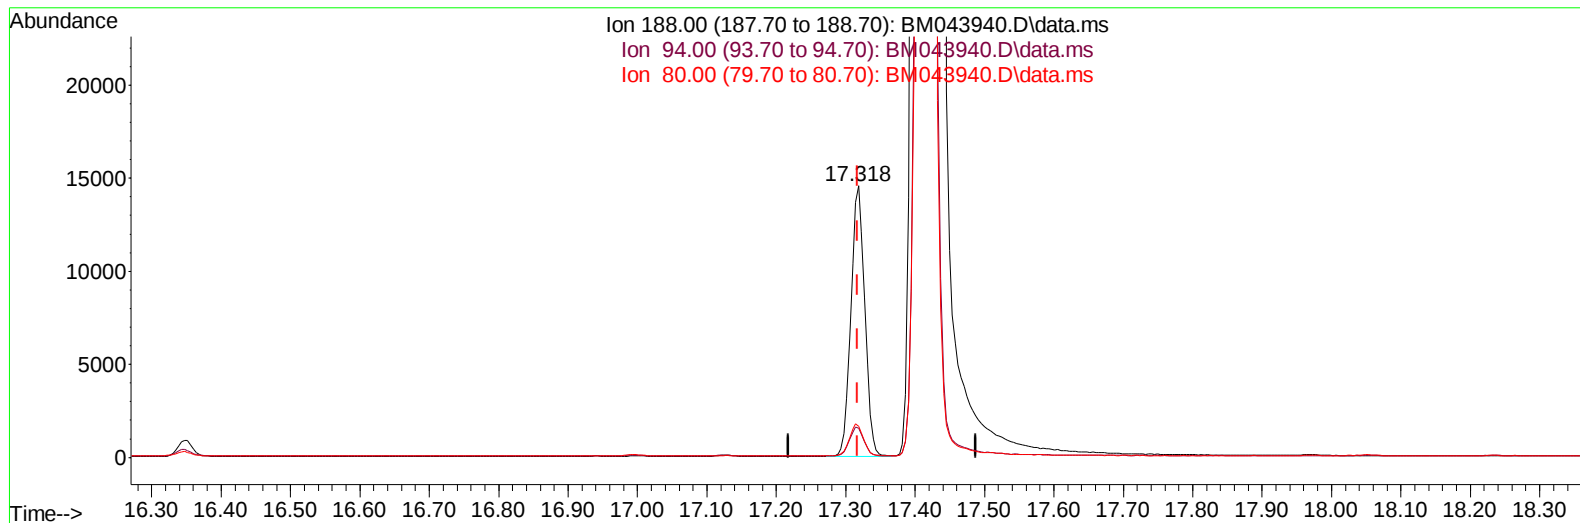

TIC: BM043940.D\data.ms

(13) Phenanthrene-d10 (I)

17.318min (+ 0.001) 0.40 ng/ul m

response 20091

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	10.79
80.00	12.90	11.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043940.D
Acq On : 01 Feb 2024 10:57
Operator : MA/JU
Sample : PB158635BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Manual IntegrationsAPPROVED

Quant Time: Feb 01 11:26:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

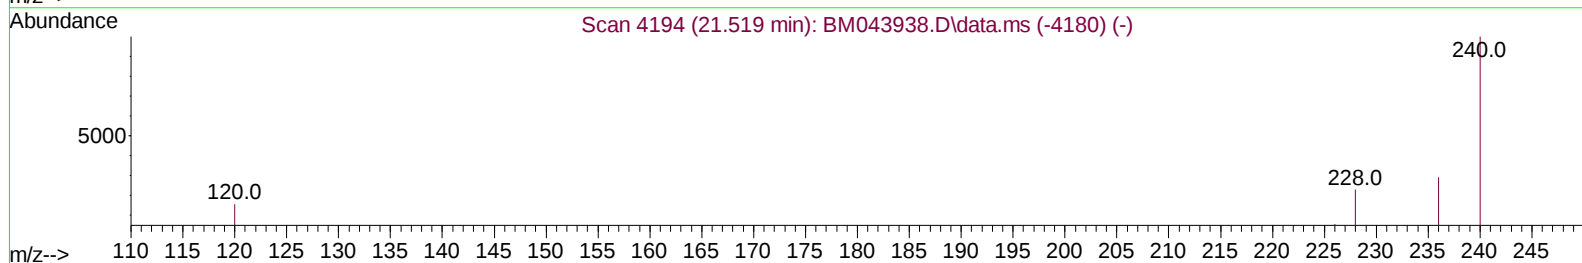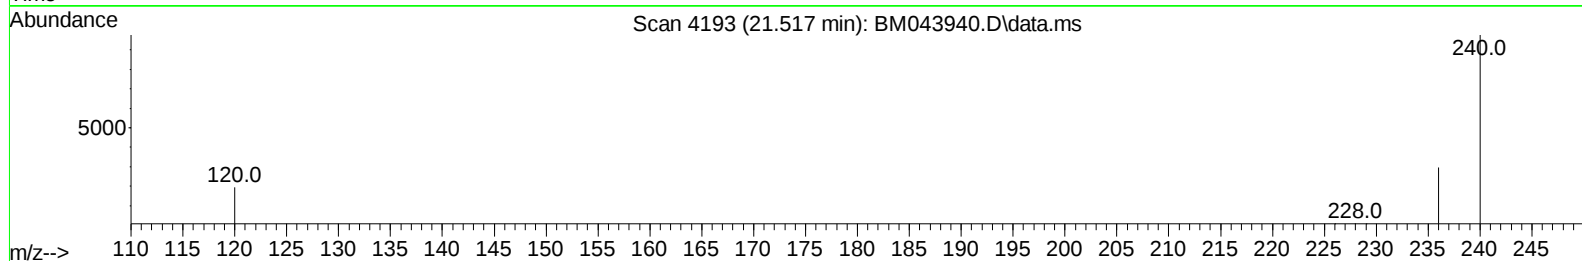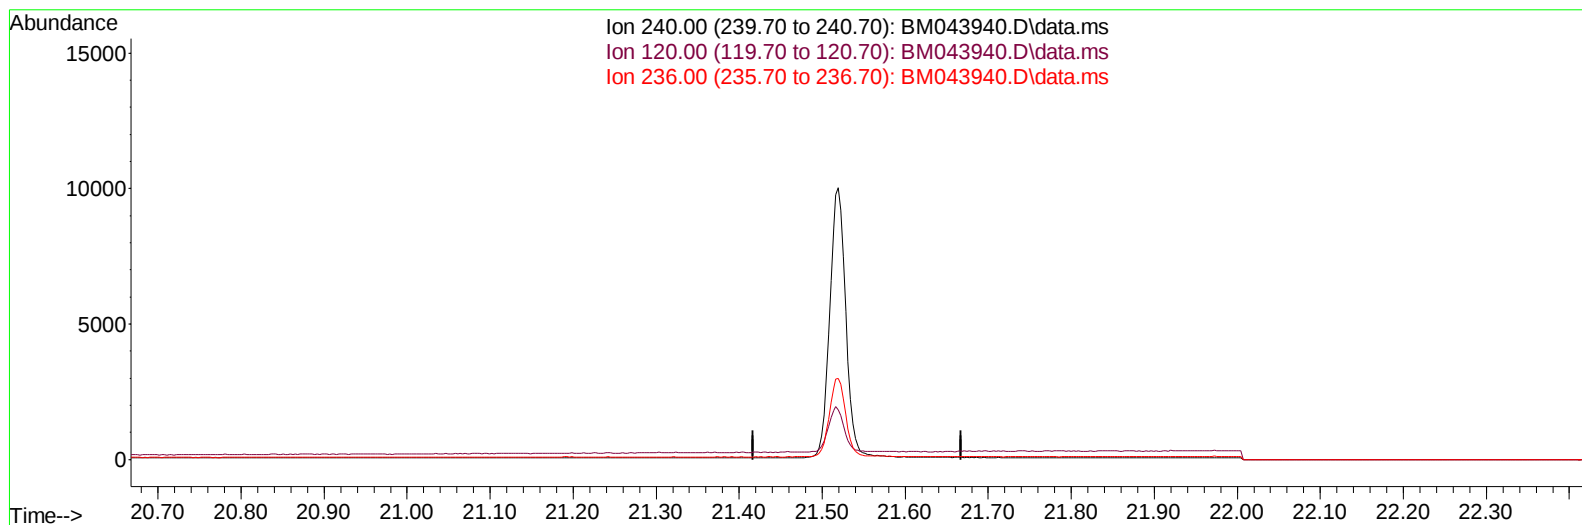

TIC: BM043940.D\data.ms

(17) Chrysene-d12

21.517min (-21.517) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	17.60	0.00#
236.00	29.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043940.D
Acq On : 01 Feb 2024 10:57
Operator : MA/JU
Sample : PB158635BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 11:26:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

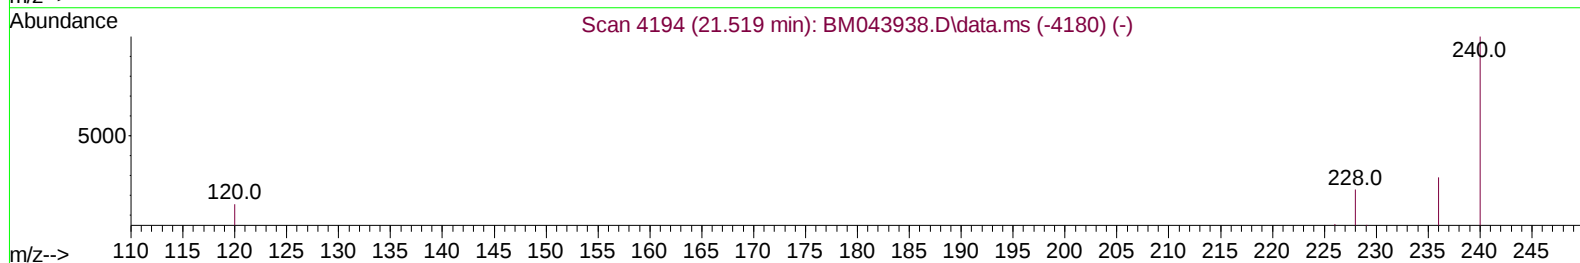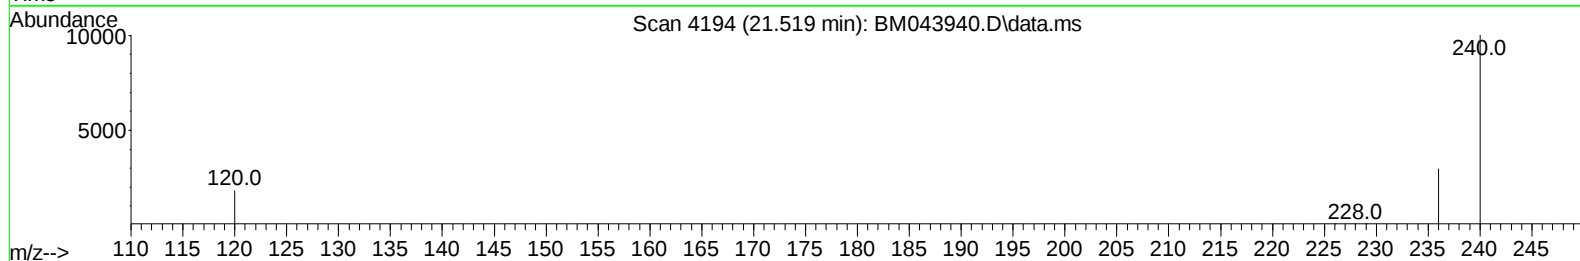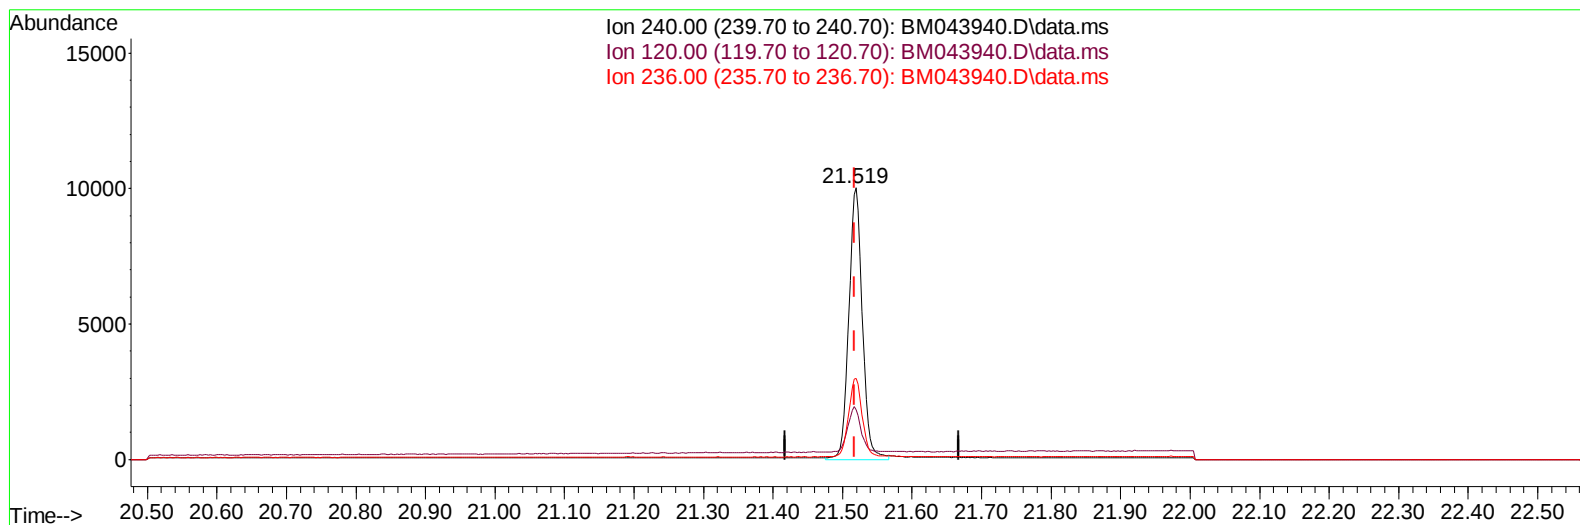

TIC: BM043940.D\data.ms

(17) Chrysene-d12

21.519min (+ 0.002) 0.40 ng/ul m

response 13698

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	17.60	18.30
236.00	29.90	29.77
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043940.D
Acq On : 01 Feb 2024 10:57
Operator : MA/JU
Sample : PB158635BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Manual IntegrationsAPPROVED

Quant Time: Feb 01 11:26:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

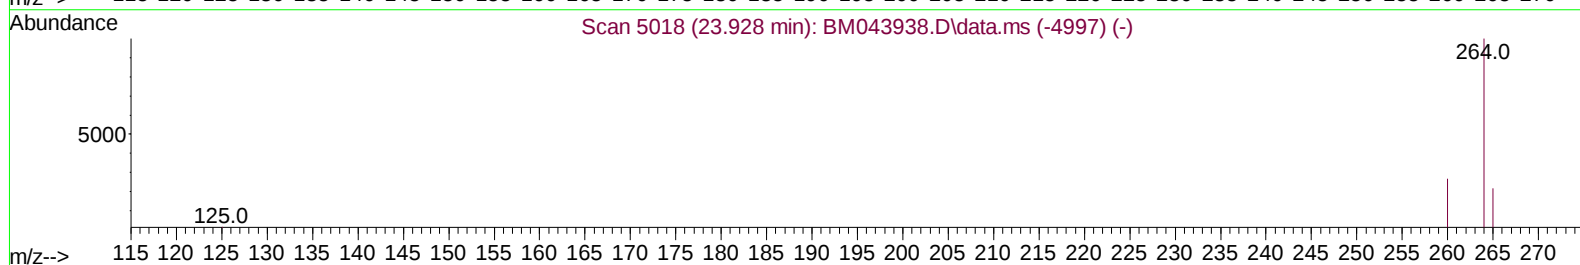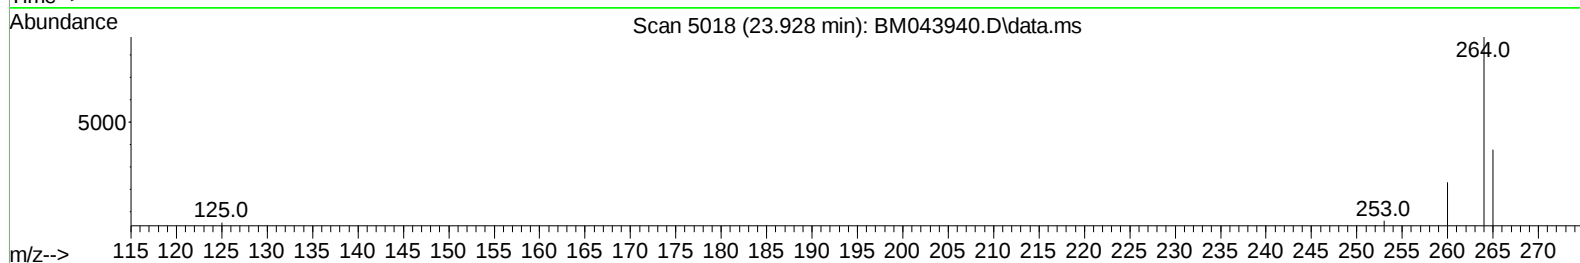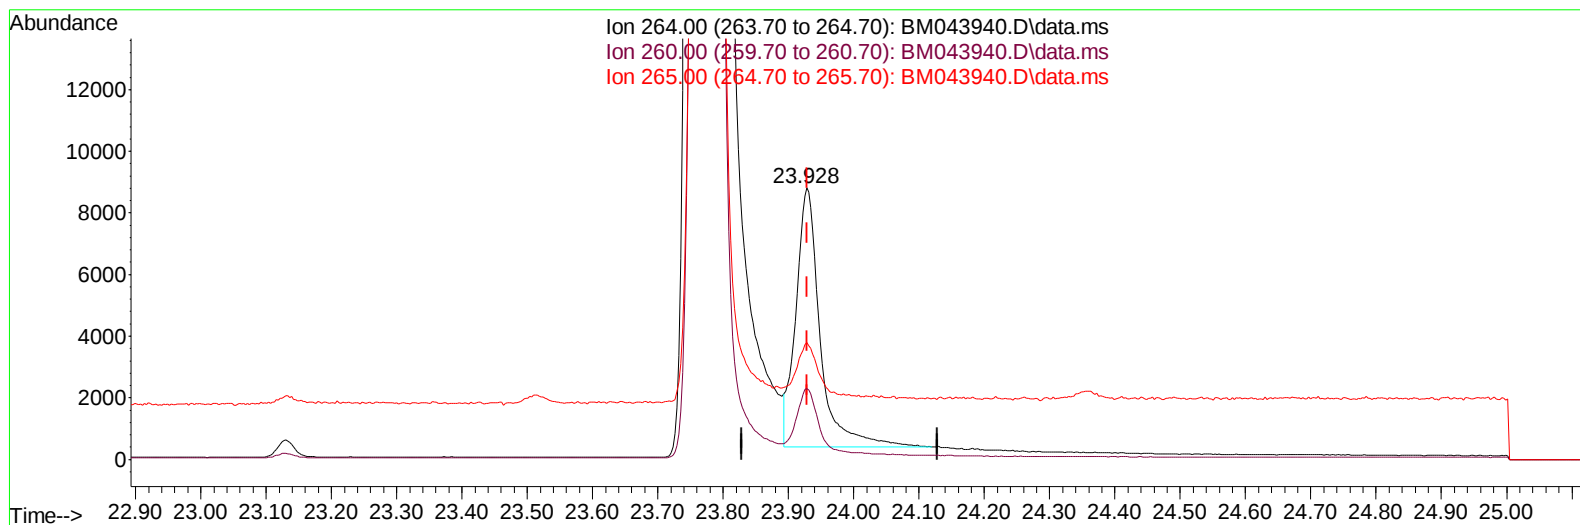

TIC: BM043940.D\data.ms

(23) Perylene-d12 (I)

23.928min (-0.001) 0.40 ng/u1

response 21617

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	26.17
265.00	42.60	42.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043940.D
Acq On : 01 Feb 2024 10:57
Operator : MA/JU
Sample : PB158635BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Manual IntegrationsAPPROVED

Quant Time: Feb 01 11:26:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

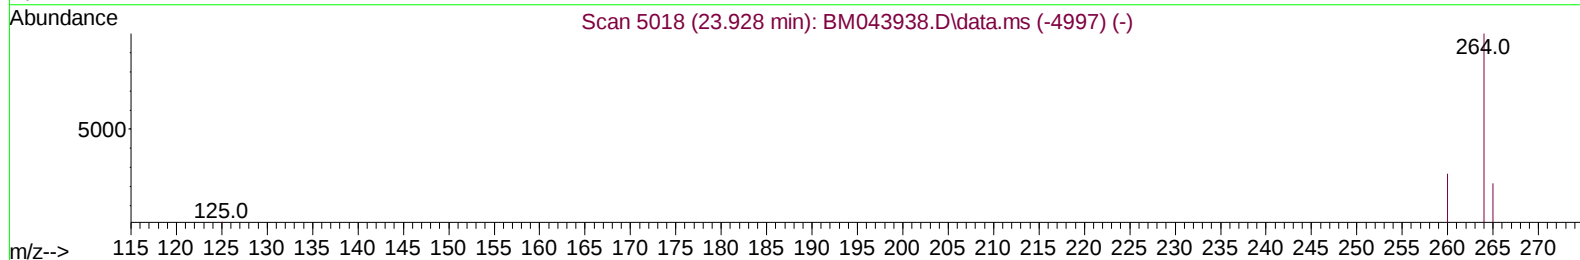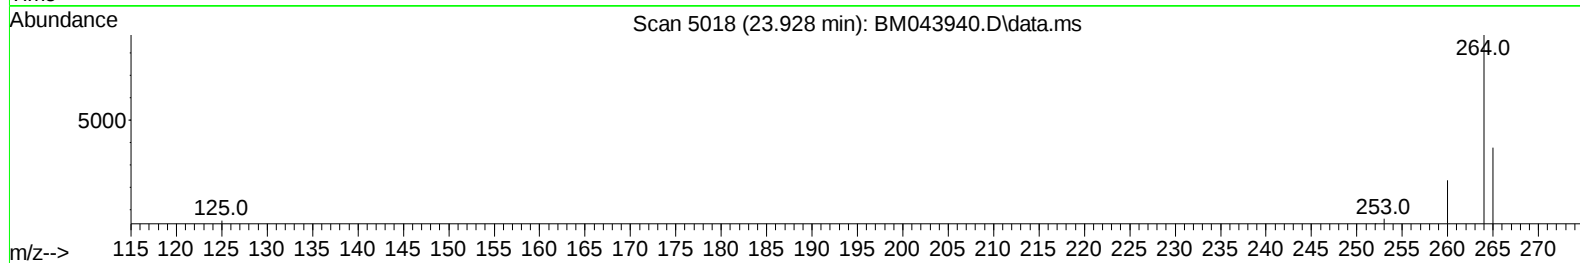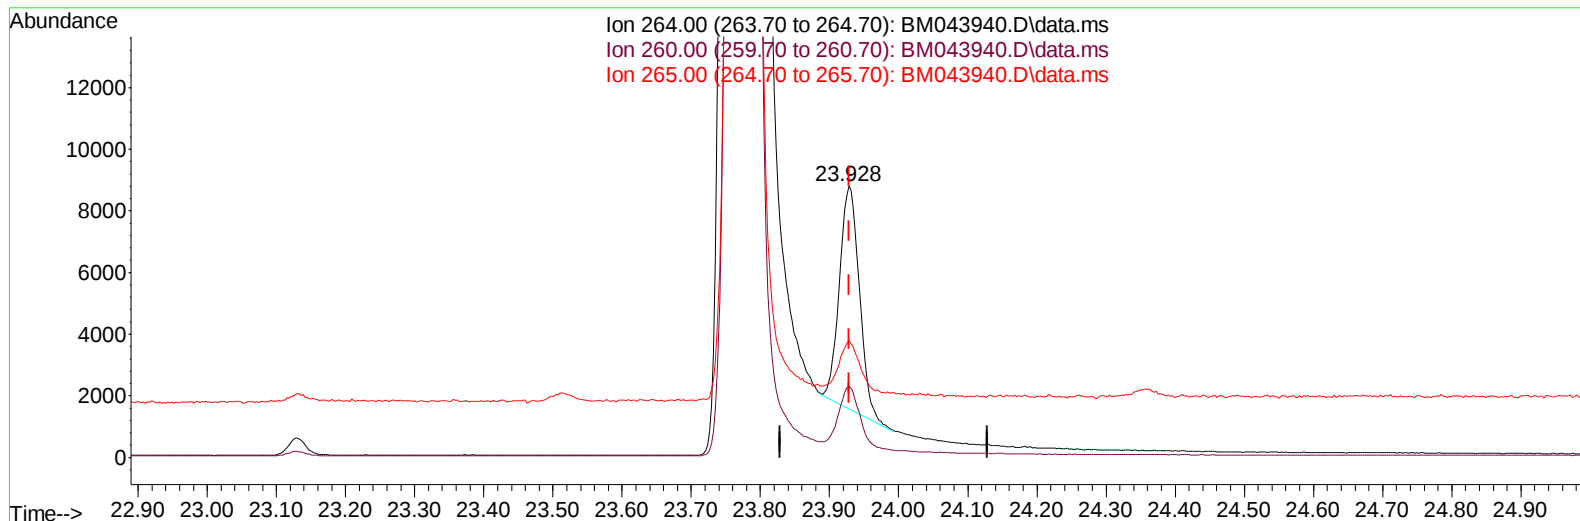

TIC: BM043940.D\data.ms

(23) Perylene-d12 (I)

23.928min (-0.001) 0.40 ng/ul m

response 14407

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	26.17
265.00	42.60	42.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043940.D
 Acq On : 01 Feb 2024 10:57
 Operator : MA/JU
 Sample : PB158635BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK635

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 11:26:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	7691	0.400	ng/ul	0.00
4) Naphthalene-d8	10.727	136	21392	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.567	164	9918	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.318	188	20091m	0.400	ng/ul	0.00
17) Chrysene-d12	21.519	240	13698m	0.400	ng/ul	0.00
23) Perylene-d12	23.928	264	14407m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.365	96	58719	5.934	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	8166	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.351	212	13806	0.321	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043940.D
Acq On : 01 Feb 2024 10:57
Operator : MA/JU
Sample : PB158635BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Manual IntegrationsAPPROVED

Quant Time: Feb 01 11:26:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

