




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

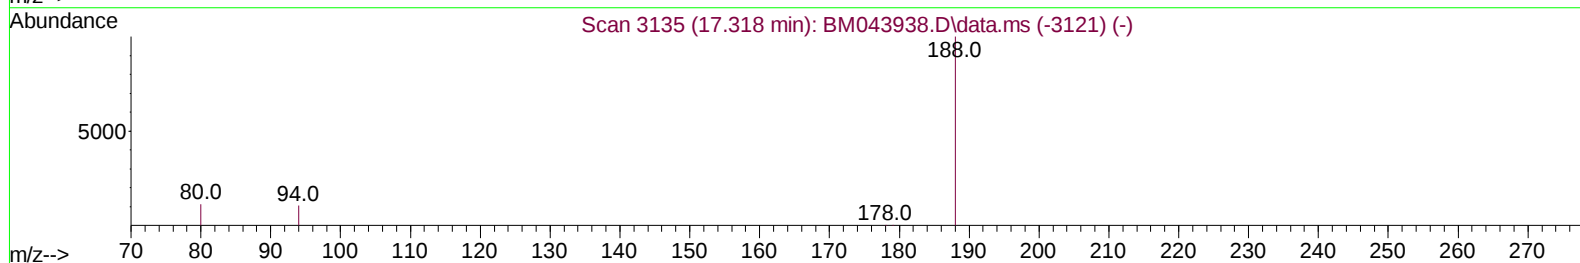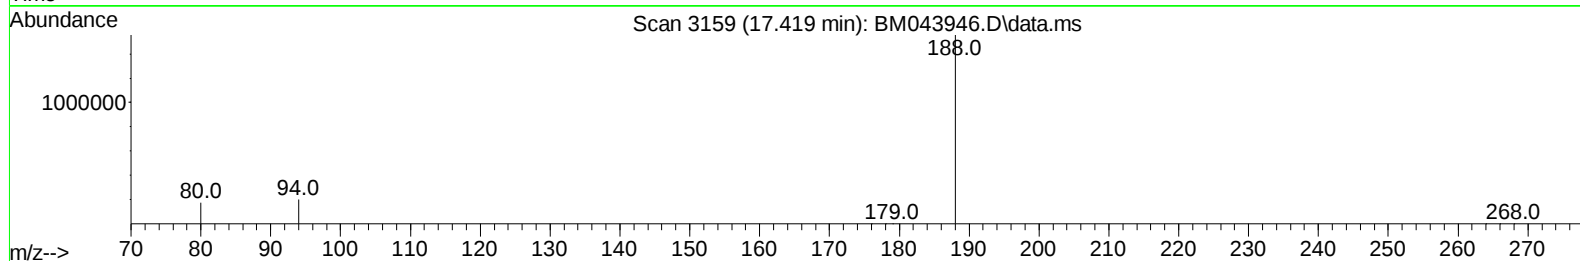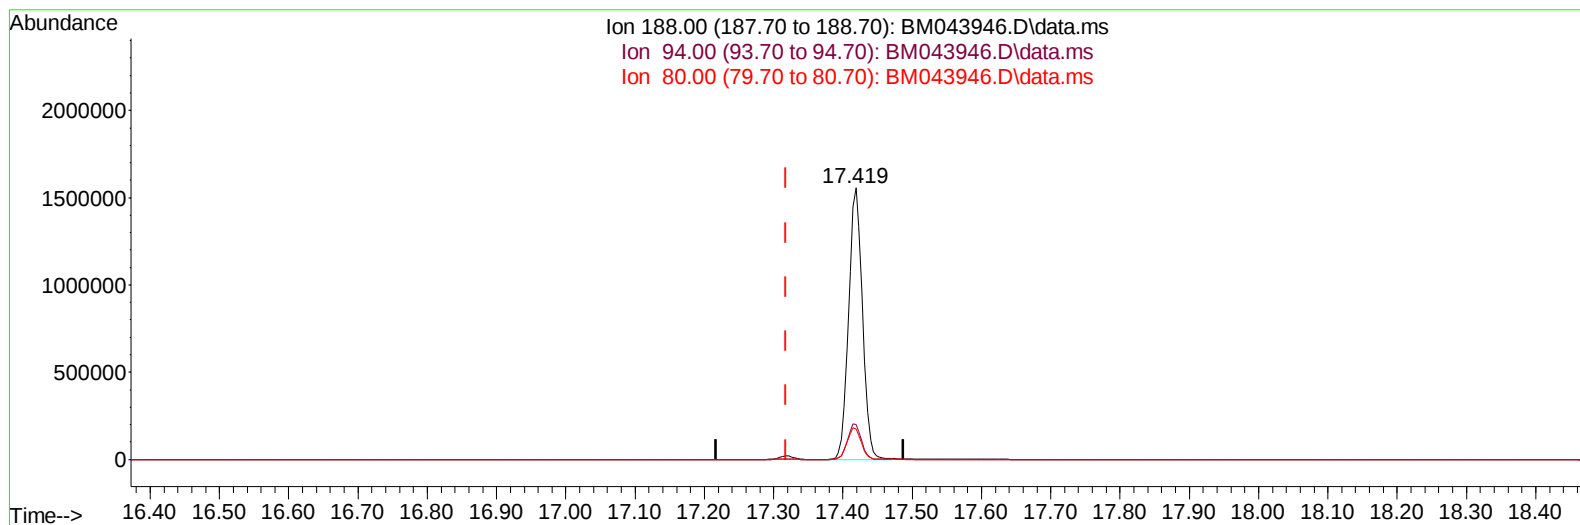

TIC: BM043946.D\data.ms

(13) Phenanthrene-d10 (I)

17.419min (+ 0.101) 0.40 ng/u1

response 2160793

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	12.81
80.00	12.90	11.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

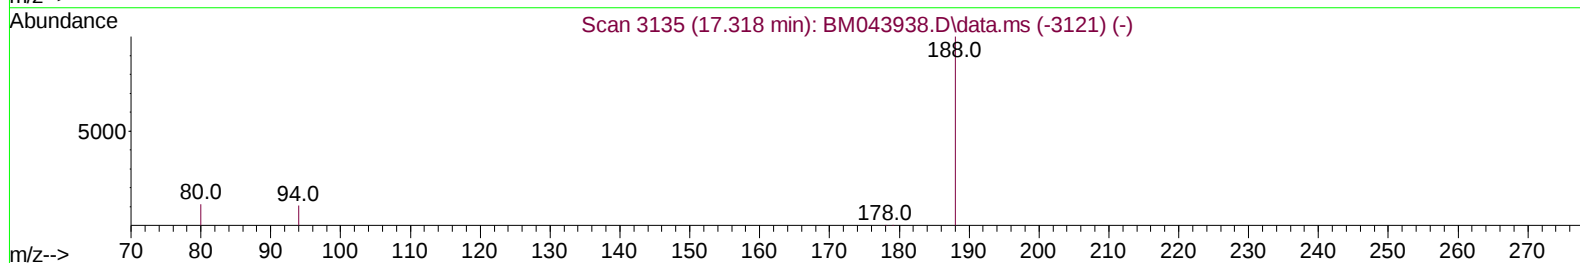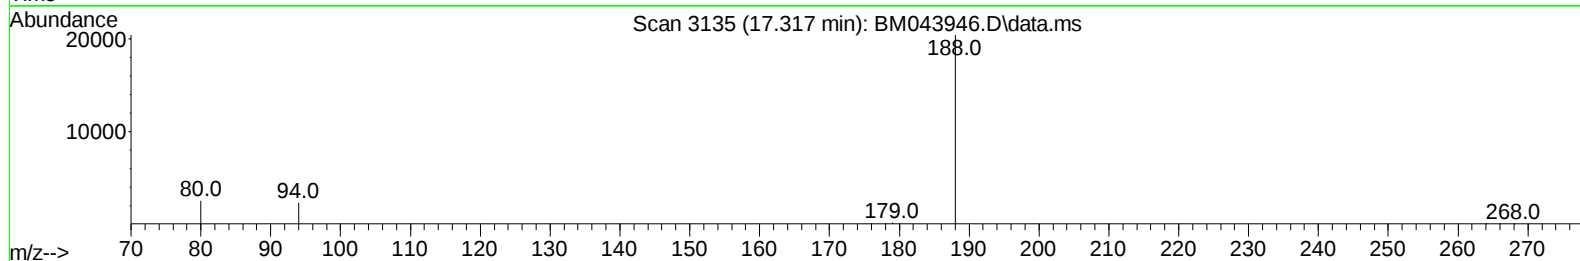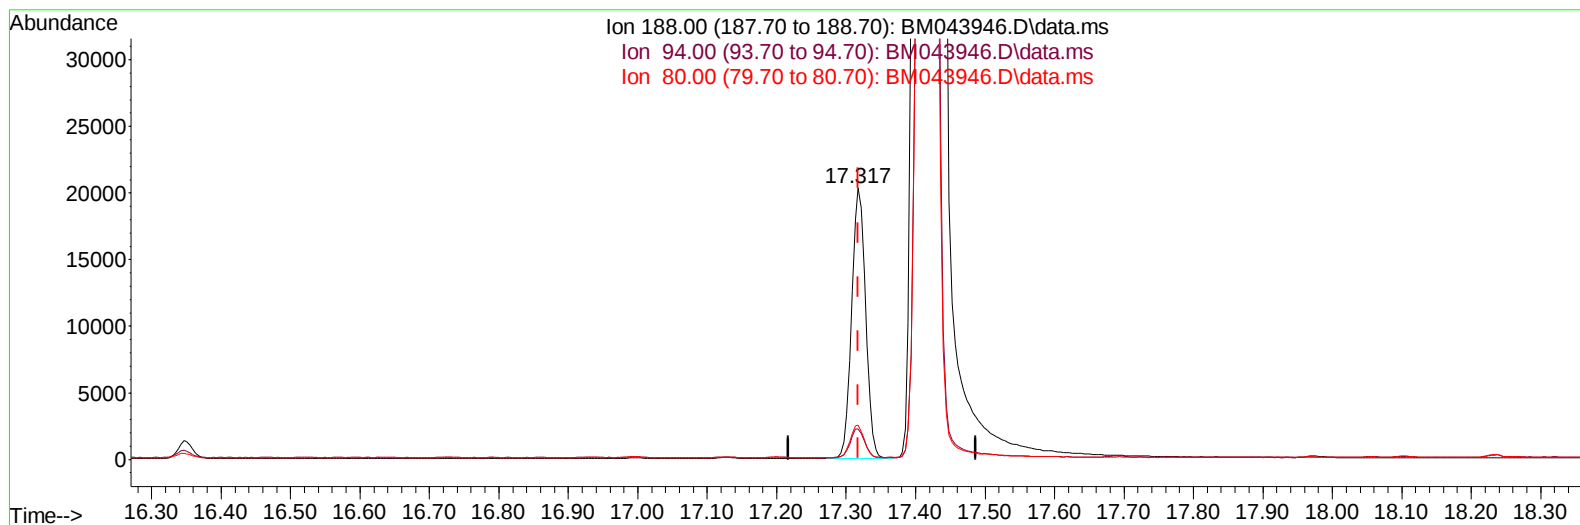

TIC: BM043946.D\data.ms

(13) Phenanthrene-d10 (I)

17.317min (-0.000) 0.40 ng/ul m

response 28359

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	11.32
80.00	12.90	12.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

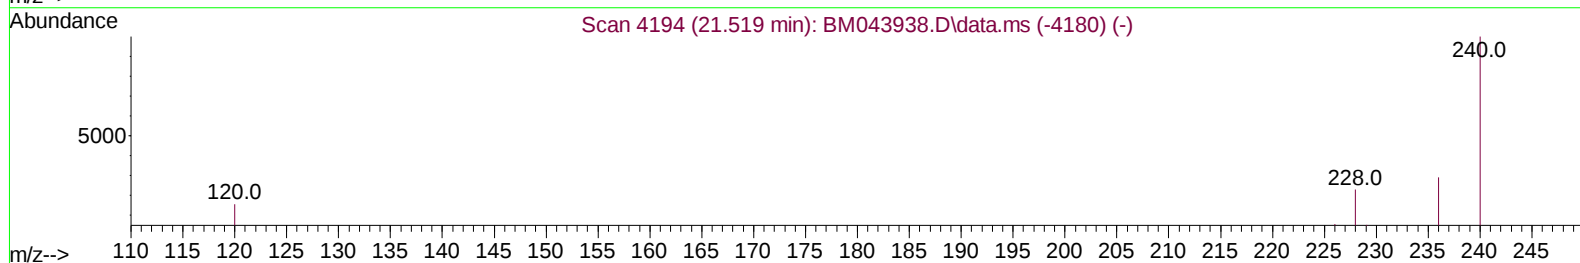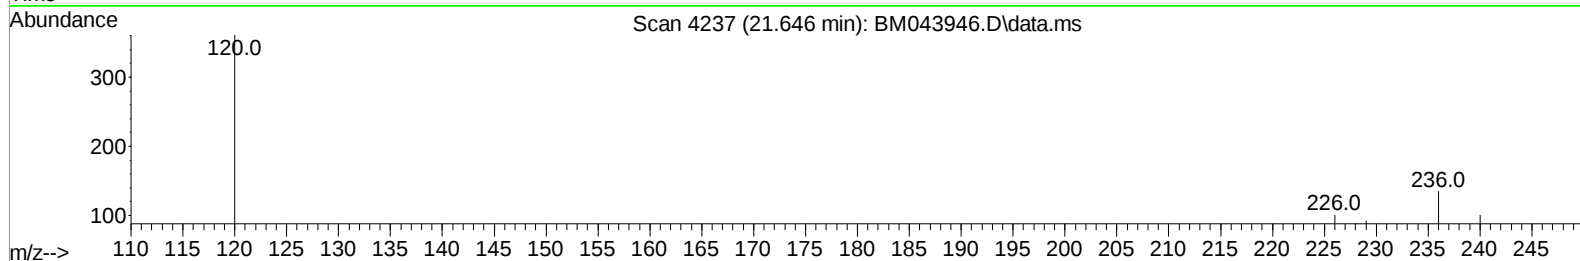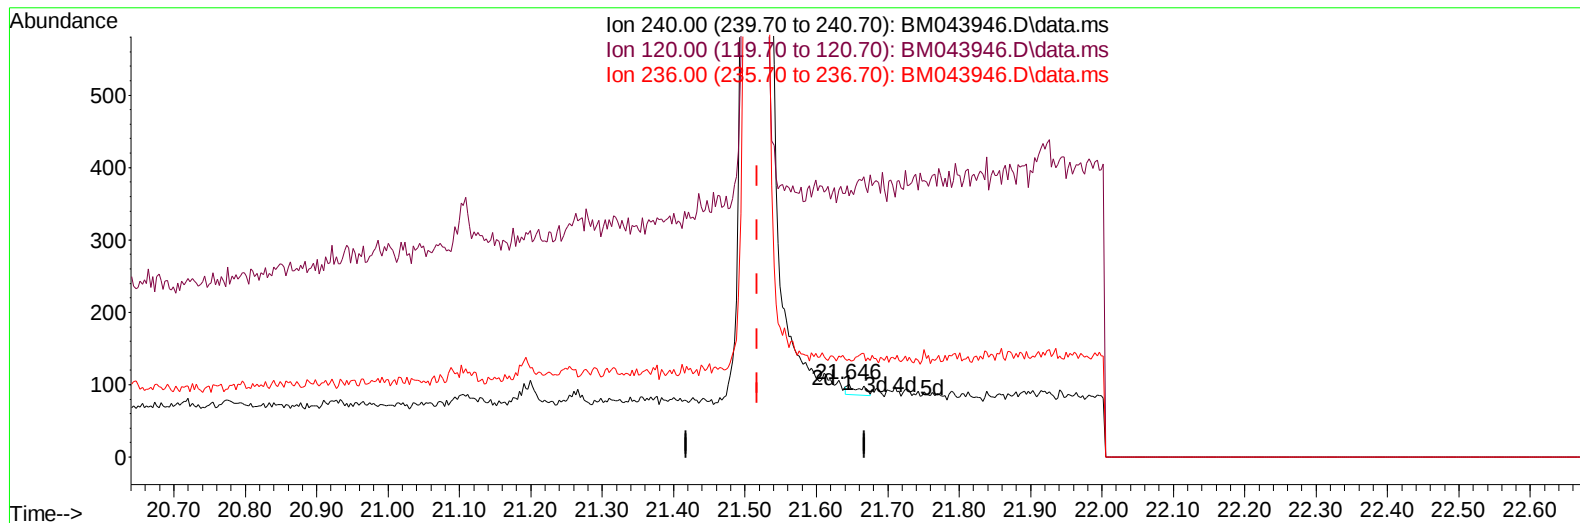

TIC: BM043946.D\data.ms

(17) Chrysene-d12

21.646min (+ 0.128) 0.40 ng/u1

response 18

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	17.60	357.43#
236.00	29.90	133.66#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

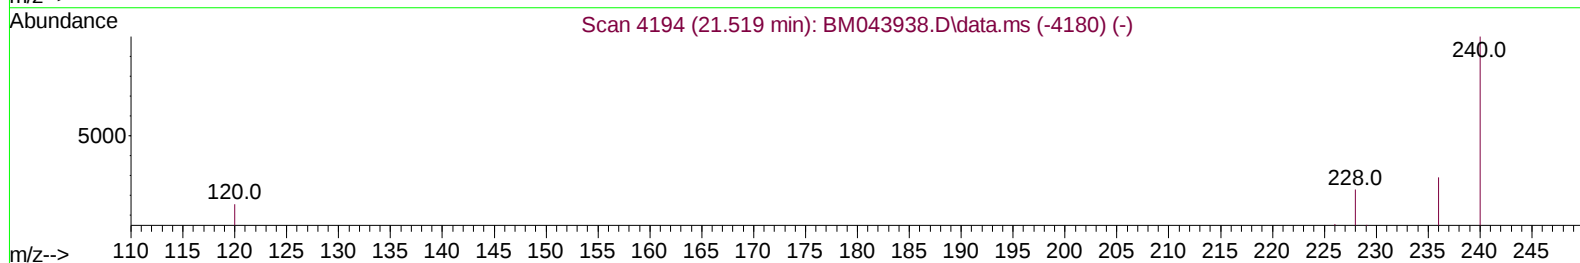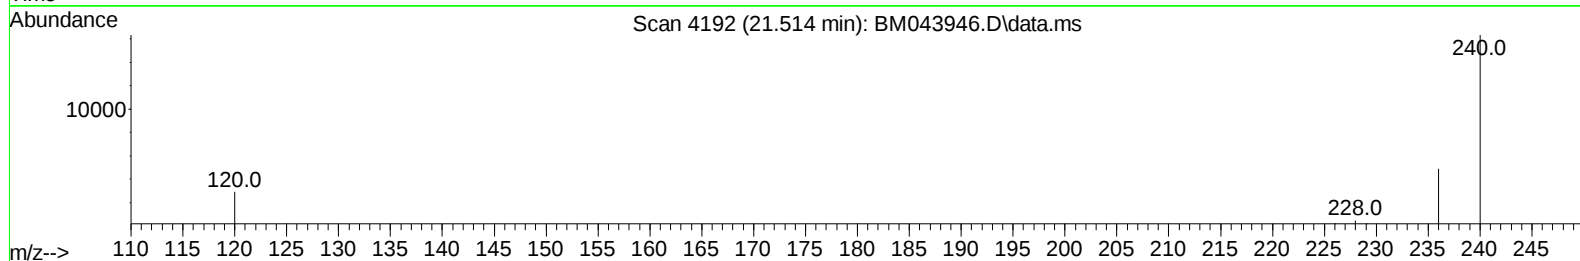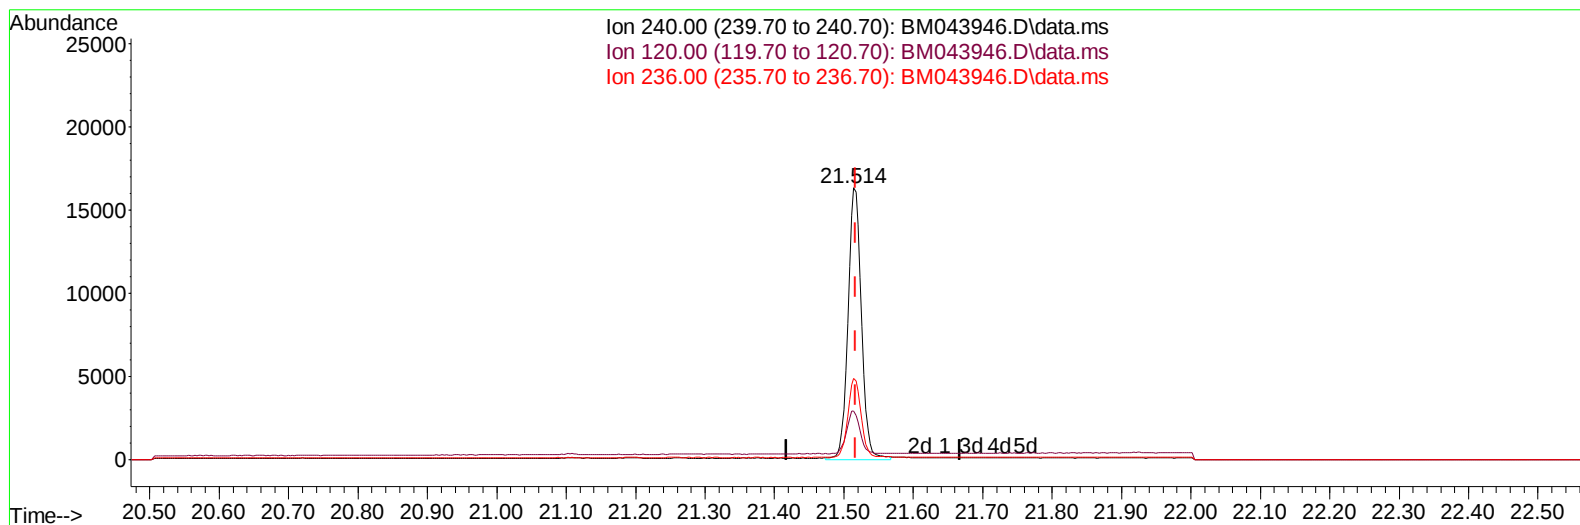

TIC: BM043946.D\data.ms

(17) Chrysene-d12

21.514min (-0.003) 0.40 ng/ul m

response 21916

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	17.60	17.79
236.00	29.90	29.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

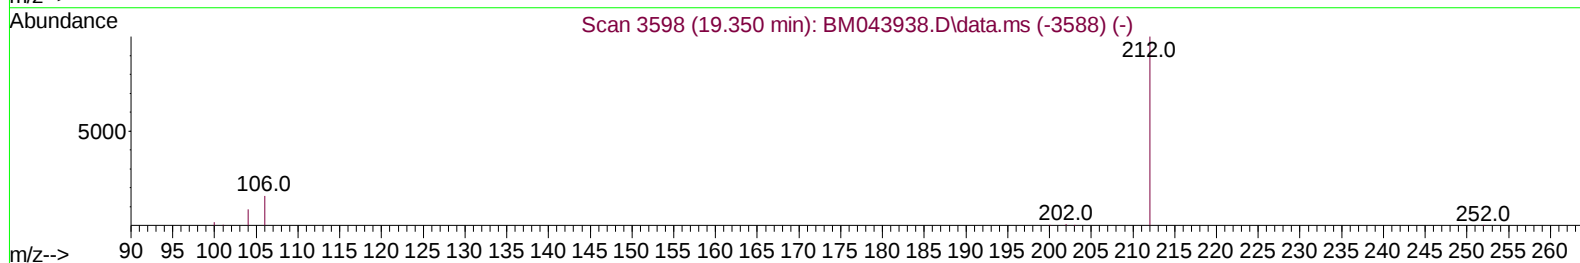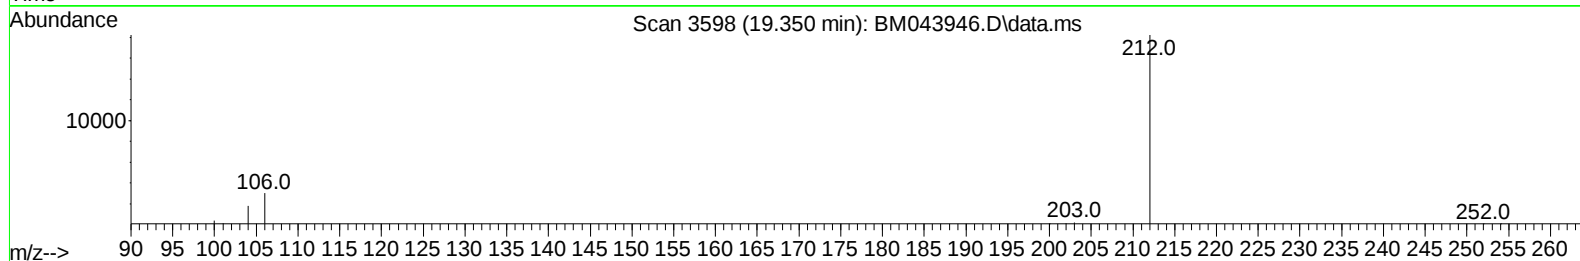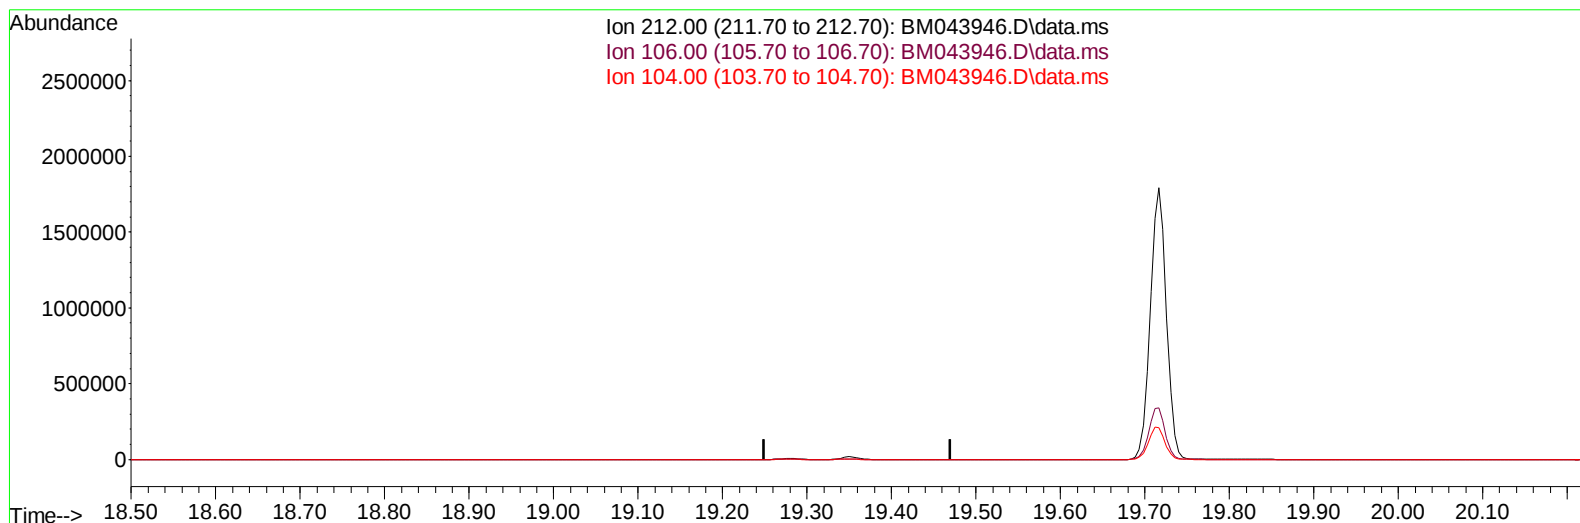

TIC: BM043946.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.350min (-19.350) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	16.20	0.00#
104.00	9.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043946.D
 Acq On : 01 Feb 2024 14:34
 Operator : MA/JU
 Sample : P1239-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

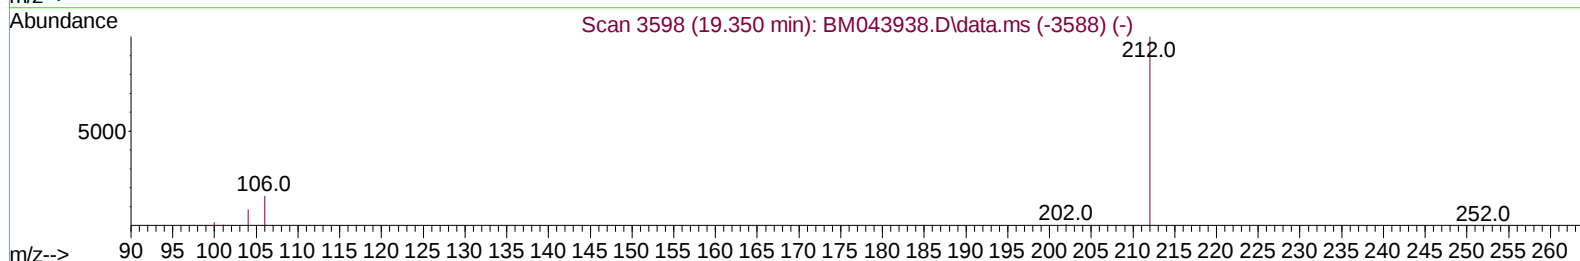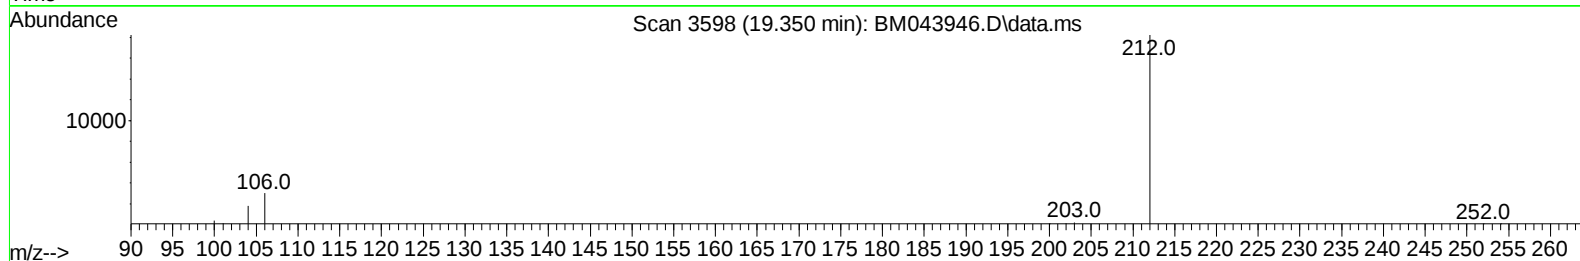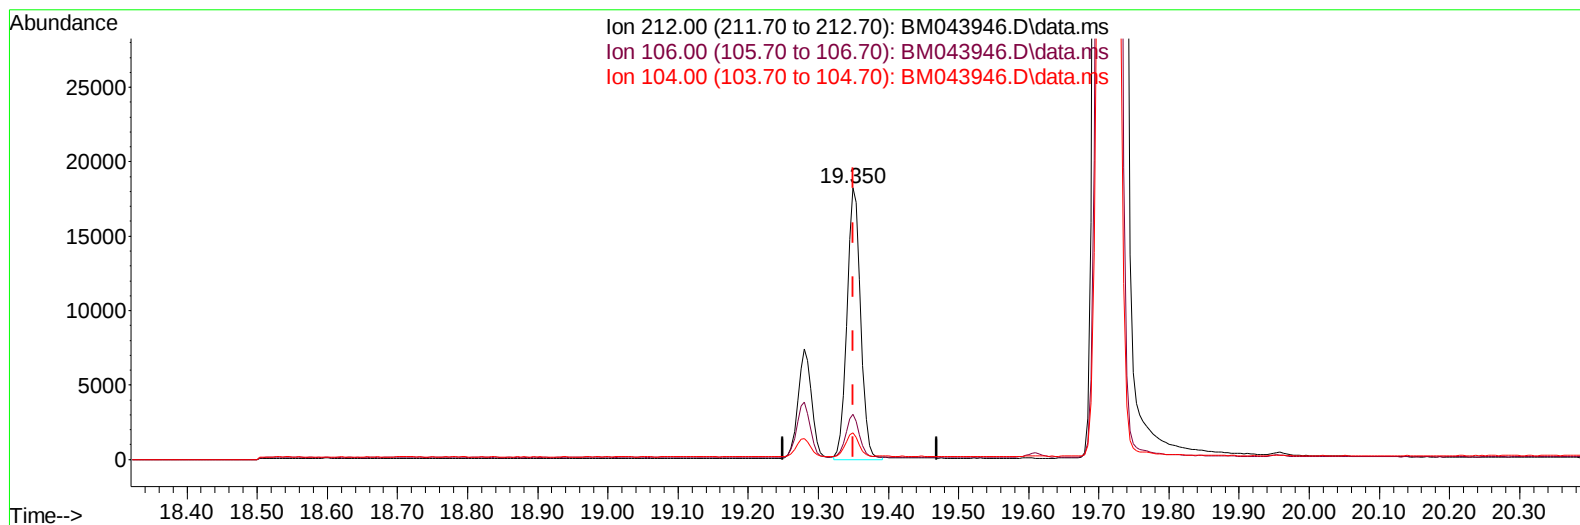

TIC: BM043946.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.350min (-0.000) 0.36 ng/u1 m

response 24717

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	16.20	0.00#
104.00	9.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

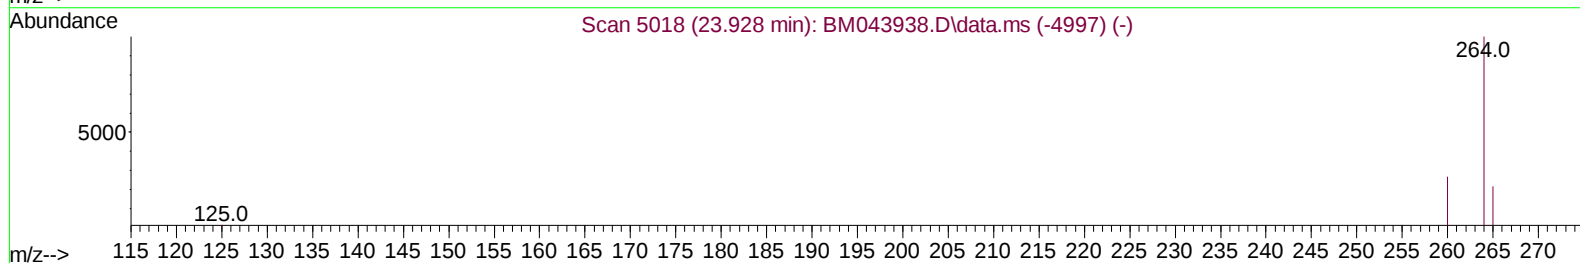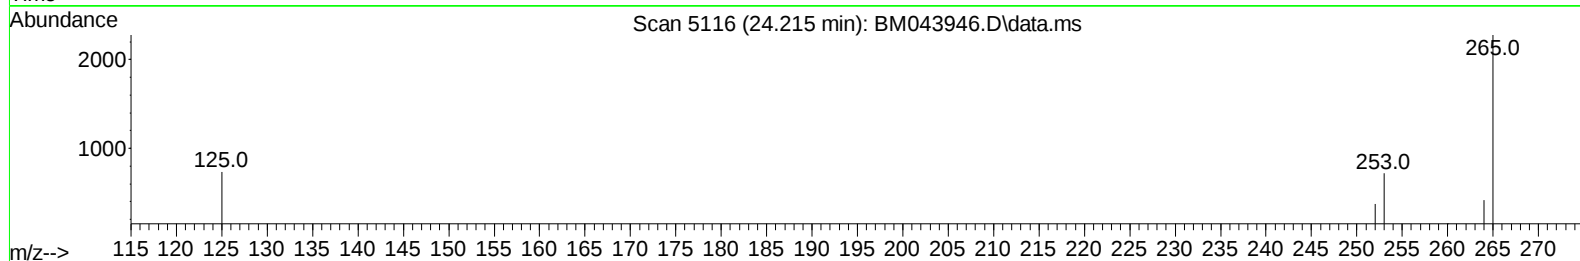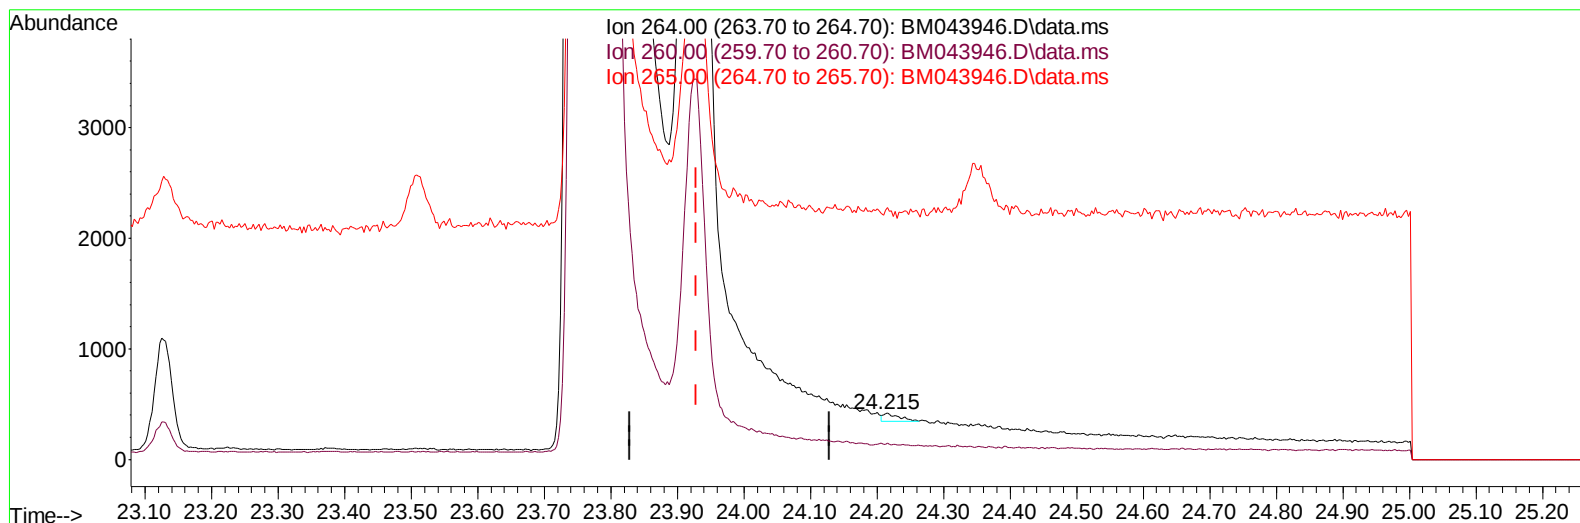

TIC: BM043946.D\data.ms

(23) Perylene-d12 (I)

24.215min (+ 0.286) 0.40 ng/u1

response 126

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	35.97#
265.00	42.60	545.80#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

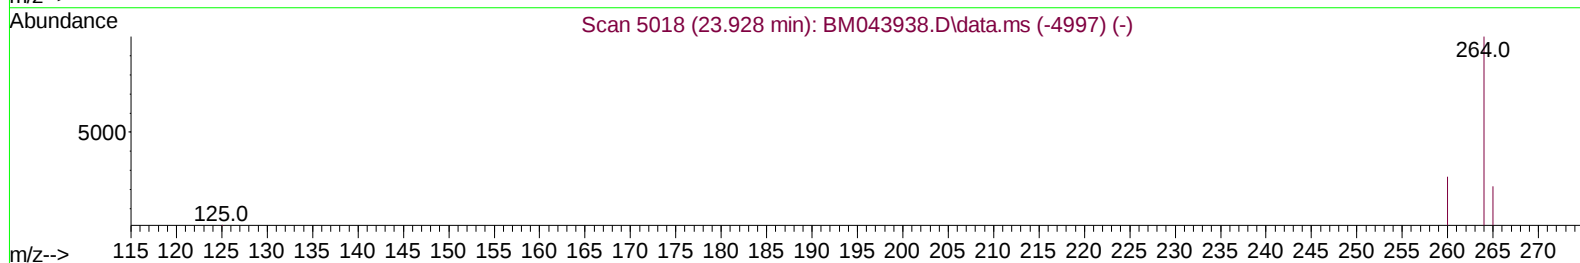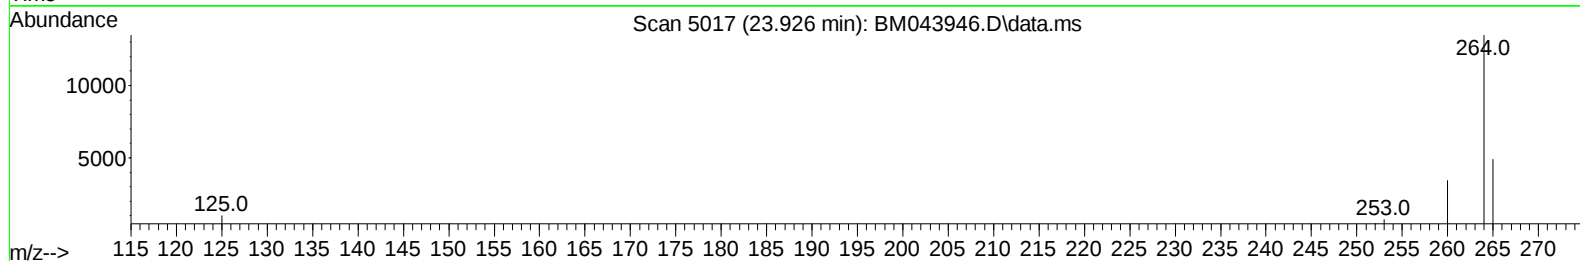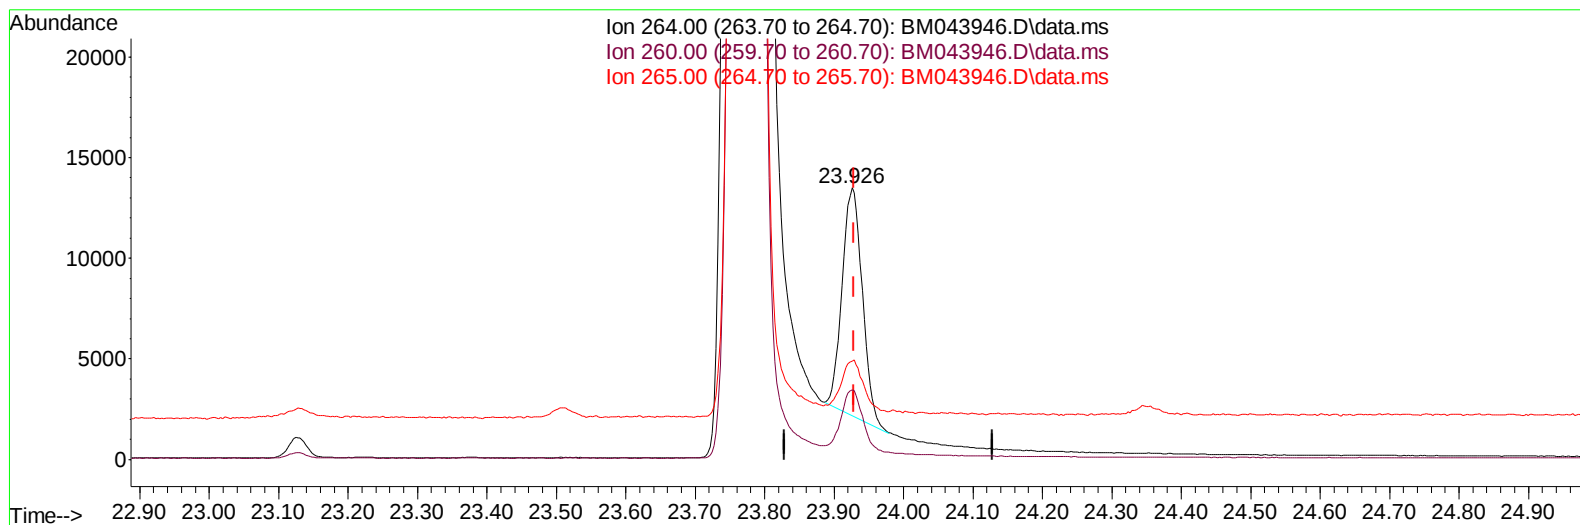

TIC: BM043946.D\data.ms

(23) Perylene-d12 (I)

23.926min (-0.003) 0.40 ng/ul m

response 22836

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	25.49
265.00	42.60	36.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

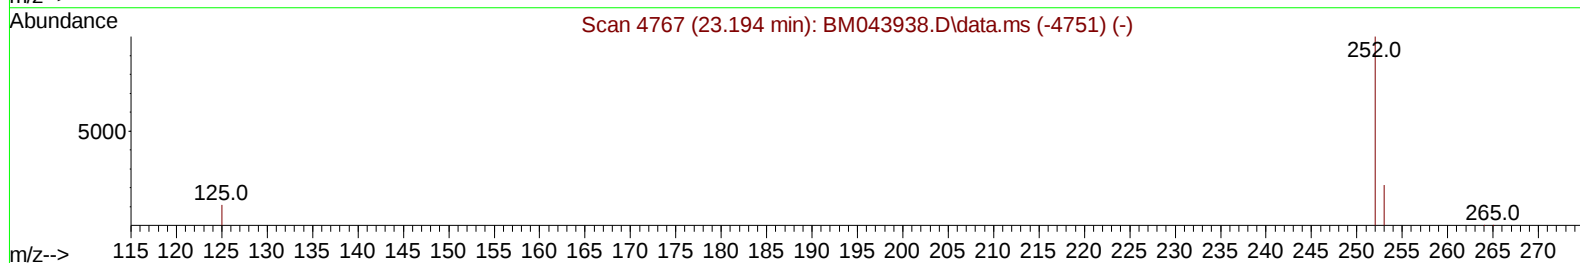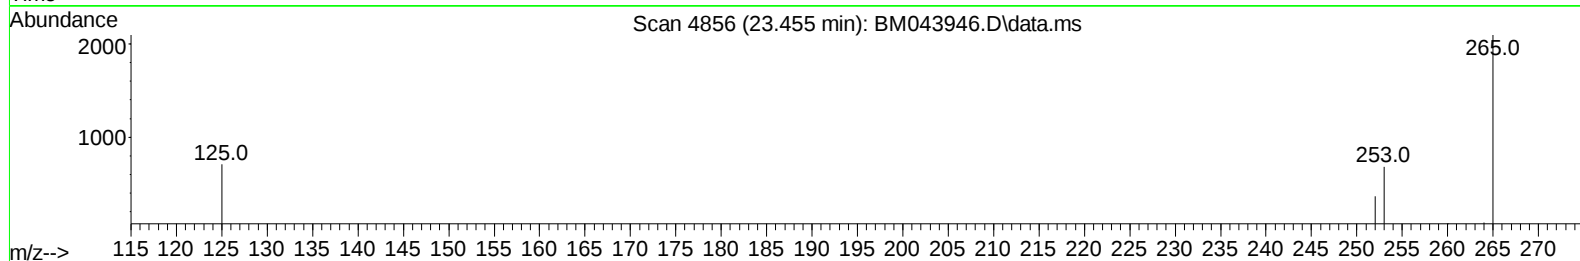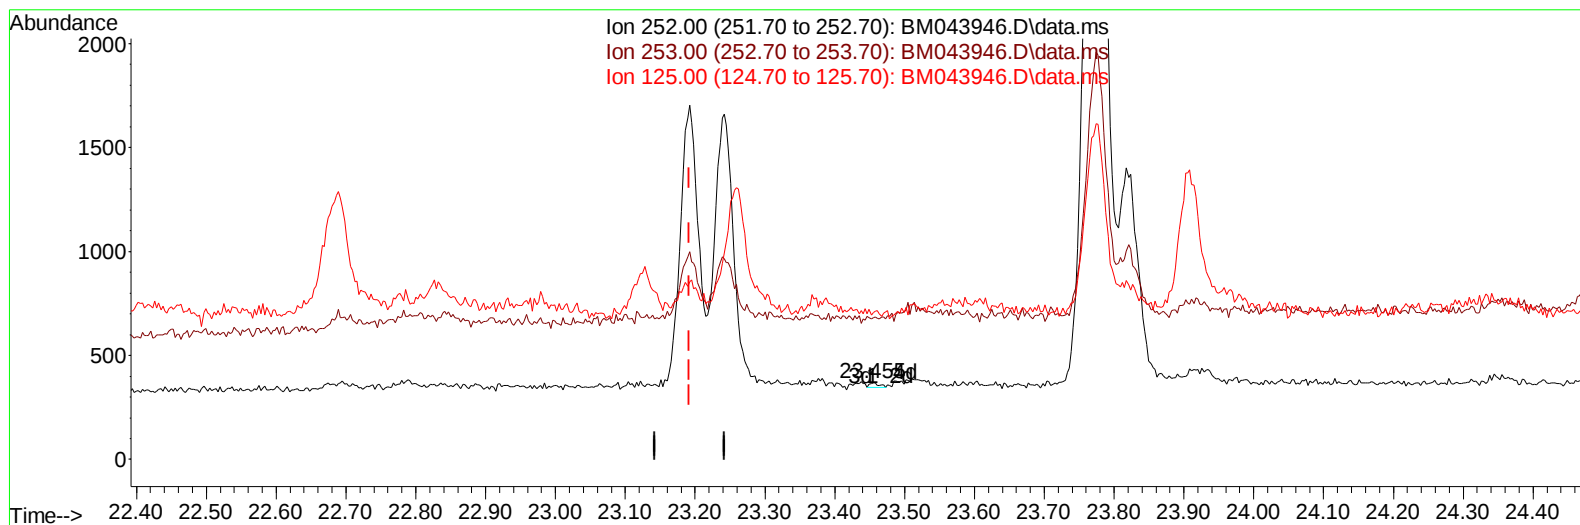

TIC: BM043946.D\data.ms

(24) Benzo(b)fluoranthene

23.455min (+ 0.263) 0.00 ng/u1

response 24

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	184.55#
125.00	13.20	191.87#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

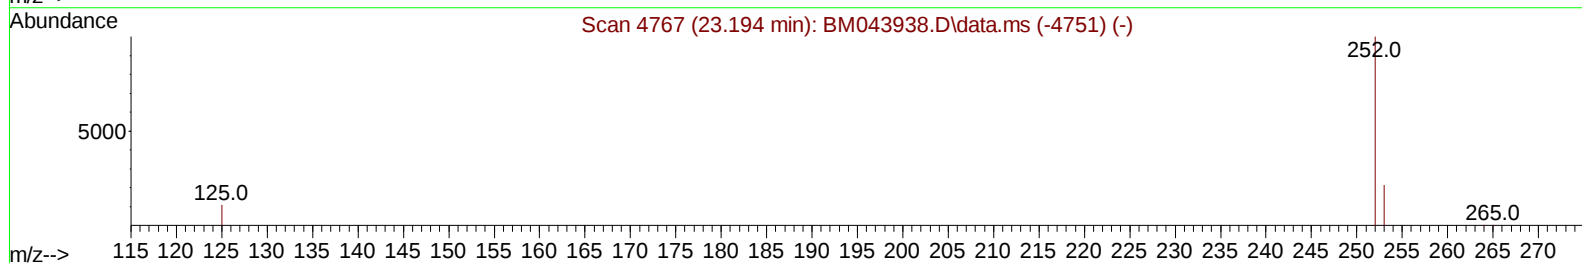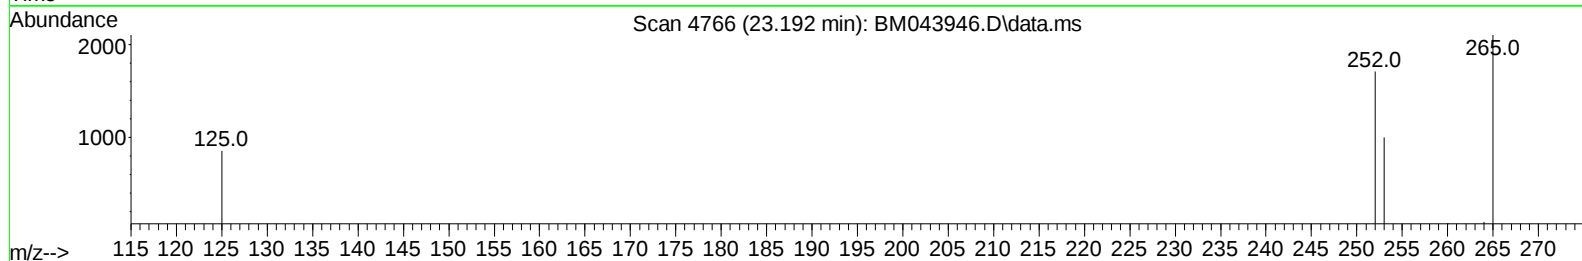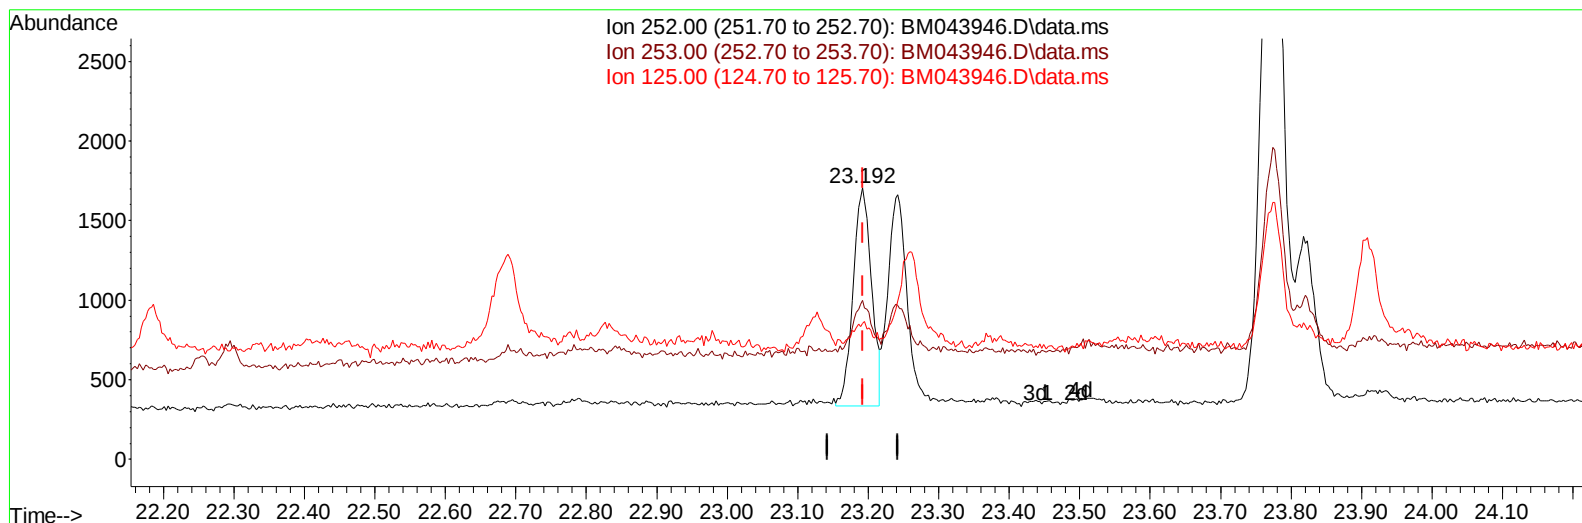

TIC: BM043946.D\data.ms

(24) Benzo(b)fluoranthene

23.192min (-0.000) 0.03 ng/u1 m

response 2462

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	58.65#
125.00	13.20	50.09#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

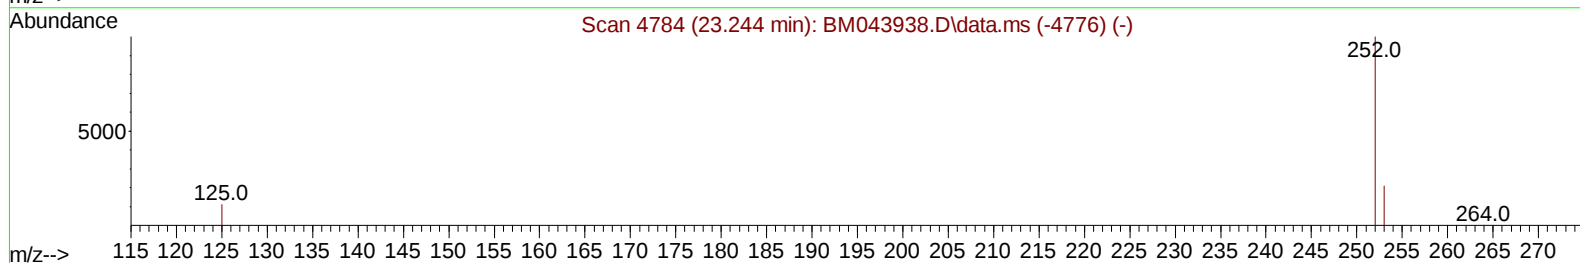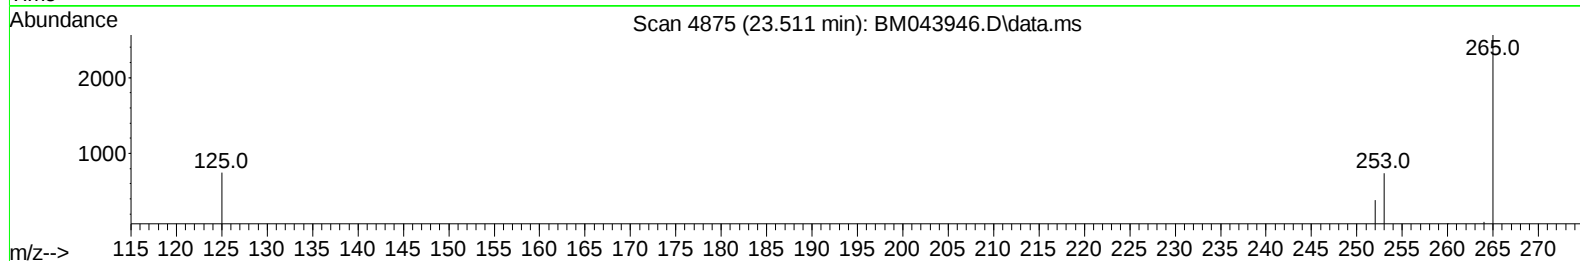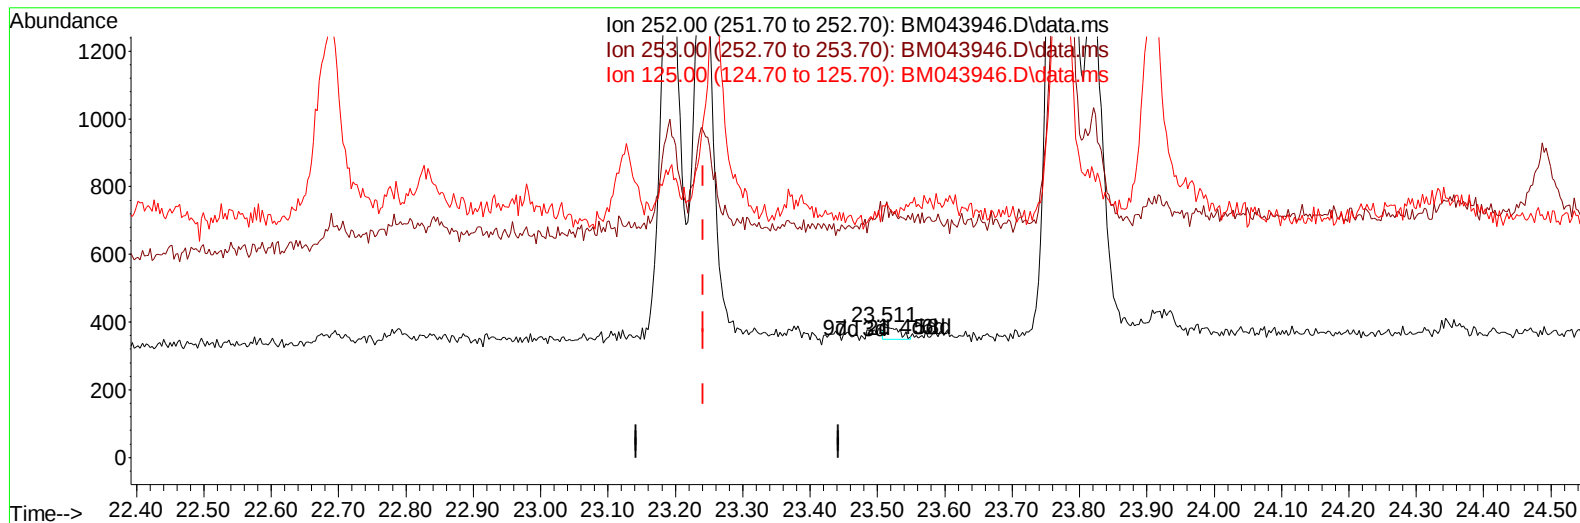

TIC: BM043946.D\data.ms

(25) Benzo(k)fluoranthene

23.511min (+ 0.269) 0.00 ng/u1

response 56

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.60	191.95#
125.00	13.30	192.99#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

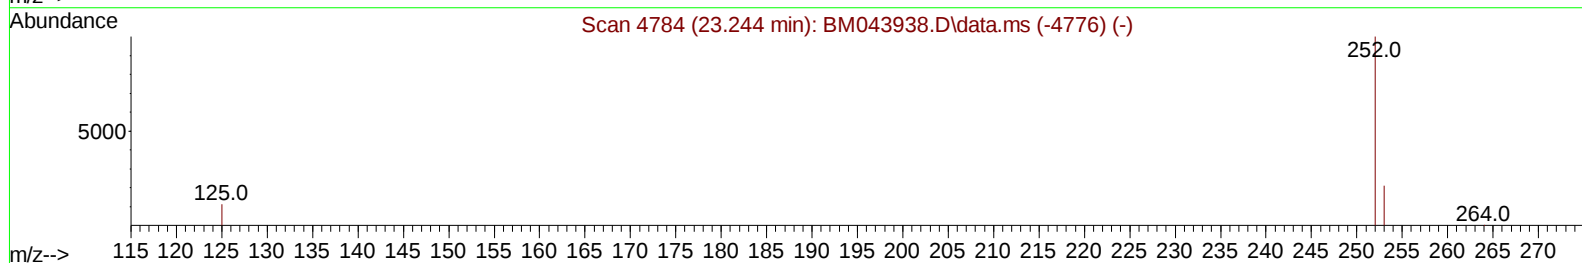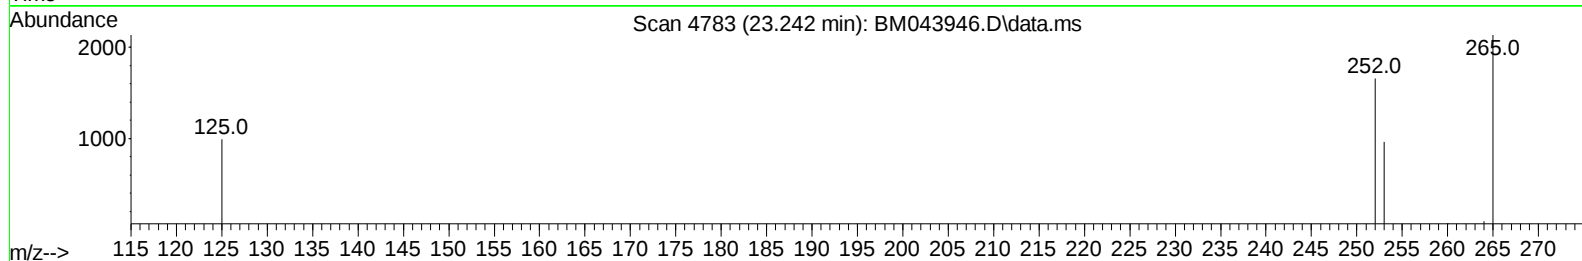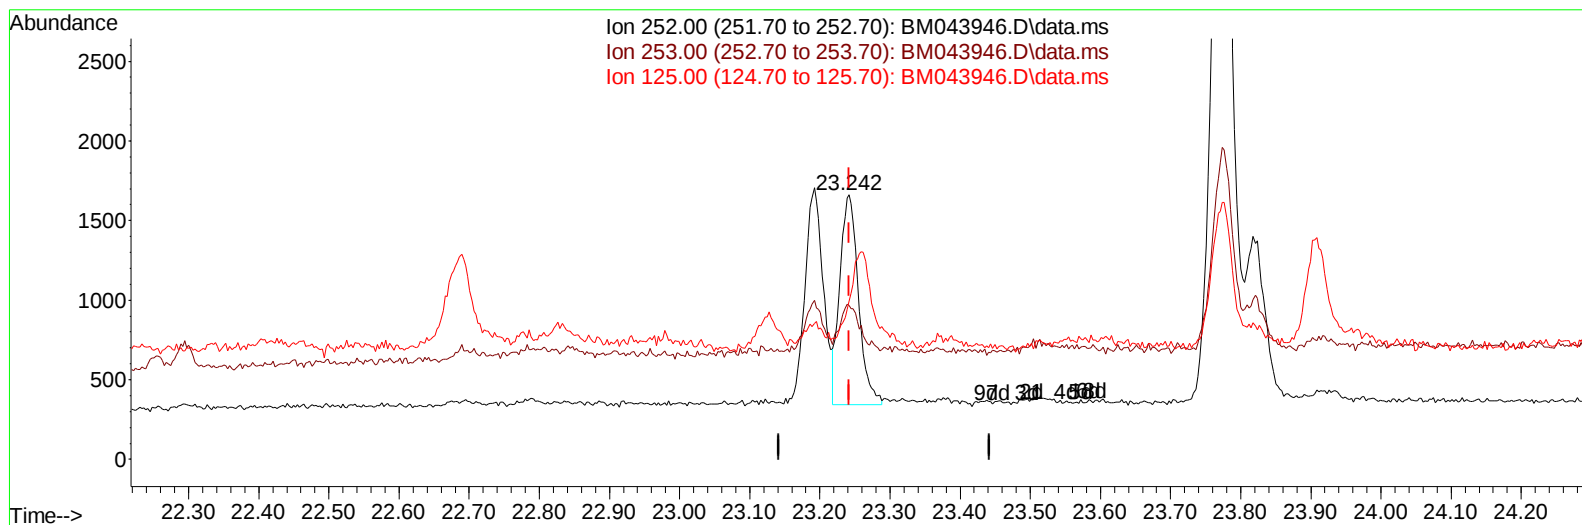

TIC: BM043946.D\data.ms

(25) Benzo(k)fluoranthene

23.242min (-0.000) 0.03 ng/u1 m

response 2427

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.60	58.16#
125.00	13.30	59.84#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

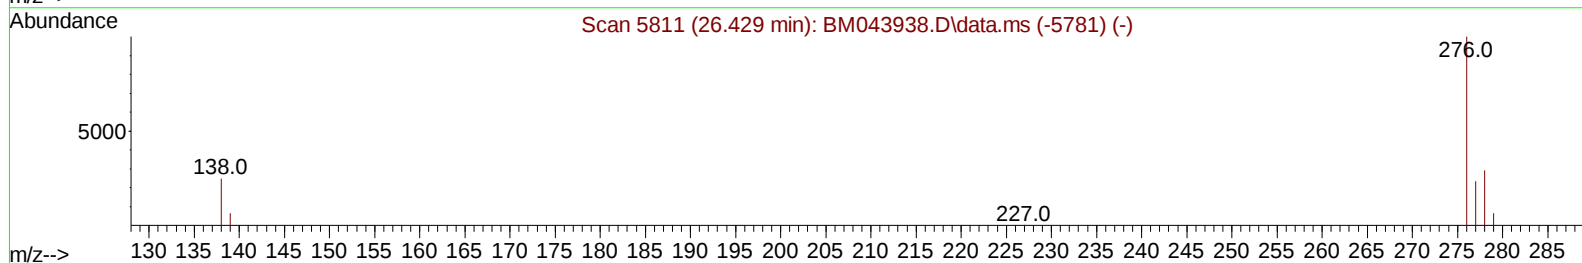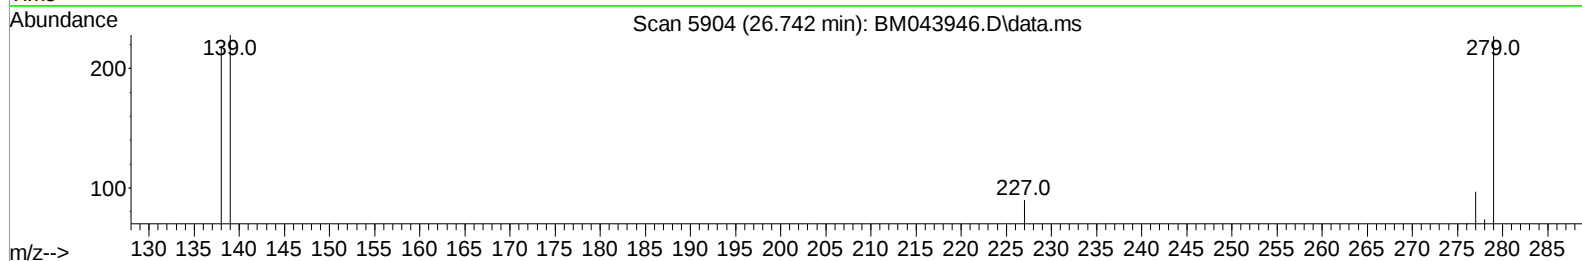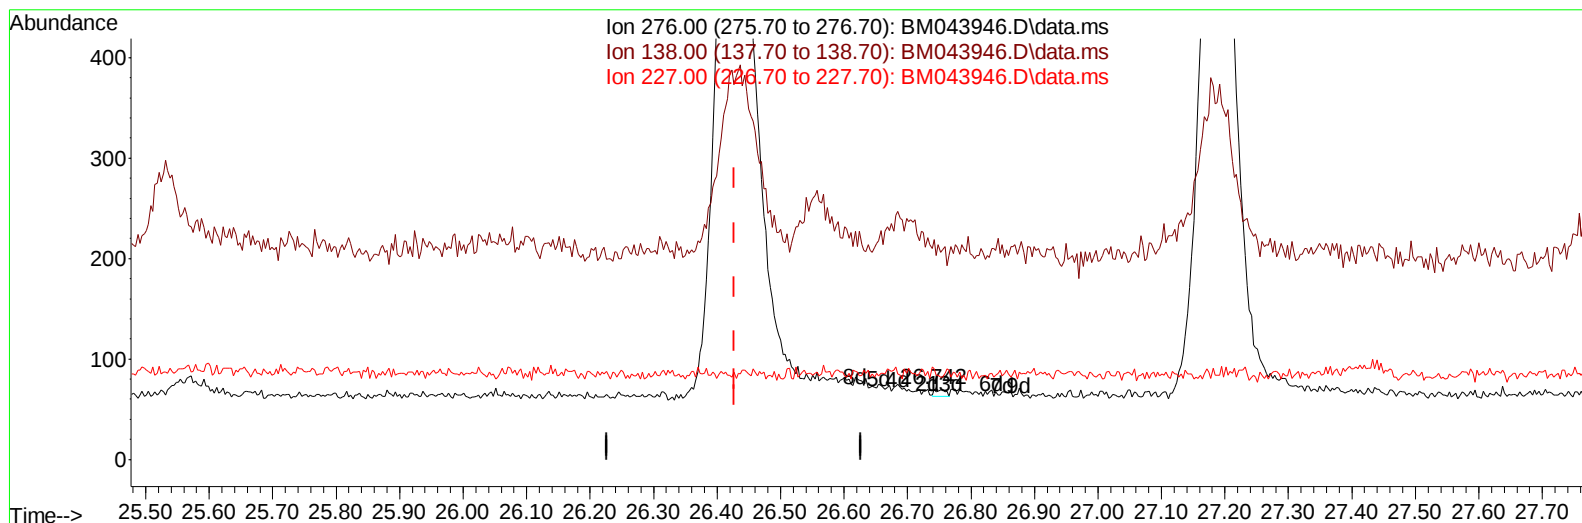

TIC: BM043946.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

26.742min (+ 0.315) 0.00 ng/u1

response 8

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	27.70	0.00#
227.00	0.00	62.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

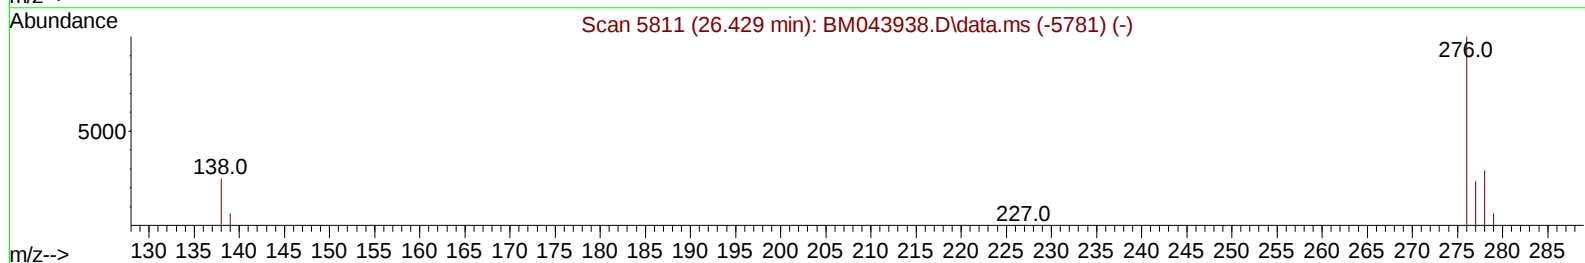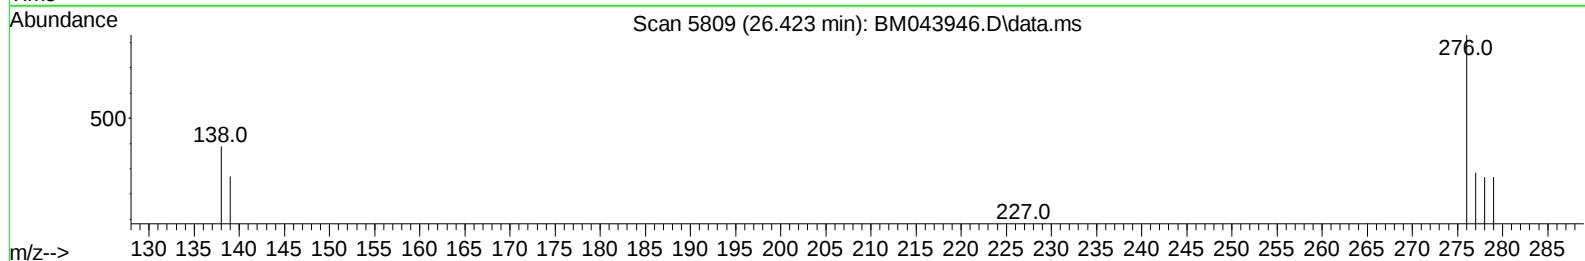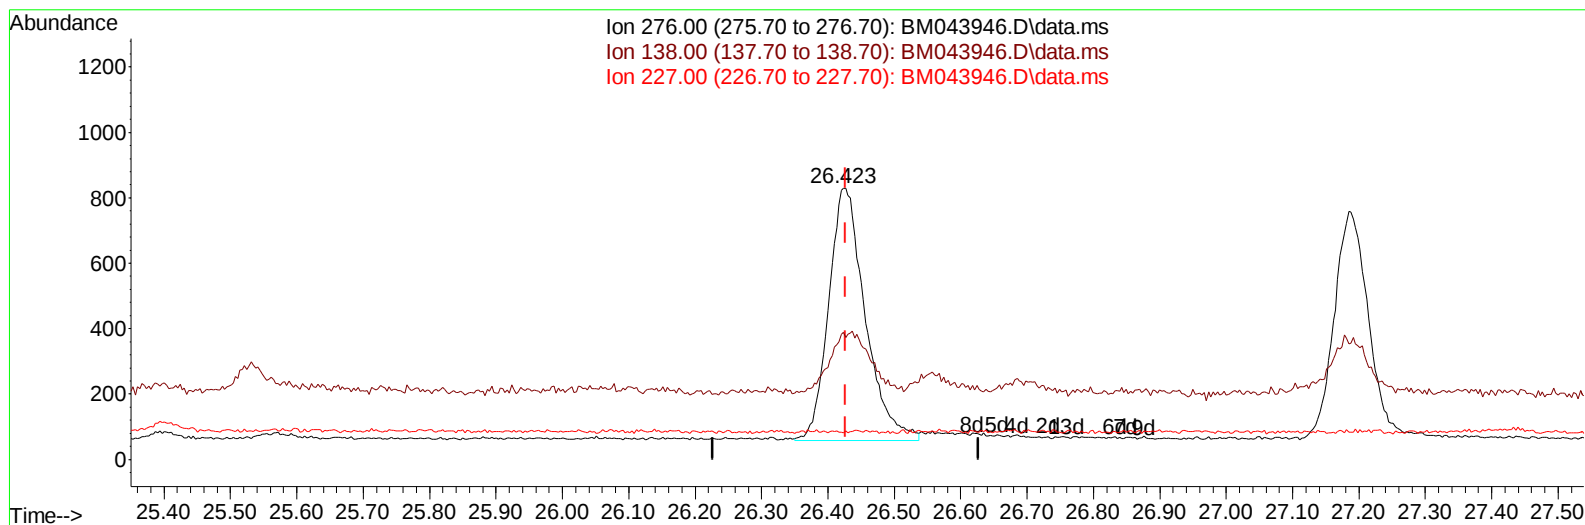

TIC: BM043946.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

26.423min (-0.003) 0.03 ng/u1 m

response 2949

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	27.70	0.00#
227.00	0.00	0.17#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

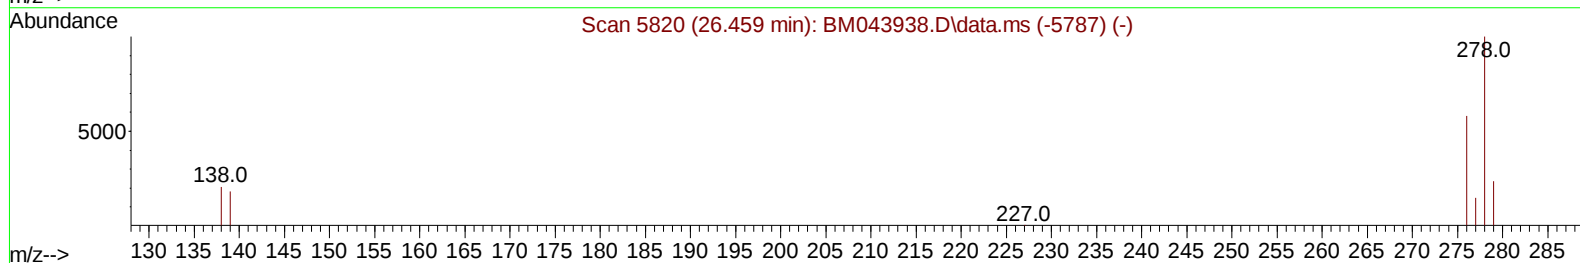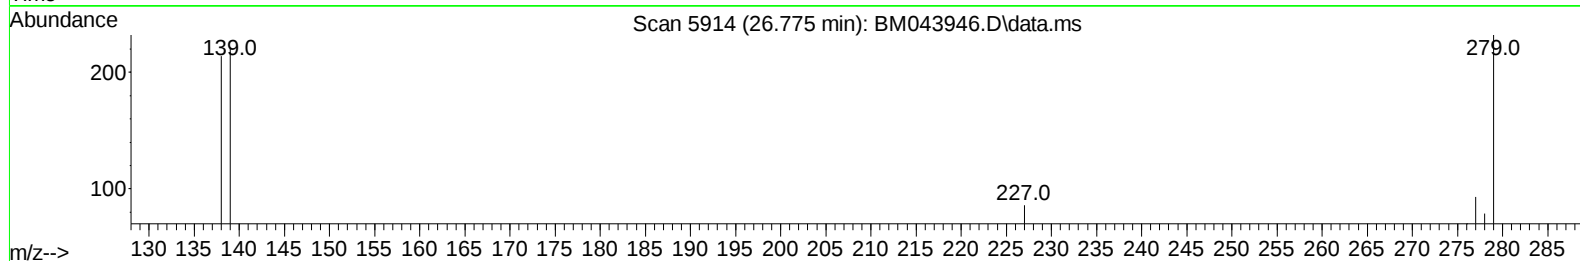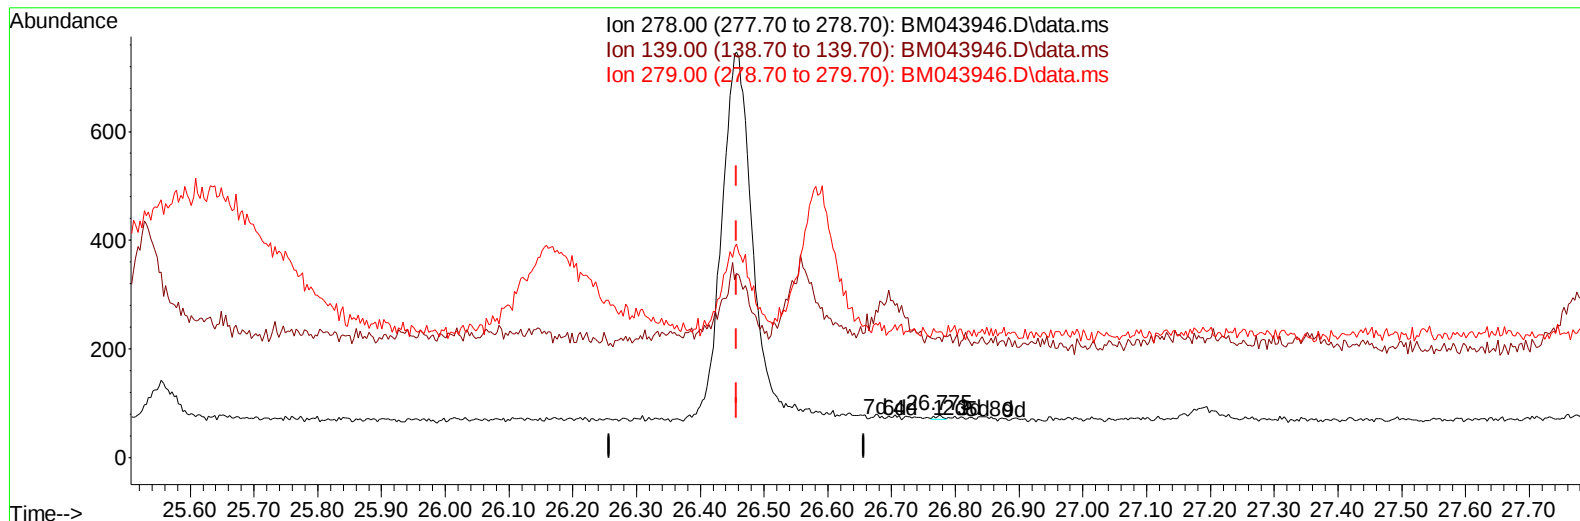

TIC: BM043946.D\data.ms

(28) Dibenzo(a,h)anthracene

26.775min (+ 0.319) 0.00 ng/u1

response 6

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	20.20	279.75#
279.00	27.10	293.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

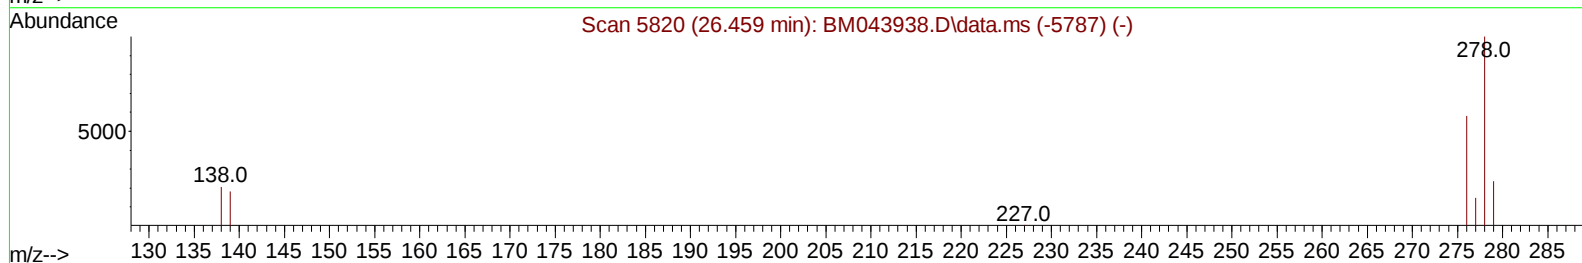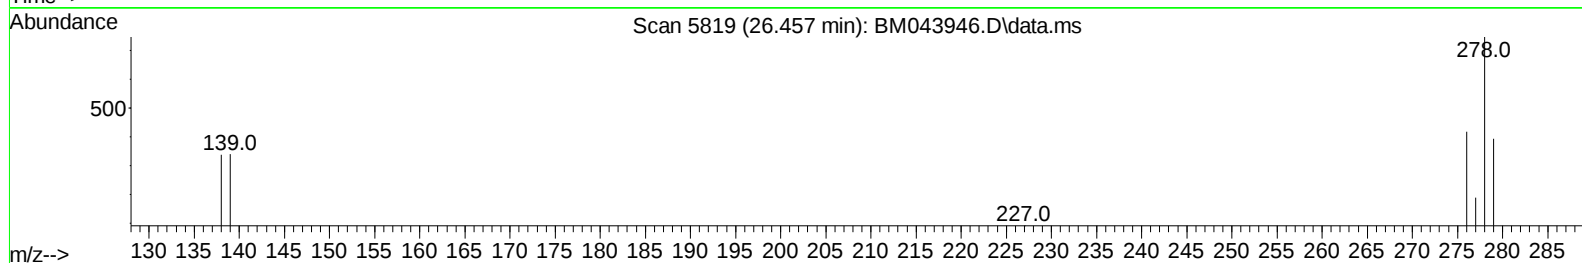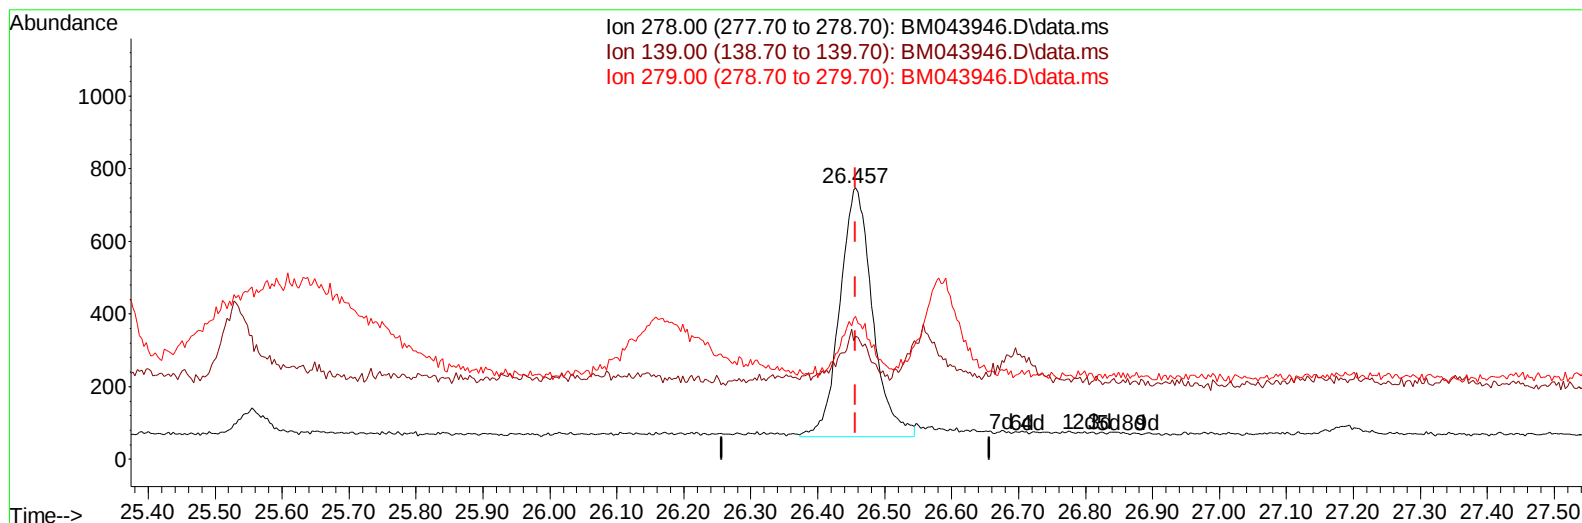

TIC: BM043946.D\data.ms

(28) Dibenzo(a,h)anthracene

26.457min (-0.000) 0.03 ng/ul m

response 2305

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	20.20	45.38#
279.00	27.10	52.61#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

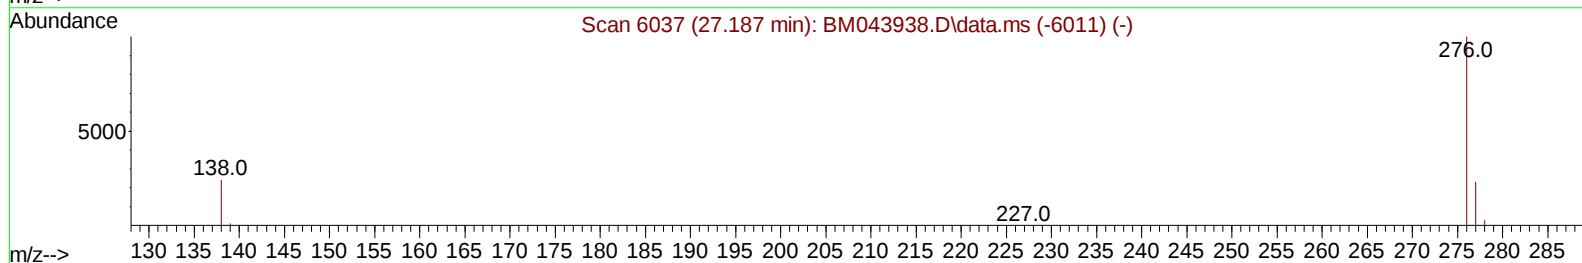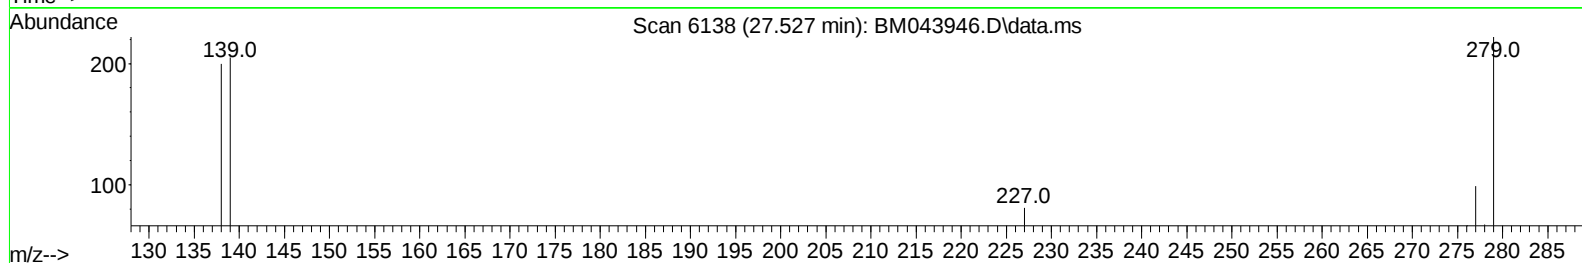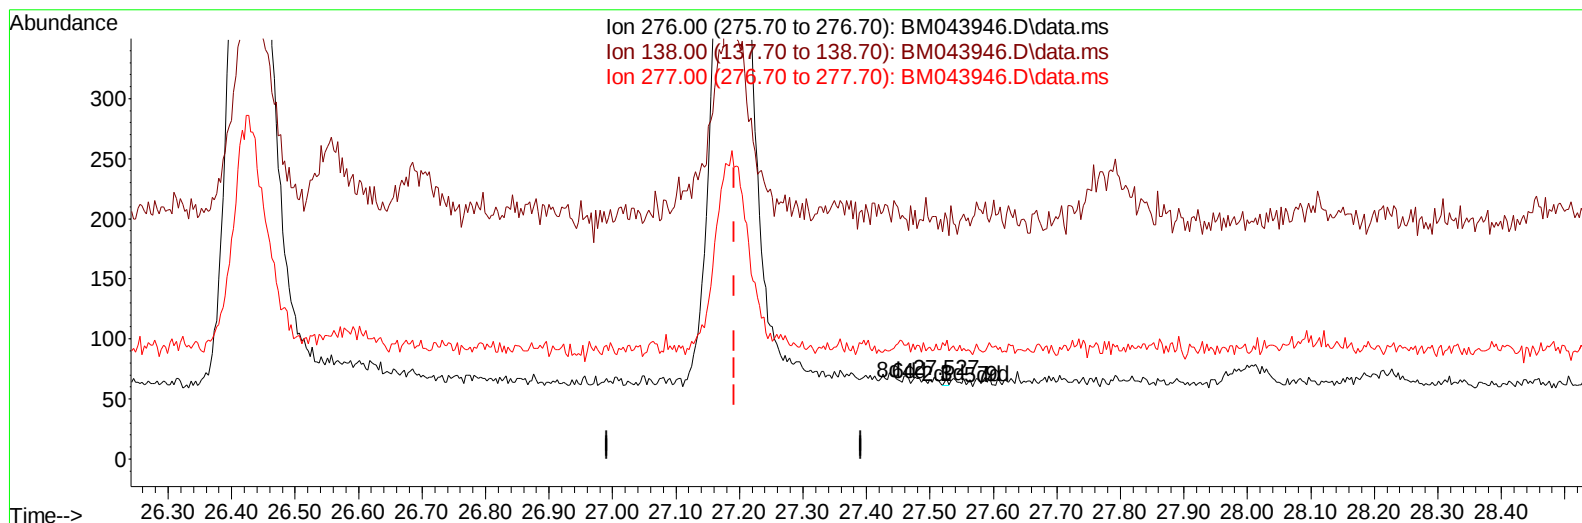

TIC: BM043946.D\data.ms

(29) Benzo(g,h,i)perylene

27.527min (+ 0.335) 0.00 ng/u1

response 2

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	25.20	303.03#
277.00	23.70	150.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

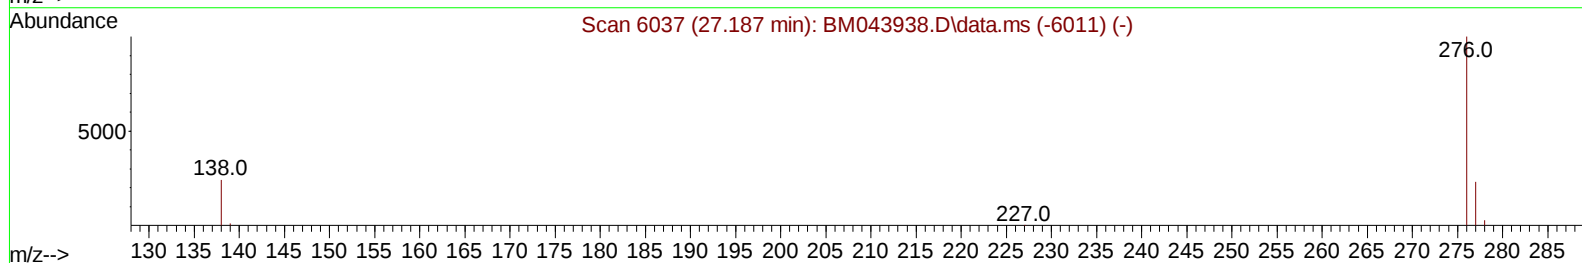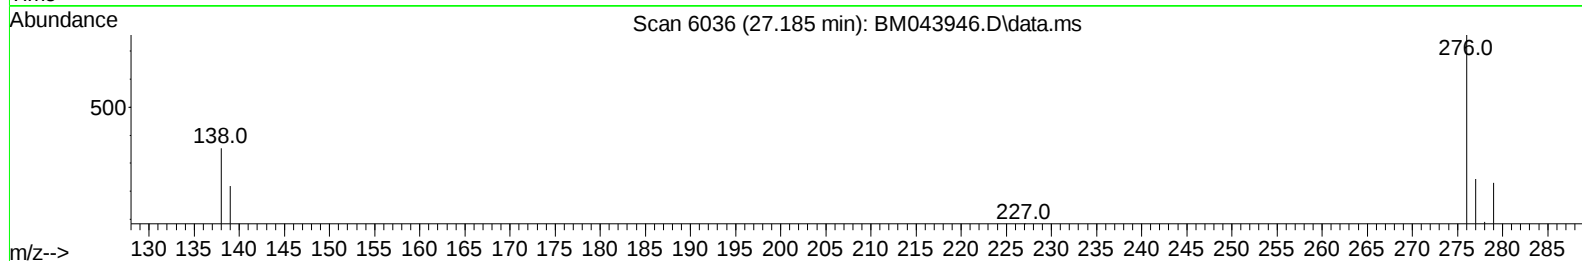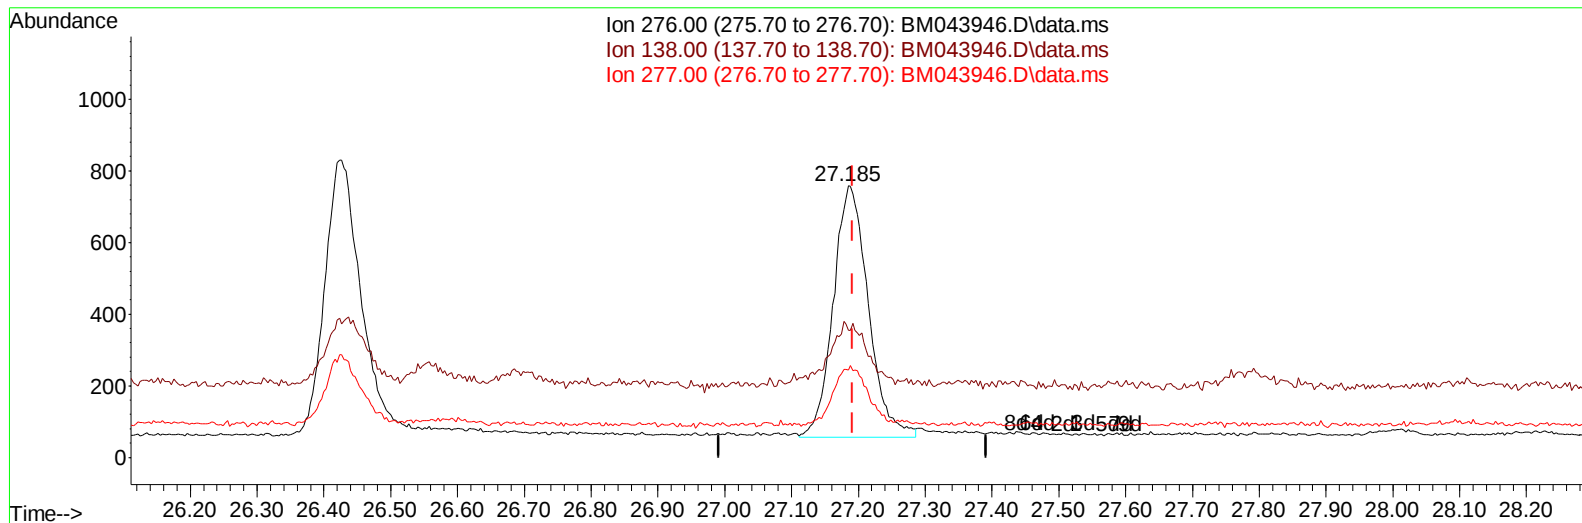

TIC: BM043946.D\data.ms

(29) Benzo(g,h,i)perylene

27.185min (-0.007) 0.03 ng/ul m

response 2544

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	25.20	46.70#
277.00	23.70	32.19#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043946.D
 Acq On : 01 Feb 2024 14:34
 Operator : MA/JU
 Sample : P1239-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FB9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 15:14:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.926	152		9291	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136		27165	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.566	164		13613	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.317	188		28359m	0.400	ng/ul	0.00
17) Chrysene-d12	21.514	240		21916m	0.400	ng/ul	0.00
23) Perylene-d12	23.926	264		22836m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.365	96		49669	4.155	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152		11648	0.327	ng/ul	0.00
18) Fluoranthene-d10	19.350	212		24717m	0.359	ng/ul	0.00
Target Compounds							Qvalue
14) Pentachlorophenol	16.959	266		494	0.074	ng/ul	98
24) Benzo(b)fluoranthene	23.192	252		2462m	0.028	ng/ul	
25) Benzo(k)fluoranthene	23.242	252		2427m	0.027	ng/ul	
27) Indeno(1,2,3-cd)pyrene	26.423	276		2949m	0.029	ng/ul	
28) Dibenzo(a,h)anthracene	26.457	278		2305m	0.028	ng/ul	
29) Benzo(g,h,i)perylene	27.185	276		2544m	0.029	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043946.D
Acq On : 01 Feb 2024 14:34
Operator : MA/JU
Sample : P1239-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB9

Manual IntegrationsAPPROVED

Quant Time: Feb 01 15:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

