




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043948.D
Acq On : 01 Feb 2024 15:47
Operator : MA/JU
Sample : P1239-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 16:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

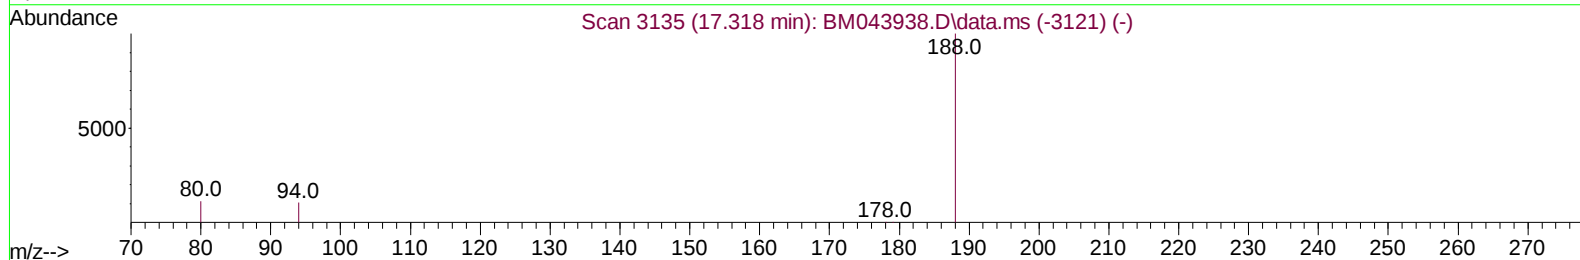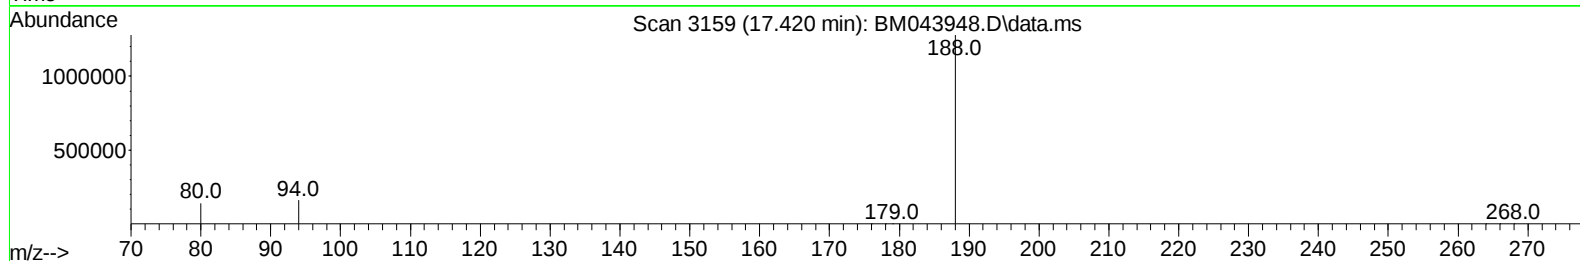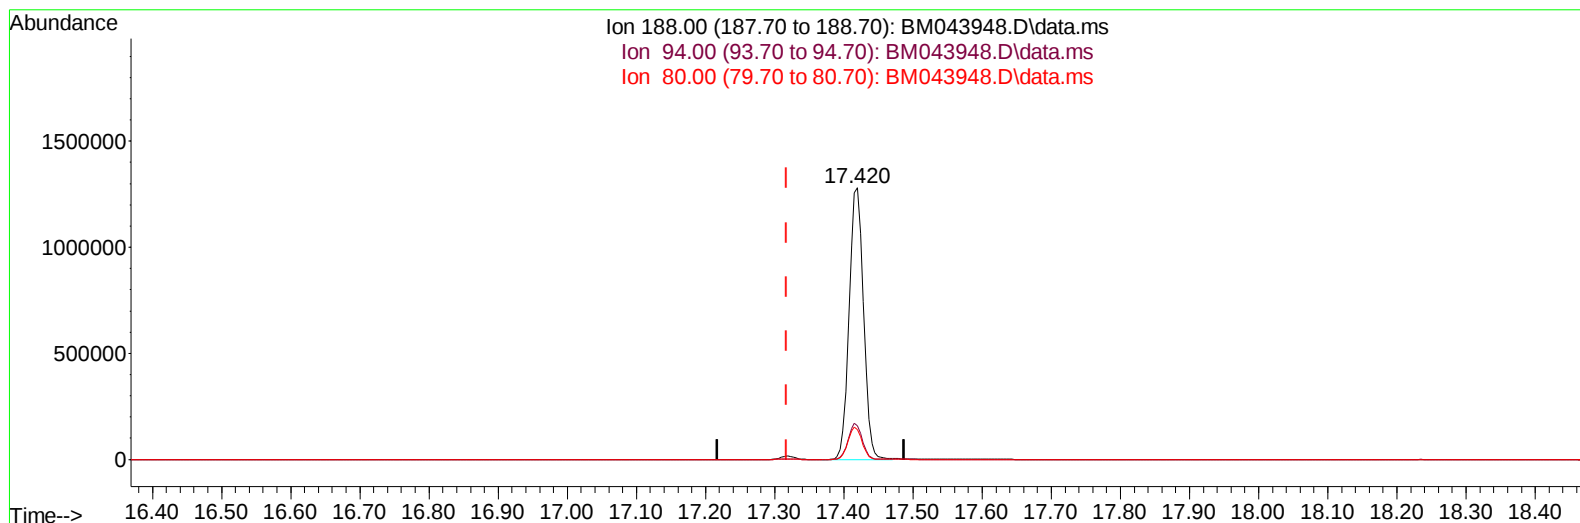

TIC: BM043948.D\data.ms

(13) Phenanthrene-d10 (I)

17.420min (+ 0.102) 0.40 ng/u1

response 1837435

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	12.50
80.00	12.90	10.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043948.D
Acq On : 01 Feb 2024 15:47
Operator : MA/JU
Sample : P1239-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 16:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

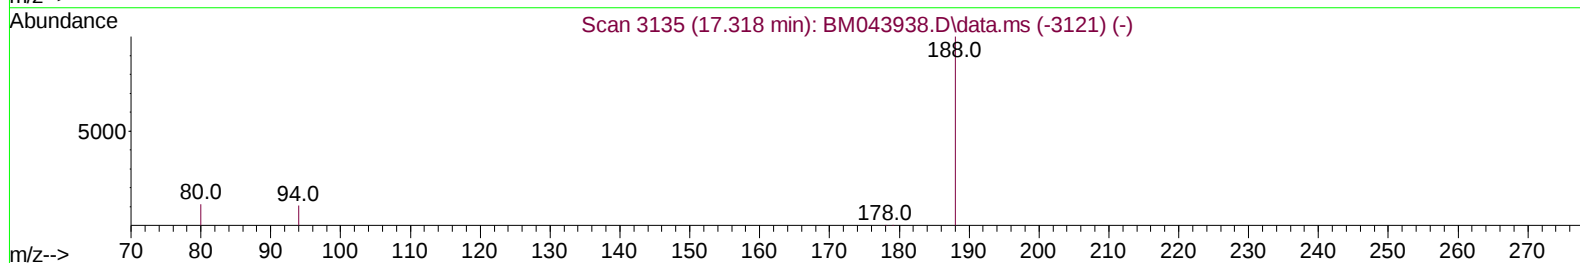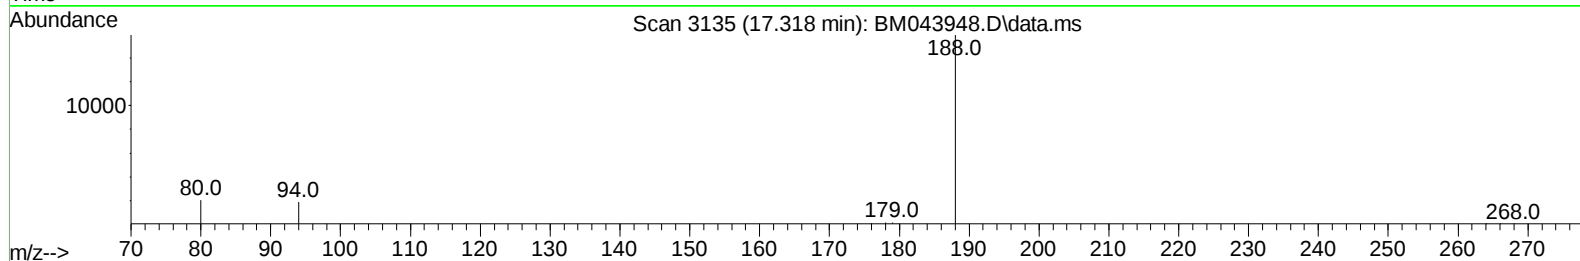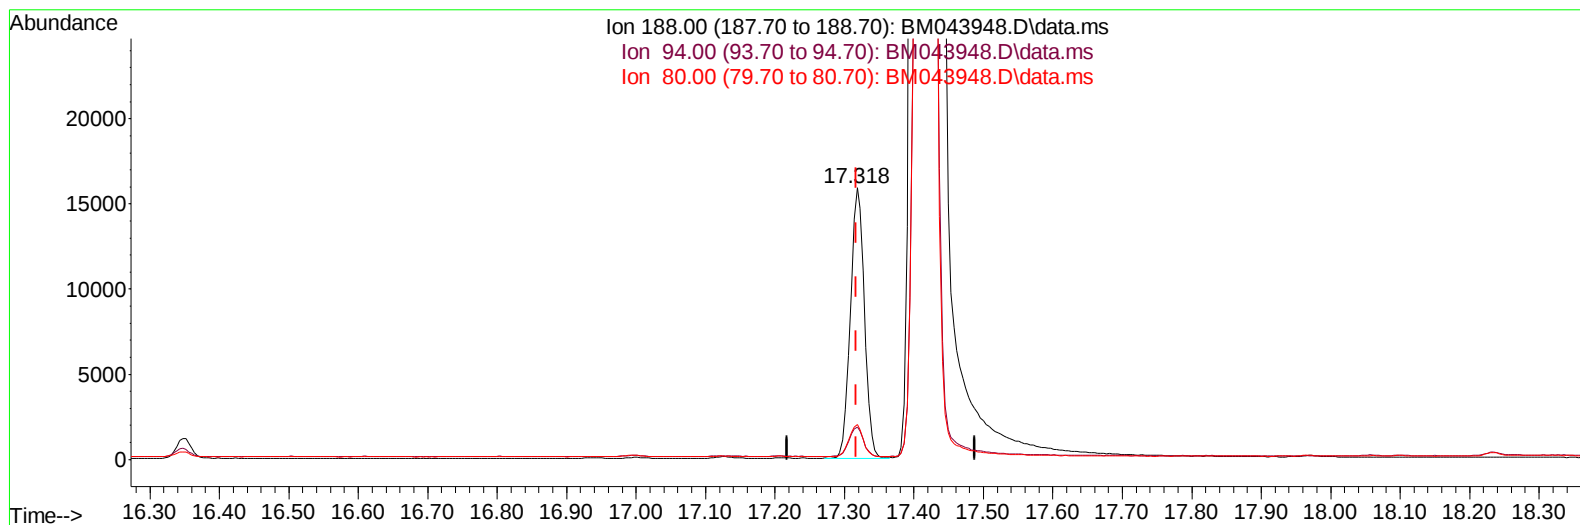

TIC: BM043948.D\data.ms

(13) Phenanthrene-d10 (I)

17.318min (+ 0.001) 0.40 ng/ul m

response 22329

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	11.91
80.00	12.90	12.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043948.D
Acq On : 01 Feb 2024 15:47
Operator : MA/JU
Sample : P1239-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 16:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

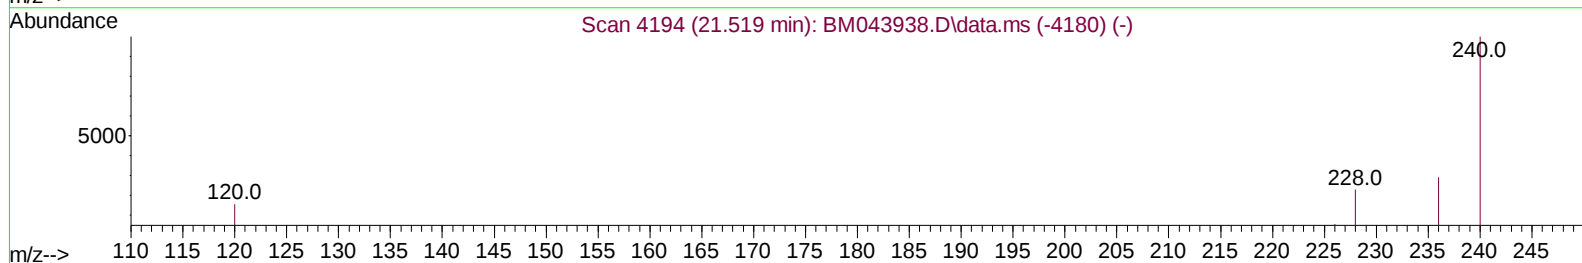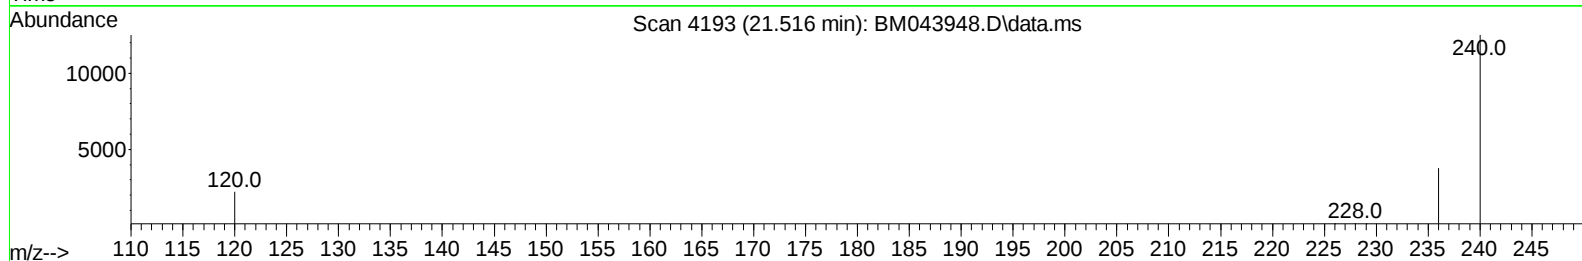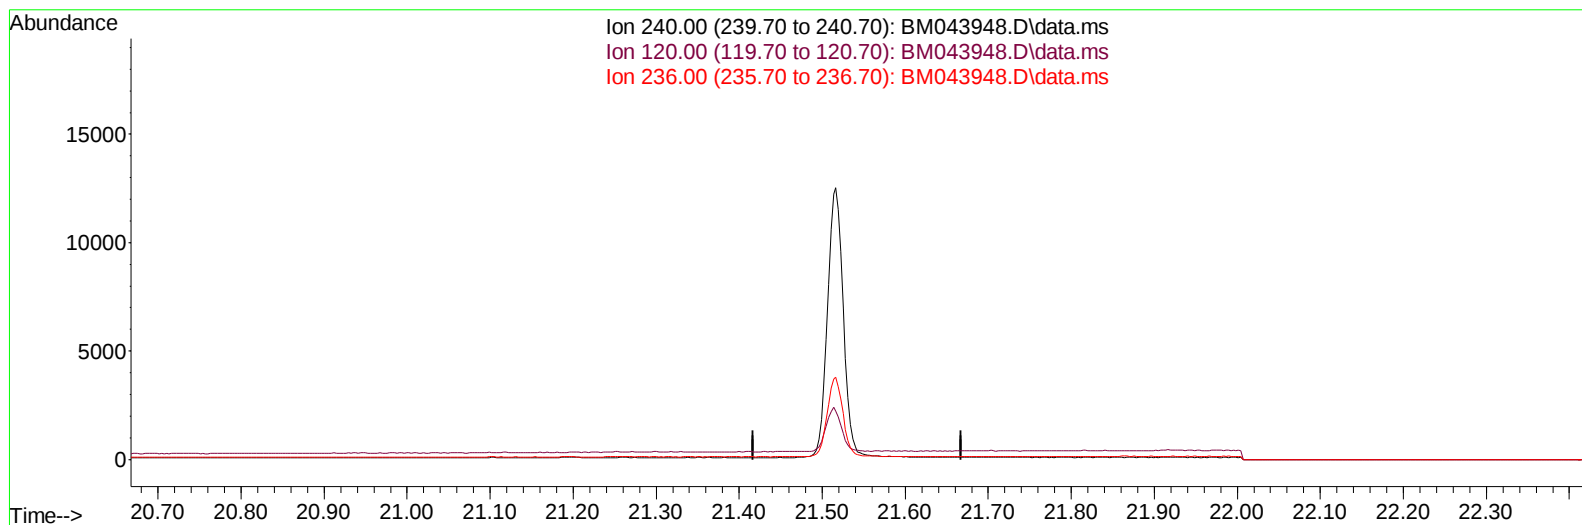

TIC: BM043948.D\data.ms

(17) Chrysene-d12

21.517min (-21.517) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	17.60	0.00#
236.00	29.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043948.D
Acq On : 01 Feb 2024 15:47
Operator : MA/JU
Sample : P1239-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 16:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

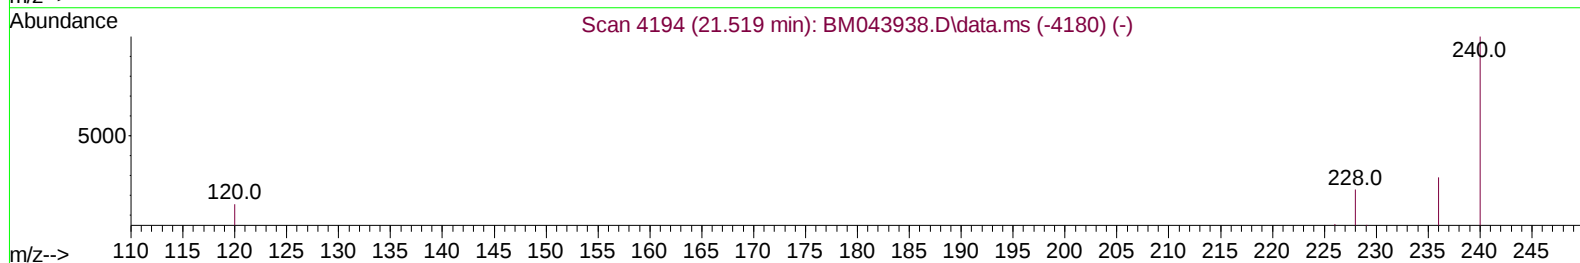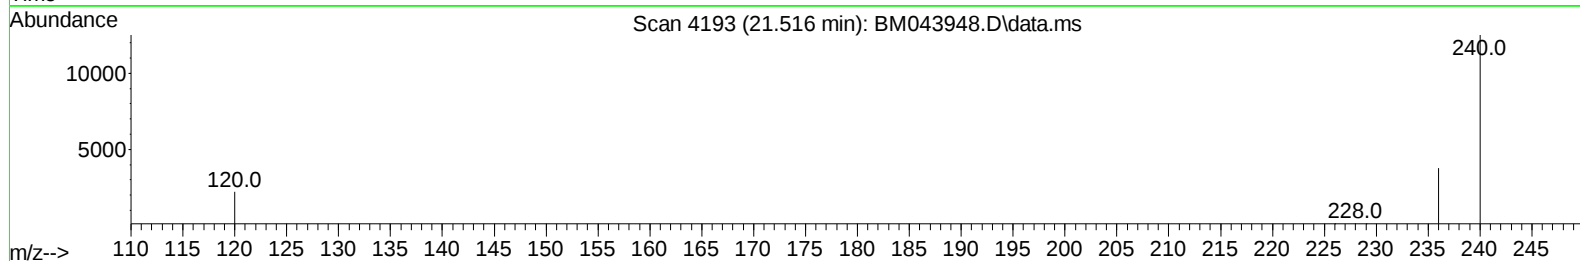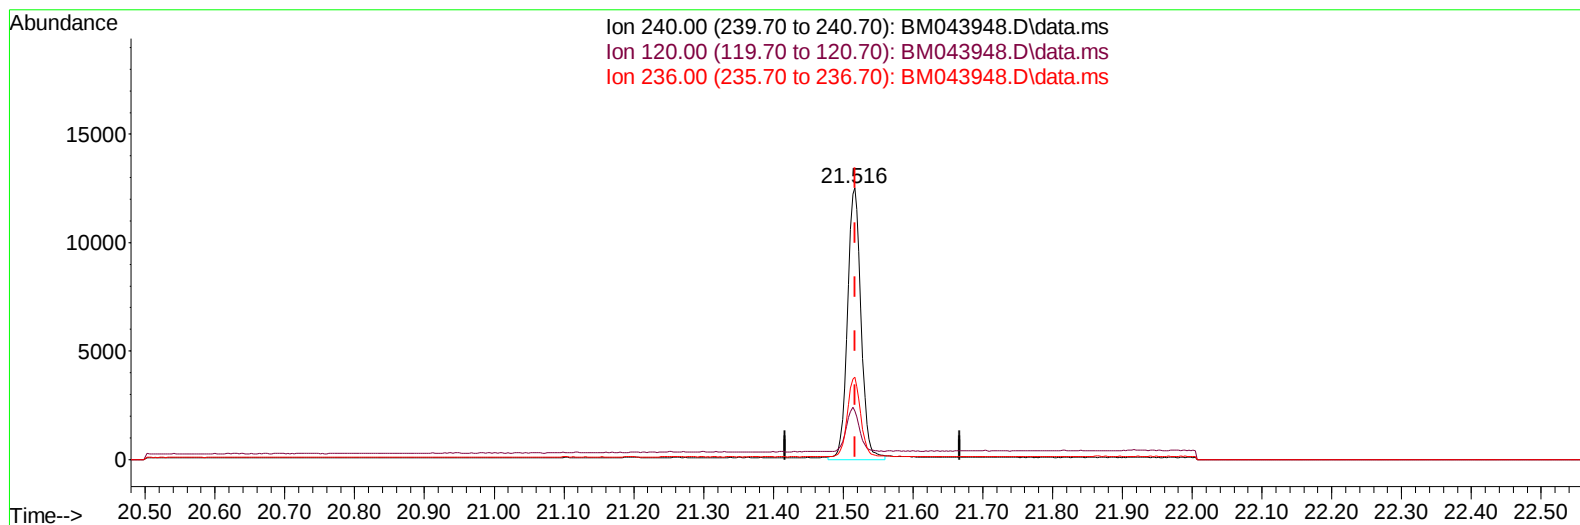

TIC: BM043948.D\data.ms

(17) Chrysene-d12

21.516min (-0.001) 0.40 ng/u1 m

response 16931

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	17.60	17.76
236.00	29.90	30.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043948.D
 Acq On : 01 Feb 2024 15:47
 Operator : MA/JU
 Sample : P1239-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FB5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 16:58:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

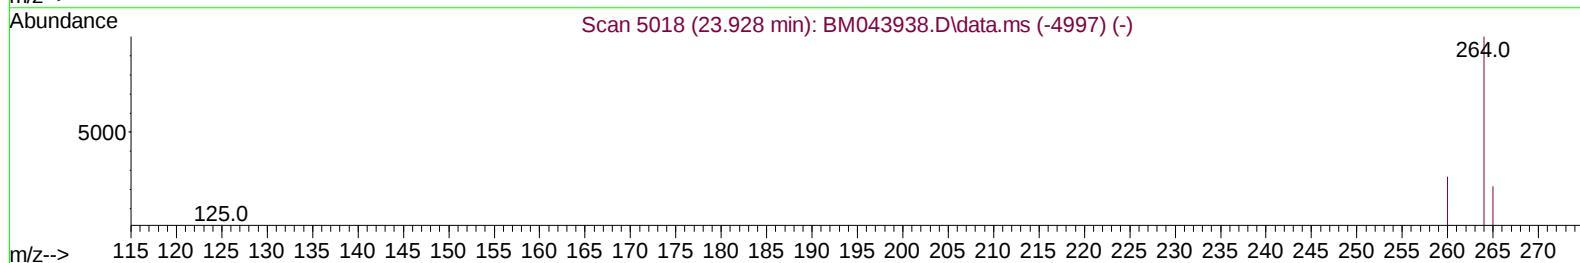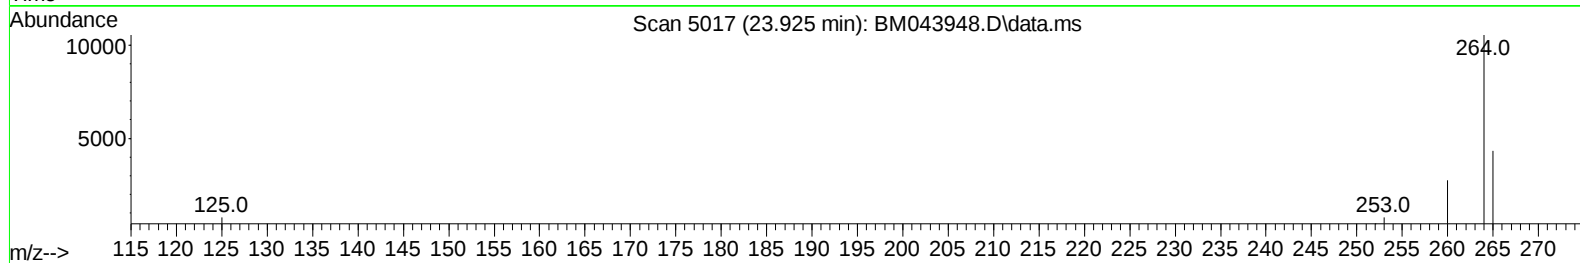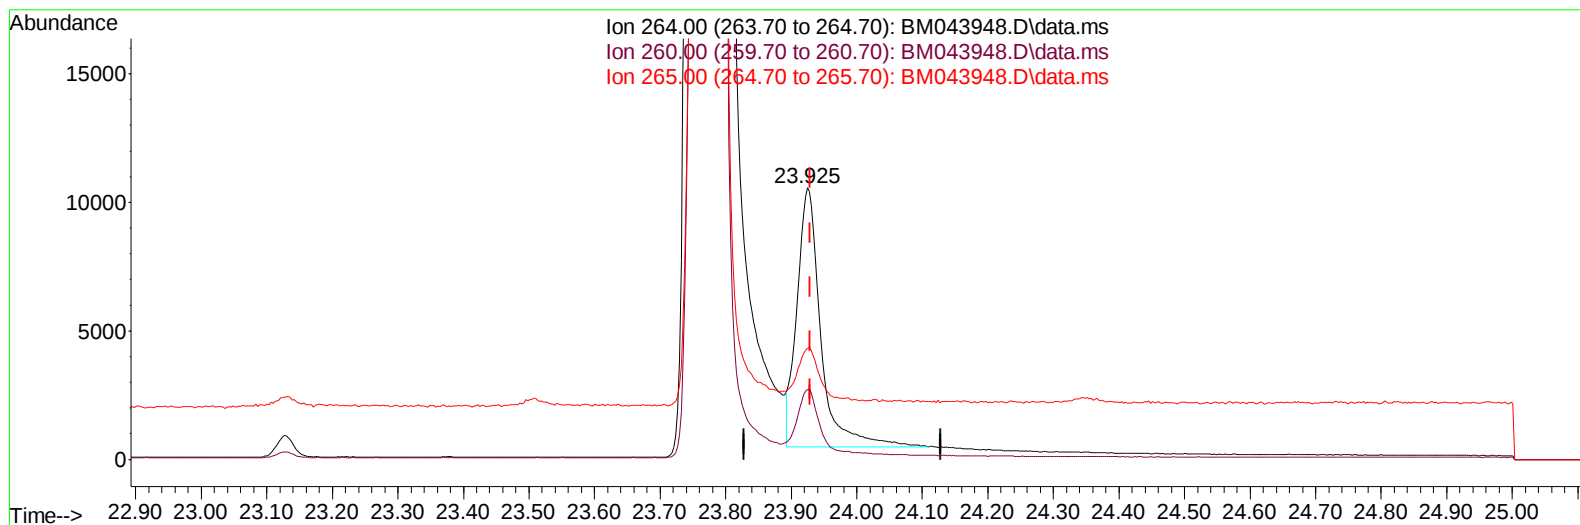

TIC: BM043948.D\data.ms

(23) Perylene-d12 (I)

23.925min (-0.004) 0.40 ng/u1

response 25489

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	25.90
265.00	42.60	40.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043948.D
Acq On : 01 Feb 2024 15:47
Operator : MA/JU
Sample : P1239-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 16:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

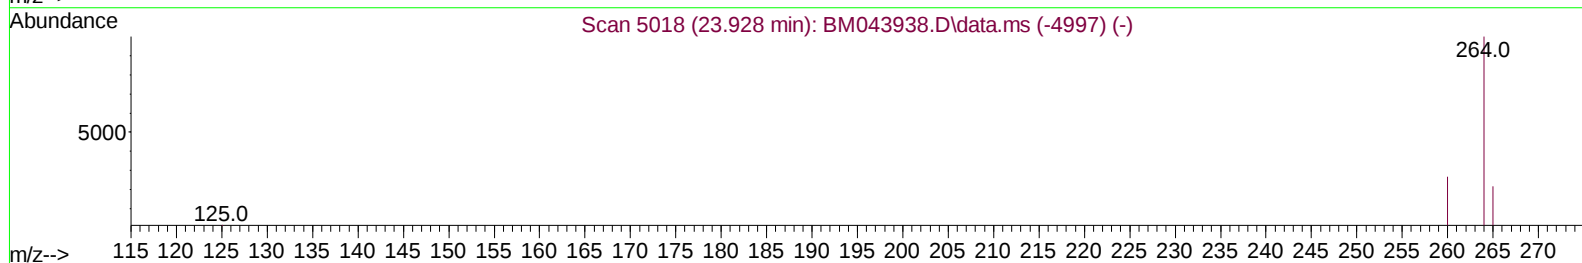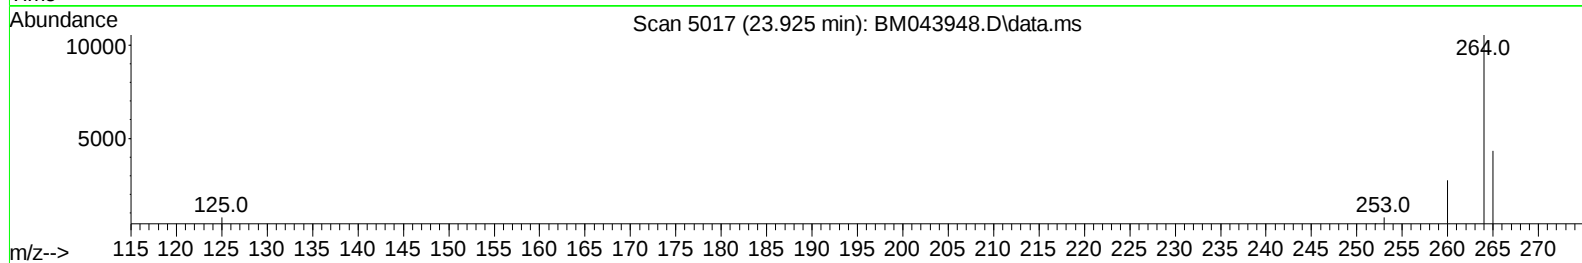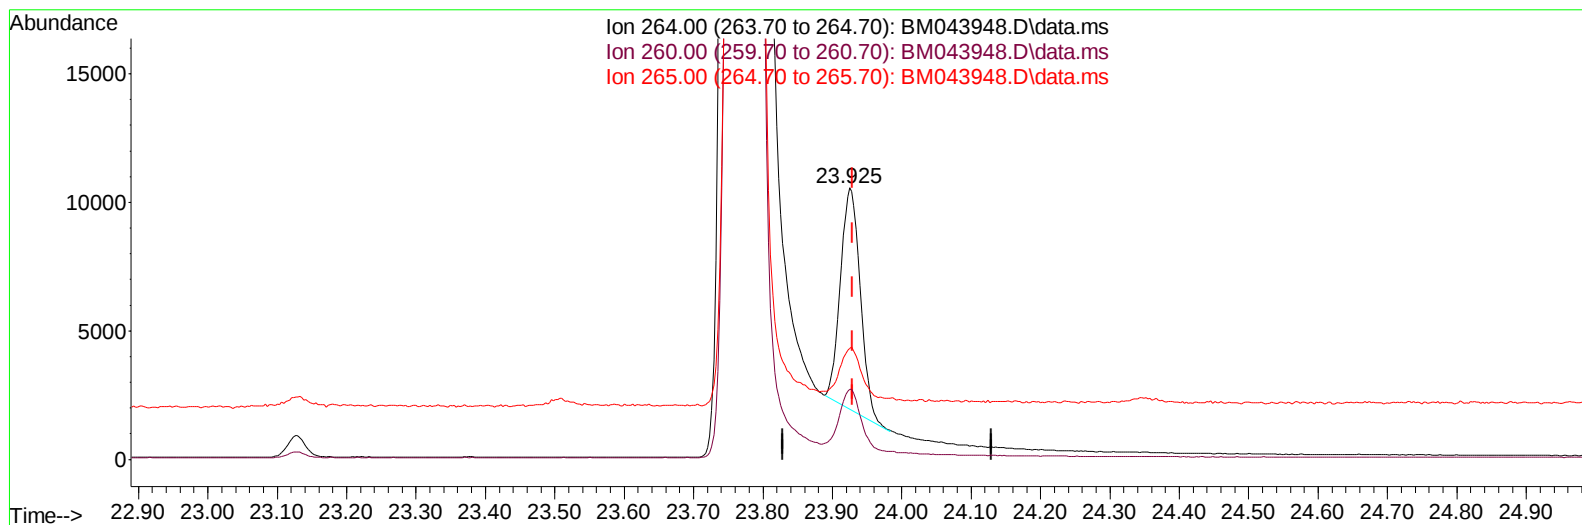

TIC: BM043948.D\data.ms

(23) Perylene-d12 (I)

23.925min (-0.004) 0.40 ng/ul m

response 16953

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	25.90
265.00	42.60	40.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043948.D
 Acq On : 01 Feb 2024 15:47
 Operator : MA/JU
 Sample : P1239-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FB5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 16:58:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	7708	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	22099	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.567	164	11688	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.318	188	22329m	0.400	ng/ul	0.00
17) Chrysene-d12	21.516	240	16931m	0.400	ng/ul	0.00
23) Perylene-d12	23.925	264	16953m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.365	96	34582	3.487	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	10600	0.366	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	20658	0.389	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043948.D
Acq On : 01 Feb 2024 15:47
Operator : MA/JU
Sample : P1239-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FB5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 16:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

