




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043956.D
Acq On : 01 Feb 2024 21:16
Operator : MA/JU
Sample : PB158662BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK662

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:55:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

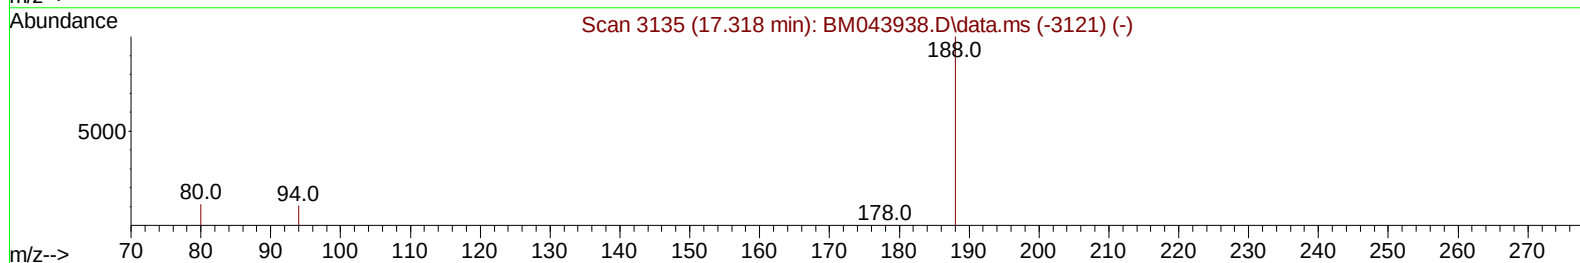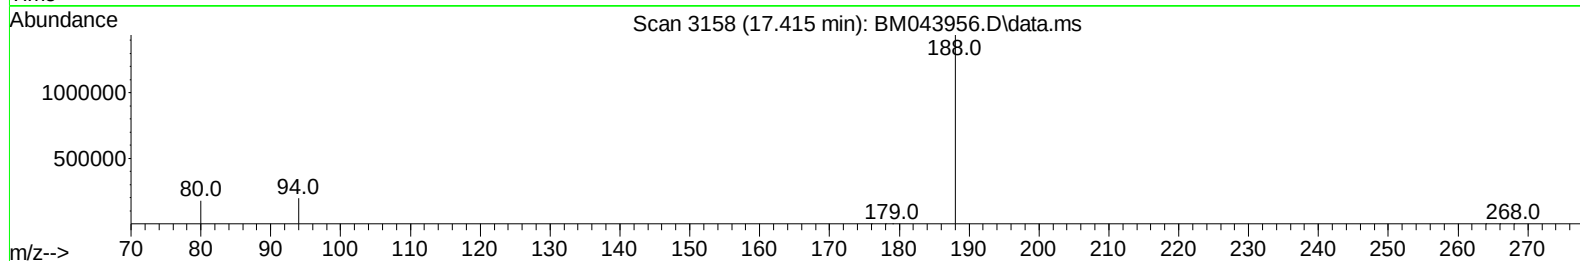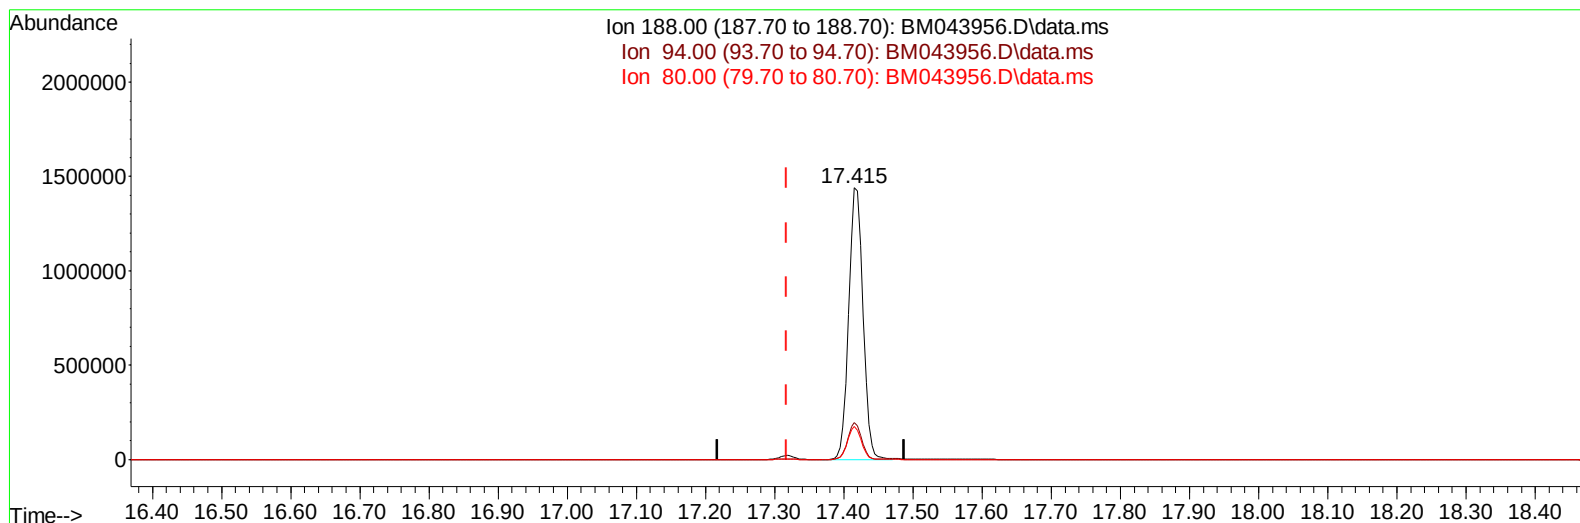

TIC: BM043956.D\data.ms

(13) Phenanthrene-d10 (I)

17.415min (+ 0.098) 0.40 ng/u1

response 2055447

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	13.55
80.00	12.90	12.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043956.D
Acq On : 01 Feb 2024 21:16
Operator : MA/JU
Sample : PB158662BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK662

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:55:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

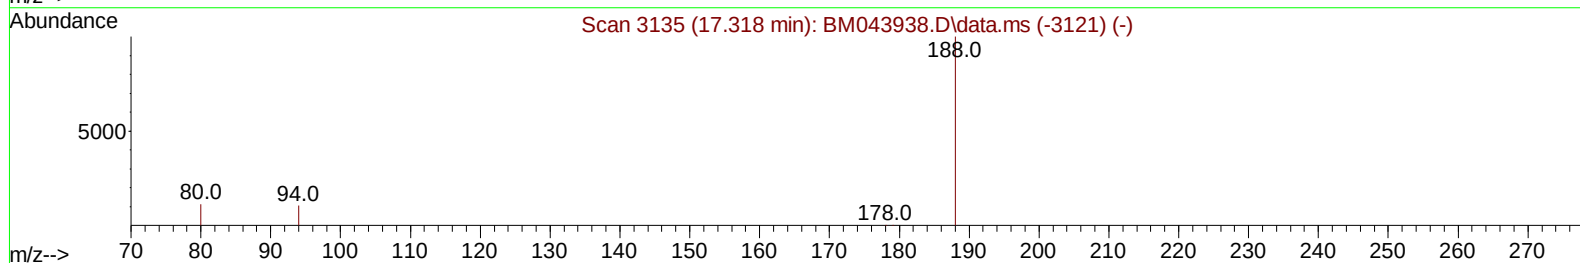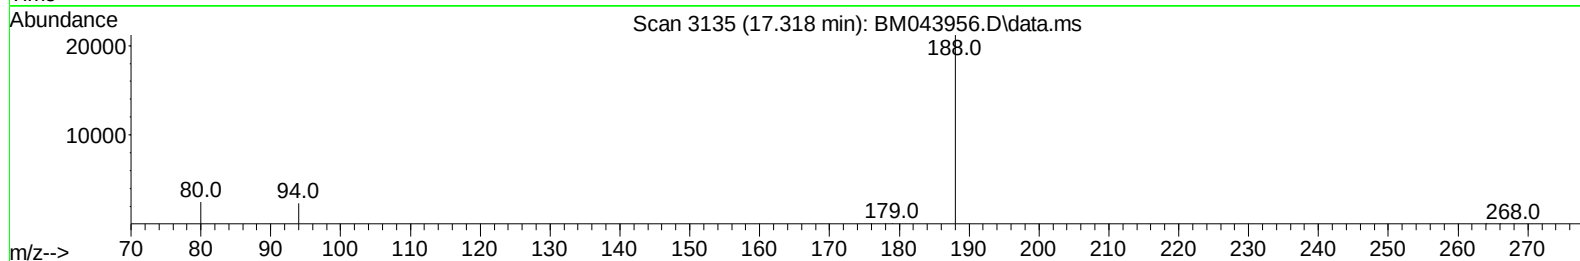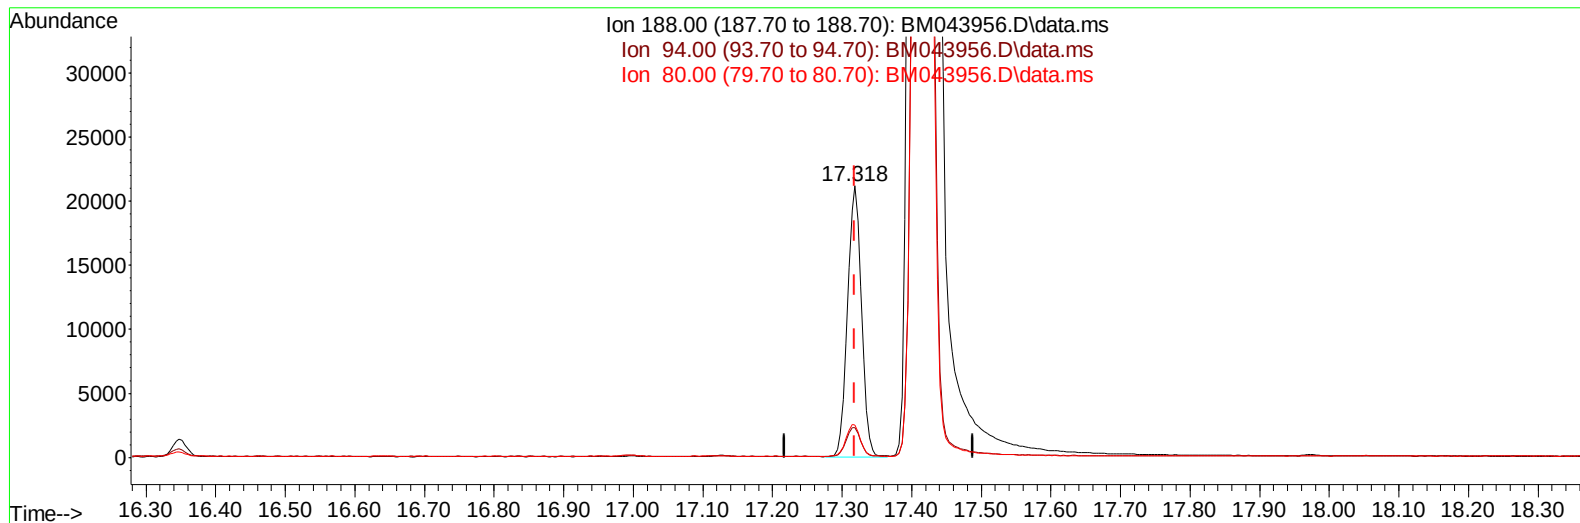

TIC: BM043956.D\data.ms

(13) Phenanthrene-d10 (I)

17.318min (+ 0.001) 0.40 ng/ul m

response 29554

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	11.07
80.00	12.90	11.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043956.D
Acq On : 01 Feb 2024 21:16
Operator : MA/JU
Sample : PB158662BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK662

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:55:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

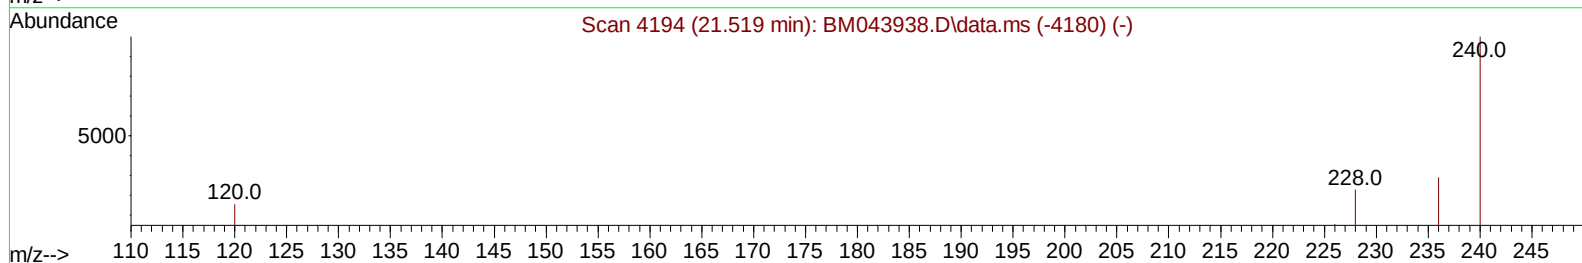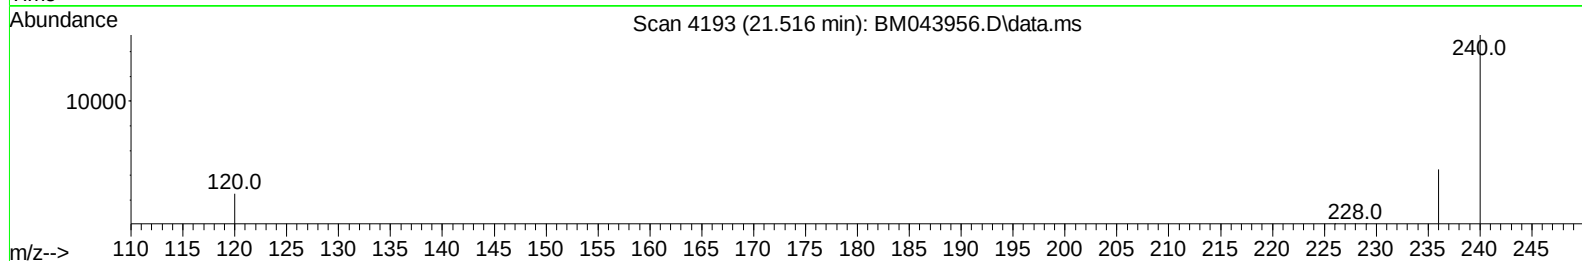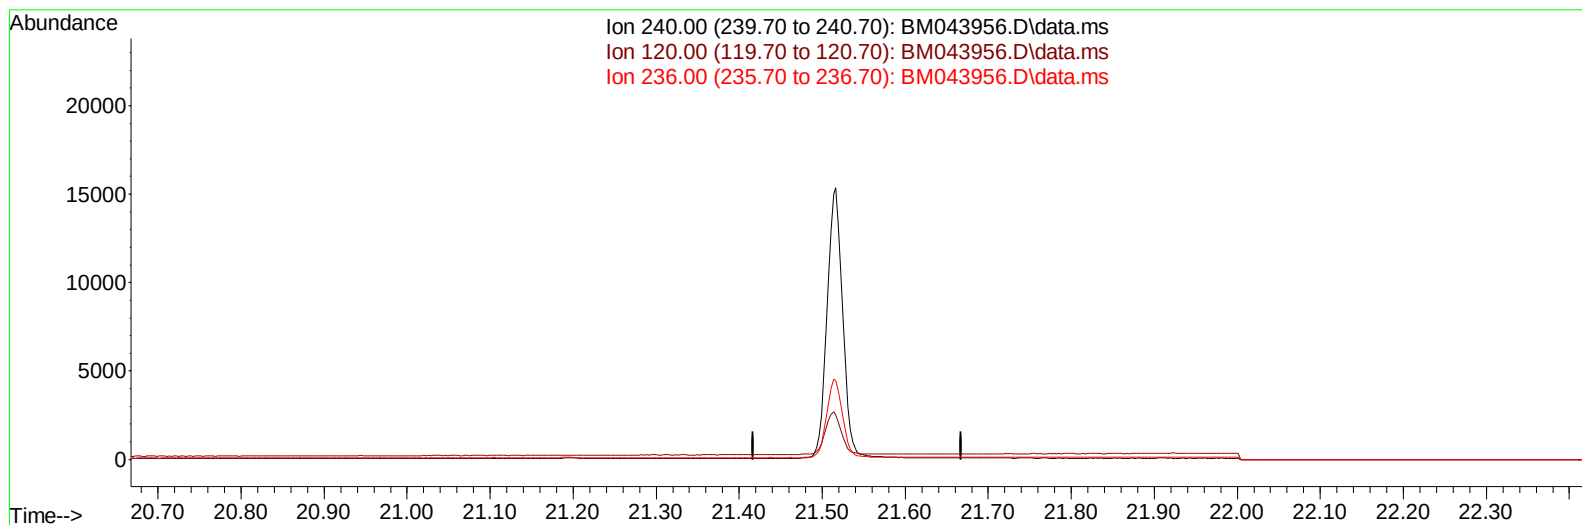

TIC: BM043956.D\data.ms

(17) Chrysene-d12

21.517min (-21.517) 0.00 ng/ul

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	17.60	0.00#
236.00	29.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043956.D
Acq On : 01 Feb 2024 21:16
Operator : MA/JU
Sample : PB158662BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK662

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:55:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

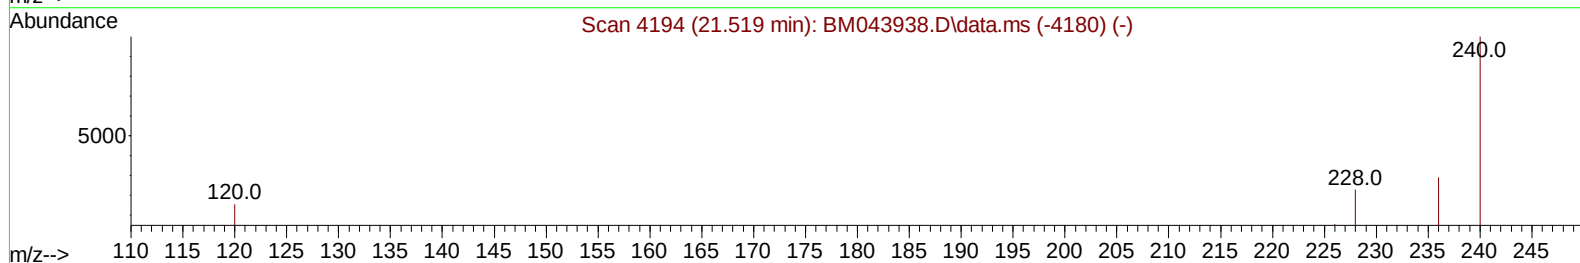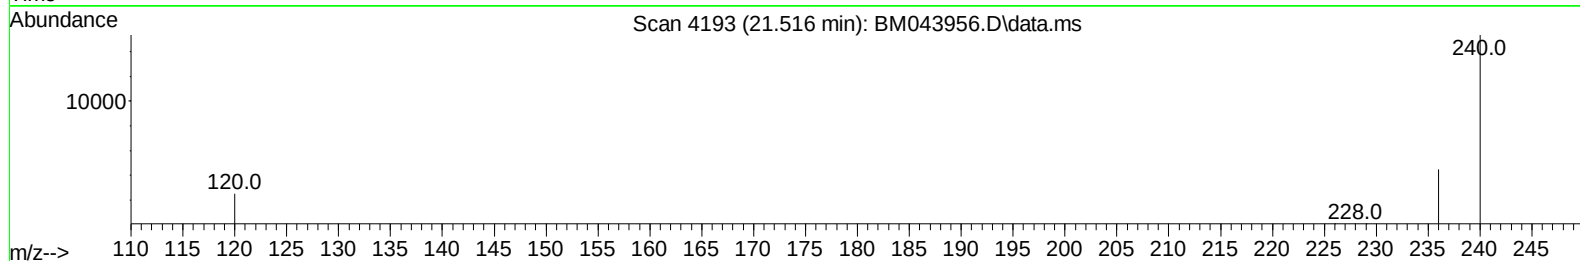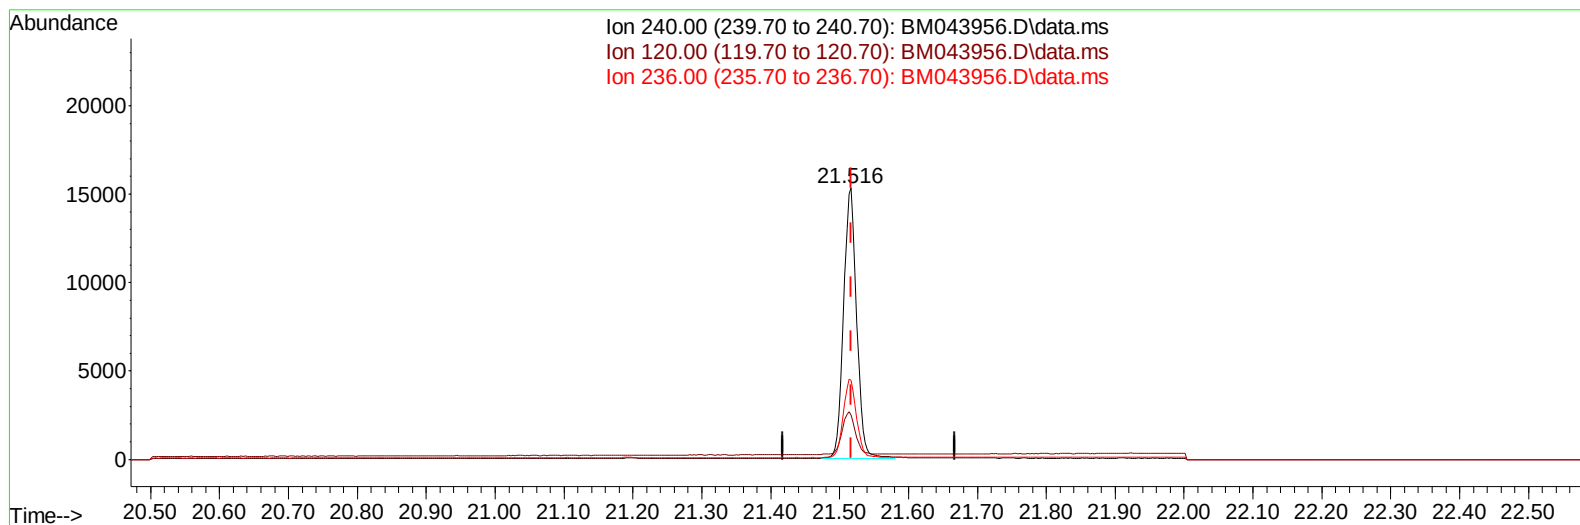

TIC: BM043956.D\data.ms

(17) Chrysene-d12

21.516min (-0.001) 0.40 ng/ul m

response 20043

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	17.60	16.47
236.00	29.90	29.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043956.D
 Acq On : 01 Feb 2024 21:16
 Operator : MA/JU
 Sample : PB158662BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK662

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 23:55:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	9350	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	27770	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.567	164	14178	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.318	188	29554m	0.400	ng/ul	0.00
17) Chrysene-d12	21.516	240	20043m	0.400	ng/ul	0.00
23) Perylene-d12	23.922	264	30864	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.365	96	72566	6.032	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	11787	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.350	212	21706	0.345	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043956.D
Acq On : 01 Feb 2024 21:16
Operator : MA/JU
Sample : PB158662BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK662

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:55:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

