

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
 Data File : BM043952.D
 Acq On : 01 Feb 2024 18:14
 Operator : MA/JU
 Sample : P1239-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FC5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 23:54:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 22:50:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	8870	0.400	ng/u1	0.00
4) Naphthalene-d8	10.726	136	26768	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.567	164	14083	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.318	188	29948m	0.400	ng/u1	0.00
17) Chrysene-d12	21.514	240	21949m	0.400	ng/u1	0.00
23) Perylene-d12	23.925	264	28518m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	47560	4.167	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.316	152	14776	0.421	ng/u1	0.00
18) Fluoranthene-d10	19.350	212	31777m	0.461	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.964	266	1735	0.245	ng/u1	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020124\
Data File : BM043952.D
Acq On : 01 Feb 2024 18:14
Operator : MA/JU
Sample : P1239-15
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0FC5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024


Quant Time: Feb 01 23:54:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 22:50:05 2024
Response via : Initial Calibration

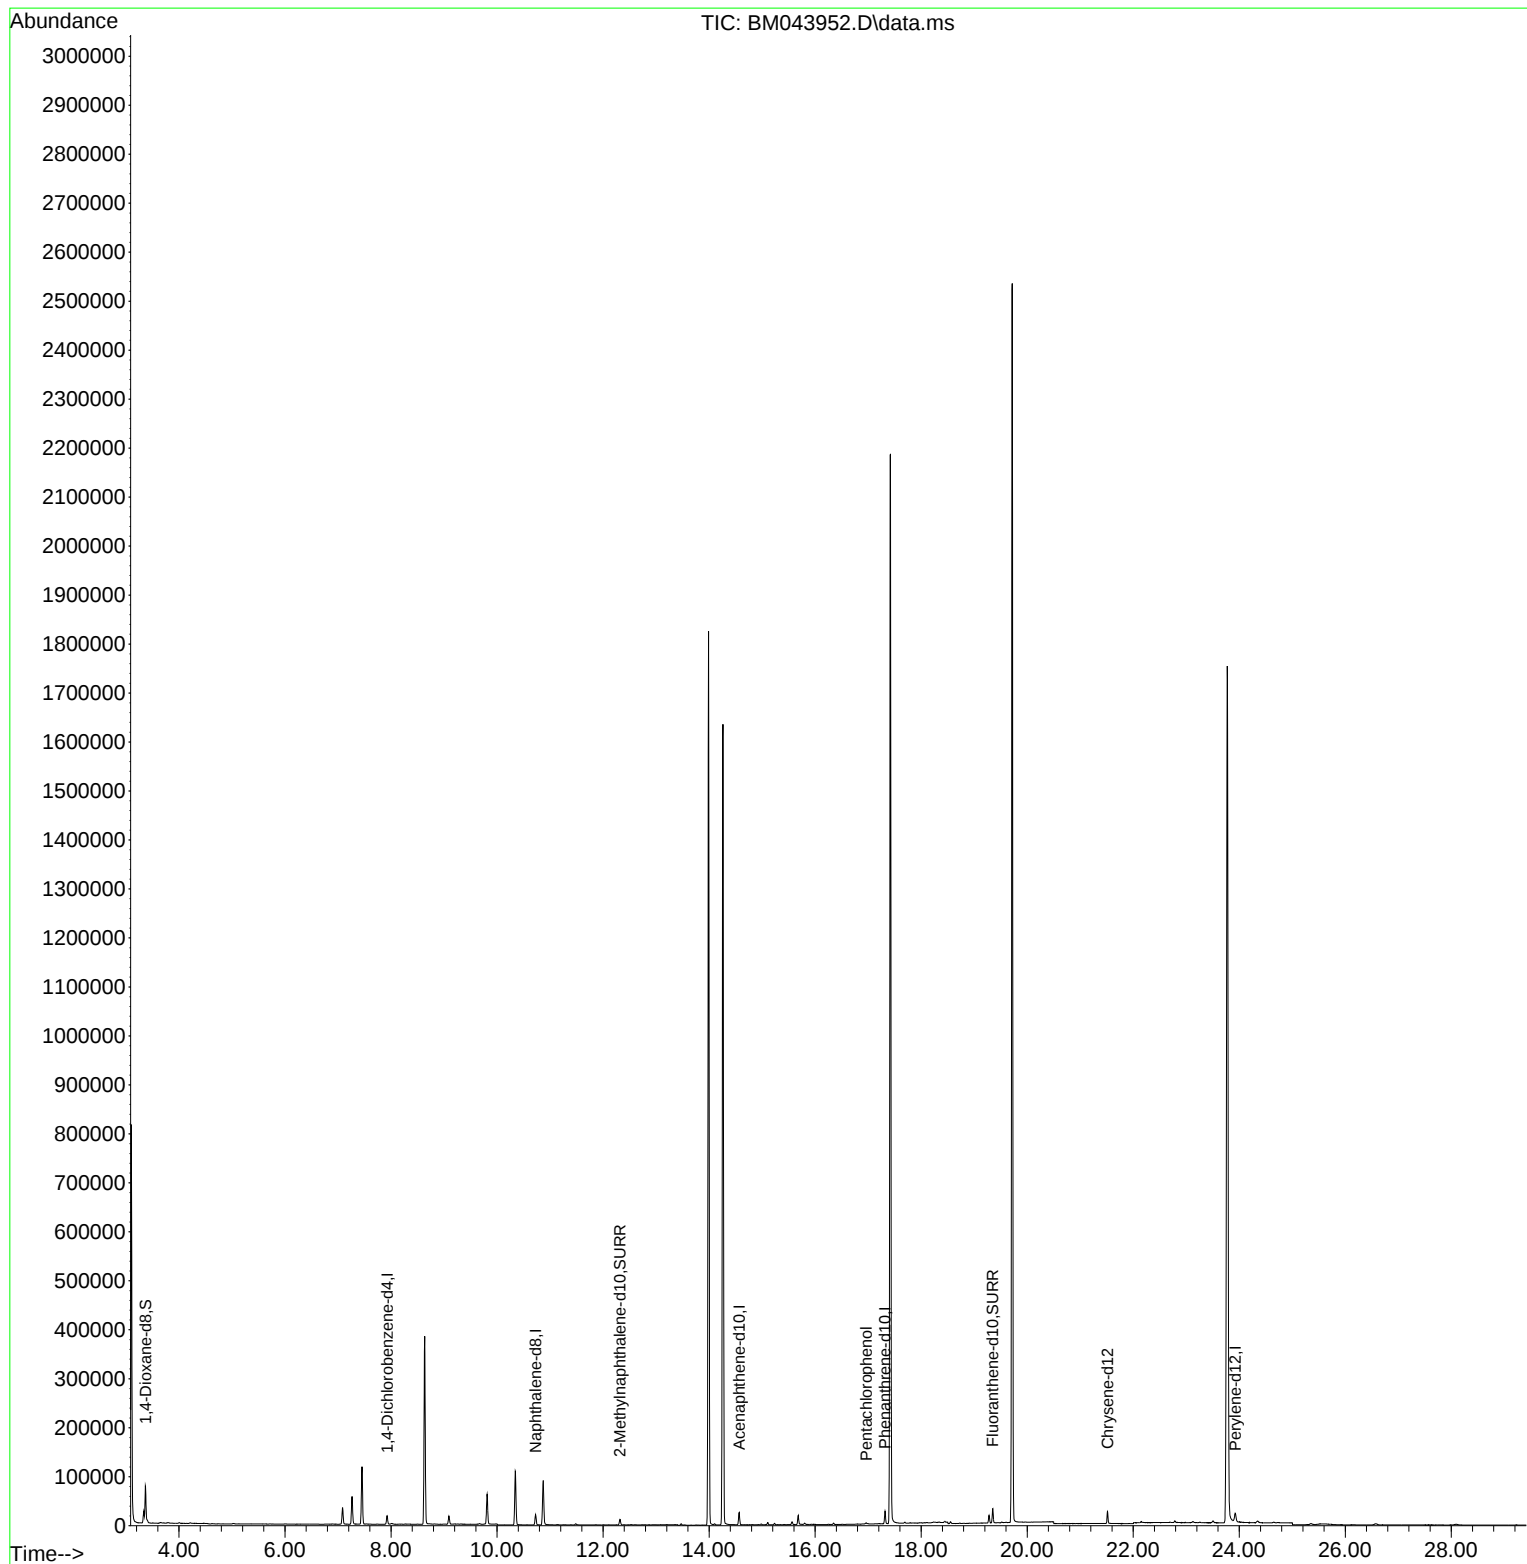

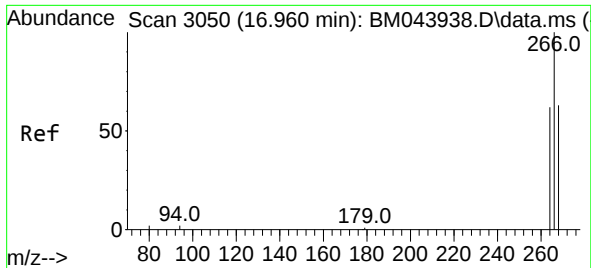

#14
 Pentachlorophenol
 Concen: 0.245 ng/ul
 RT: 16.964 min Scan# 3051
 Delta R.T. 0.005 min
 Lab File: BM043952.D
 Acq: 01 Feb 2024 18:14

Instrument :
 BNA_M
 ClientSampleId :
 C0FC5

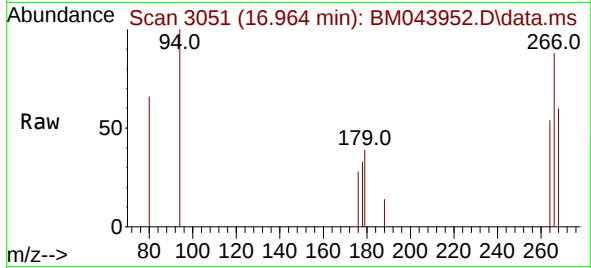

Tgt Ion:	266	Resp:	173
Ion	Ratio	Lower	Upper
266	100		
264	66.5	51.3	76.9
268	62.1	54.7	82.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

