


Data Path : Z:\HPCHEM1\BNA M\Data\BM020216\
 Data File : BM004164.D
 Acq On : 02 Feb 2016 13:30
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM012216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 22 14:46:41 2016

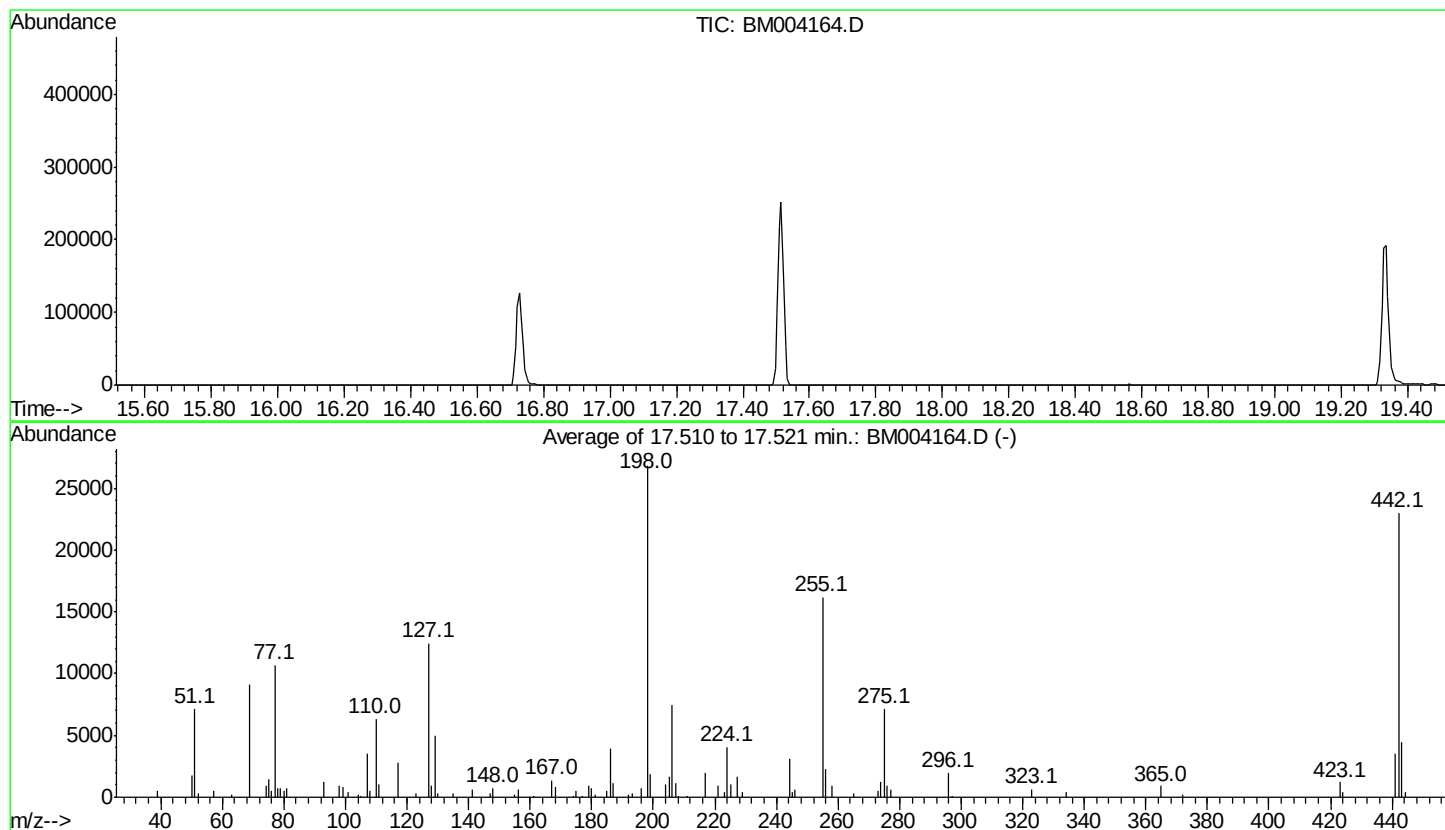

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	7156	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	9090	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	12480	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26832	PASS
199	198	5	9	7.0	1886	PASS
275	198	10	60	26.6	7149	PASS
365	198	1	100	3.3	894	PASS
441	442	0.01	24	15.3	3520	PASS
442	198	50	100	85.9	23037	PASS
443	442	15	24	19.2	4417	PASS