

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020217\
 Data File : BM008960.D
 Acq On : 02 Feb 2017 13:53
 Operator : SJ/MA
 Sample : I1449-13MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FJ4MS

Quant Time: Feb 02 17:40:52 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 17:33:49 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	59241	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	247455	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.55	164	181100	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	425285	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	528367	20.00	ng/ul	0.00
83) Perylene-d12	23.82	264	457299	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	4535	3.06	ng/uL	0.00
5) Phenol-d5	7.06	99	124511	22.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.24	67	114172	25.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	84379	24.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.61	113	96209	23.00	ng/ul	0.00
19) Nitrobenzene-d5	9.07	128	43858	24.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.80	143	41848	21.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.33	165	95574	22.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.85	131	68983	18.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	211998	15.97	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	409853	27.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.74	143	32869	15.17	ng/ul	0.00
57) Fluorene-d10	15.55	176	329201	26.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	20941	7.61	ng/ul	0.00
70) Anthracene-d10	17.40	188	552142	27.17	ng/ul	0.00
76) Pyrene-d10	19.69	212	667943	28.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.67	264	546057	26.30	ng/ul	0.00

Target Compounds


						Qvalue
6) Phenol	7.09	94	151632	25.83	ng/ul#	92
10) 2-Chlorophenol	7.48	128	83724	23.72	ng/ul	94
15) N-Nitroso-di-n-propylamine	8.72	70	68201	13.22	ng/ul#	96
33) 4-Chloro-3-methylphenol	11.99	107	133139	23.88	ng/ul	93
44) Dimethylphthalate	14.00	163	52637	4.06	ng/ul#	94
49) Acenaphthene	14.62	153	272360	25.61	ng/ul	99
52) 4-Nitrophenol	14.75	109	82796	17.52	ng/ul	97
54) 2,4-Dinitrotoluene	14.92	165	67195	17.84	ng/ul#	97
68) Pentachlorophenol	16.94	266	72620	21.25	ng/ul	90
77) Pyrene	19.72	202	820183	28.06	ng/ul#	97
81) Bis(2-ethylhexyl)phthalate	21.36	149	48507	3.20	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020217\
Data File : BM008960.D
Acq On : 02 Feb 2017 13:53
Operator : SJ/MA
Sample : I1449-13MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0FJ4MS

Quant Time: Feb 02 17:40:52 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 17:33:49 2017
Response via : Initial Calibration

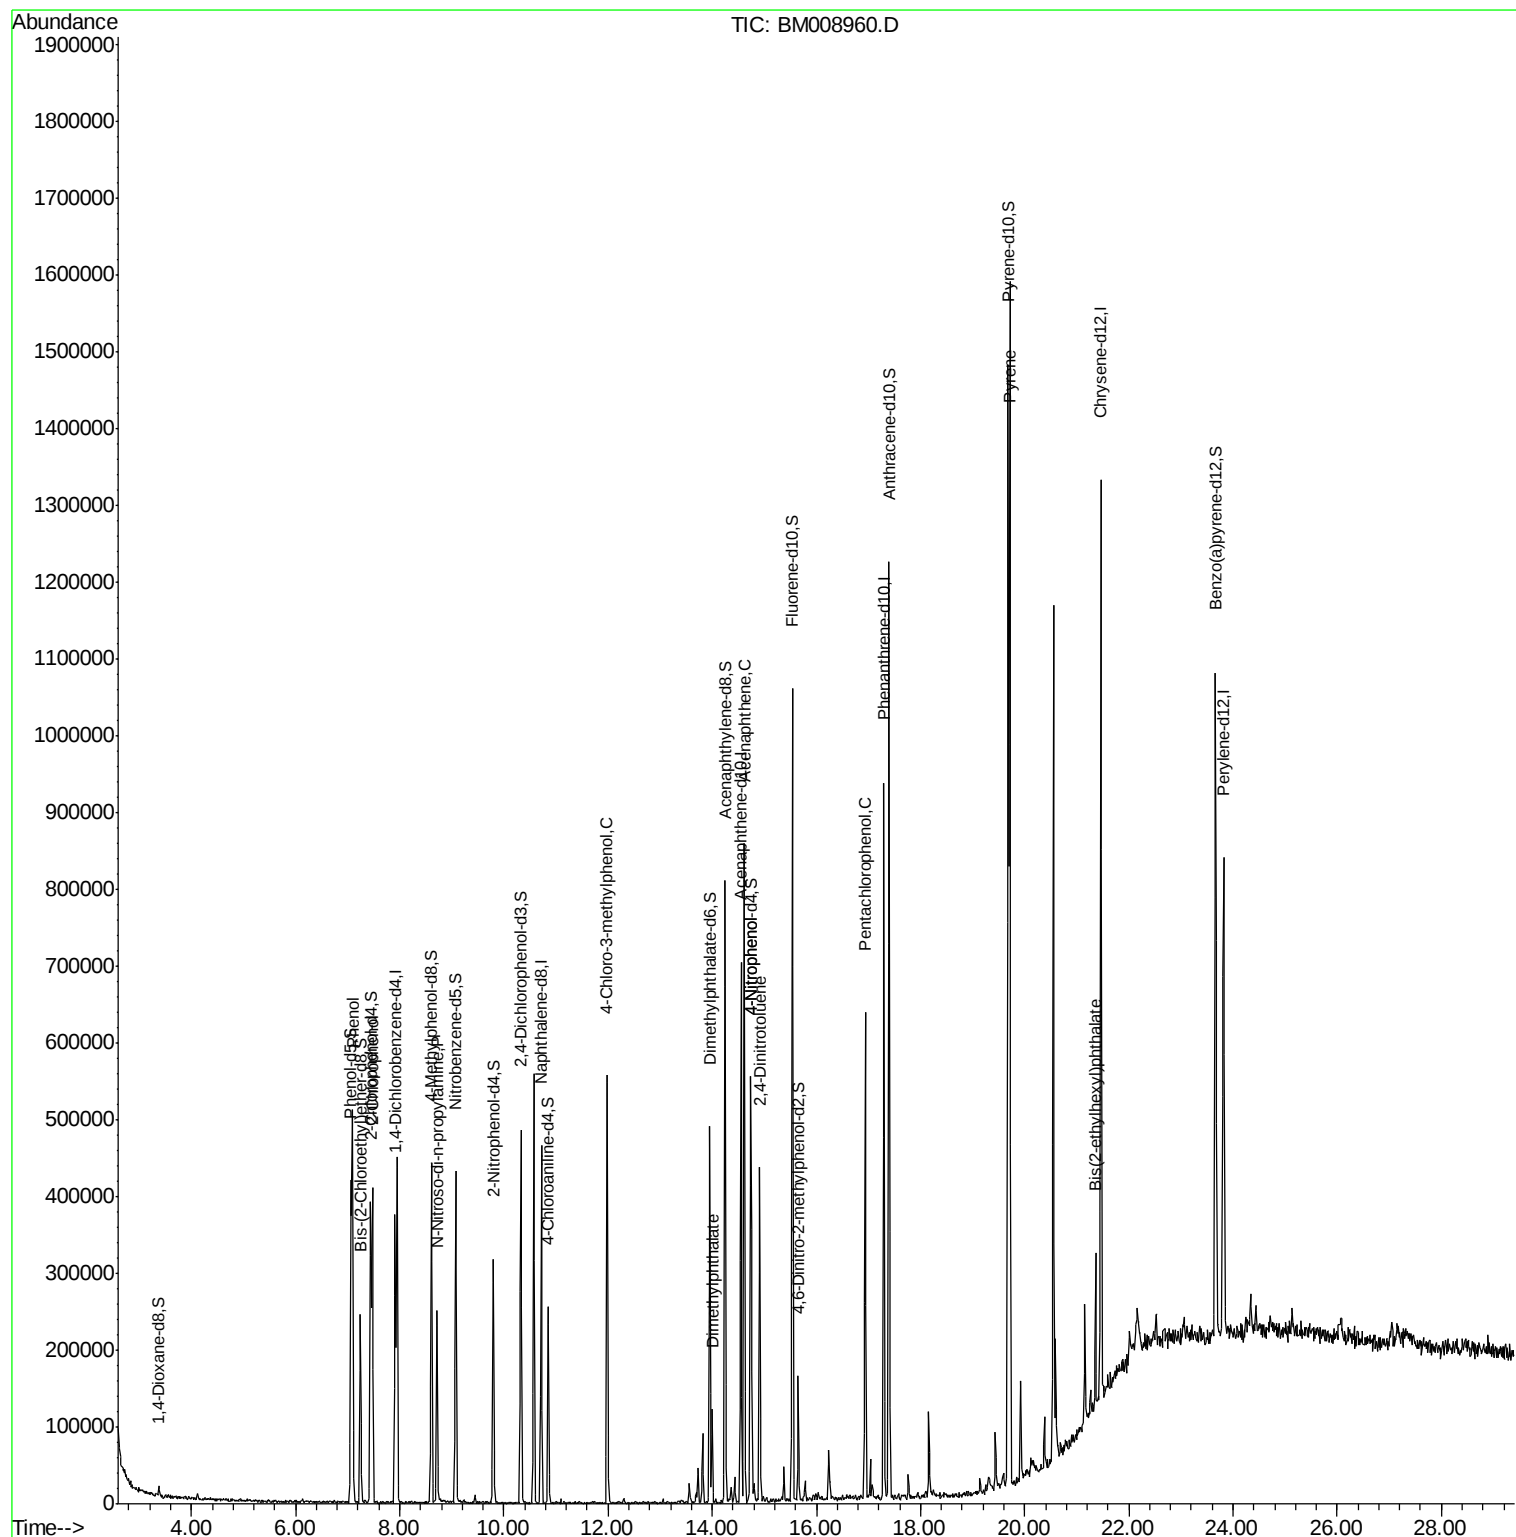

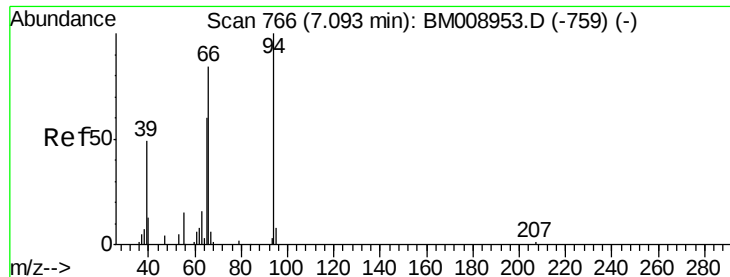

#6

Phenol

Concen: 25.83 ng/ul

RT: 7.09 min Scan# 766

Delta R.T. 0.00 min

Lab File: BM008960.D

Acq: 02 Feb 2017 13:53

Instrument :

BNA_M

ClientSampleId :

H0FJ4MS





Tgt Ion: 94 Resp: 151632

Ion Ratio Lower Upper

94 100

65 62.1 39.8 59.6#

66 85.7 69.9 104.9

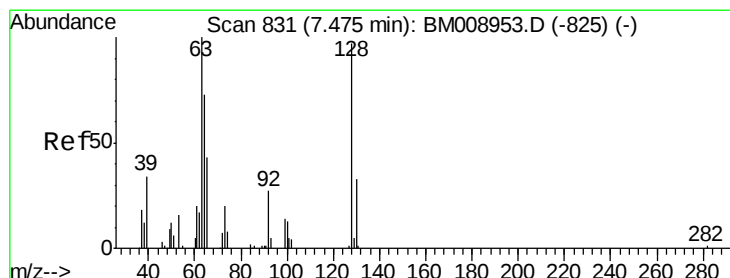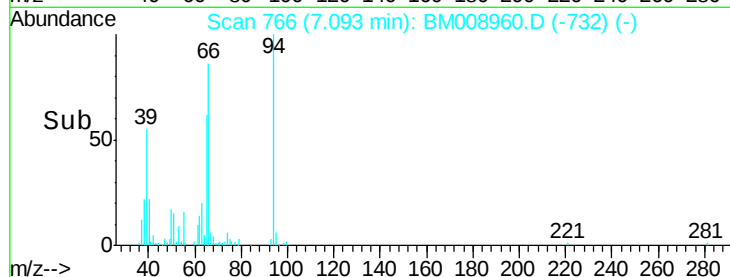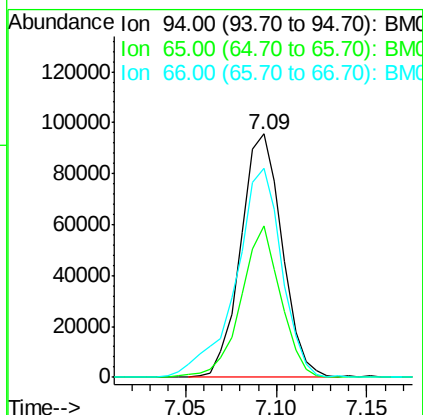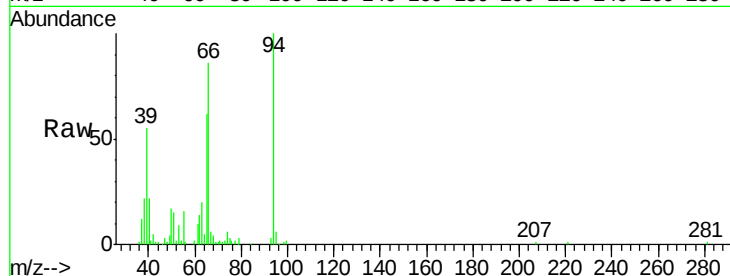

#10

2-Chlorophenol

Concen: 23.72 ng/ul

RT: 7.48 min Scan# 831

Delta R.T. 0.00 min

Lab File: BM008960.D

Acq: 02 Feb 2017 13:53




Tgt Ion: 128 Resp: 83724


Ion Ratio Lower Upper

128 100

64 102.1 76.6 115.0

130 31.0 26.5 39.7


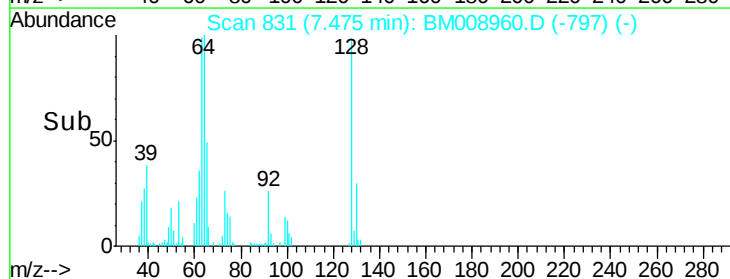
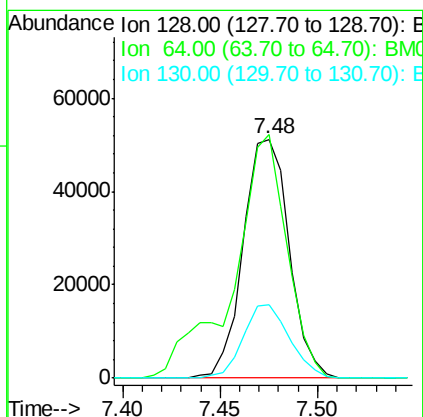
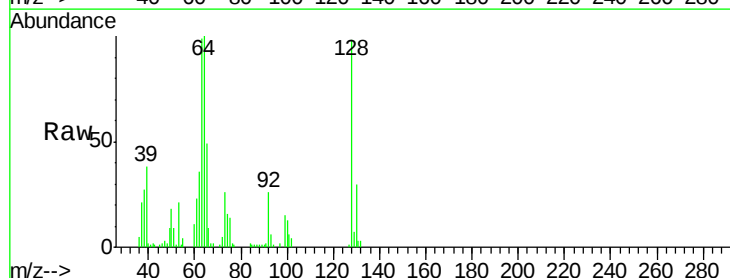


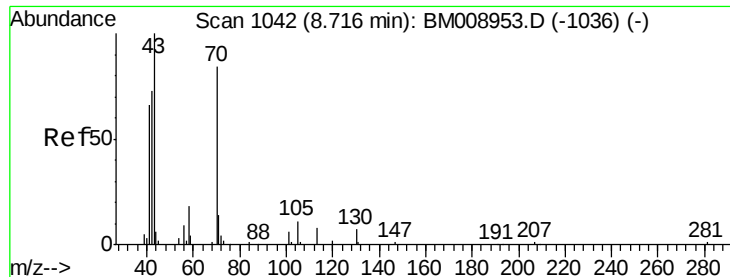

#15
N-Nitroso-di-n-propylamine
Concen: 13.22 ng/ul
RT: 8.72 min Scan# 1042
Delta R.T. 0.00 min
Lab File: BM008960.D
Acq: 02 Feb 2017 13:53




Instrument :
BNA_M
ClientSampleId :
H0FJ4MS


Tgt Ion: 70 Resp: 68201
Ion Ratio Lower Upper
70 100
42 83.2 64.2 96.2
101 5.4 5.1 7.7
130 15.1 8.3 12.5#

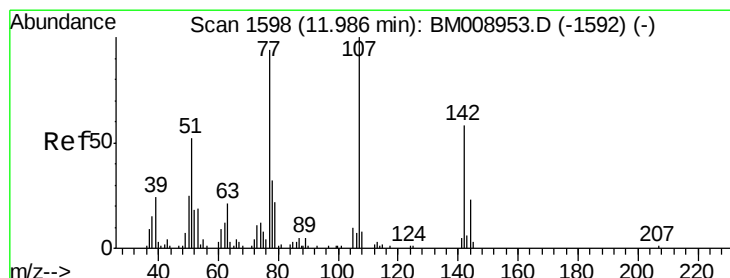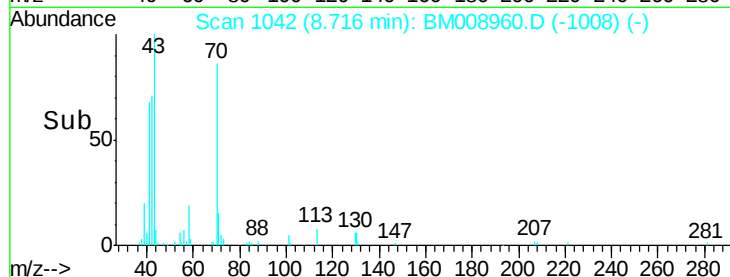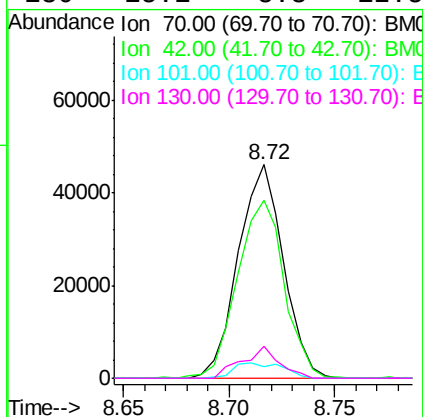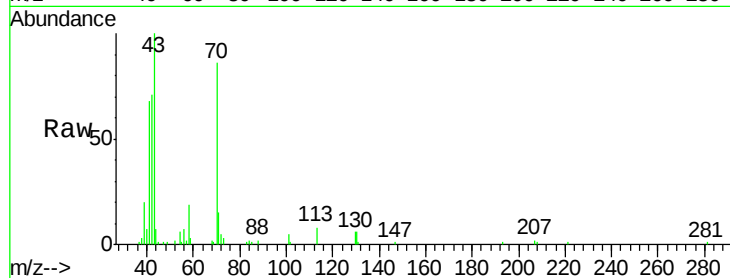

#33
4-Chloro-3-methylphenol
Concen: 23.88 ng/ul
RT: 11.99 min Scan# 1598
Delta R.T. 0.00 min
Lab File: BM008960.D
Acq: 02 Feb 2017 13:53

Tgt Ion: 107 Resp: 133139
Ion Ratio Lower Upper
107 100
144 18.2 14.4 21.6
142 56.1 50.7 76.1

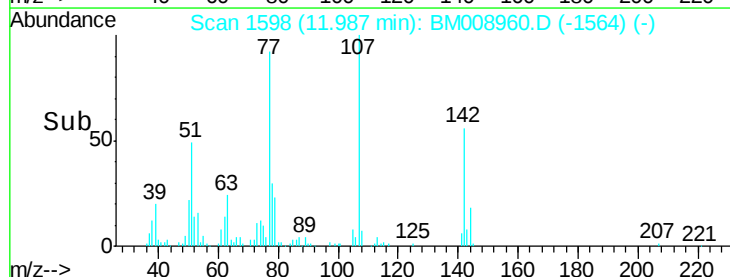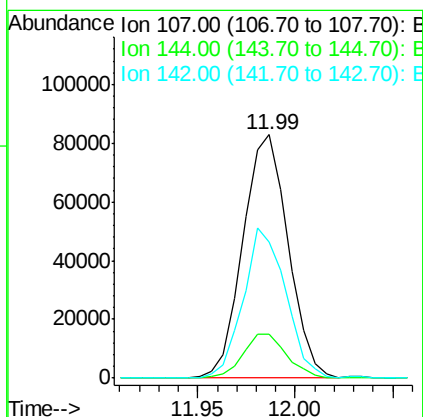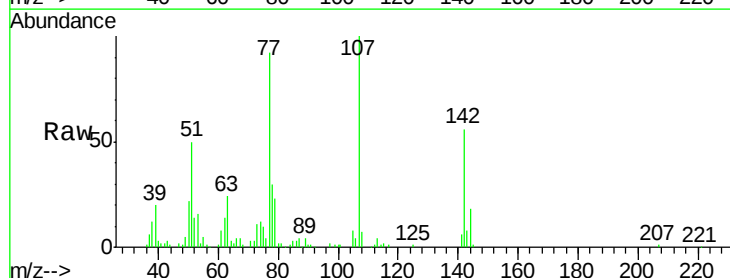

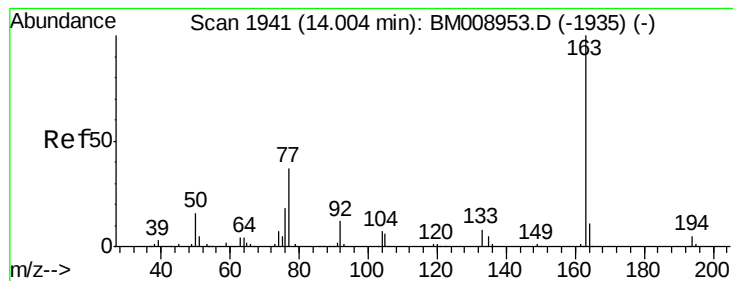

#44

Dimethylphthalate

Concen: 4.06 ng/ul

RT: 14.00 min Scan# 1941

Delta R.T. 0.00 min

Lab File: BM008960.D

Acq: 02 Feb 2017 13:53

Instrument :





BNA_M

ClientSampleId :

H0FJ4MS

Tgt Ion:163 Resp: 52637

Ion	Ratio	Lower	Upper
163	100		
194	6.2	3.0	4.6#
164	8.6	8.6	12.8

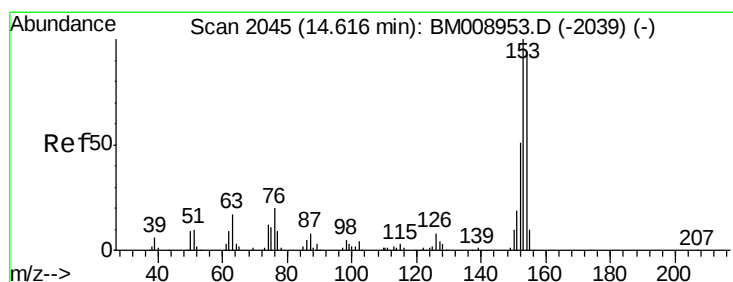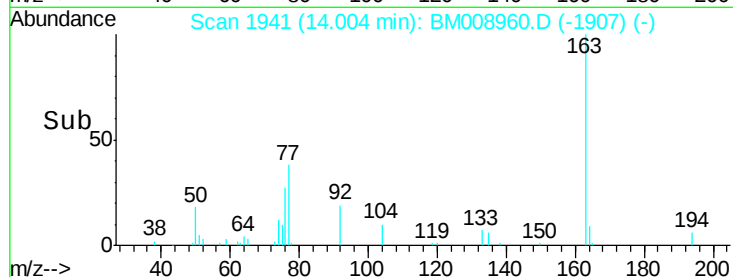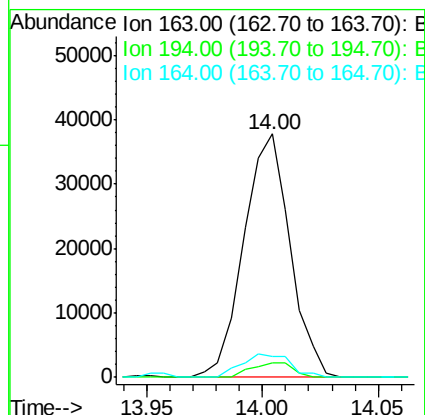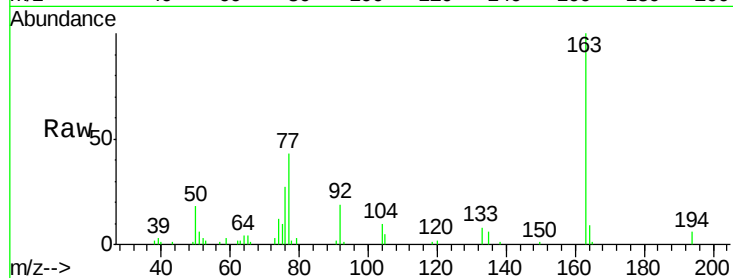

#49

Acenaphthene

Concen: 25.61 ng/ul

RT: 14.62 min Scan# 2045




Delta R.T. 0.00 min


Lab File: BM008960.D

Acq: 02 Feb 2017 13:53

Tgt Ion:153 Resp: 272360

Ion	Ratio	Lower	Upper
153	100		
152	46.1	36.7	55.1
154	86.2	68.3	102.5


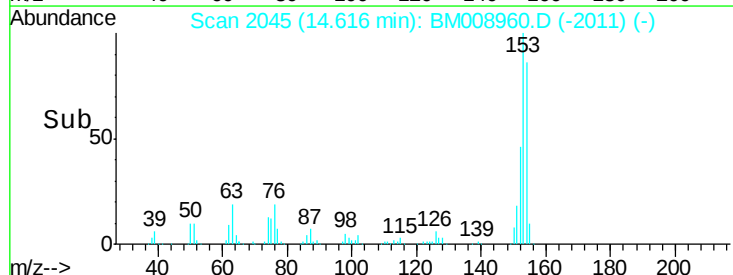
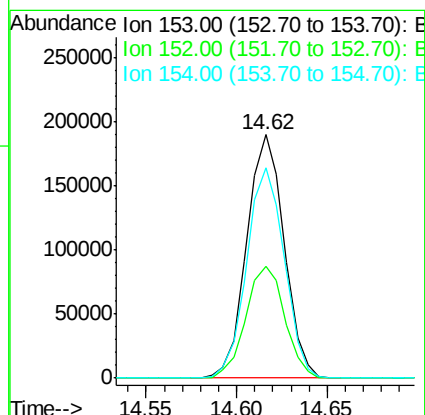
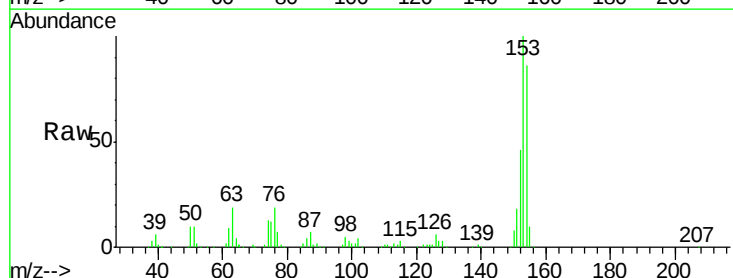


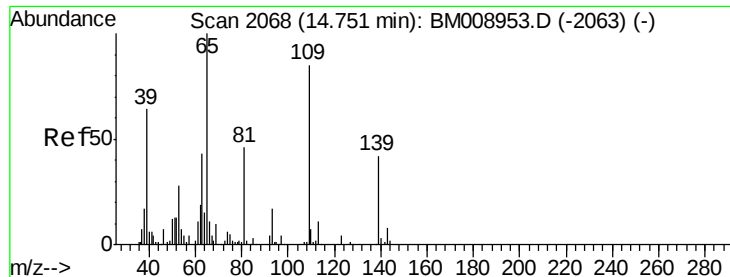

#52
4-Nitrophenol
Concen: 17.52 ng/ul
RT: 14.75 min Scan# 2068
Delta R.T. 0.00 min
Lab File: BM008960.D
Acq: 02 Feb 2017 13:53




Instrument :
BNA_M
ClientSampleId :
H0FJ4MS


Tgt Ion:109 Resp: 82796
Ion Ratio Lower Upper
109 100
139 47.9 33.9 50.9
65 116.4 92.2 138.2

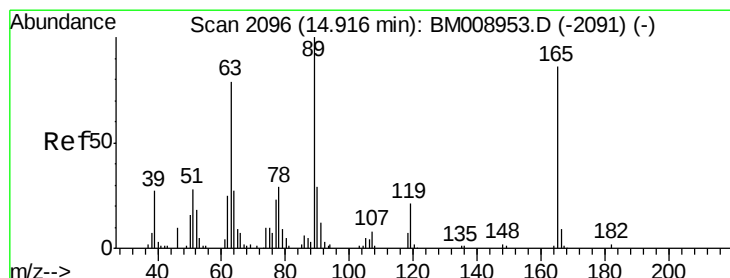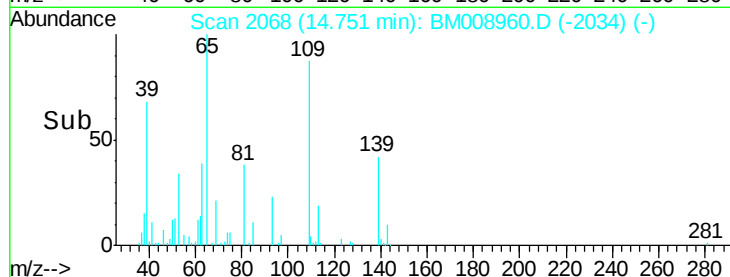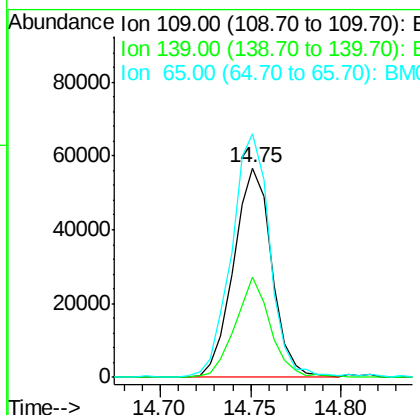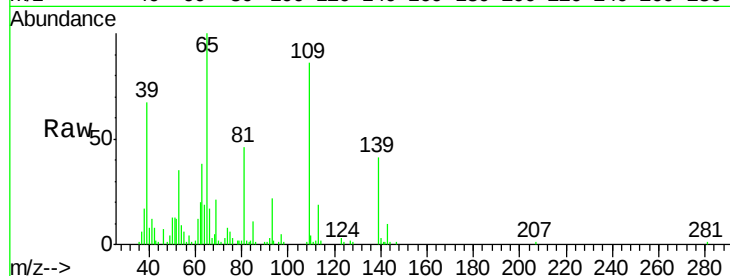

#54
2,4-Dinitrotoluene
Concen: 17.84 ng/ul
RT: 14.92 min Scan# 2096
Delta R.T. 0.00 min
Lab File: BM008960.D
Acq: 02 Feb 2017 13:53

Tgt Ion:165 Resp: 67195
Ion Ratio Lower Upper
165 100
63 97.9 75.7 113.5
182 2.7 1.7 2.5#

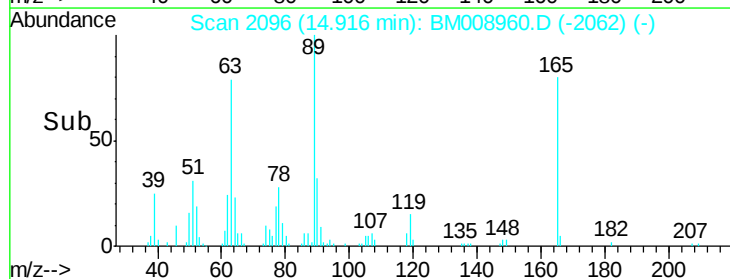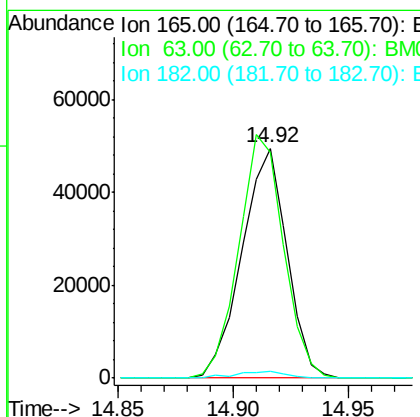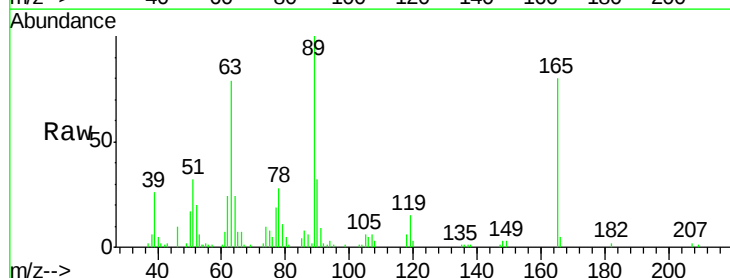


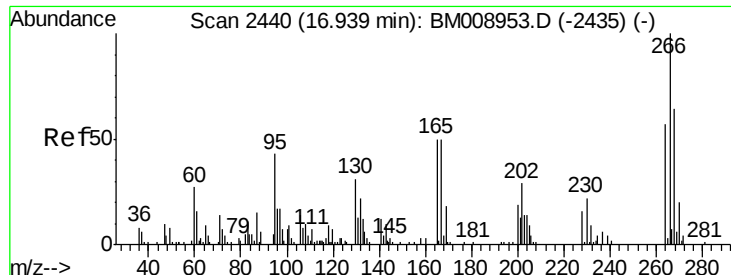




#68
 Pentachlorophenol
 Concen: 21.25 ng/ul
 RT: 16.94 min Scan# 2440
 Delta R.T. 0.00 min
 Lab File: BM008960.D
 Acq: 02 Feb 2017 13:53

Instrument :
 BNA_M
 ClientSampleId :
 H0FJ4MS

Tgt Ion:266 Resp: 72620
 Ion Ratio Lower Upper
 266 100
 264 62.3 54.8 82.2
 268 66.8 62.1 93.1

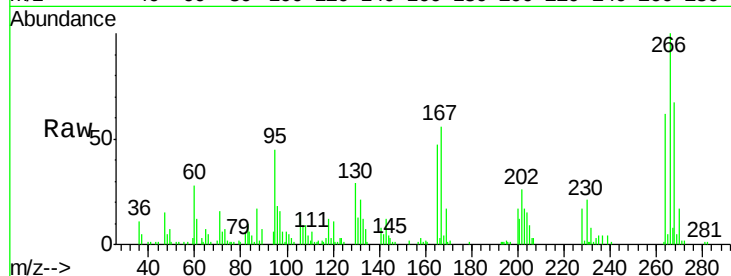


Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

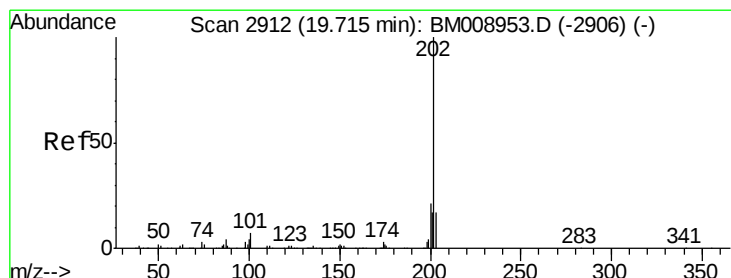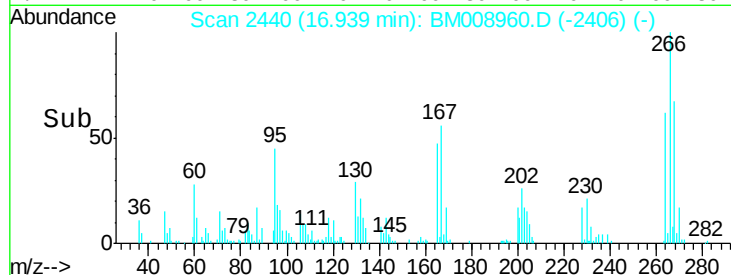
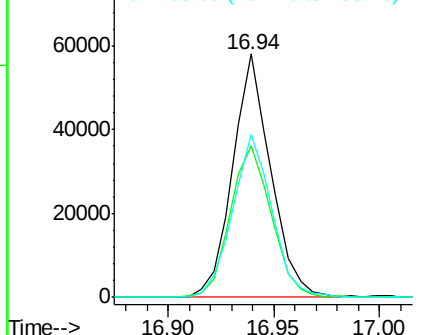



#77
 Pyrene
 Concen: 28.06 ng/ul
 RT: 19.72 min Scan# 2912
 Delta R.T. 0.00 min
 Lab File: BM008960.D
 Acq: 02 Feb 2017 13:53

Tgt Ion:202 Resp: 820183
 Ion Ratio Lower Upper
 202 100
 101 7.2 6.2 9.4
 100 6.4 6.4 9.6#

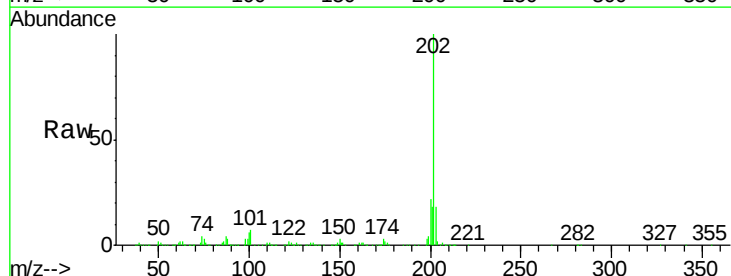

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

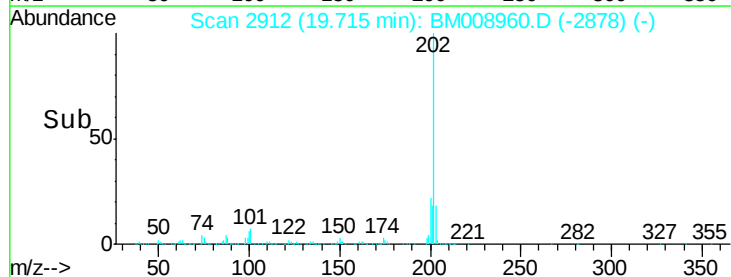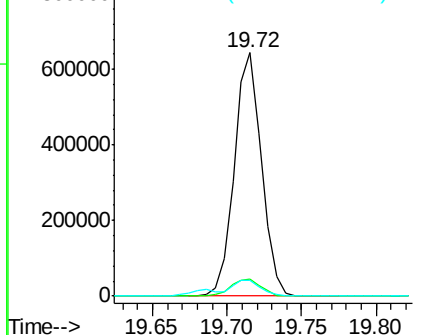

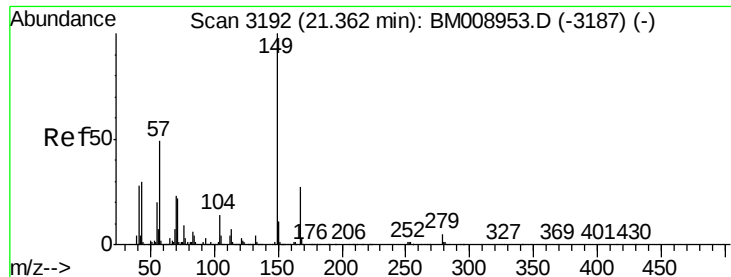

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 3.20 ng/ul
 RT: 21.36 min Scan# 3192
 Delta R.T. 0.00 min
 Lab File: BM008960.D
 Acq: 02 Feb 2017 13:53

Instrument :
 BNA_M
 ClientSampleId :
 H0FJ4MS

Tgt Ion:149 Resp: 48507
 Ion Ratio Lower Upper
 149 100
 167 25.8 20.2 30.2
 279 6.0 4.0 6.0

