

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020218\
 Data File : BM014141.D
 Acq On : 03 Feb 2018 07:41
 Operator : SJ/JU
 Sample : J1339-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6C94

Manual Integrations
 APPROVED

Sohil
 2/5/2018 3:57:50 PM

Quant Time: Feb 14 15:28:47 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 03 04:17:00 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	103336	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	415747	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	273613	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	654135	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	763183	20.00	ng/ul	0.00
83) Perylene-d12	23.34	264	780616	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	9781	4.34	ng/uL	0.00
5) Phenol-d5	6.74	99	186635	24.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	122048	26.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	159986	26.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	166783	25.65	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	85277	28.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	97761	29.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	173139	24.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	192510	31.78	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	645676	28.43	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	791983	28.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	65060m	20.79	ng/ul	0.00
57) Fluorene-d10	15.21	176	566382	27.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	76770	19.11	ng/ul	0.00
70) Anthracene-d10	17.06	188	907271	28.57	ng/ul	0.00
76) Pyrene-d10	19.37	212	1064470	28.96	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.21	264	1088453	28.41	ng/ul	0.00

Target Compounds					Ovalue	
44) Dimethylphthalate	13.67	163	86089	3.933	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020218\
Data File : BM014141.D
Acq On : 03 Feb 2018 07:41
Operator : SJ/JU
Sample : J1339-04
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6C94

Quant Time: Feb 14 15:28:47 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 03 04:17:00 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
2/5/2018 3:57:50 PM

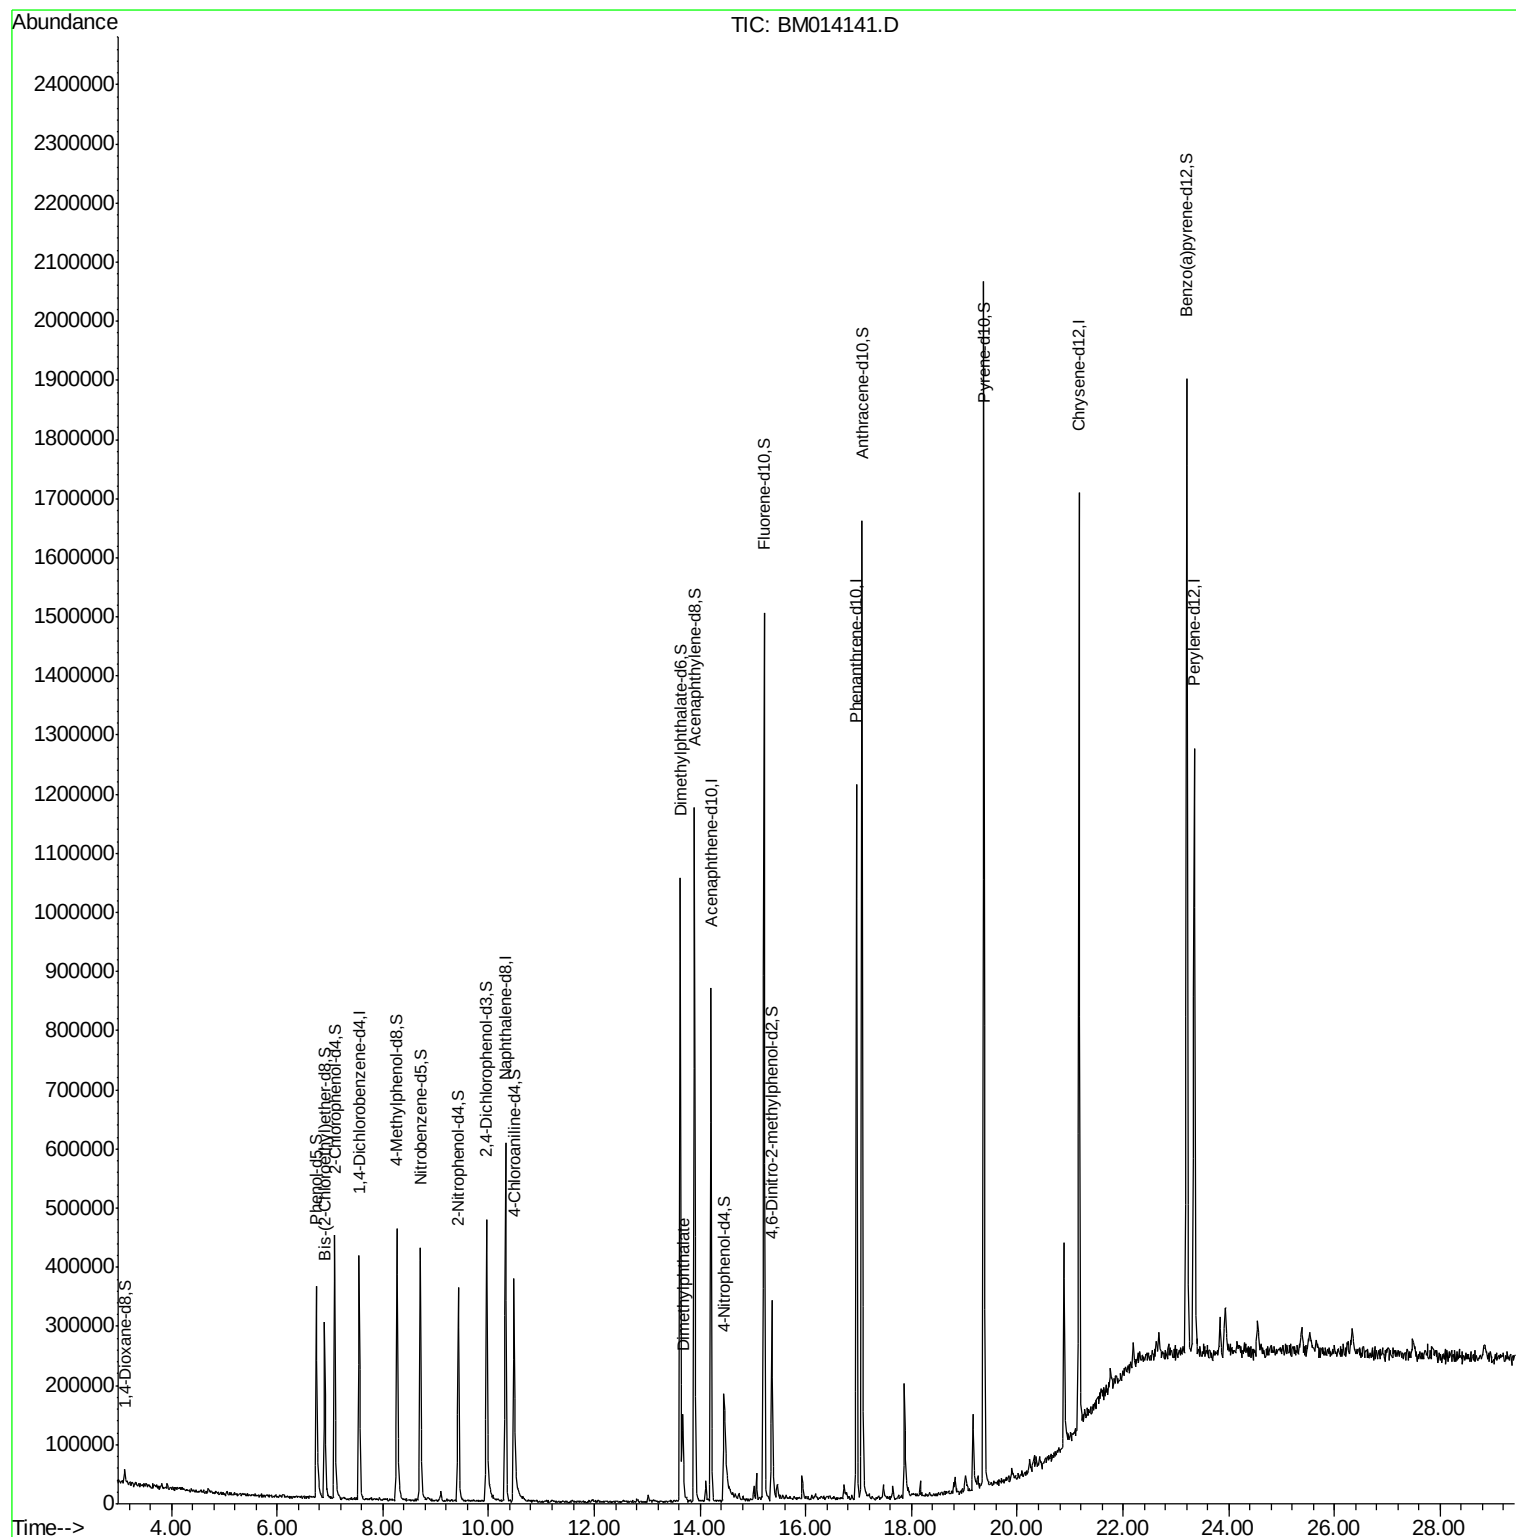

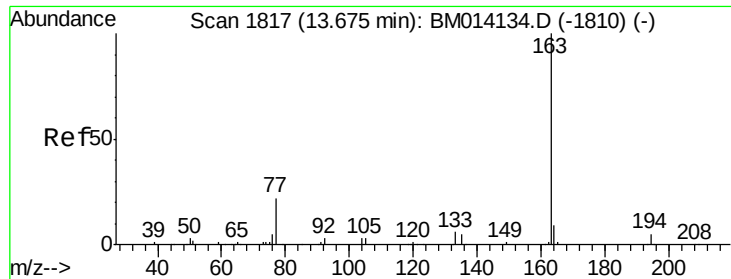


#44
 Dimethylphthalate
 Concen: 3.933 ng/ul
 RT: 13.67 min Scan# 1817
 Delta R.T. -0.00 min
 Lab File: BM014141.D
 Acq: 03 Feb 2018 07:41

Instrument :
 BNA_M
 ClientSampleId :
 F6C94

Tot Ion	Ratio	Resp	Lower	Upper
163	100	86089		
194	4.7		3.5	5.3
164	12.8		8.2	12.4

Manual Integrations
 APPROVED

Sohil
 2/5/2018 3:57:50 PM

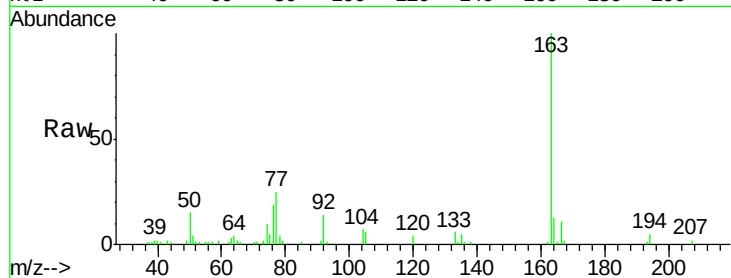

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

