

Data Path : U:\HPCHEM1\BNA M\DATA\BM020218\
 Data File : BM014144.D
 Acq On : 03 Feb 2018 09:28
 Operator : SJ/JU
 Sample : J1355-11
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6A86

Manual Integrations
 APPROVED

Sohil
 2/5/2018 3:58:05 PM

Quant Time: Feb 05 06:15:58 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 03 04:17:00 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	105015	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	418176	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	264421	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	632877	20.00	ng/ul	0.00
75) Chrysene-d12	21.17	240	746046	20.00	ng/ul	0.00
83) Perylene-d12	23.34	264	734704	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	11592	5.07	ng/uL	0.00
5) Phenol-d5	6.74	99	238085	30.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	152574	32.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	206427	33.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	214210	32.41	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	111483	36.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	101456	30.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	221678	31.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	257277	42.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	755153	34.41	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	997782	37.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	63070m	20.86	ng/ul	0.00
57) Fluorene-d10	15.21	176	696856	35.48	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	37391	9.62	ng/ul	0.00
70) Anthracene-d10	17.06	188	1123937m	36.58	ng/ul	0.00
76) Pyrene-d10	19.37	212	1297548	36.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.21	264	1292914	35.86	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.77	94	19414	2.459	ng/ul 91
44) Dimethylphthalate	13.67	163	128663	6.082	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : U:\HPCHEM1\BNA M\DATA\BM020218\
Data File : BM014144.D
Acq On : 03 Feb 2018 09:28
Operator : SJ/JU
Sample : J1355-11
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6A86

Manual Integrations
APPROVED

Sohil
2/5/2018 3:58:05 PM

Quant Time: Feb 05 06:15:58 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM013118.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 03 04:17:00 2018
Response via : Initial Calibration

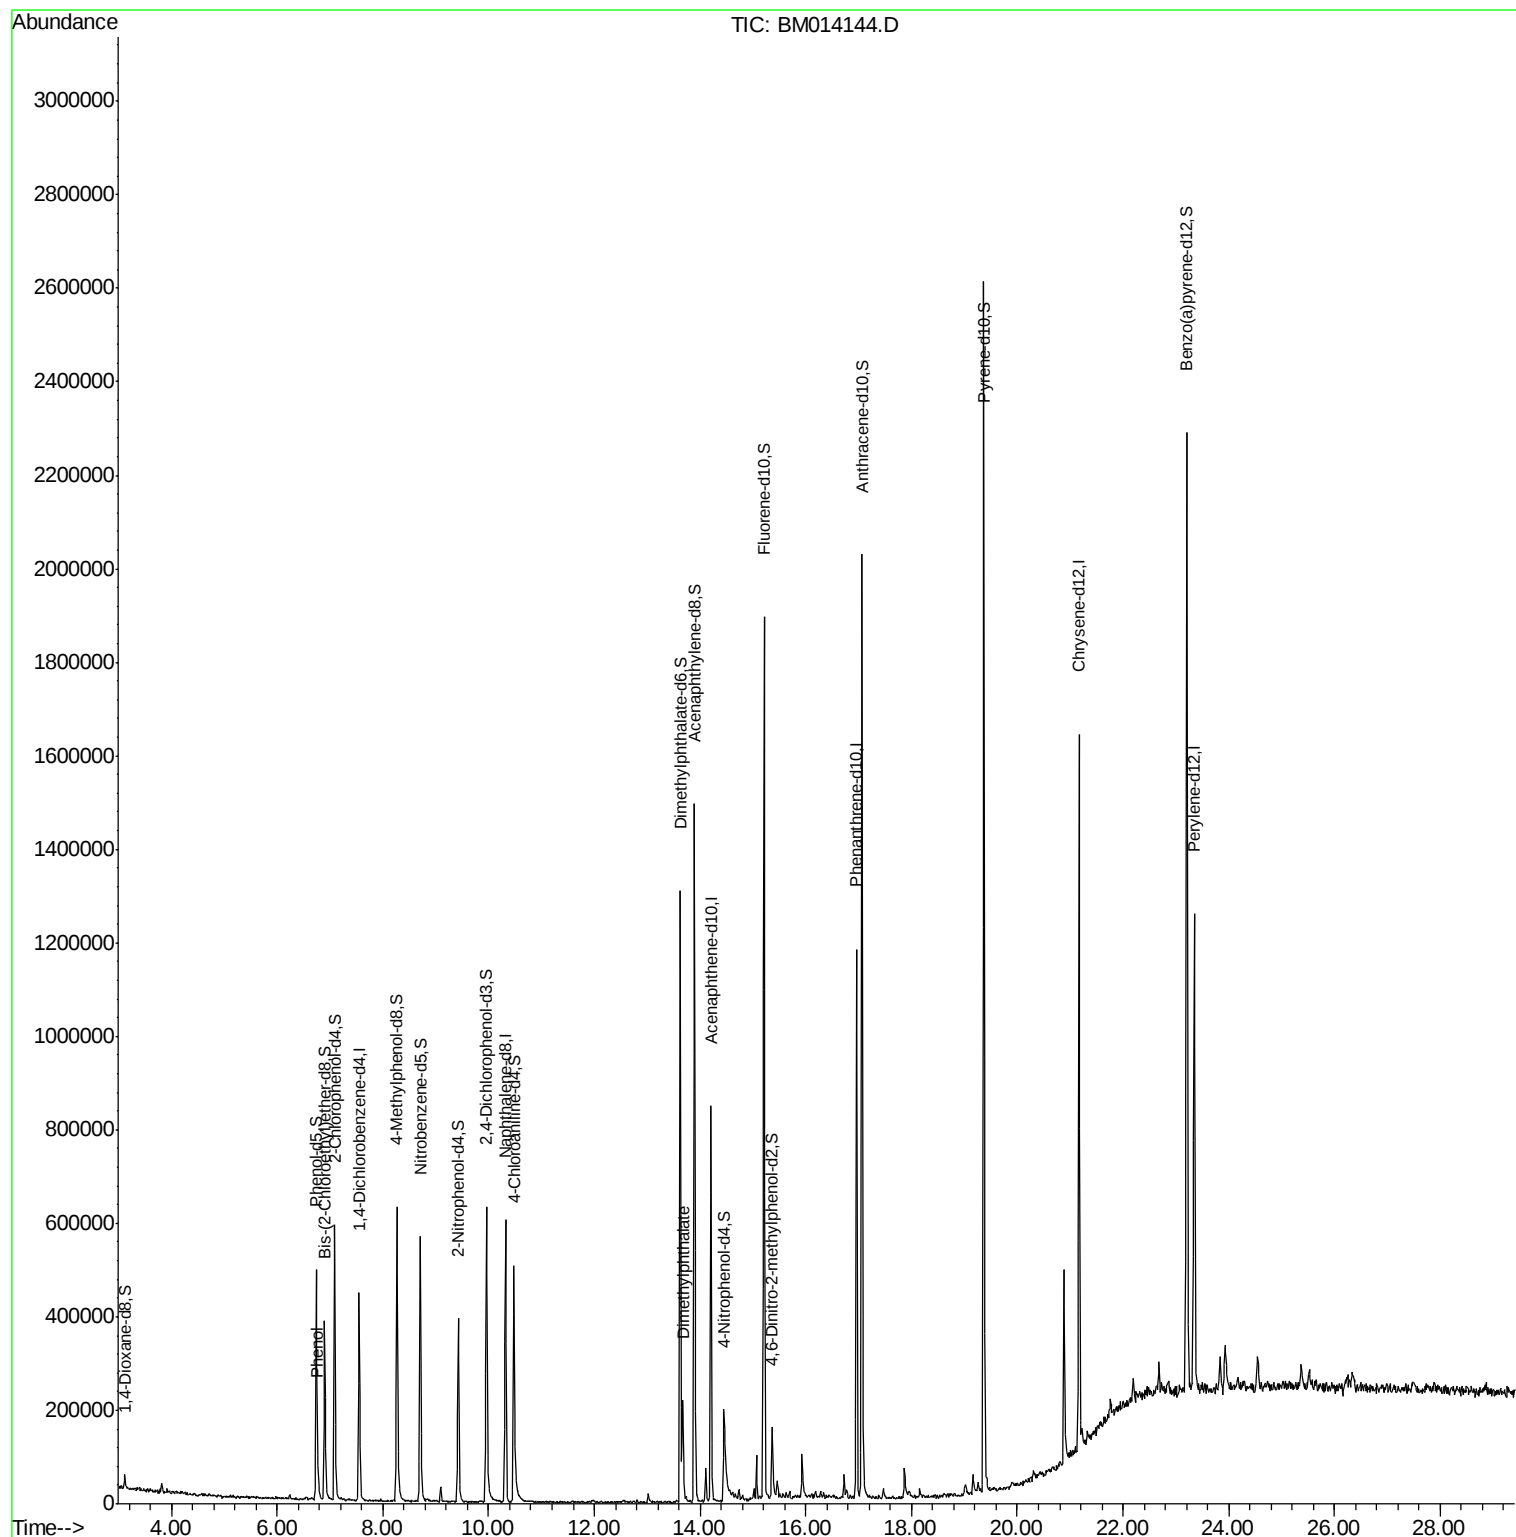

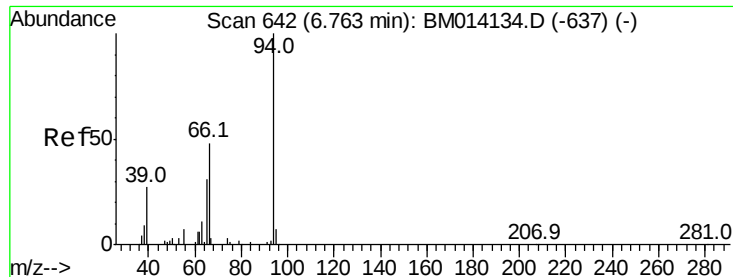

#6

Phenol

Concen: 2.459 ng/ul

RT: 6.77 min Scan# 643

Delta R.T. 0.01 min

Lab File: BM014144.D

Acq: 03 Feb 2018 09:28

Instrument :

BNA_M





ClientSampleId :

F6A86

Tot Ion:	94	Resp:	19414
Ion Ratio	Lower	Upper	
94	100		
65	40.6	28.2	42.4
66	66.1	47.2	70.8

Manual Integrations
APPROVED

Sohil
2/5/2018 3:58:05 PM

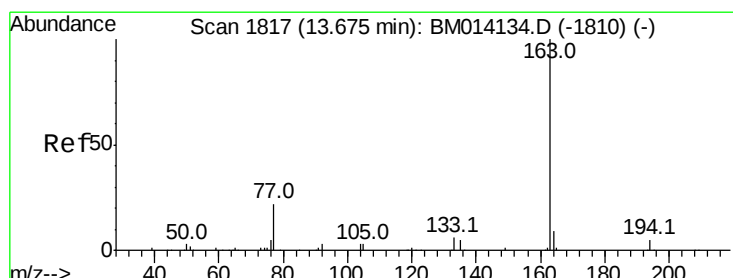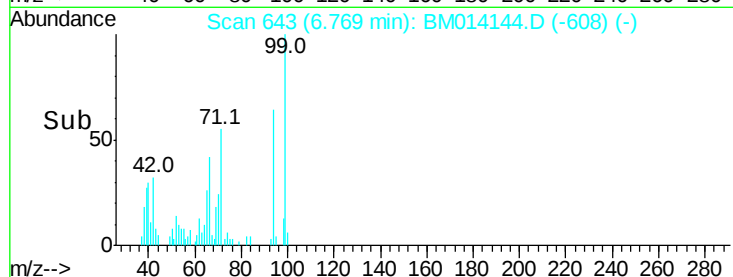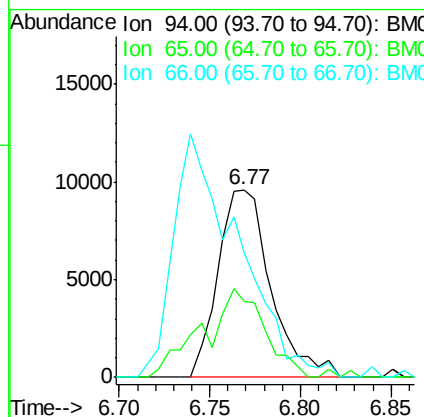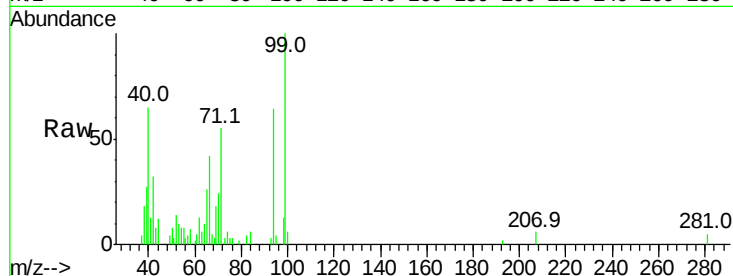

#44

Dimethylphthalate

Concen: 6.082 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BM014144.D

Acq: 03 Feb 2018 09:28

Tgt Ion:	163	Resp:	128663
Ion Ratio	Lower	Upper	
163	100		
194	4.0	3.5	5.3
164	9.6	8.2	12.4

