
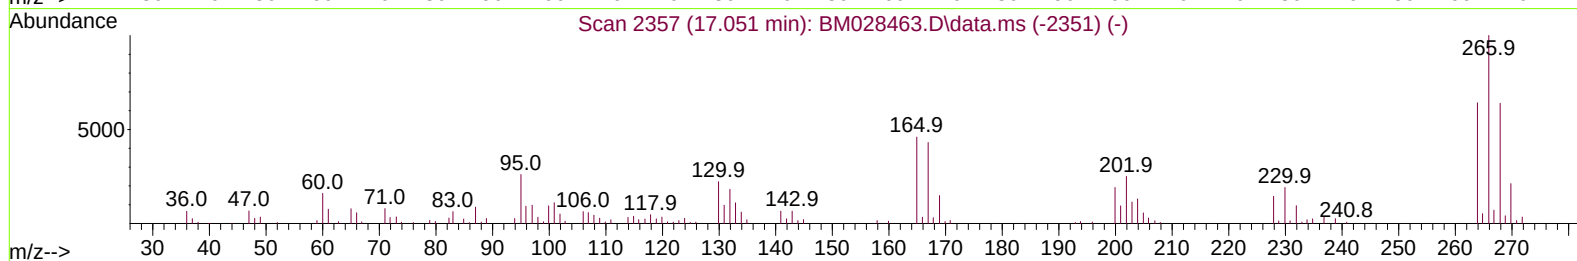
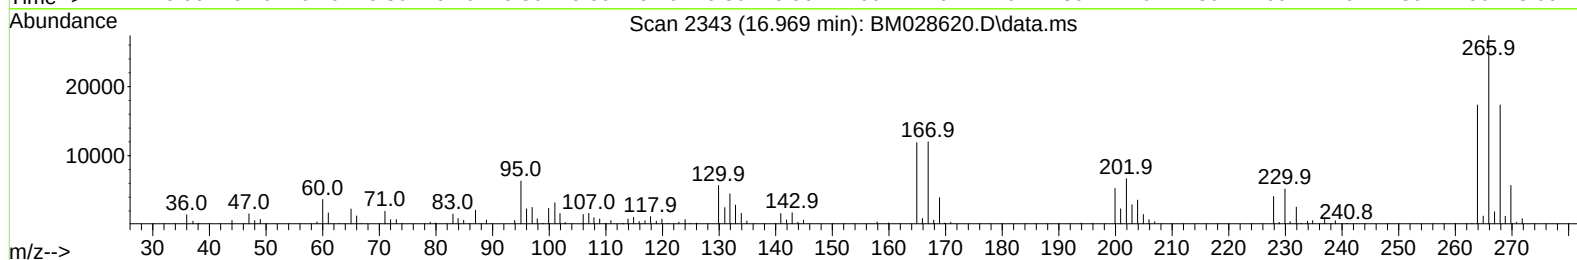


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020221\
Data File : BM028620.D
Acq On : 02 Feb 2021 13:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 01:21:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

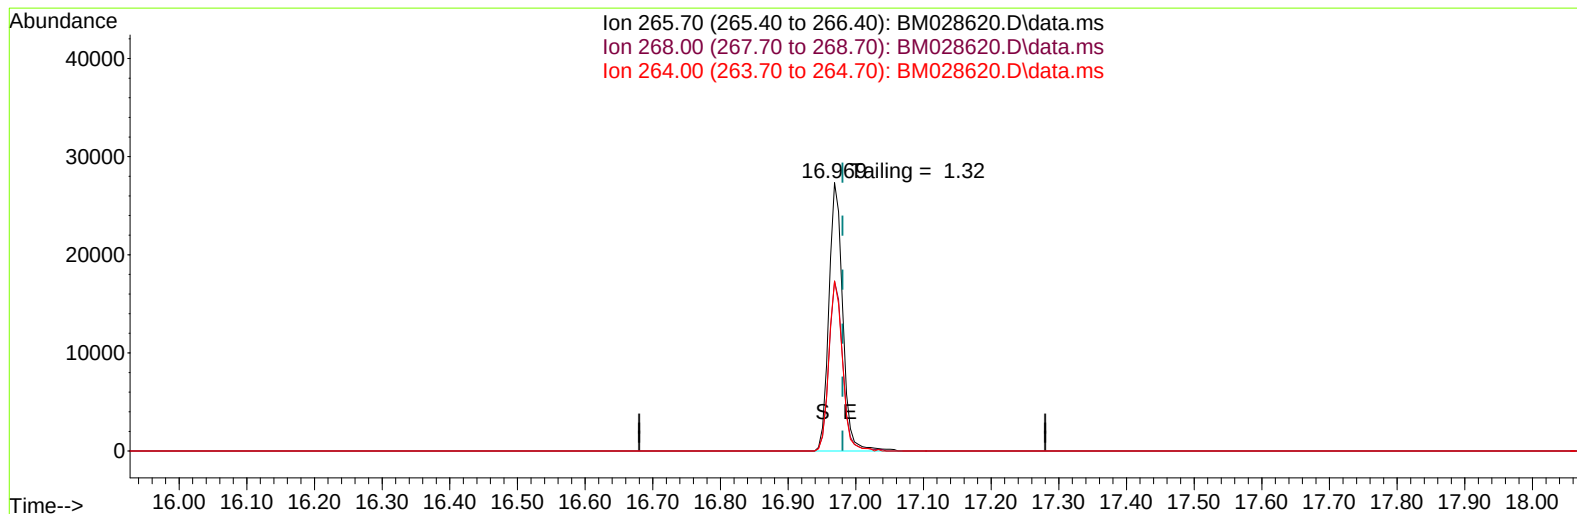

TIC: BM028620.D\data.ms

(70) Pentachlorophenol (C)




16.969min (-0.012) 0.00 ng

response 38735

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.32
264.00	63.30	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020221\
Data File : BM028620.D
Acq On : 02 Feb 2021 13:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 01:21:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

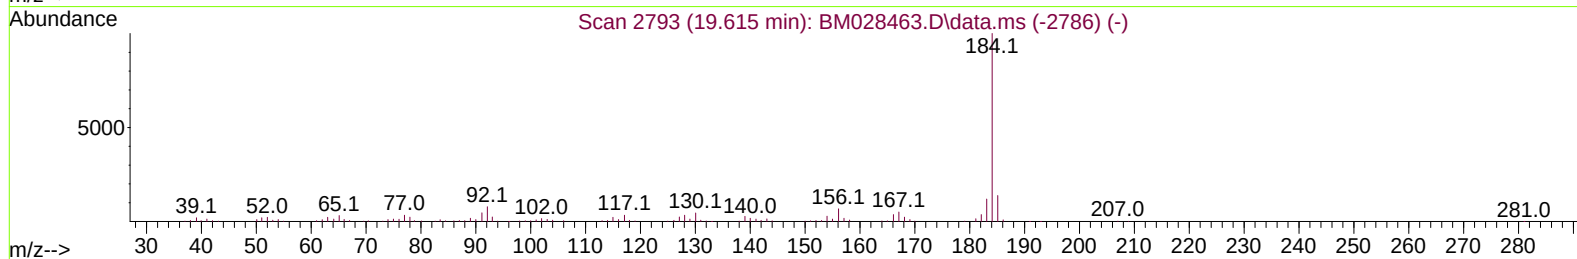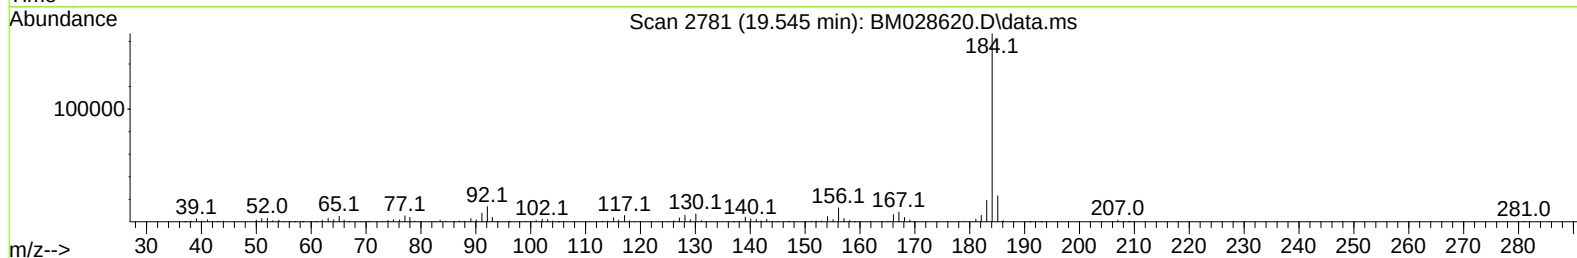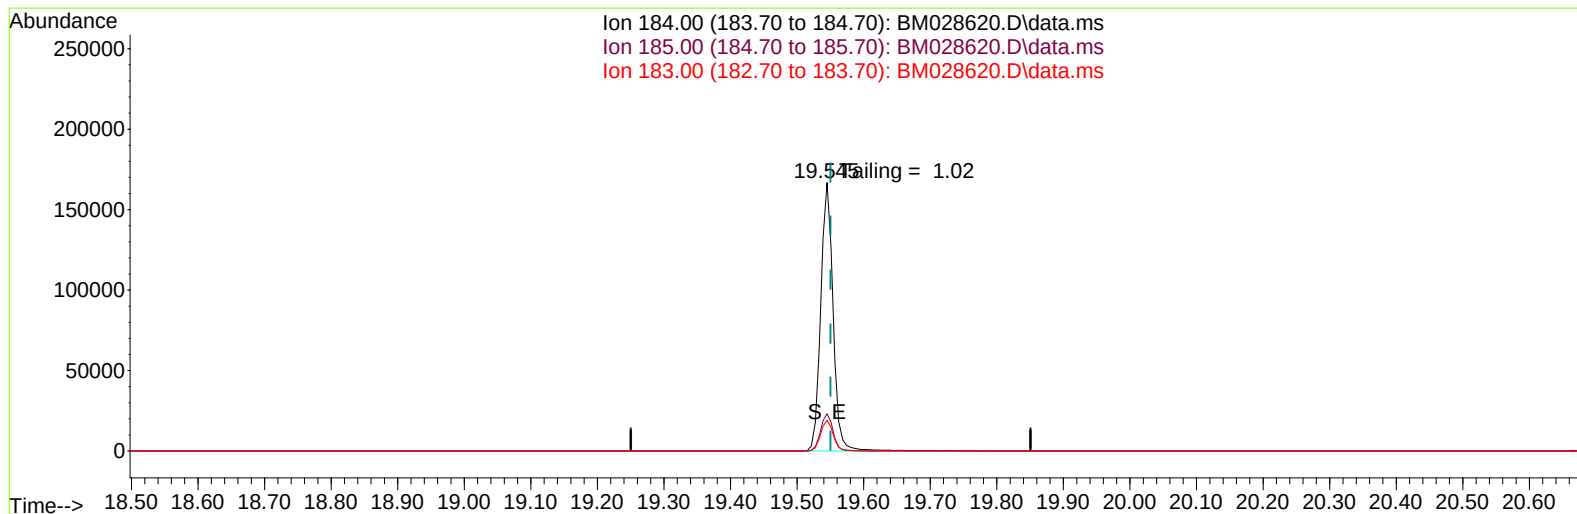

TIC: BM028620.D\data.ms

(77) Benzidine

19.545min (-0.006) 173375.51 ng

response 214435

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.91
183.00	12.10	11.48
0.00	0.00	0.00