

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020221\
 Data File : BM028635.D
 Acq On : 02 Feb 2021 22:48
 Operator : CG/JU
 Sample : M1286-09 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JJ BH 02 0-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	382	388	397	rBV	68116	99509	27.51%	4.054%
2	7.104	660	666	676	rBV	61657	96343	26.64%	3.925%
3	7.928	800	806	813	rVB	113972	172895	47.81%	7.044%
4	9.098	1000	1005	1014	rBV	37446	59379	16.42%	2.419%
5	10.739	1277	1284	1291	rBV	143663	233619	64.60%	9.518%
6	13.198	1695	1702	1709	rBV	90166	123653	34.19%	5.038%
7	14.033	1837	1844	1849	rVB	4988	6196	1.71%	0.252%
8	14.427	1902	1911	1916	rBV3	4783	11738	3.25%	0.478%
9	14.580	1931	1937	1944	rVB	198232	280811	77.64%	11.441%
10	16.062	2185	2189	2195	rVB	61329	84147	23.27%	3.428%
11	17.315	2396	2402	2407	rBV	228666	309159	85.48%	12.595%
12	17.356	2407	2409	2413	rVB	5173	5466	1.51%	0.223%
13	18.192	2546	2551	2557	rBV3	14012	20358	5.63%	0.829%
14	19.356	2745	2749	2752	rBV	14517	18138	5.02%	0.739%
15	19.462	2764	2767	2772	rBV4	6584	9359	2.59%	0.381%
16	19.721	2807	2811	2817	rVB	10862	13740	3.80%	0.560%
17	19.915	2839	2844	2849	rBV	151826	172871	47.80%	7.043%
18	21.162	3054	3056	3060	rVB3	18320	19488	5.39%	0.794%
19	21.456	3101	3106	3111	rBV2	280536	361661	100.00%	14.734%
20	23.715	3485	3490	3501	rVB2	187454	355993	98.43%	14.504%




Sum of corrected areas: 2454523

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020221\
Data File : BM028635.D
Acq On : 02 Feb 2021 22:48
Operator : CG/JU
Sample : M1286-09 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
JJ BH 02 0-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

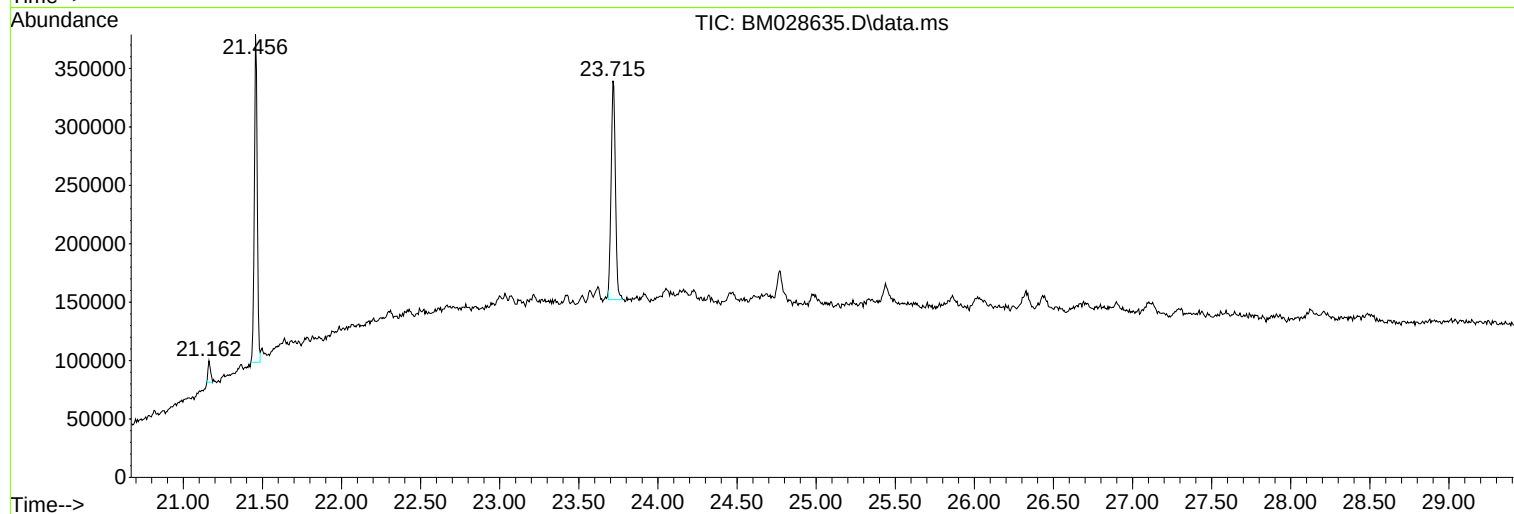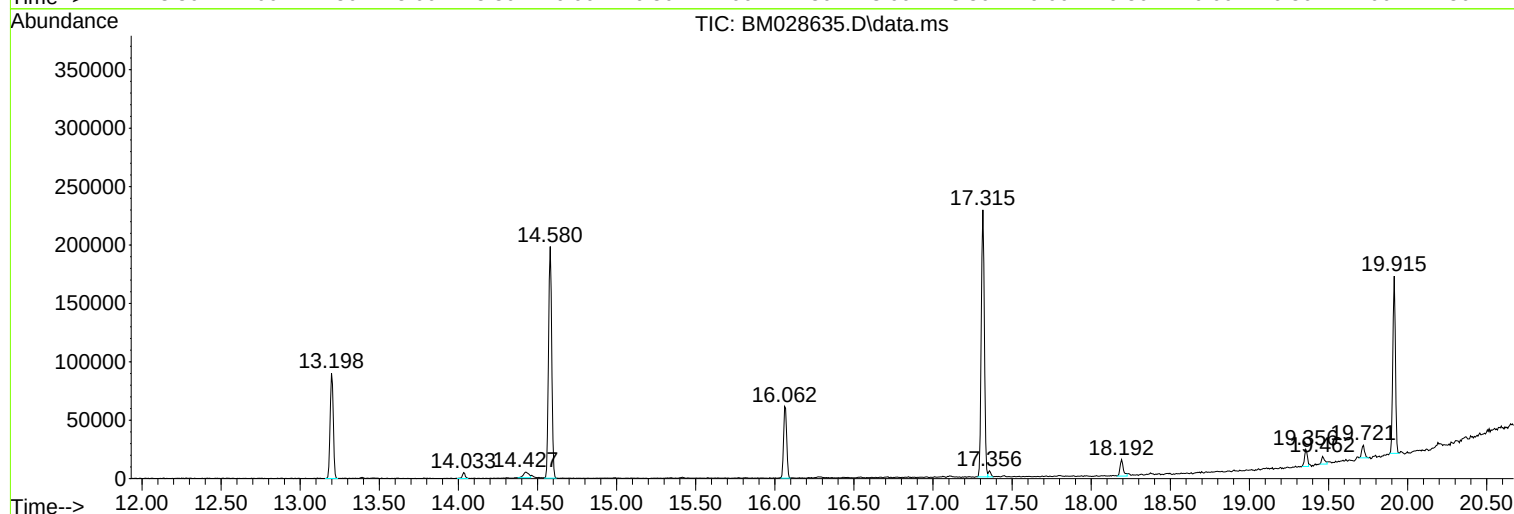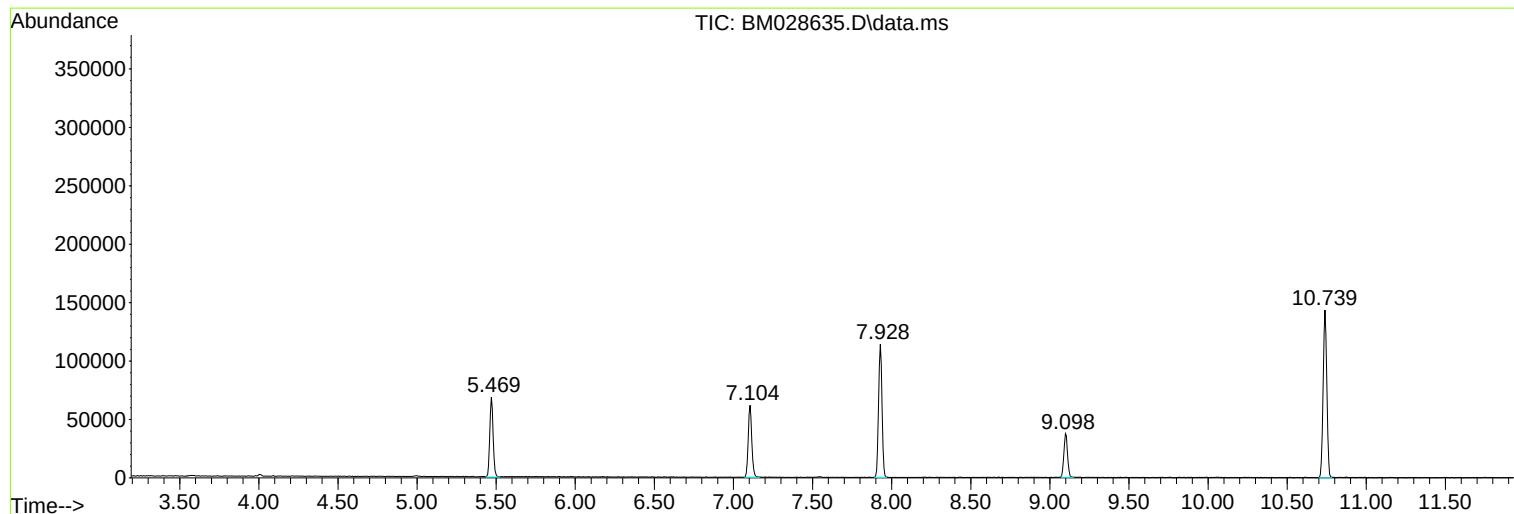

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020221\
Data File : BM028635.D
Acq On : 02 Feb 2021 22:48
Operator : CG/JU
Sample : M1286-09 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JJ_BH_02_0-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020221\
Data File : BM028635.D
Acq On : 02 Feb 2021 22:48
Operator : CG/JU
Sample : M1286-09 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JJ BH 02 0-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------