
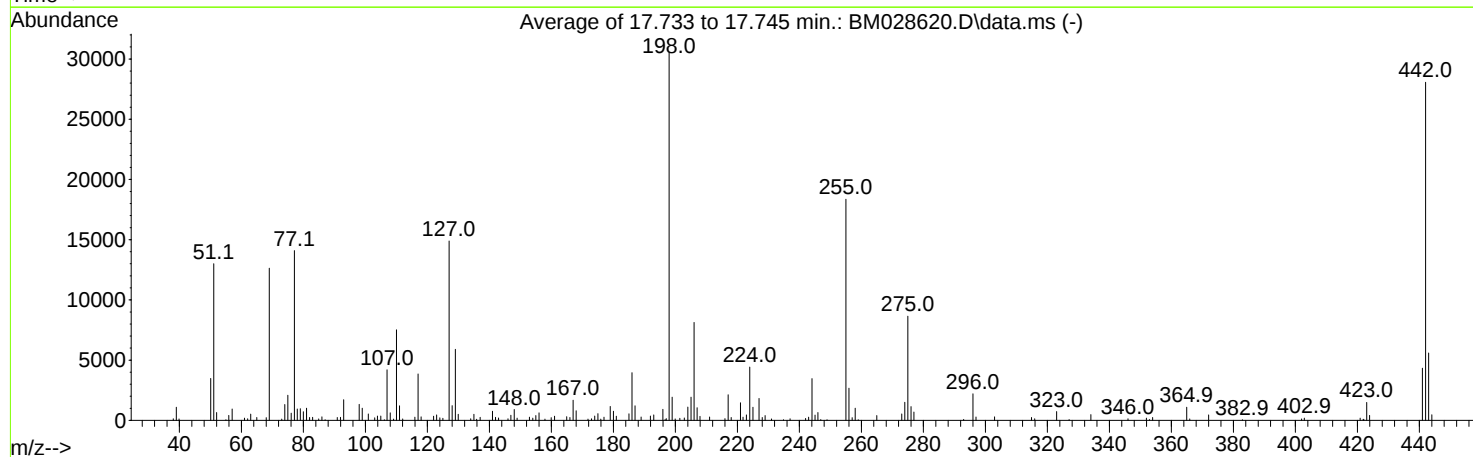


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020221\
 Data File : BM028620.D
 Acq On : 02 Feb 2021 13:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 16:19:07 2021

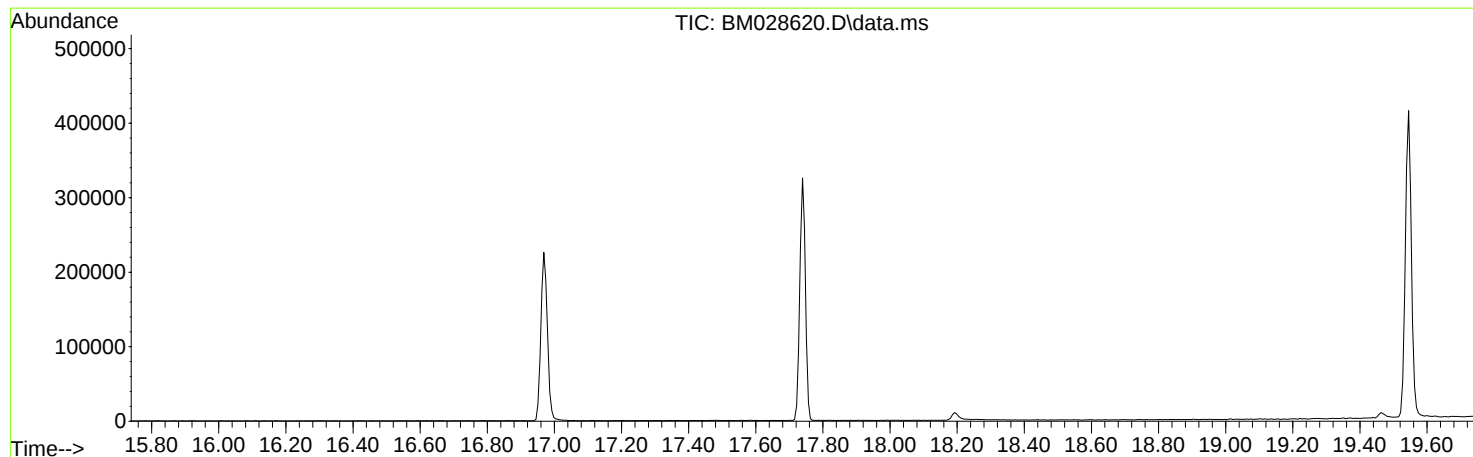

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	13002	PASS
68	69	0.00	2	1.7	220	PASS
69	198	0.00	100	41.4	12629	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	14896	PASS
197	198	0.00	2	0.5	149	PASS
198	198	100	100	100.0	30541	PASS
199	198	5	9	6.3	1927	PASS
275	198	10	60	28.3	8655	PASS
365	198	1	100	3.6	1096	PASS
441	198	0.01	100	14.2	4327	PASS
442	442	50	100	100.0	28067	PASS
443	442	15	24	19.9	5595	PASS