

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020224\
 Data File : BM043970.D
 Acq On : 02 Feb 2024 16:54
 Operator : MA/JU
 Sample : SSTD020ICV
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SICV012

Quant Time: Feb 02 21:58:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM020224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 02 21:58:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	363261	20.000	ng/u1	0.00
20) Naphthalene-d8	10.722	136	1588025	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.562	164	939931	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.315	188	1986298	20.000	ng/u1	0.00
79) Chrysene-d12	21.515	240	1882274	20.000	ng/u1	0.00
88) Perylene-d12	23.927	264	2123254	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	73689	7.078	ng/uL	0.00
4) Pyridine-d5	3.763	84	585973	19.563	ng/u1	0.00
7) Phenol-d5	7.081	99	705837	20.088	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	479062	21.794	ng/u1	0.00
11) 2-Chlorophenol-d4	7.445	132	547590	21.528	ng/u1	0.00
15) 4-Methylphenol-d8	8.628	113	543806	20.387	ng/u1	0.00
21) Nitrobenzene-d5	9.086	128	271132	21.416	ng/u1	0.00
24) 2-Nitrophenol-d4	9.804	143	273880	21.986	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.339	165	516306	21.680	ng/u1	0.00
31) 4-Chloroaniline-d4	10.863	131	802720	19.964	ng/u1	0.00
46) Dimethylphthalate-d6	13.986	166	1492234	21.001	ng/u1	0.00
49) Acenaphthylene-d8	14.257	160	1813948	21.475	ng/u1	0.00
54) 4-Nitrophenol-d4	14.762	143	306404	20.310	ng/u1	0.00
60) Fluorene-d10	15.557	176	1296115	20.882	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	219141	19.087	ng/u1	0.00
73) Anthracene-d10	17.415	188	1986104	20.607	ng/u1	0.00
81) Pyrene-d10	19.709	212	2231069	20.617	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.768	264	2248636	20.559	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.393	88	73338	6.909	ng/uL	100
5) Pyridine	3.787	79	488528	16.069	ng/u1	99
6) Benzaldehyde	7.063	77	399326	26.689	ng/u1	99
8) Phenol	7.110	94	657693	18.237	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.351	93	531238	18.321	ng/u1	98
12) 2-Chlorophenol	7.475	128	520391	19.430	ng/u1	98
13) 2-Methylphenol	8.363	108	483454	18.371	ng/u1	95
14) 2,2'-oxybis(1-Chloropr...	8.457	45	712958	17.333	ng/u1	98
16) Acetophenone	8.745	105	838033	19.393	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.733	70	426462	19.567	ng/u1	98
18) 4-Methylphenol	8.692	108	523921	18.386	ng/u1	97
19) Hexachloroethane	8.992	117	216123	18.717	ng/u1	96
22) Nitrobenzene	9.128	77	595703	18.519	ng/u1	98
23) Isophorone	9.651	82	1132392	18.652	ng/u1	99
25) 2-Nitrophenol	9.839	139	279371	19.867	ng/u1	97
26) 2,4-Dimethylphenol	9.898	107	434834	15.143	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.145	93	706548	18.630	ng/u1	99
29) 2,4-Dichlorophenol	10.369	162	466958	19.616	ng/u1	97
30) Naphthalene	10.774	128	1639111	18.548	ng/u1	100
32) 4-Chloroaniline	10.892	127	721093	18.272	ng/u1	100
33) Hexachlorobutadiene	11.045	225	272116	18.220	ng/u1	97
34) Caprolactam	11.663	113	158034	18.918	ng/u1	94
35) 4-Chloro-3-methylphenol	12.010	107	509233	19.730	ng/u1	99
36) 2-Methylnaphthalene	12.386	142	1103138	18.819	ng/u1	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020224\
 Data File : BM043970.D
 Acq On : 02 Feb 2024 16:54
 Operator : MA/JU
 Sample : SSTD020ICV
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SICV012


Quant Time: Feb 02 21:58:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM020224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 02 21:58:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.604	142	1076033	18.584	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.745	216	557559	19.177	ng/ul	100
40) Hexachlorocyclopentadiene	12.721	237	272712	14.454	ng/ul	99
41) 2,4,6-Trichlorophenol	12.992	196	350074	19.258	ng/ul	99
42) 2,4,5-Trichlorophenol	13.063	196	388000	19.732	ng/ul	98
43) 1,1'-Biphenyl	13.398	154	1467439	19.339	ng/ul	99
44) 2-Chloronaphthalene	13.439	162	1108953	18.449	ng/ul	99
45) 2-Nitroaniline	13.651	65	346813	19.650	ng/ul	97
47) Dimethylphthalate	14.033	163	1349179	18.414	ng/ul	100
48) 2,6-Dinitrotoluene	14.151	165	285682	21.246	ng/ul	95
50) Acenaphthylene	14.286	152	1837388	18.646	ng/ul	100
51) 3-Nitroaniline	14.474	138	334980	21.680	ng/ul	98
52) Acenaphthene	14.627	153	1177837	18.219	ng/ul	100
53) 2,4-Dinitrophenol	14.680	184	132850	17.124	ng/ul	96
55) 4-Nitrophenol	14.780	109	222449	18.644	ng/ul	99
56) Dibenzofuran	14.962	168	1659976	19.001	ng/ul	99
57) 2,4-Dinitrotoluene	14.933	165	388713	19.874	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.186	232	332933	20.339	ng/ul	99
59) Diethylphthalate	15.398	149	1358172	18.330	ng/ul	100
61) Fluorene	15.609	166	1360031	18.459	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.615	204	643748	18.164	ng/ul	100
63) 4-Nitroaniline	15.639	138	349566	23.361	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.692	198	212383	16.631	ng/ul	98
67) N-Nitrosodiphenylamine	15.827	169	1168412	19.151	ng/ul	100
68) 4-Bromophenyl-phenylether	16.509	248	377189	18.085	ng/ul	99
69) Hexachlorobenzene	16.604	284	433098	17.928	ng/ul	97
70) Atrazine	16.786	200	355538	17.440	ng/ul	97
71) Pentachlorophenol	16.956	266	253491	16.305	ng/ul	97
72) Phenanthrene	17.356	178	2100955	18.312	ng/ul	100
74) Anthracene	17.451	178	2112465	18.076	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.357	216	525759	18.492	ng/ul	98
76) Pentachlorobenzene	14.874	250	510082	18.656	ng/ul	98
77) Carbazole	17.727	167	1993303	18.068	ng/ul	99
78) Di-n-butylphthalate	18.303	149	2320649	18.200	ng/ul	100
80) Fluoranthene	19.374	202	2337225	18.107	ng/ul	98
82) Pyrene	19.739	202	2506943	18.332	ng/ul	100
83) Butylbenzylphthalate	20.662	149	1025767	18.780	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.438	252	885293	22.116	ng/ul	100
85) Benzo(a)anthracene	21.497	228	2517527	18.135	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.450	149	1548527	18.802	ng/ul	99
87) Chrysene	21.550	228	2293033	17.726	ng/ul	99
89) Di-n-octyl phthalate	22.397	149	2576054	17.761	ng/ul	100
90) Benzo(b)fluoranthene	23.191	252	2478602	18.129	ng/ul	100
91) Benzo(k)fluoranthene	23.238	252	2364128	17.337	ng/ul	100
93) Benzo(a)pyrene	23.815	252	2217465	17.012	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.426	276	2927083	18.280	ng/ul	99
95) Dibenzo(a,h)anthracene	26.450	278	2440839	18.322	ng/ul	98
96) Benzo(g,h,i)perylene	27.191	276	2324116	18.098	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Feb 02 21:58:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM020224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 02 21:58:08 2024
Response via : Initial Calibration




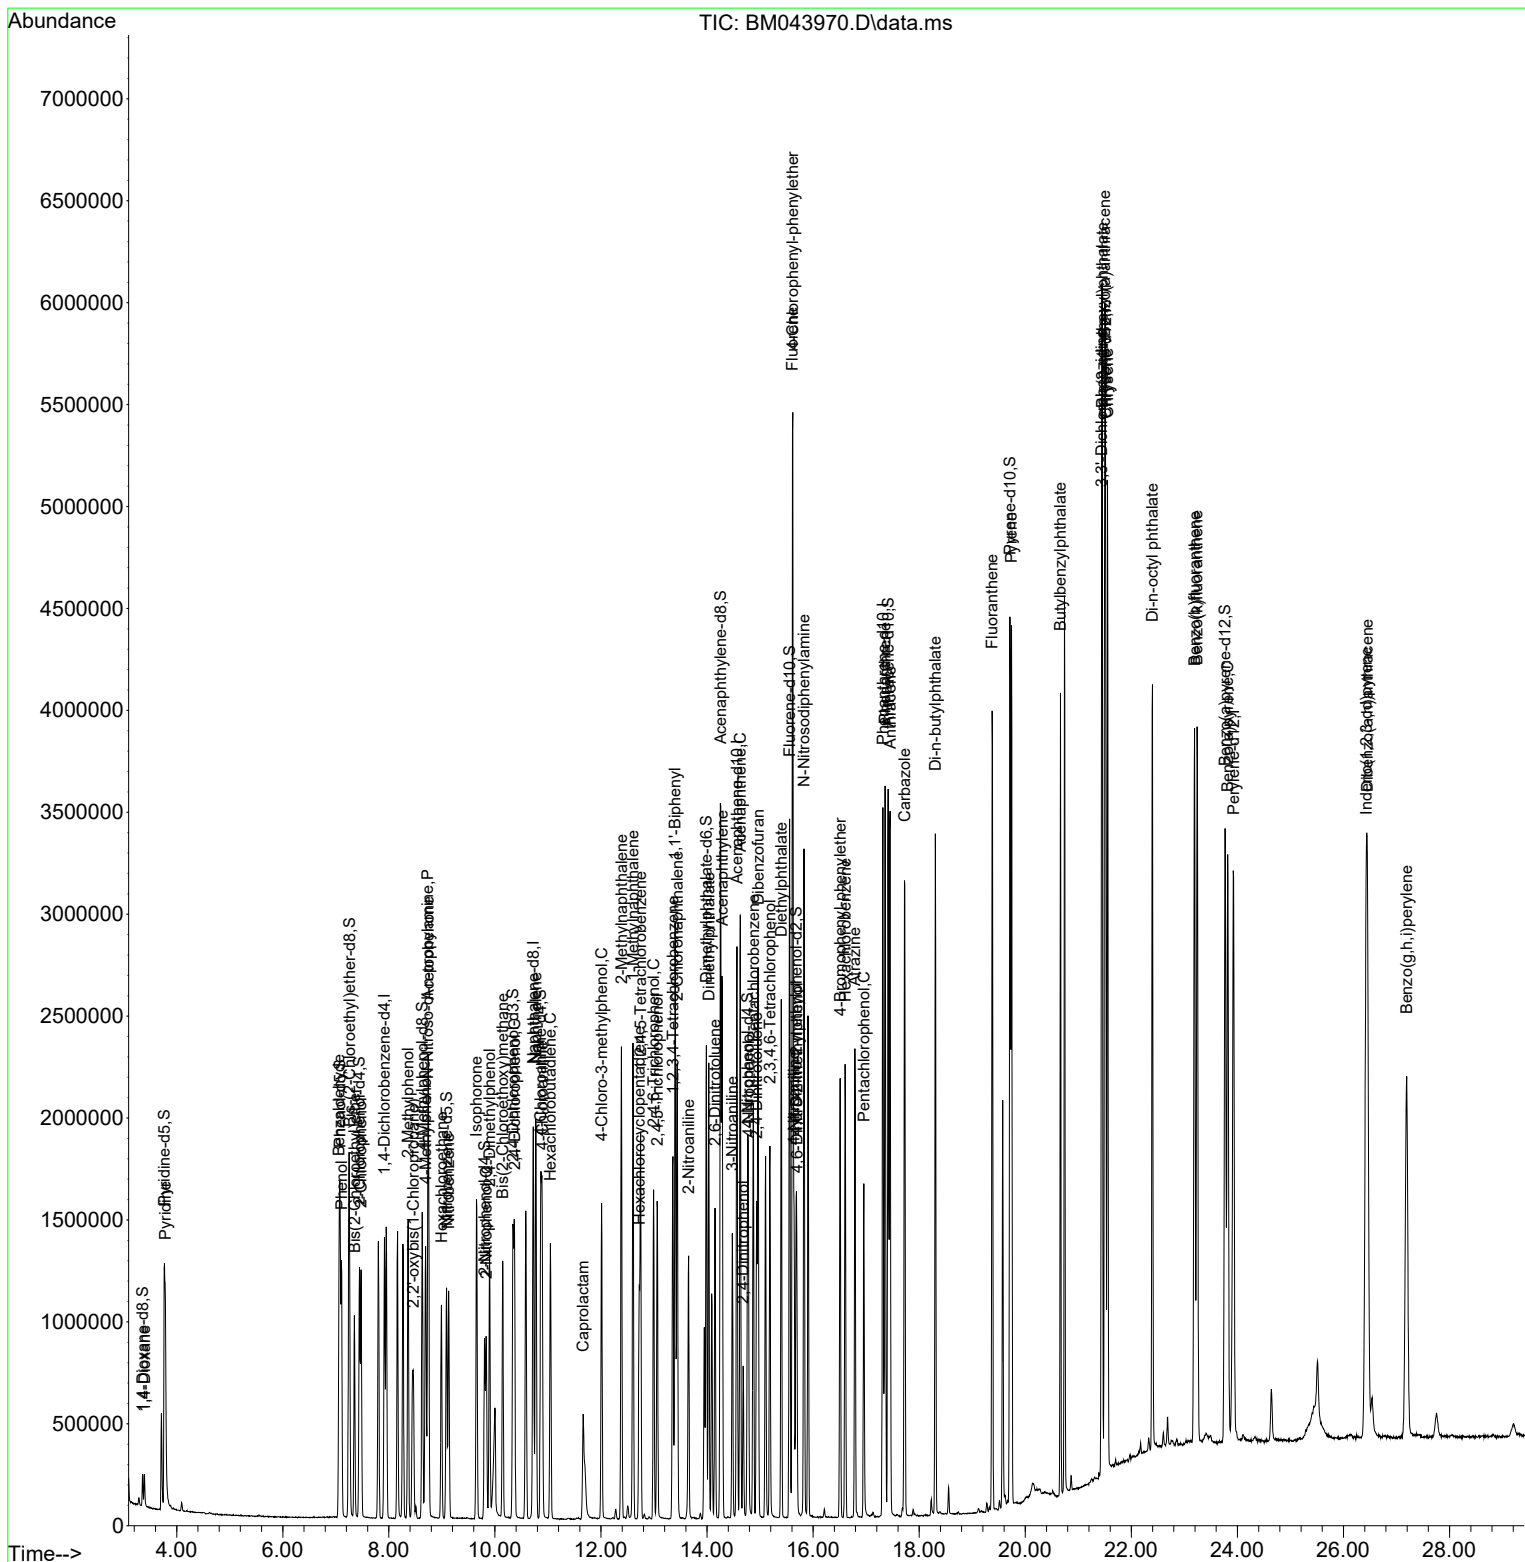




#2
1,4-Dioxane
Concen: 6.909 ng/uL
RT: 3.393 min Scan# 51
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion: 88 Resp: 73338
Ion Ratio Lower Upper
88 100
43 29.9 24.2 36.2
58 74.1 59.0 88.6



#5
Pyridine
Concen: 16.069 ng/uL
RT: 3.787 min Scan# 119
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion: 79 Resp: 488528
Ion Ratio Lower Upper
79 100
52 75.2 60.0 90.0
51 35.4 29.8 44.8









#6
Benzaldehyde
Concen: 26.689 ng/ul
RT: 7.063 min Scan# 611
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion: 77 Resp: 399326
Ion Ratio Lower Upper
77 100
105 97.4 77.0 115.4
106 94.8 76.0 114.0



#8
Phenol
Concen: 18.237 ng/ul
RT: 7.110 min Scan# 684
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion: 94 Resp: 657693
Ion Ratio Lower Upper
94 100
65 28.9 22.9 34.3
66 36.2 28.6 43.0




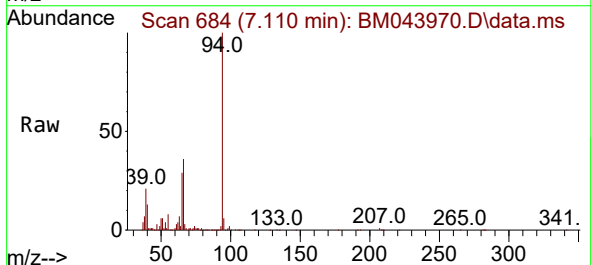


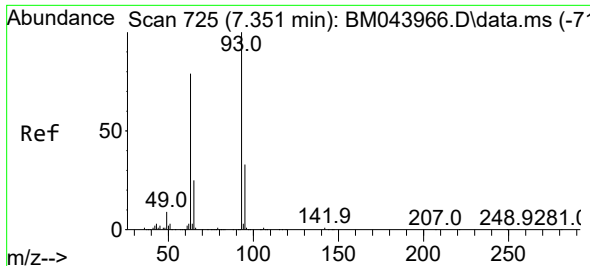

#10
 Bis(2-Chloroethyl)ether
 Concen: 18.321 ng/ul
 RT: 7.351 min Scan# 725
 Delta R.T. -0.000 min
 Lab File: BM043970.D
 Acq: 02 Feb 2024 16:54




Instrument :
 BNA_M
 ClientSampleId :
 SICV012


Tgt Ion: 93 Resp: 531238
 Ion Ratio Lower Upper
 93 100
 63 76.9 62.9 94.3
 95 32.4 26.3 39.5

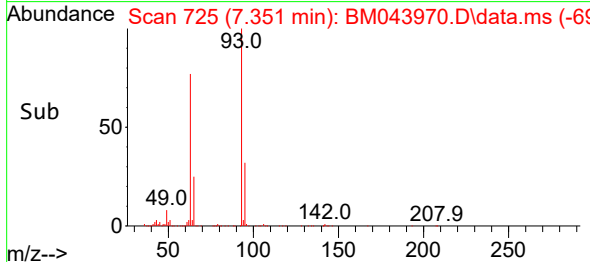

#12
 2-Chlorophenol
 Concen: 19.430 ng/ul
 RT: 7.475 min Scan# 746
 Delta R.T. -0.000 min
 Lab File: BM043970.D
 Acq: 02 Feb 2024 16:54

Tgt Ion:128 Resp: 520391
 Ion Ratio Lower Upper
 128 100
 64 47.4 38.6 58.0
 130 31.3 25.9 38.9


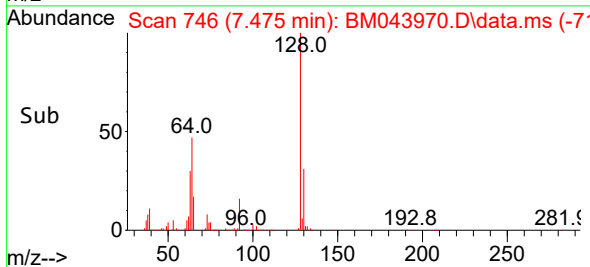

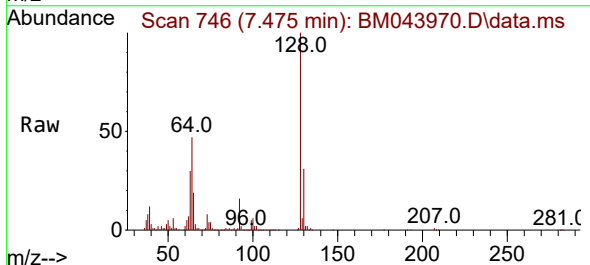




#13
2-Methylphenol
Concen: 18.371 ng/ul
RT: 8.363 min Scan# 897
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:108 Resp: 483454
Ion Ratio Lower Upper
108 100
107 85.2 71.7 107.5



#14
2,2'-oxybis(1-Chloropropane)
Concen: 17.333 ng/ul
RT: 8.457 min Scan# 913
Delta R.T. 0.012 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion: 45 Resp: 712958
Ion Ratio Lower Upper
45 100
77 15.1 11.2 16.8
79 11.1 8.3 12.5


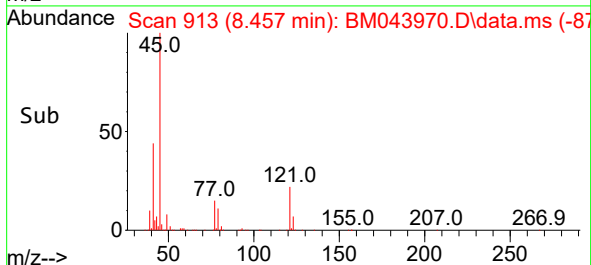






#16
Acetophenone
Concen: 19.393 ng/ul
RT: 8.745 min Scan# 962
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:105 Resp: 838033
Ion Ratio Lower Upper
105 100
77 78.6 63.2 94.8
51 28.5 23.0 34.4



#17
N-Nitroso-di-n-propylamine
Concen: 19.567 ng/ul
RT: 8.733 min Scan# 960
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion: 70 Resp: 426462
Ion Ratio Lower Upper
70 100
42 56.5 46.9 70.3
101 9.2 7.6 11.4
130 20.9 16.2 24.2


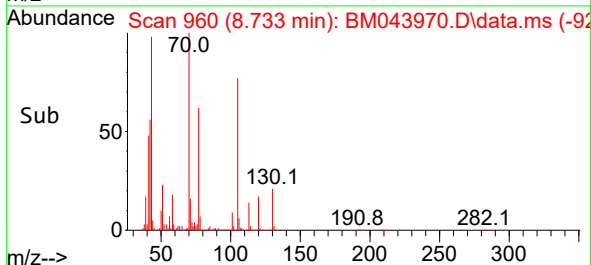
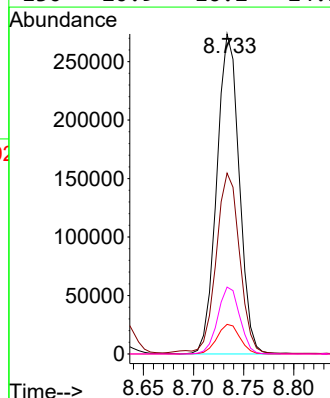
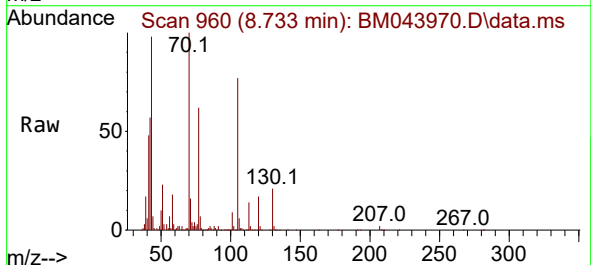




#18
4-Methylphenol
Concen: 18.386 ng/ul
RT: 8.692 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:108 Resp: 523921
Ion Ratio Lower Upper
108 100
107 110.1 85.8 128.6

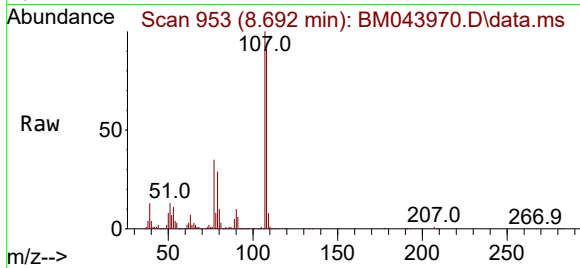

#19
Hexachloroethane
Concen: 18.717 ng/ul
RT: 8.992 min Scan# 1004
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:117 Resp: 216123
Ion Ratio Lower Upper
117 100
201 94.0 72.9 109.3
199 59.9 45.4 68.0




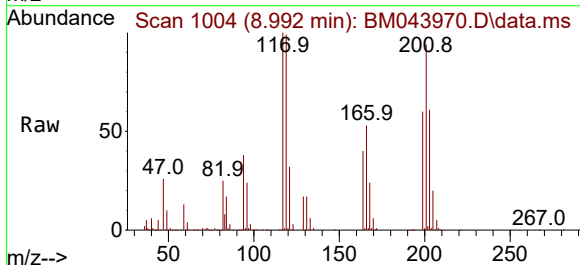


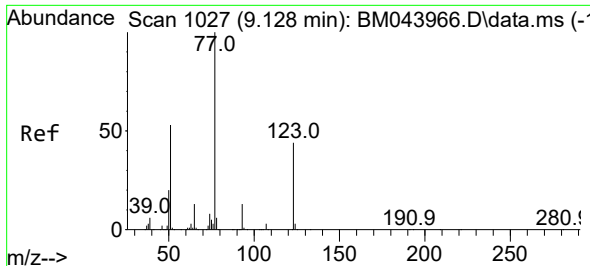

#22
Nitrobenzene
Concen: 18.519 ng/ul
RT: 9.128 min Scan# 1027
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion: 77 Resp: 595703
Ion Ratio Lower Upper
77 100
123 45.8 35.1 52.7
65 13.3 10.4 15.6

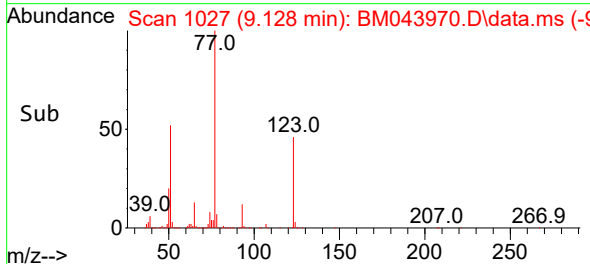

#23
Isophorone
Concen: 18.652 ng/ul
RT: 9.651 min Scan# 1116
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion: 82 Resp: 1132392
Ion Ratio Lower Upper
82 100
95 6.6 5.4 8.0
138 16.9 13.3 19.9


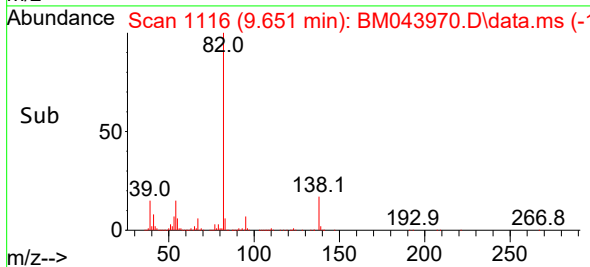

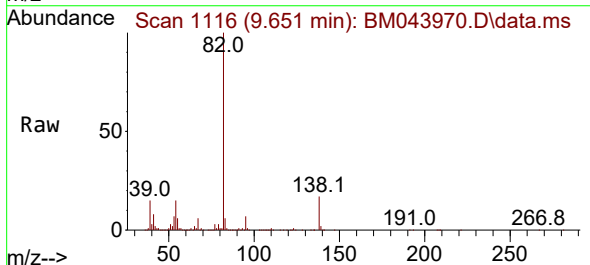




#25
2-Nitrophenol
Concen: 19.867 ng/ul
RT: 9.839 min Scan# 1148
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:139 Resp: 279371
Ion Ratio Lower Upper
139 100
65 49.7 42.3 63.5
109 28.2 23.1 34.7

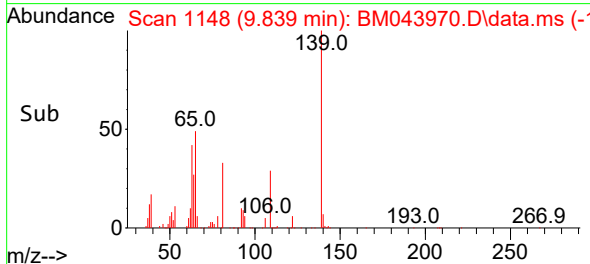

#26
2,4-Dimethylphenol
Concen: 15.143 ng/ul
RT: 9.898 min Scan# 1158
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:107 Resp: 434834
Ion Ratio Lower Upper
107 100
121 49.8 40.2 60.2
122 89.5 70.1 105.1

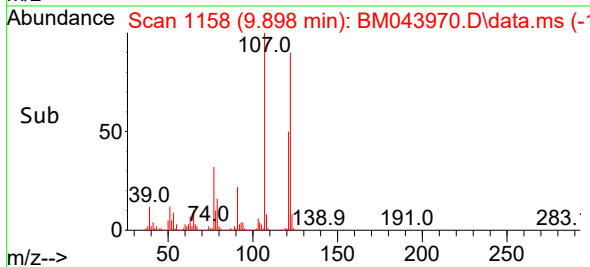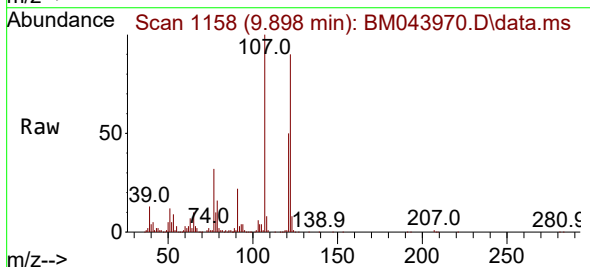



#27

Bis(2-Chloroethoxy)methane

Concen: 18.630 ng/ul

RT: 10.145 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion: 93 Resp: 706548

Ion Ratio Lower Upper

93 100

95 32.3 26.2 39.4

123 12.2 8.9 13.3



#29

2,4-Dichlorophenol

Concen: 19.616 ng/ul

RT: 10.369 min Scan# 1238

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion:162 Resp: 466958


Ion Ratio Lower Upper

162 100

164 67.0 51.7 77.5

98 38.2 29.1 43.7




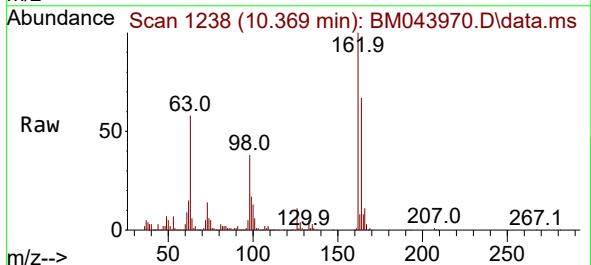




#30
Naphthalene
Concen: 18.548 ng/ul
RT: 10.774 min Scan# 1307
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:128 Resp: 1639111
Ion Ratio Lower Upper
128 100
129 11.0 8.9 13.3
127 12.9 10.2 15.4



#32
4-Chloroaniline
Concen: 18.272 ng/ul
RT: 10.892 min Scan# 1327
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:127 Resp: 721093
Ion Ratio Lower Upper
127 100
129 32.8 26.1 39.1









#33
Hexachlorobutadiene
Concen: 18.220 ng/ul
RT: 11.045 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:225 Resp: 272116
Ion Ratio Lower Upper
225 100
223 61.4 52.2 78.2
227 63.4 51.0 76.4



#34
Caprolactam
Concen: 18.918 ng/ul
RT: 11.663 min Scan# 1458
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:113 Resp: 158034
Ion Ratio Lower Upper
113 100
55 167.1 144.4 216.6
56 125.4 100.6 151.0




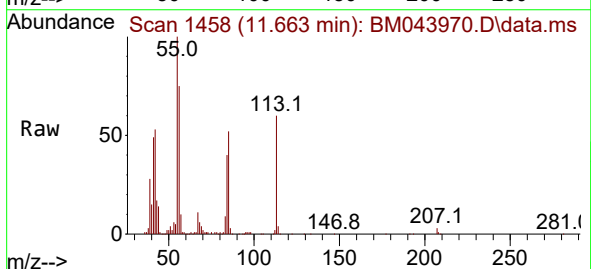




#35
4-Chloro-3-methylphenol
Concen: 19.730 ng/ul
RT: 12.010 min Scan# 1517
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:107 Resp: 509233
Ion Ratio Lower Upper
107 100
144 26.4 21.0 31.6
142 82.2 66.6 99.8

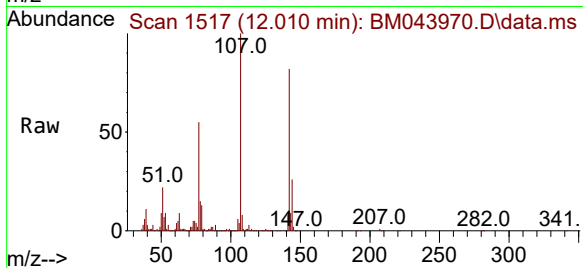

#36
2-Methylnaphthalene
Concen: 18.819 ng/ul
RT: 12.386 min Scan# 1581
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:142 Resp: 1103138
Ion Ratio Lower Upper
142 100
141 86.4 71.2 106.8




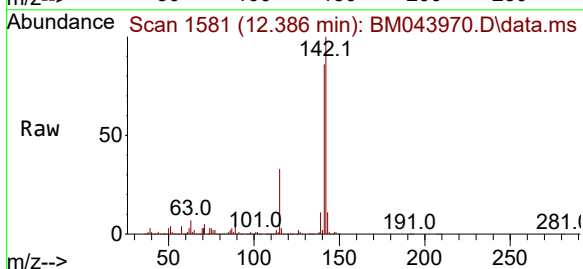


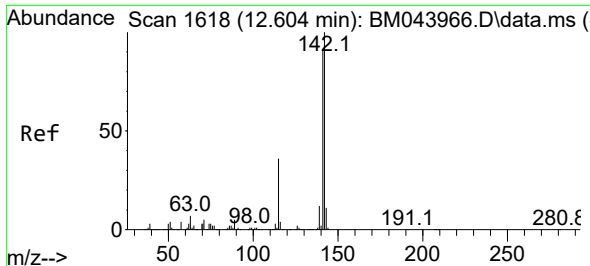

#37
1-Methylnaphthalene
Concen: 18.584 ng/ul
RT: 12.604 min Scan# 1618
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:142 Resp: 1076033
Ion Ratio Lower Upper
142 100
141 90.3 72.8 109.2
116 3.7 3.1 4.7

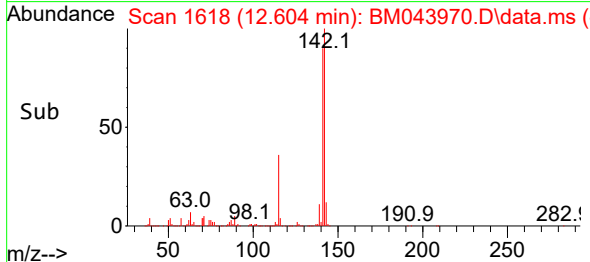

#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.177 ng/ul
RT: 12.745 min Scan# 1642
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:216 Resp: 557559
Ion Ratio Lower Upper
216 100
214 77.9 62.1 93.1
179 20.9 16.7 25.1
108 18.5 15.2 22.8


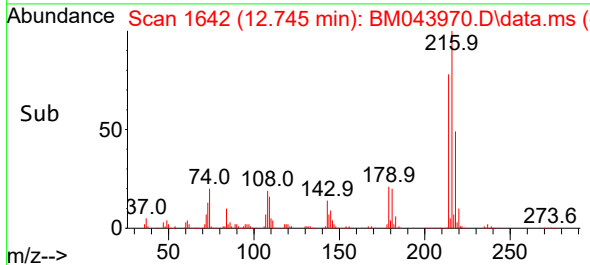

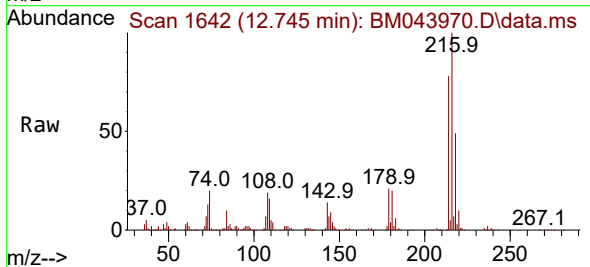




#40
Hexachlorocyclopentadiene
Concen: 14.454 ng/ul
RT: 12.721 min Scan# 1638
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:237 Resp: 272712
Ion Ratio Lower Upper
237 100
235 63.7 50.5 75.7
272 13.4 11.5 17.3



#41
2,4,6-Trichlorophenol
Concen: 19.258 ng/ul
RT: 12.992 min Scan# 1684
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:196 Resp: 350074
Ion Ratio Lower Upper
196 100
198 94.7 75.3 112.9
200 30.2 24.5 36.7

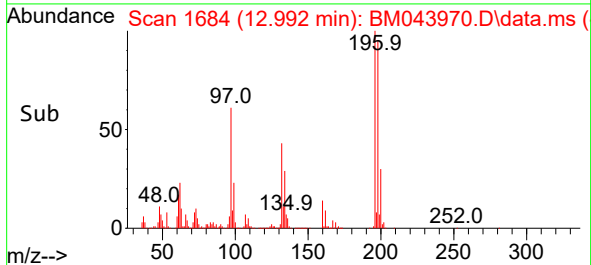



#42

2,4,5-Trichlorophenol

Concen: 19.732 ng/ul

RT: 13.063 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:196 Resp: 388000

Ion Ratio Lower Upper

196 100

198 94.9 77.5 116.3

200 29.8 24.6 37.0



#43

1,1'-Biphenyl

Concen: 19.339 ng/ul

RT: 13.398 min Scan# 1753

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion:154 Resp: 1467439


Ion Ratio Lower Upper

154 100

153 38.8 31.4 47.0

76 12.7 10.5 15.7





#44

2-Chloronaphthalene

Concen: 18.449 ng/ul

RT: 13.439 min Scan# 1760

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:162 Resp: 1108953

Ion Ratio Lower Upper

162 100

164 32.7 26.2 39.2

127 37.7 31.2 46.8



#45

2-Nitroaniline

Concen: 19.650 ng/ul

RT: 13.651 min Scan# 1796

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion: 65 Resp: 346813


Ion Ratio Lower Upper

65 100

92 68.2 52.5 78.7

138 105.2 82.2 123.4









#47
Dimethylphthalate
Concen: 18.414 ng/ul
RT: 14.033 min Scan# 1861
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:163 Resp: 1349179
Ion Ratio Lower Upper
163 100
194 3.9 3.1 4.7
164 9.7 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 21.246 ng/ul
RT: 14.151 min Scan# 1881
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:165 Resp: 285682
Ion Ratio Lower Upper
165 100
89 60.4 51.4 77.2
121 22.4 19.4 29.2




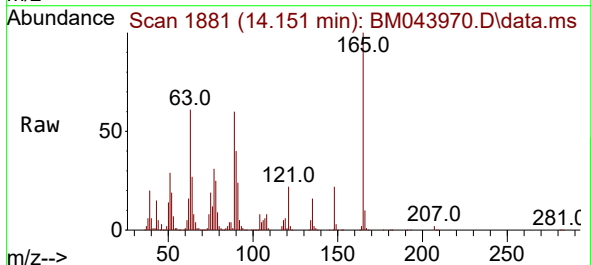


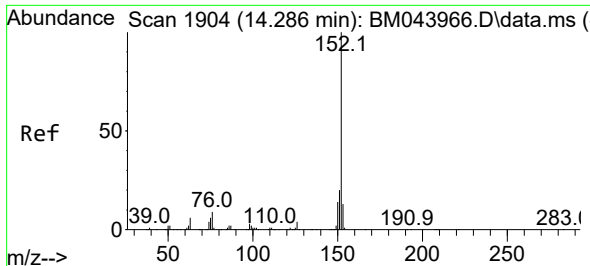

#50
Acenaphthylene
Concen: 18.646 ng/ul
RT: 14.286 min Scan# 1904
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:152 Resp: 1837388
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.8
153 12.7 10.4 15.6

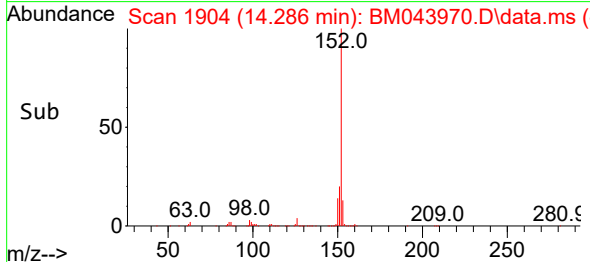

#51
3-Nitroaniline
Concen: 21.680 ng/ul
RT: 14.474 min Scan# 1936
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:138 Resp: 334980
Ion Ratio Lower Upper
138 100
108 10.5 9.0 13.6
92 114.6 93.8 140.6


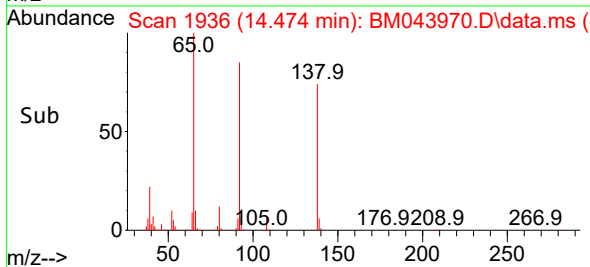

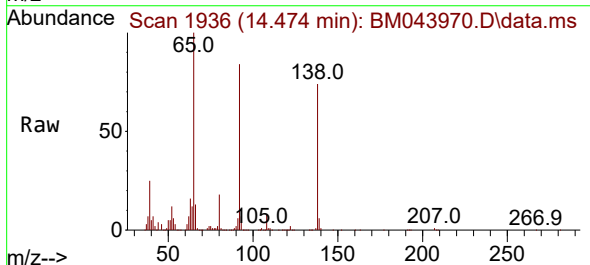




#52
Acenaphthene
Concen: 18.219 ng/ul
RT: 14.627 min Scan# 1962
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:153 Resp: 1177837
Ion Ratio Lower Upper
153 100
152 47.2 37.9 56.9
154 88.4 71.0 106.6

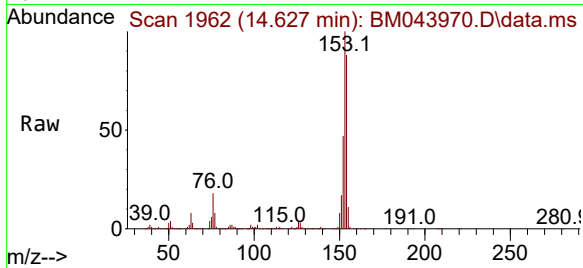

#53
2,4-Dinitrophenol
Concen: 17.124 ng/ul
RT: 14.680 min Scan# 1971
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:184 Resp: 132850
Ion Ratio Lower Upper
184 100
63 76.4 59.0 88.4
154 63.7 53.5 80.3




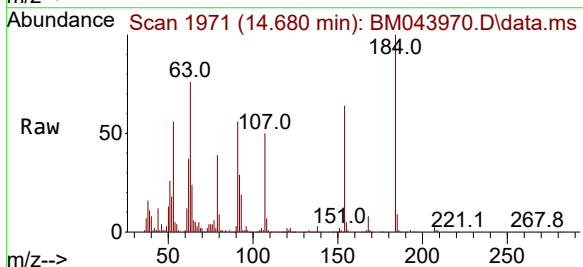




#55
4-Nitrophenol
Concen: 18.644 ng/ul
RT: 14.780 min Scan# 1988
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:109 Resp: 222449
Ion Ratio Lower Upper
109 100
139 137.0 110.6 165.8
65 133.7 107.6 161.4

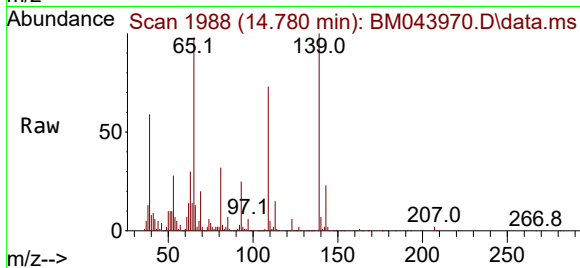

#56
Dibenzofuran
Concen: 19.001 ng/ul
RT: 14.962 min Scan# 2019
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:168 Resp: 1659976
Ion Ratio Lower Upper
168 100
139 38.1 31.1 46.7




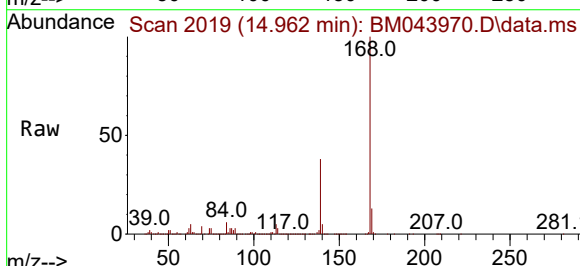




#57
 2,4-Dinitrotoluene
 Concen: 19.874 ng/ul
 RT: 14.933 min Scan# 2014
 Delta R.T. -0.000 min
 Lab File: BM043970.D
 Acq: 02 Feb 2024 16:54




Instrument :
 BNA_M
 ClientSampleId :
 SICV012


Tgt Ion:165 Resp: 388713
 Ion Ratio Lower Upper
 165 100
 63 48.7 40.6 61.0
 182 2.7 2.1 3.1

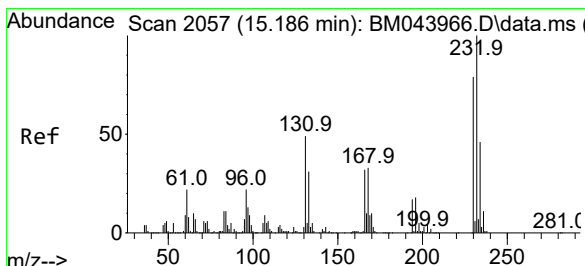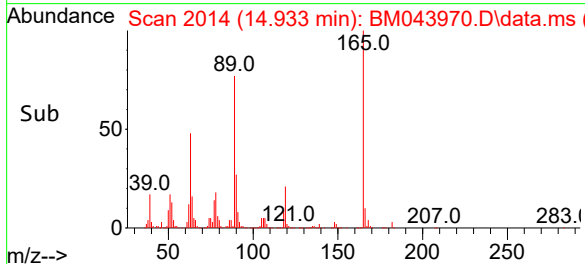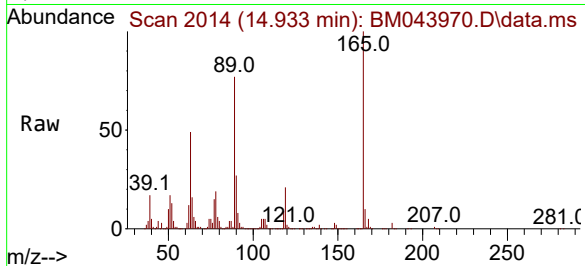

#58
 2,3,4,6-Tetrachlorophenol
 Concen: 20.339 ng/ul
 RT: 15.186 min Scan# 2057
 Delta R.T. -0.000 min
 Lab File: BM043970.D
 Acq: 02 Feb 2024 16:54

Tgt Ion:232 Resp: 332933
 Ion Ratio Lower Upper
 232 100
 131 47.9 39.2 58.8
 130 2.6 2.1 3.1
 166 32.3 25.3 37.9


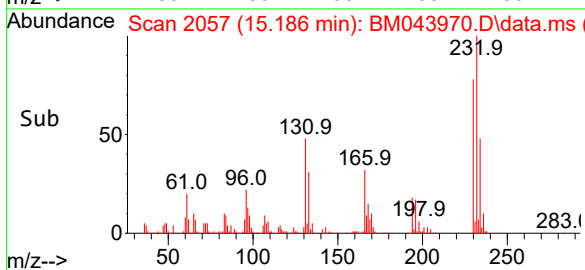

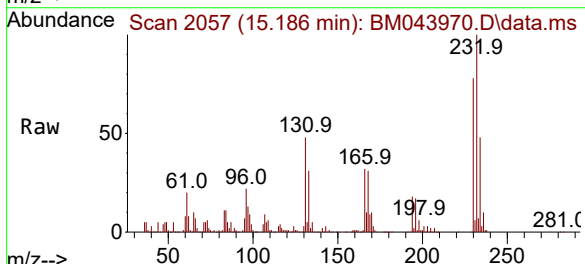




#59
Diethylphthalate
Concen: 18.330 ng/ul
RT: 15.398 min Scan# 2093
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:149 Resp: 1358172
Ion Ratio Lower Upper
149 100
177 20.9 16.6 25.0
150 12.2 9.8 14.8

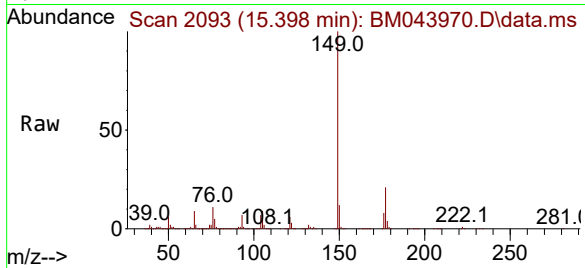

#61
Fluorene
Concen: 18.459 ng/ul
RT: 15.609 min Scan# 2129
Delta R.T. -0.006 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:166 Resp: 1360031
Ion Ratio Lower Upper
166 100
165 97.2 76.9 115.3
167 13.6 10.6 16.0




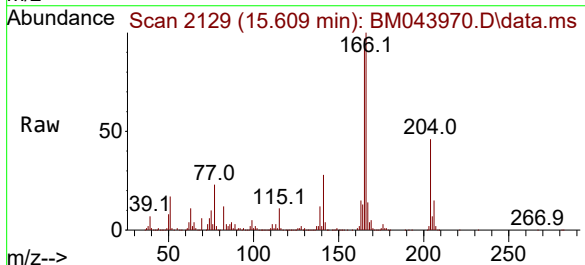




#62
4-Chlorophenyl-phenylether
Concen: 18.164 ng/ul
RT: 15.615 min Scan# 2130
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:204 Resp: 643748
Ion Ratio Lower Upper
204 100
206 32.1 26.1 39.1
141 58.9 47.0 70.4



#63
4-Nitroaniline
Concen: 23.361 ng/ul
RT: 15.639 min Scan# 2134
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:138 Resp: 349566
Ion Ratio Lower Upper
138 100
92 52.1 41.4 62.2
108 79.1 63.7 95.5




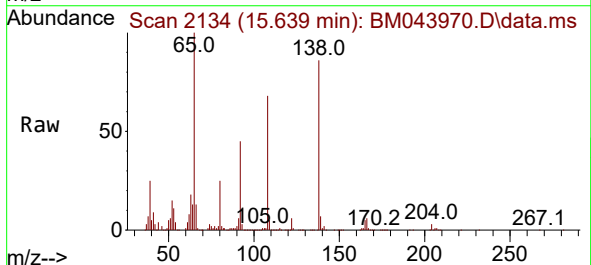




#66
 4,6-Dinitro-2-methylphenol
 Concen: 16.631 ng/ul
 RT: 15.692 min Scan# 2143
 Delta R.T. -0.000 min
 Lab File: BM043970.D
 Acq: 02 Feb 2024 16:54




Instrument :
 BNA_M
 ClientSampleId :
 SICV012


Tgt Ion:198 Resp: 212383
 Ion Ratio Lower Upper
 198 100
 182 4.8 4.0 6.0
 77 27.9 23.0 34.6



#67
 N-Nitrosodiphenylamine
 Concen: 19.151 ng/ul
 RT: 15.827 min Scan# 2166
 Delta R.T. -0.000 min
 Lab File: BM043970.D
 Acq: 02 Feb 2024 16:54

Tgt Ion:169 Resp: 1168412
 Ion Ratio Lower Upper
 169 100
 168 66.5 53.2 79.8
 167 36.0 28.9 43.3


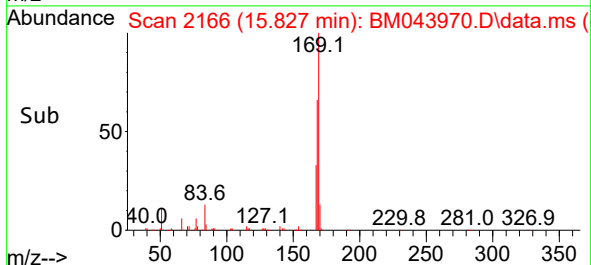






#68
4-Bromophenyl-phenylether
Concen: 18.085 ng/ul
RT: 16.509 min Scan# 2189
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:248 Resp: 377189
Ion Ratio Lower Upper
248 100
250 96.6 77.7 116.5
141 74.5 61.4 92.2



#69
Hexachlorobenzene
Concen: 17.928 ng/ul
RT: 16.604 min Scan# 2298
Delta R.T. -0.006 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:284 Resp: 433098
Ion Ratio Lower Upper
284 100
142 39.5 30.1 45.1
249 30.7 23.8 35.6





#70

Atrazine

Concen: 17.440 ng/ul

RT: 16.786 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:200 Resp: 355538

Ion Ratio Lower Upper

200 100

173 28.5 21.8 32.6

215 48.5 41.0 61.6

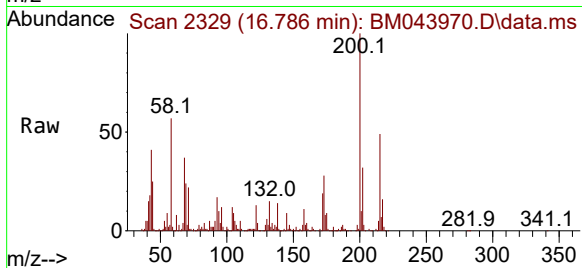

#71

Pentachlorophenol

Concen: 16.305 ng/ul

RT: 16.956 min Scan# 2358

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion:266 Resp: 253491


Ion Ratio Lower Upper

266 100

264 63.7 48.9 73.3

268 63.8 49.4 74.2




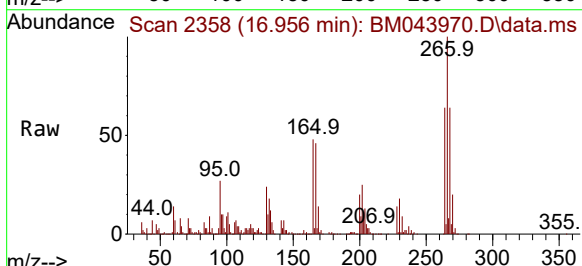




#72
Phenanthrene
Concen: 18.312 ng/ul
RT: 17.356 min Scan# 2426
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:178 Resp: 2100955
Ion Ratio Lower Upper
178 100
179 15.1 12.2 18.4
176 19.3 15.6 23.4



#74
Anthracene
Concen: 18.076 ng/ul
RT: 17.451 min Scan# 2442
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:178 Resp: 2112465
Ion Ratio Lower Upper
178 100
179 15.3 12.2 18.4
176 18.5 15.0 22.6





#75

1,2,3,4-Tetrachlorobenzene

Concen: 18.492 ng/uL

RT: 13.357 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:216 Resp: 525759

Ion Ratio Lower Upper

216 100

214 78.1 63.7 95.5

218 50.1 39.4 59.0

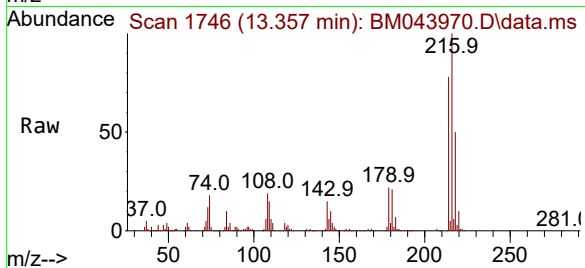

#76

Pentachlorobenzene

Concen: 18.656 ng/uL

RT: 14.874 min Scan# 2004

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion:250 Resp: 510082


Ion Ratio Lower Upper

250 100

248 62.9 49.7 74.5

252 63.0 51.8 77.8




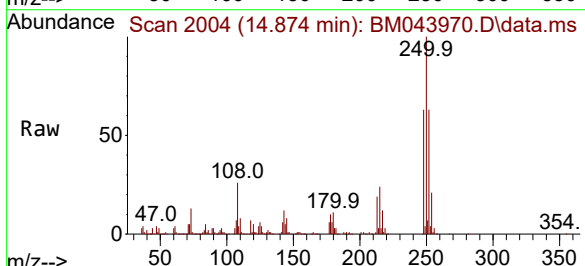




#77
 Carbazole
 Concen: 18.068 ng/ul
 RT: 17.727 min Scan# 2489
 Delta R.T. -0.000 min
 Lab File: BM043970.D
 Acq: 02 Feb 2024 16:54




Instrument :
 BNA_M
 ClientSampleId :
 SICV012


Tgt Ion:167 Resp: 1993303
 Ion Ratio Lower Upper
 167 100
 166 21.1 17.1 25.7
 139 12.8 10.6 15.8

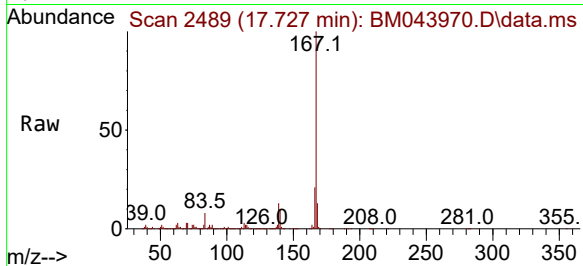

#78
 Di-n-butylphthalate
 Concen: 18.200 ng/ul
 RT: 18.303 min Scan# 2587
 Delta R.T. -0.000 min
 Lab File: BM043970.D
 Acq: 02 Feb 2024 16:54

Tgt Ion:149 Resp: 2320649
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.2 10.8
 104 5.2 4.2 6.4




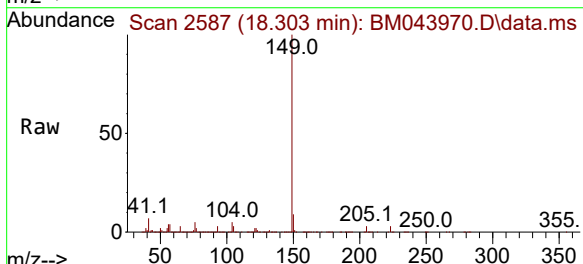




#80
Fluoranthene
Concen: 18.107 ng/ul
RT: 19.374 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54




Instrument :
BNA_M
ClientSampleId :
SICV012


Tgt Ion:202 Resp: 2337225
Ion Ratio Lower Upper
202 100
101 12.3 9.2 13.8
100 9.2 6.7 10.1

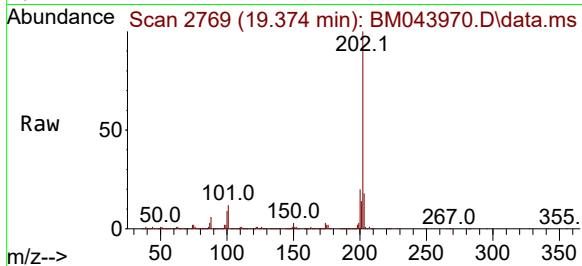

#82
Pyrene
Concen: 18.332 ng/ul
RT: 19.739 min Scan# 2831
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:202 Resp: 2506943
Ion Ratio Lower Upper
202 100
101 14.1 11.3 16.9
100 11.5 9.2 13.8

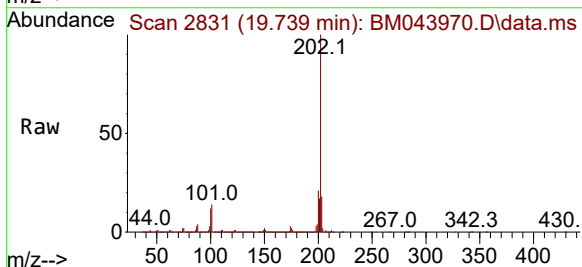



#83

Butylbenzylphthalate

Concen: 18.780 ng/ul

RT: 20.662 min Scan# 2988

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:149 Resp: 1025767

Ion Ratio Lower Upper

149 100

91 74.1 60.2 90.4

206 20.1 15.8 23.6

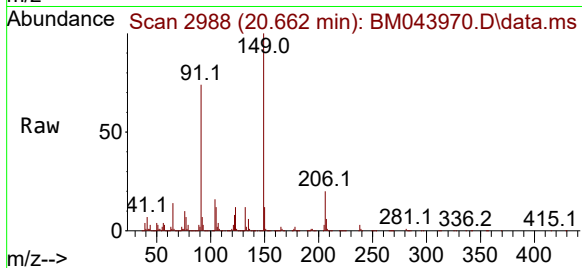

#84

3,3'-Dichlorobenzidine

Concen: 22.116 ng/ul

RT: 21.438 min Scan# 3120

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion:252 Resp: 885293


Ion Ratio Lower Upper

252 100

254 65.2 52.5 78.7

126 11.7 9.4 14.2

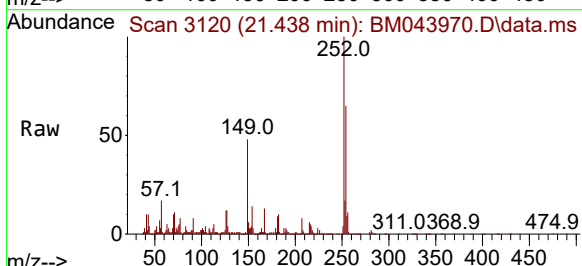



#85

Benzo(a)anthracene

Concen: 18.135 ng/ul

RT: 21.497 min Scan# 3130

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:228 Resp: 2517527

Ion Ratio Lower Upper

228 100

229 19.5 15.5 23.3

226 27.3 21.7 32.5

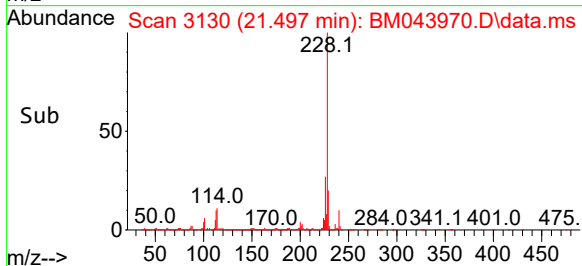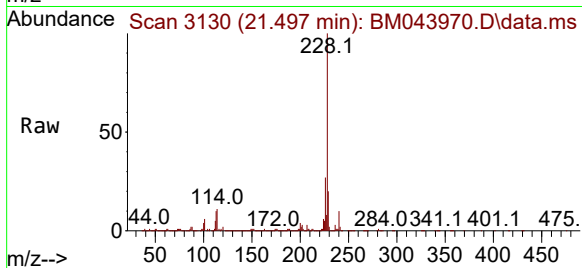

#86

Bis(2-ethylhexyl)phthalate

Concen: 18.802 ng/ul

RT: 21.450 min Scan# 3122

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion:149 Resp: 1548527


Ion Ratio Lower Upper

149 100

167 27.7 21.6 32.4

279 3.8 2.9 4.3

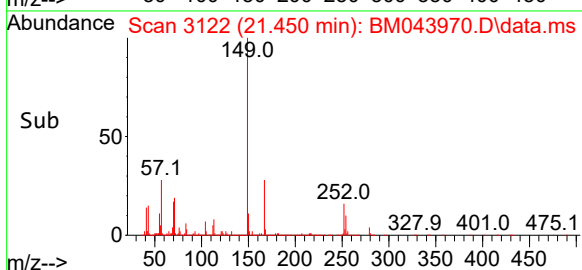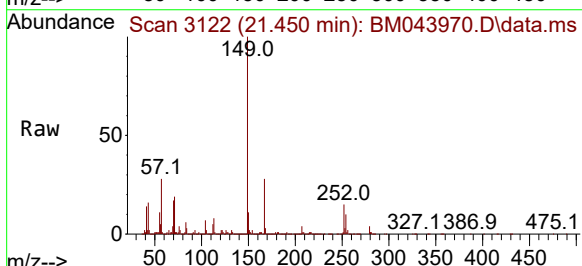



#87

Chrysene

Concen: 17.726 ng/ul

RT: 21.550 min Scan# 3139

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:228 Resp: 2293033

Ion Ratio Lower Upper

228 100

226 29.6 24.3 36.5

229 19.5 15.8 23.8



#89

Di-n-octyl phthalate

Concen: 17.761 ng/ul




RT: 22.397 min Scan# 3283


Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Tgt Ion:149 Resp: 2576054





#90

Benzo(b)fluoranthene

Concen: 18.129 ng/ul

RT: 23.191 min Scan# 3418

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:252 Resp: 2478602

Ion Ratio Lower Upper

252 100

253 21.8 17.4 26.0

125 10.7 8.2 12.4



#91

Benzo(k)fluoranthene

Concen: 17.337 ng/ul

RT: 23.238 min Scan# 3426

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion:252 Resp: 2364128


Ion Ratio Lower Upper

252 100

253 21.9 17.3 25.9

125 10.7 8.5 12.7





#93

Benzo(a)pyrene

Concen: 17.012 ng/ul

RT: 23.815 min Scan# 3

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54

Instrument :

BNA_M

ClientSampleId :

SICV012





Tgt Ion:252 Resp: 2217465

Ion Ratio Lower Upper

252 100

253 21.5 17.5 26.3

125 12.2 9.2 13.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 18.280 ng/ul

RT: 26.426 min Scan# 3968

Delta R.T. -0.000 min

Lab File: BM043970.D

Acq: 02 Feb 2024 16:54




Tgt Ion:276 Resp: 2927083


Ion Ratio Lower Upper

276 100

138 24.3 19.4 29.2

277 23.9 19.8 29.8









#95
Dibenzo(a,h)anthracene
Concen: 18.322 ng/ul
RT: 26.450 min Scan# 3972
Delta R.T. -0.000 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Instrument :
BNA_M
ClientSampleId :
SICV012

Tgt Ion:278 Resp: 2440839
Ion Ratio Lower Upper
278 100
139 17.6 14.3 21.5
279 24.2 18.4 27.6



#96
Benzo(g,h,i)perylene
Concen: 18.098 ng/ul
RT: 27.191 min Scan# 4098
Delta R.T. 0.006 min
Lab File: BM043970.D
Acq: 02 Feb 2024 16:54

Tgt Ion:276 Resp: 2324116
Ion Ratio Lower Upper
276 100
138 23.3 19.2 28.8
277 23.3 18.3 27.5

