


Data Path : Z:\HPCHEM1\BNA_M\Data\BM020315\
 Data File : BM000408.D
 Acq On : 03 Feb 2015 08:45
 Operator : TP/IZ
 Sample : DFTPP15
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP15

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM020315.M
 Title : SVOA CALIBRATION
 Last Update : Tue Feb 03 12:57:43 2015

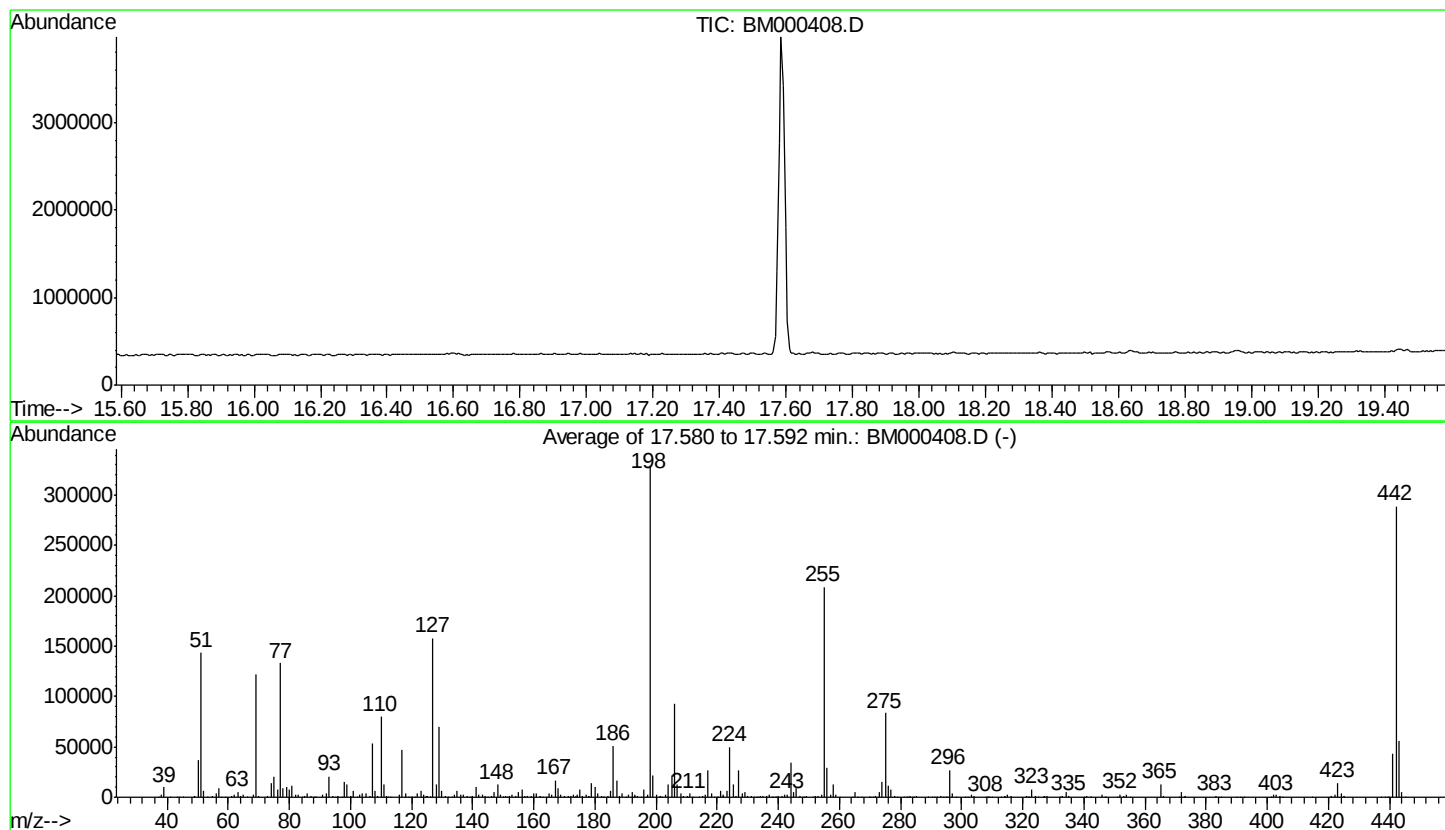

AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	143450	PASS
68	69	0.00	2	1.7	2026	PASS
69	198	0.00	100	37.2	122525	PASS
70	69	0.00	2	0.6	727	PASS
127	198	10	80	47.9	157824	PASS
197	198	0.00	2	0.7	2293	PASS
198	198	100	100	100.0	329301	PASS
199	198	5	9	6.7	21973	PASS
275	198	10	60	25.3	83376	PASS
365	198	1	100	4.0	13093	PASS
441	443	0.01	100	77.5	43162	PASS
442	198	50	100	87.7	288810	PASS
443	442	15	24	19.3	55725	PASS