

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020317\
 Data File : BM008971.D
 Acq On : 03 Feb 2017 19:52
 Operator : SJ/MA
 Sample : I1681-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB1

Quant Time: Feb 03 22:30:12 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 03 22:25:40 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	53340	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	228918	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.55	164	163526	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	339335	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	412984	20.00	ng/ul	-0.01
83) Perylene-d12	23.82	264	395904	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.37	96	7861	5.89	ng/uL	0.00
5) Phenol-d5	7.06	99	26318	5.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.24	67	119132	29.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.44	132	73707	23.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.60	113	49260	13.08	ng/ul	-0.01
19) Nitrobenzene-d5	9.07	128	46940	28.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	54217	29.51	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.33	165	96270	24.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	163	0.05	ng/ul	-0.13
43) Dimethylphthalate-d6	13.96	166	372227	31.05	ng/ul	0.00
46) Acenaphthylene-d8	14.24	160	404924	29.80	ng/ul	0.00
51) 4-Nitrophenol-d4	14.73	143	9810	5.01	ng/ul	-0.01
57) Fluorene-d10	15.54	176	339895	30.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	68829	31.33	ng/ul	0.00
70) Anthracene-d10	17.39	188	601701	37.11	ng/ul	0.00
76) Pyrene-d10	19.69	212	684659	37.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.67	264	637177	35.44	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
21) Isophorone	9.80	82	13509	1.20	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020317\
Data File : BM008971.D
Acq On : 03 Feb 2017 19:52
Operator : SJ/MA
Sample : I1681-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB1

Quant Time: Feb 03 22:30:12 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 03 22:25:40 2017
Response via : Initial Calibration

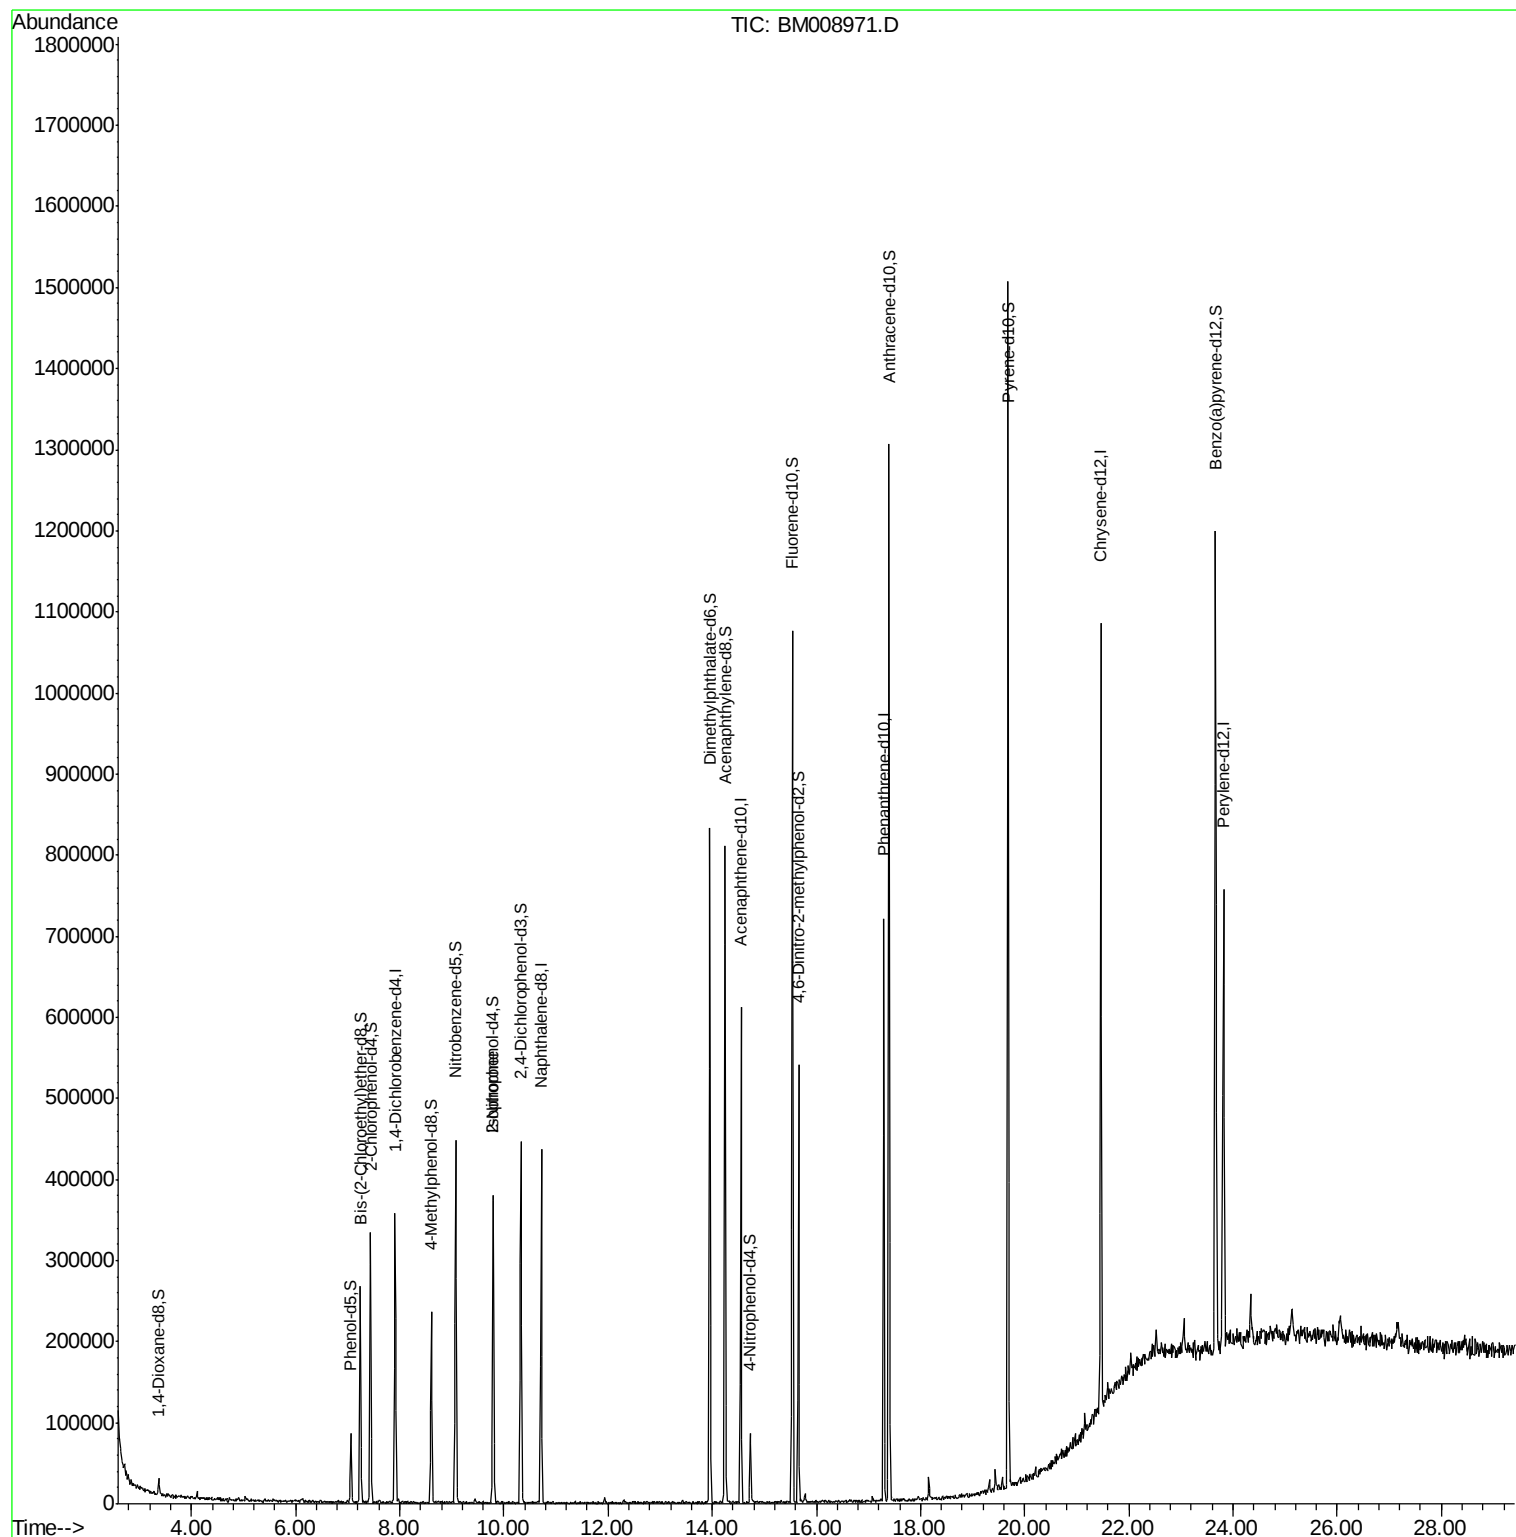

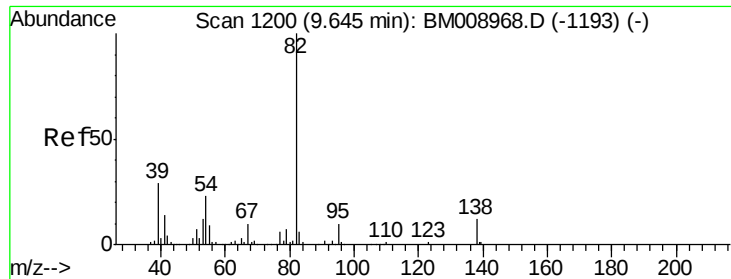

#21

Isophorone

Concen: 1.20 ng/ul

RT: 9.80 min Scan# 1226

Delta R.T. 0.15 min

Lab File: BM008971.D


Acq: 03 Feb 2017 19:52

Instrument :

BNA_M

ClientSampleId :

C0AB1

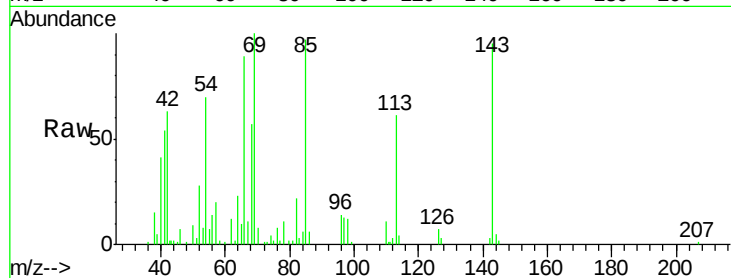

Tgt Ion: 82 Resp: 13509

Ion Ratio Lower Upper

82 100

95 0.0 7.7 11.5#

138 0.0 9.4 14.0#

