
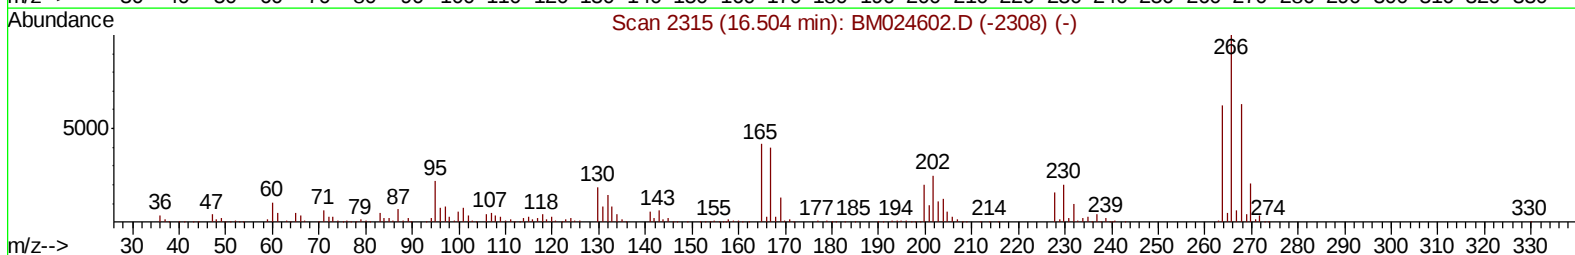
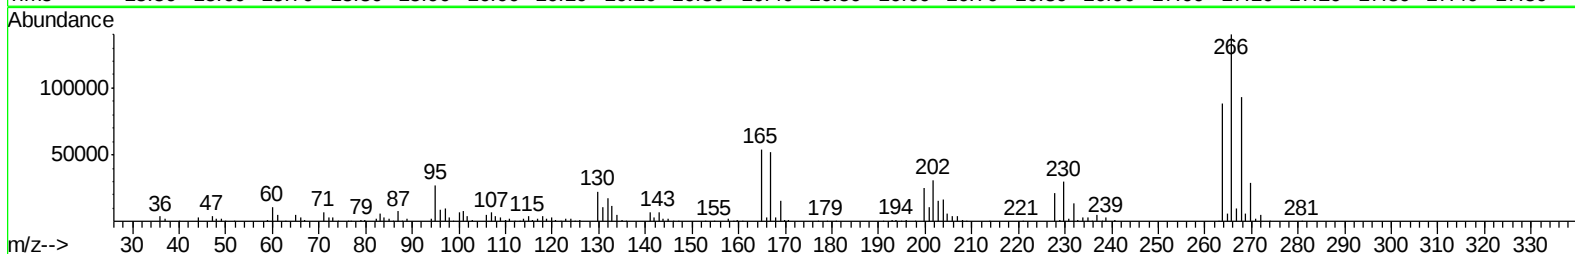


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020320\
Data File : BM024695.D
Acq On : 03 Feb 2020 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 04:15:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 23 14:57:07 2020
Response via : Initial Calibration

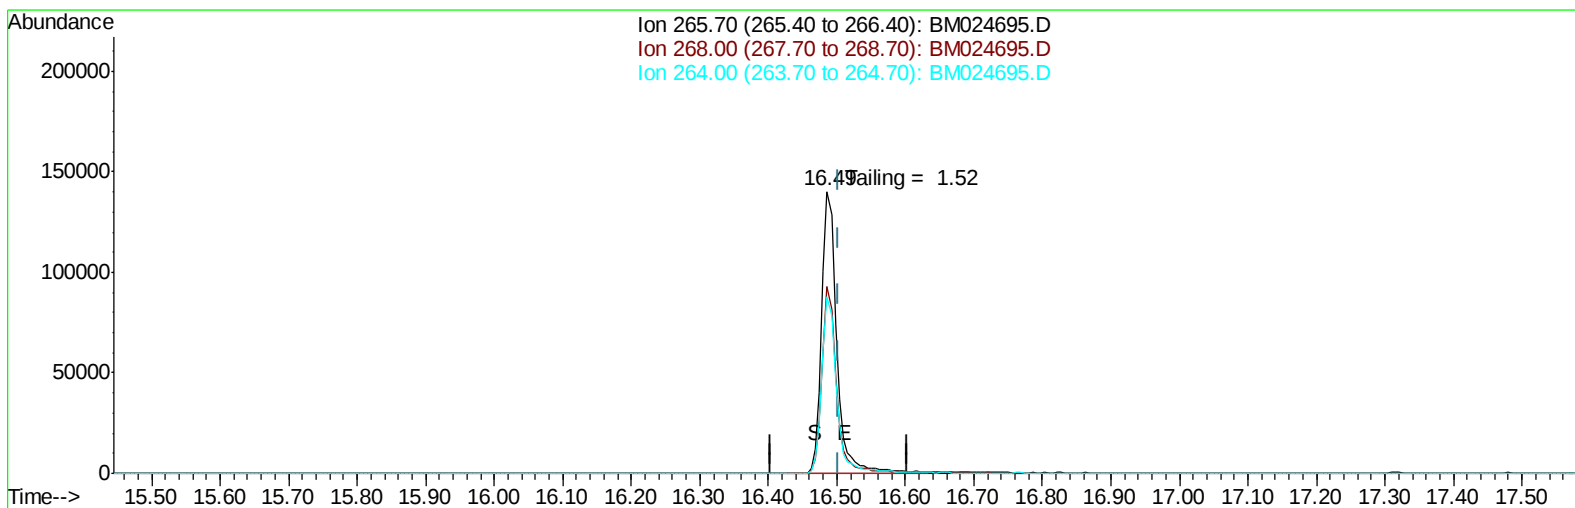

TIC: BM024695.D

(70) Pentachlorophenol (C)




16.486min (-0.018) 0.00ng

response 211546

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	66.29
264.00	62.40	62.96
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020320\
 Data File : BM024695.D
 Acq On : 03 Feb 2020 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 04:15:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 23 14:57:07 2020
 Response via : Initial Calibration

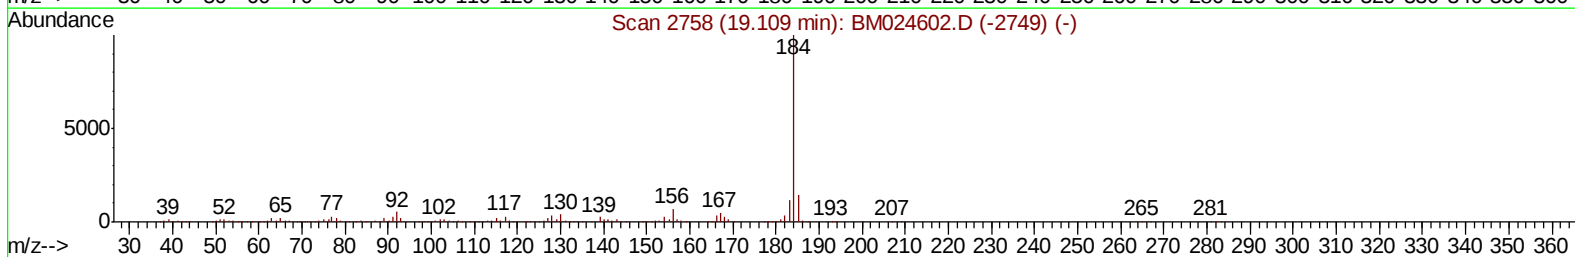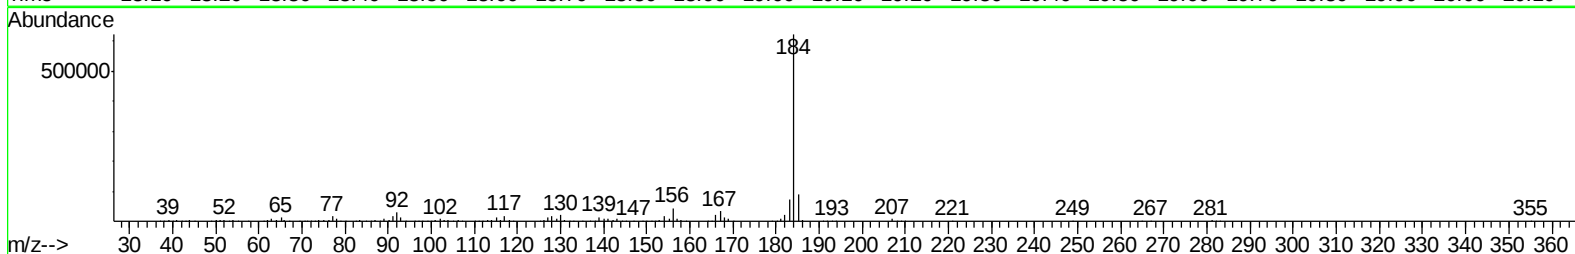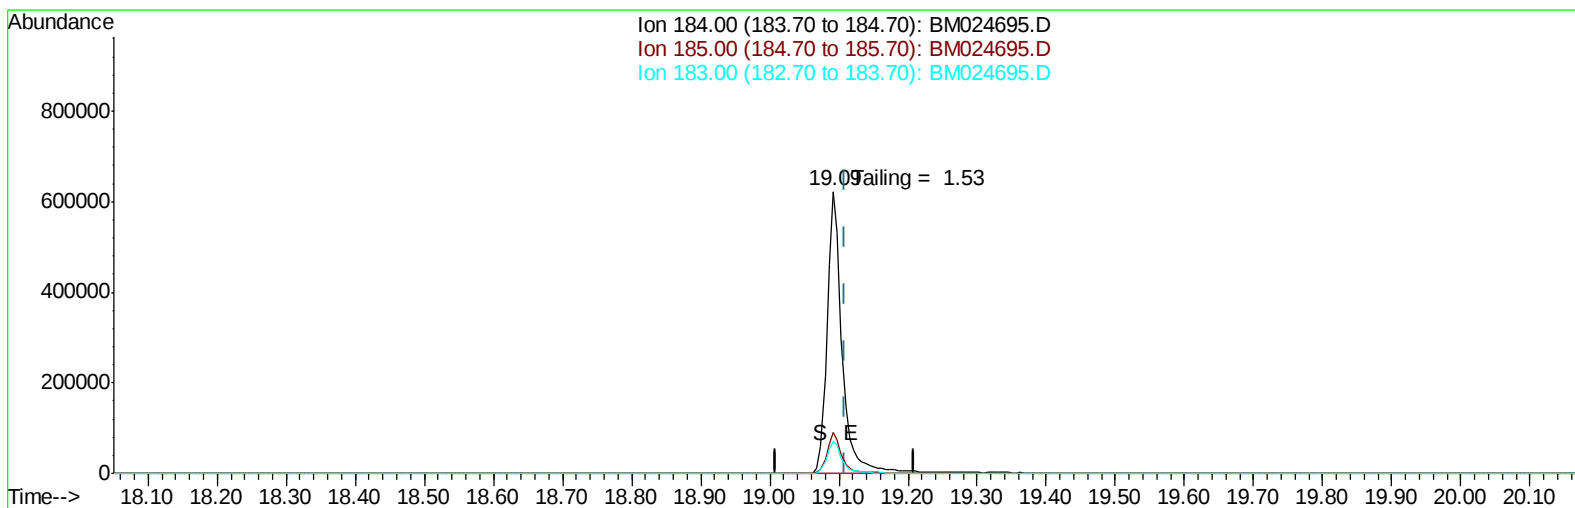

TIC: BM024695.D

(77) Benzidine

19.092min (-0.018) 50354.45ng

response 925251

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.50
183.00	12.00	11.47
0.00	0.00	0.00