

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020320\
 Data File : BM024701.D
 Acq On : 03 Feb 2020 16:23
 Operator : CG/JU
 Sample : L1346-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PD-2-(35-36)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	364	371	381	rBV	4178952	5679482	47.12%	8.570%
2	6.628	628	636	646	rBV	3776859	5790224	48.04%	8.737%
3	7.422	764	771	781	rBV	802205	1218822	10.11%	1.839%
4	7.739	817	825	835	rBV	3431205	5269582	43.72%	7.951%
5	8.563	957	965	977	rBV	2386783	3849300	31.94%	5.808%
6	10.181	1233	1240	1249	rBV	950595	1562950	12.97%	2.358%
7	12.686	1658	1666	1683	rBV	6126163	8989191	74.58%	13.564%
8	13.545	1807	1812	1821	rBV	126872	185781	1.54%	0.280%
9	14.074	1896	1902	1912	rBV	1535043	2228229	18.49%	3.362%
10	15.574	2150	2157	2176	rBV	6334837	8817840	73.16%	13.305%
11	16.827	2363	2370	2380	rBV	2012897	2804818	23.27%	4.232%
12	17.768	2525	2530	2535	rBV	147283	203496	1.69%	0.307%
13	19.486	2816	2822	2832	rBV	10302056	12053031	100.00%	18.186%
14	20.797	3041	3045	3049	rBV	257690	345031	2.86%	0.521%
15	21.039	3081	3086	3095	rVB	2744260	3467028	28.76%	5.231%
16	22.215	3284	3286	3293	rVB2	169137	214700	1.78%	0.324%
17	23.144	3438	3444	3453	rVB	2001611	3595173	29.83%	5.425%


Sum of corrected areas: 66274678

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020320\
Data File : BM024701.D
Acq On : 03 Feb 2020 16:23
Operator : CG/JU
Sample : L1346-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PD-2-(35-36)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

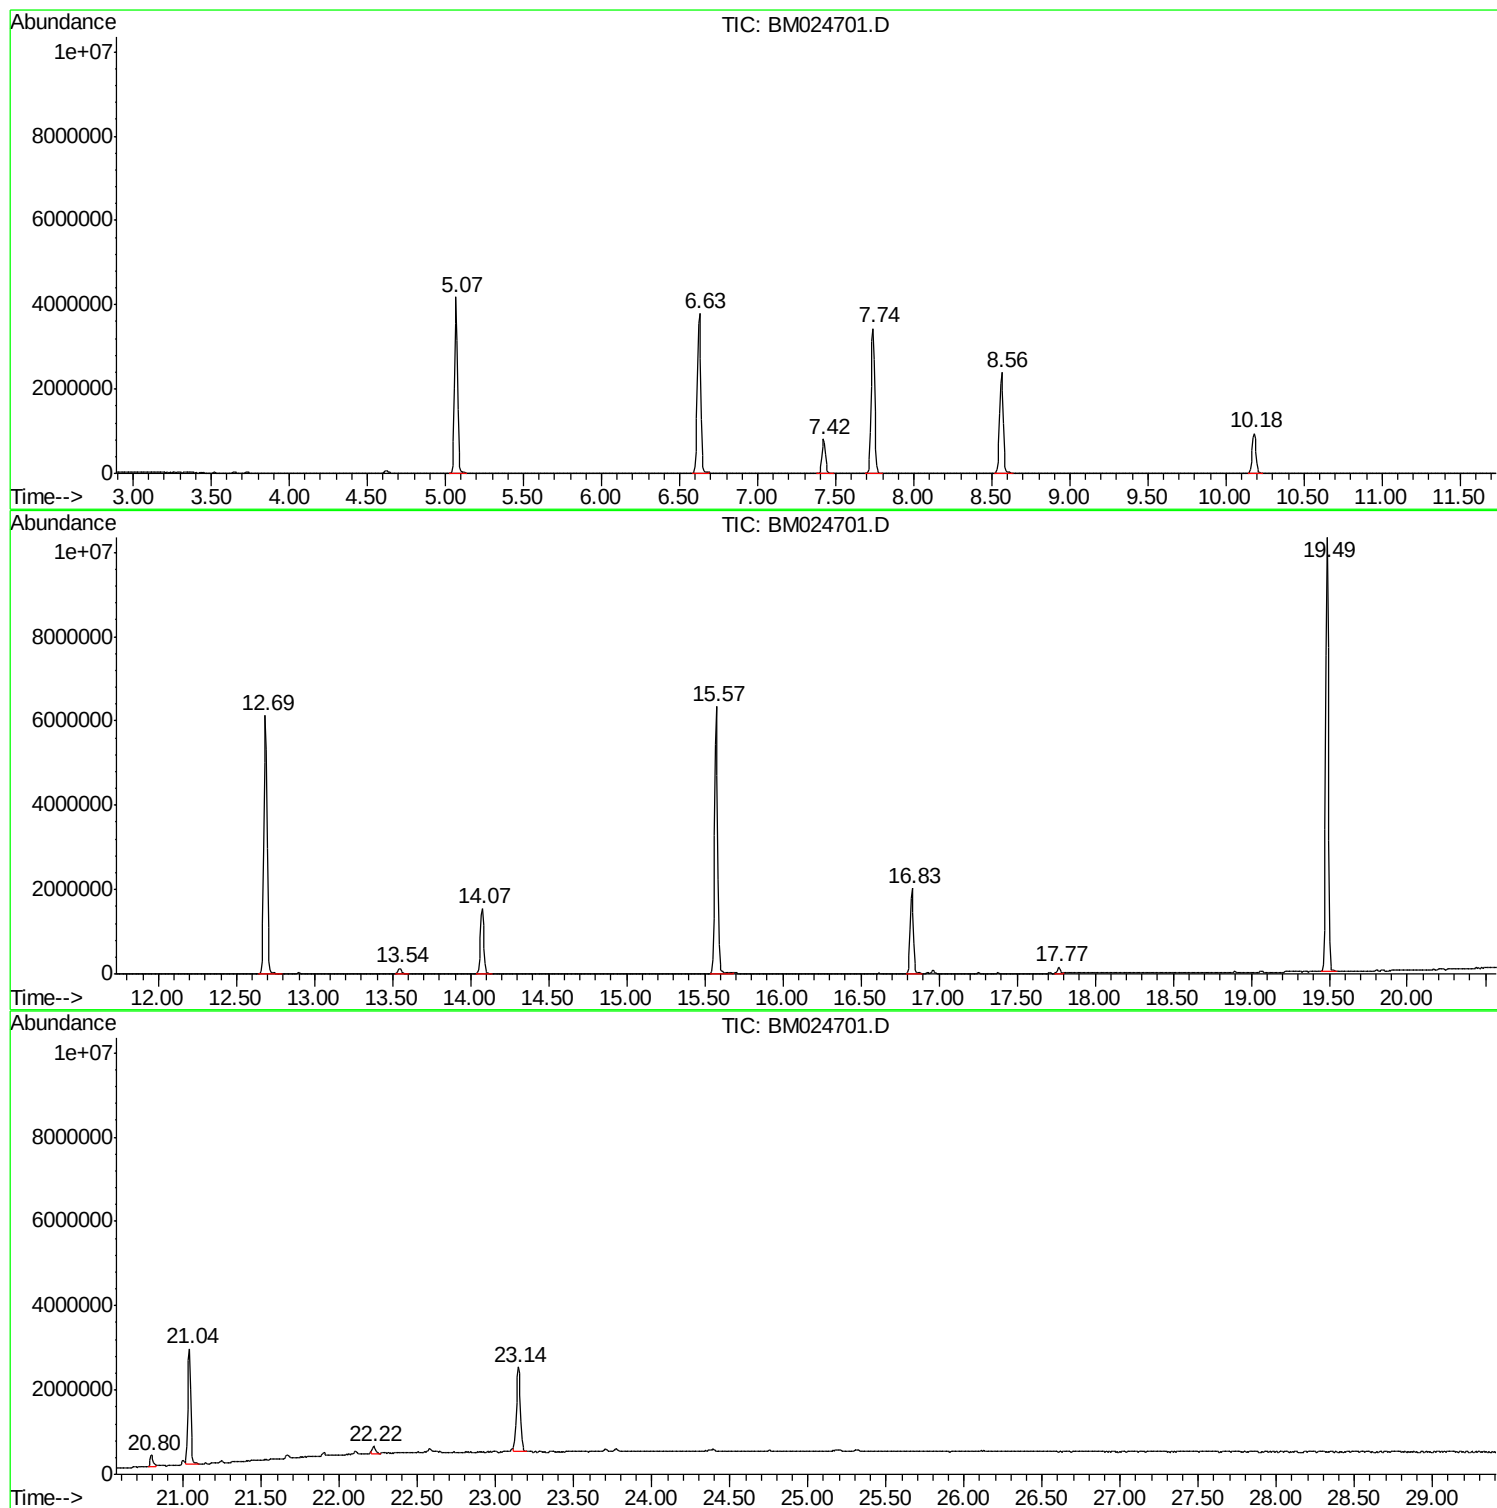

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020320\
Data_File : BM024701.D
Acq_On : 03_Feb_2020 16:233
Operator : CG/JUU
Sample : L1346-033
Misc :
ALS_Vial : 7 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
PD-2-(35-36)

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
