


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020320\
 Data File : BM024695.D
 Acq On : 03 Feb 2020 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 23 14:57:07 2020

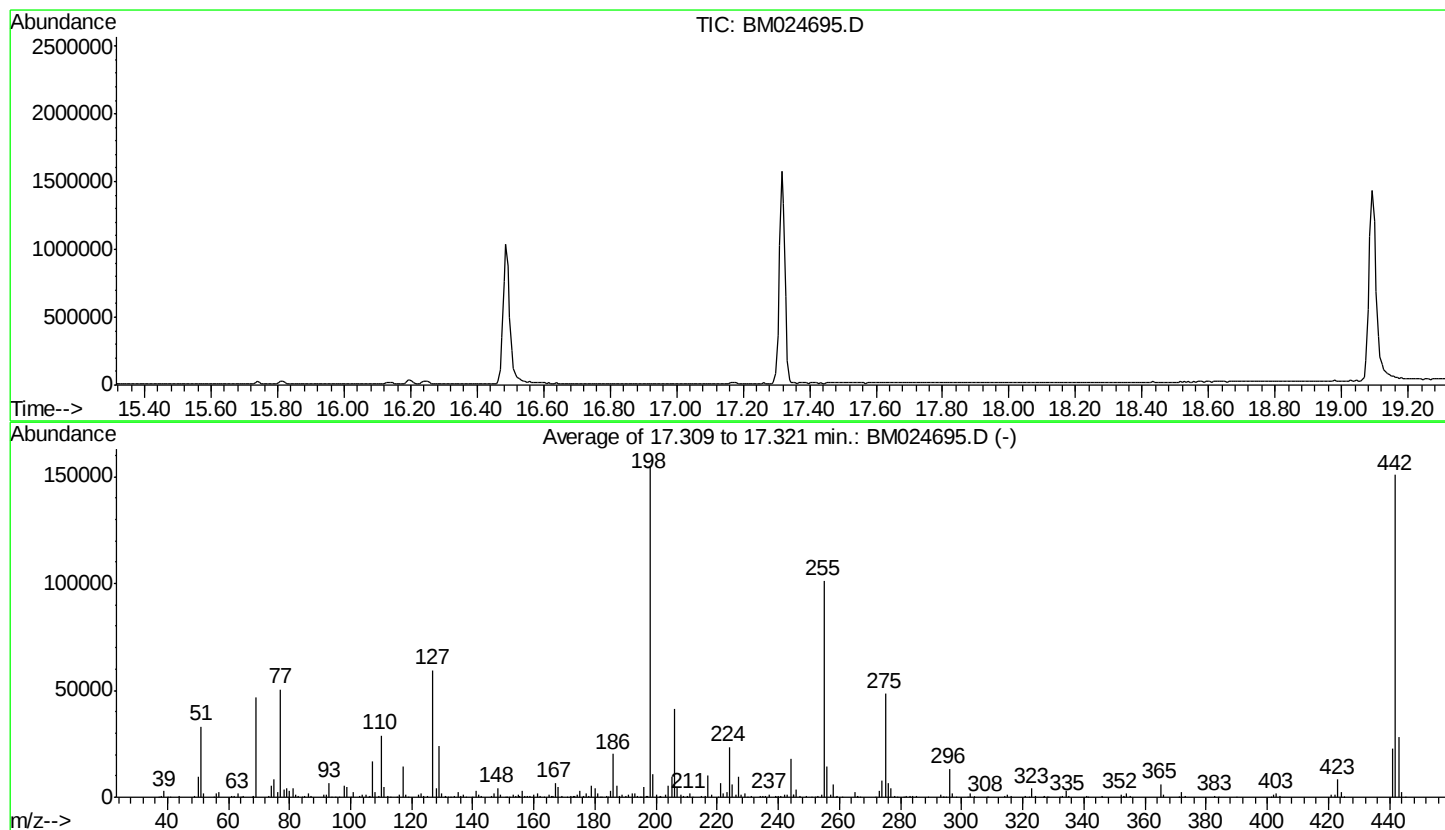

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	33128	PASS
68	69	0.00	2	1.5	712	PASS
69	198	0.00	100	30.2	46909	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.3	59368	PASS
197	198	0.00	2	0.4	600	PASS
198	198	100	100	100.0	155117	PASS
199	198	5	9	6.9	10744	PASS
275	198	10	60	31.2	48357	PASS
365	198	1	100	4.0	6132	PASS
441	198	0.01	100	14.6	22712	PASS
442	198	50	100	97.1	150680	PASS
443	442	15	24	18.8	28298	PASS