
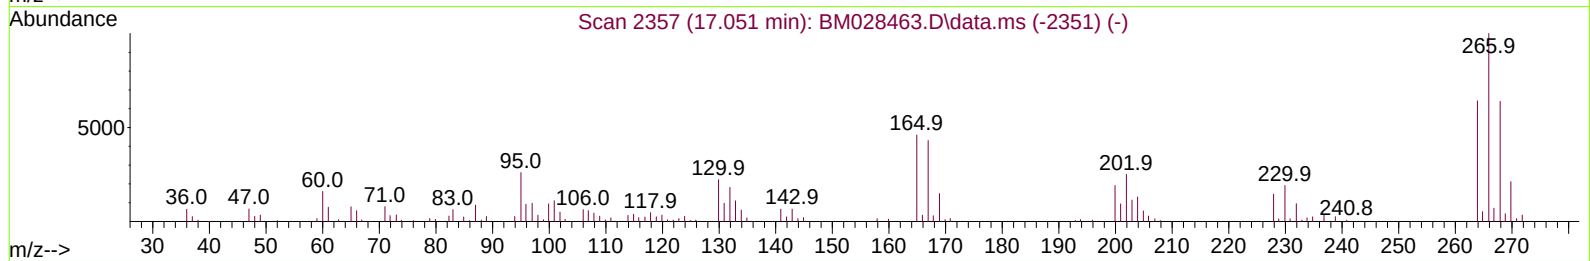
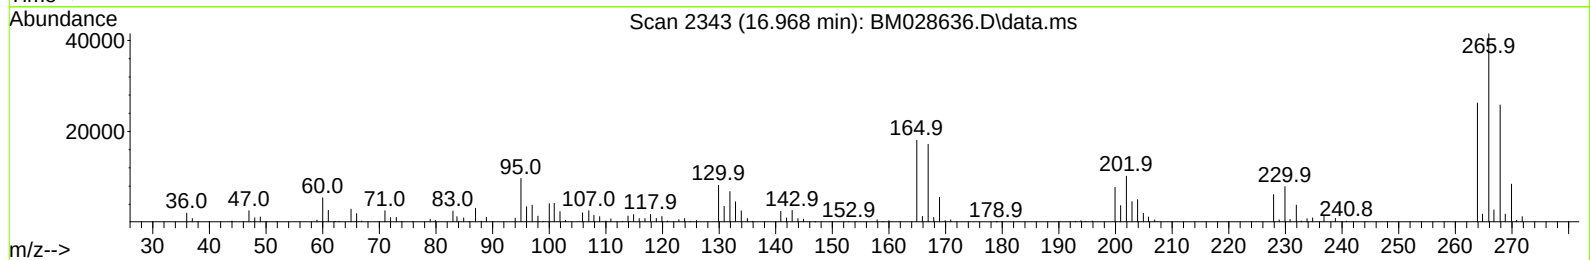


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028636.D
Acq On : 03 Feb 2021 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 01:24:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

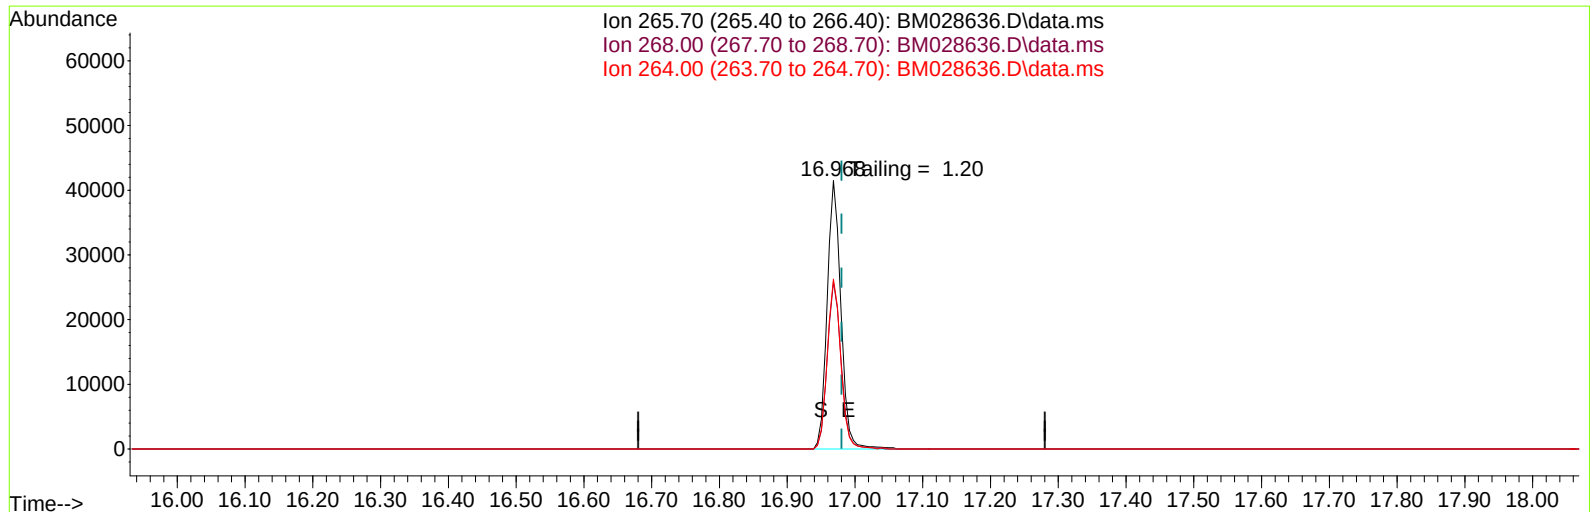

TIC: BM028636.D\data.ms

(70) Pentachlorophenol (C)




16.968min (-0.012) 0.00 ng

response 58352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.26
264.00	63.30	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028636.D
Acq On : 03 Feb 2021 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 01:24:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

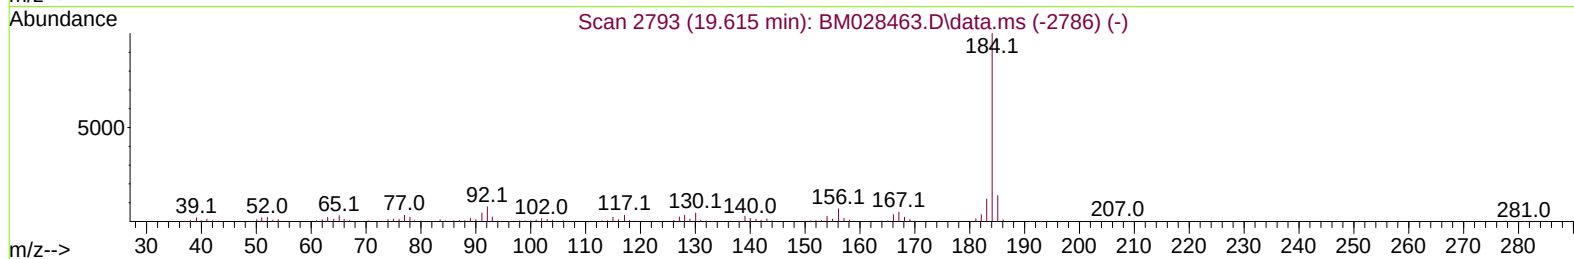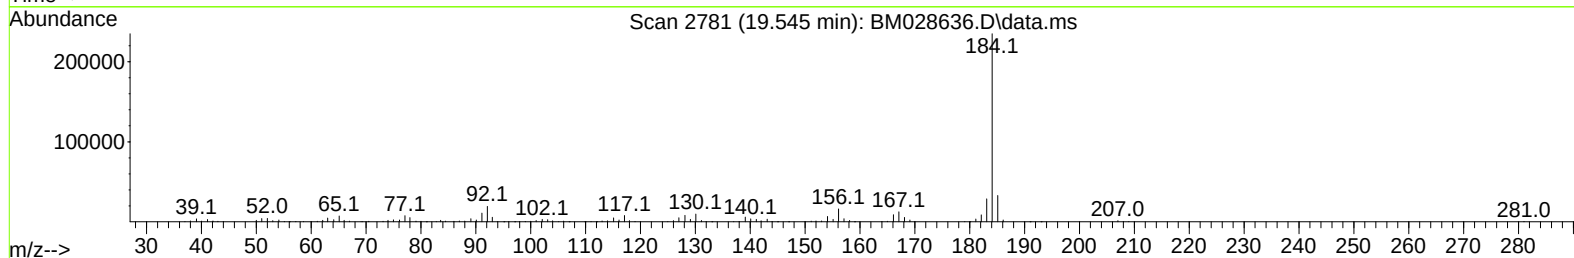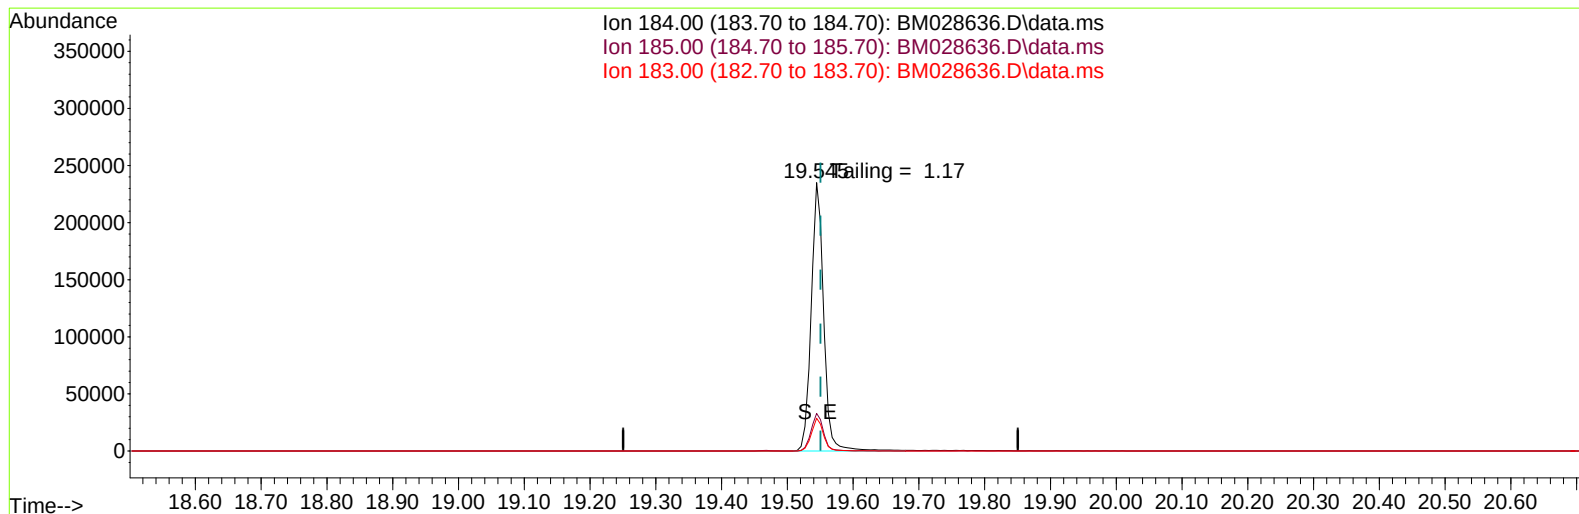

TIC: BM028636.D\data.ms

(77) Benzidine

19.545min (-0.006) 250751.91 ng

response 310136

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.01
183.00	12.10	12.25
0.00	0.00	0.00