

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
 Data File : BM028639.D
 Acq On : 03 Feb 2021 12:06
 Operator : CG/JU
 Sample : M1292-14
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-010-0205

Integration Parameters: rteint.p

Integrator: RTE

Smothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	301	306	312	rVB	9714	14783	1.60%	0.170%
2	5.469	381	388	396	rBV	301223	437858	47.44%	5.041%
3	7.104	657	666	678	rBV	291775	466487	50.54%	5.371%
4	7.928	799	806	811	rVB	88911	140080	15.18%	1.613%
5	9.098	998	1005	1016	rBV	184043	297159	32.19%	3.421%
6	10.739	1277	1284	1292	rBV	121562	206665	22.39%	2.379%
7	12.080	1506	1512	1520	rBV	125136	191658	20.76%	2.207%
8	12.374	1559	1562	1569	rVB2	7711	12481	1.35%	0.144%
9	13.198	1696	1702	1706	rBV	448750	669635	72.55%	7.710%
10	13.233	1706	1708	1716	rVB	97780	122020	13.22%	1.405%
11	14.033	1840	1844	1852	rBV2	11384	21814	2.36%	0.251%
12	14.510	1922	1925	1930	rBV	6074	10319	1.12%	0.119%
13	14.580	1931	1937	1944	rVB	187871	283434	30.71%	3.263%
14	14.992	2004	2007	2013	rVB3	11228	14836	1.61%	0.171%
15	15.786	2137	2142	2146	rBV	71945	102237	11.08%	1.177%
16	16.062	2184	2189	2198	rVB	355346	501543	54.34%	5.775%
17	16.357	2234	2239	2248	rVB2	127675	185478	20.09%	2.136%
18	16.704	2294	2298	2310	rVB2	73530	139138	15.07%	1.602%
19	17.315	2396	2402	2412	rBV	210646	317545	34.40%	3.656%
20	17.968	2510	2513	2517	rBV5	8975	12709	1.38%	0.146%
21	18.198	2546	2552	2561	rBV	371943	521370	56.48%	6.003%
22	18.480	2595	2600	2603	rBV	122743	176094	19.08%	2.027%
23	18.521	2603	2607	2619	rVB2	137121	228542	24.76%	2.631%
24	18.945	2675	2679	2691	rVB2	20827	41281	4.47%	0.475%
25	19.321	2739	2743	2744	rBV2	35202	41576	4.50%	0.479%
26	19.345	2744	2747	2757	rVB2	53410	93835	10.17%	1.080%
27	19.462	2762	2767	2784	rVB2	369894	555289	60.16%	6.393%
28	19.715	2808	2810	2816	rVB2	10168	13729	1.49%	0.158%
29	19.915	2839	2844	2849	rVB	767156	923045	100.00%	10.628%
30	20.186	2887	2890	2891	rBV3	11891	12822	1.39%	0.148%
31	20.215	2892	2895	2899	rVB4	17876	22979	2.49%	0.265%
32	20.533	2946	2949	2954	rBV4	15099	18912	2.05%	0.218%
33	20.786	2989	2992	2995	rBV	25287	25817	2.80%	0.297%
34	21.062	3036	3039	3044	rBV2	25905	37430	4.06%	0.431%
35	21.162	3052	3056	3064	rVB	200869	252424	27.35%	2.906%
36	21.233	3065	3068	3072	rVV	20165	22162	2.40%	0.255%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028639.D
Acq On : 03 Feb 2021 12:06
Operator : CG/JU
Sample : M1292-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-010-0205

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.456	3102	3106	3111	rBV	303777	389027	42.15%	4.479%
38	22.050	3204	3207	3216	rVB2	96333	139586	15.12%	1.607%
39	22.727	3319	3322	3329	rVB	34293	47464	5.14%	0.546%
40	23.003	3365	3369	3373	rBV	71070	112823	12.22%	1.299%
41	23.050	3373	3377	3388	rVB2	86858	164971	17.87%	1.899%
42	23.715	3484	3490	3501	rVB2	191958	375994	40.73%	4.329%
43	24.227	3572	3577	3584	rVB	58455	112064	12.14%	1.290%
44	24.315	3587	3592	3602	rVB2	93920	208263	22.56%	2.398%




Sum of corrected areas: 8685378

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028639.D
Acq On : 03 Feb 2021 12:06
Operator : CG/JU
Sample : M1292-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-010-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

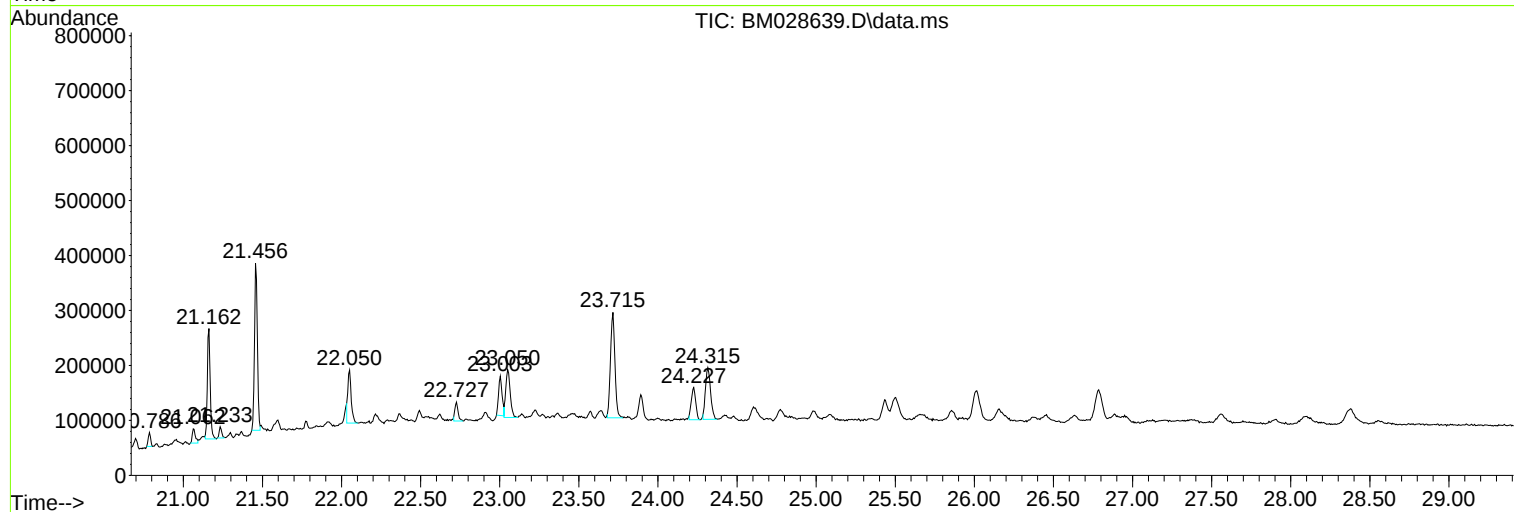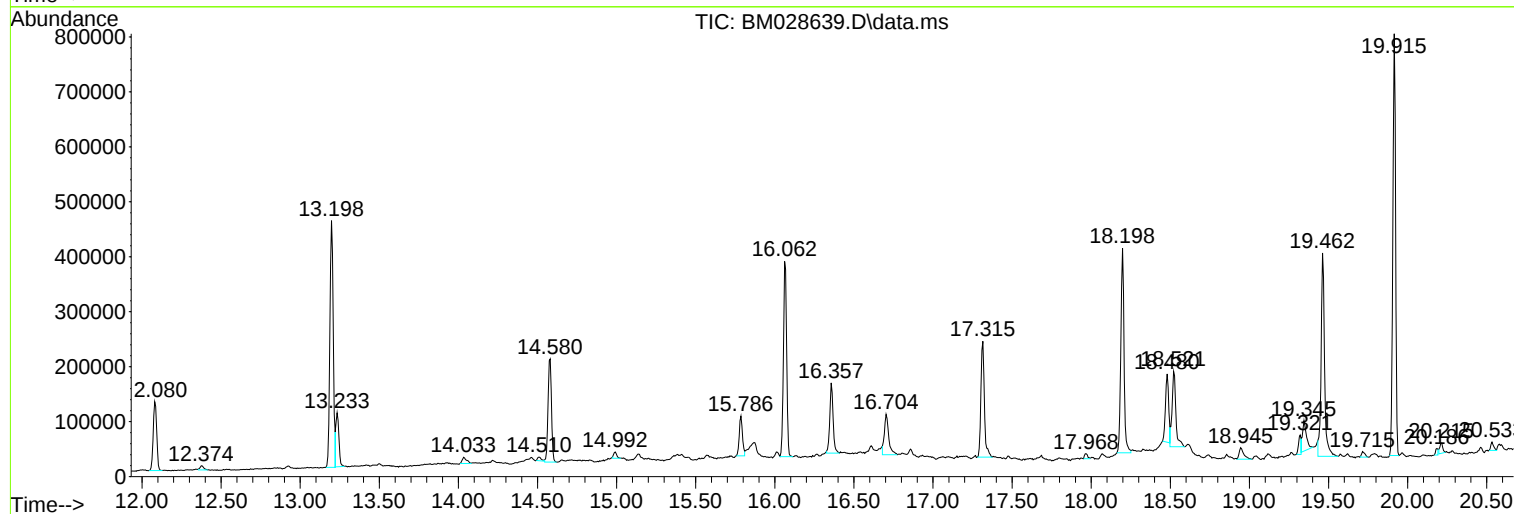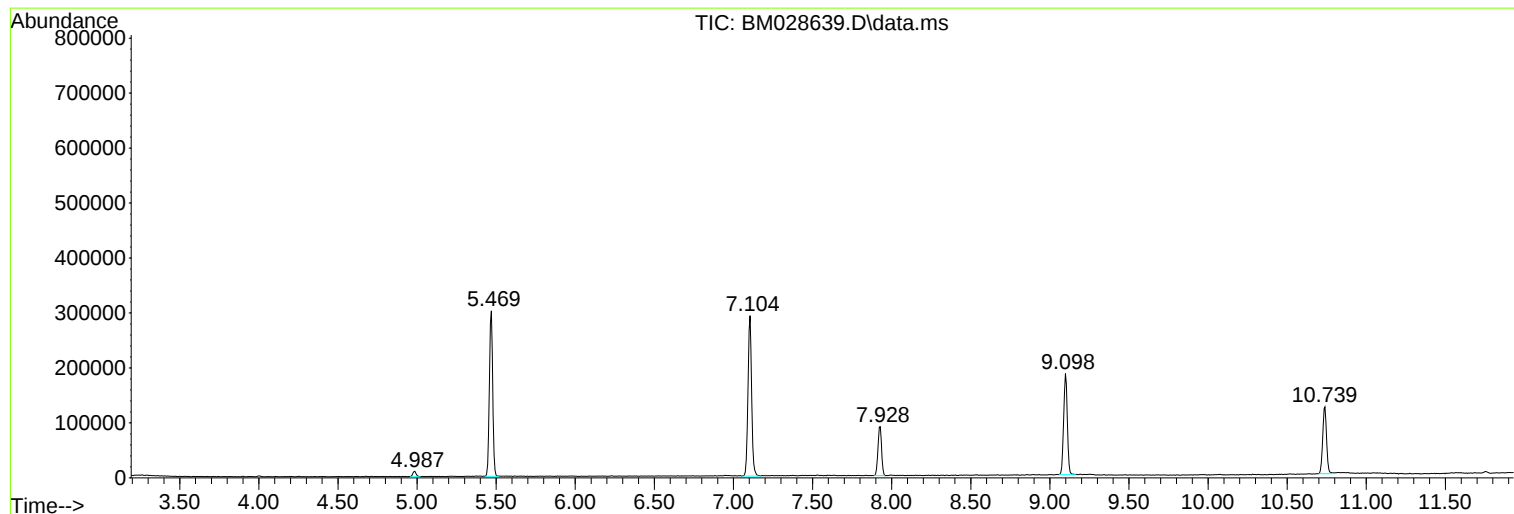

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028639.D
Acq On : 03 Feb 2021 12:06
Operator : CG/JU
Sample : M1292-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-010-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028639.D
Acq On : 03 Feb 2021 12:06
Operator : CG/JU
Sample : M1292-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-010-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------