

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
 Data File : BM028640.D
 Acq On : 03 Feb 2021 12:42
 Operator : CG/JU
 Sample : M1292-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-010-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	302	305	312	rVB	9830	13946	1.23%	0.204%
2	5.463	381	387	395	rBV	385603	572728	50.56%	8.396%
3	7.104	658	666	675	rBV	370202	593538	52.40%	8.701%
4	7.922	799	805	812	rBV	93489	143815	12.70%	2.108%
5	9.098	998	1005	1013	rBV	235429	380872	33.62%	5.583%
6	10.739	1277	1284	1291	rVB	121691	199819	17.64%	2.929%
7	13.198	1694	1702	1713	rVB	577513	825776	72.90%	12.105%
8	14.033	1839	1844	1850	rVB	13000	17473	1.54%	0.256%
9	14.580	1931	1937	1944	rVB	170521	248749	21.96%	3.646%
10	16.062	2184	2189	2197	rBV	429789	609592	53.81%	8.936%
11	17.315	2396	2402	2406	rBV	203740	279812	24.70%	4.102%
12	17.351	2406	2408	2413	rVB	12030	14785	1.31%	0.217%
13	18.192	2546	2551	2565	rBV	189415	272479	24.05%	3.994%
14	19.356	2744	2749	2756	rVB	38032	56667	5.00%	0.831%
15	19.462	2762	2767	2782	rBV	92748	139800	12.34%	2.049%
16	19.721	2807	2811	2818	rVB	29293	42110	3.72%	0.617%
17	19.915	2839	2844	2849	rBV	941548	1132812	100.00%	16.606%
18	20.186	2886	2890	2892	rBV3	10111	14080	1.24%	0.206%
19	20.209	2892	2894	2898	rVB3	12078	15173	1.34%	0.222%
20	20.703	2975	2978	2981	rVB2	15740	17787	1.57%	0.261%
21	21.162	3051	3056	3065	rBV	193895	257642	22.74%	3.777%
22	21.456	3101	3106	3110	rBV	286997	356330	31.46%	5.224%
23	21.591	3127	3129	3136	rVB3	20544	25711	2.27%	0.377%
24	22.050	3201	3207	3215	rVB4	35602	75086	6.63%	1.101%
25	22.621	3301	3304	3309	rVB	28863	39002	3.44%	0.572%
26	23.003	3366	3369	3372	rBV	27575	33808	2.98%	0.496%
27	23.715	3484	3490	3498	rVB	171684	322052	28.43%	4.721%
28	24.315	3588	3592	3602	rVB4	56116	120159	10.61%	1.761%




Sum of corrected areas: 6821603

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028640.D
Acq On : 03 Feb 2021 12:42
Operator : CG/JU
Sample : M1292-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-010-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

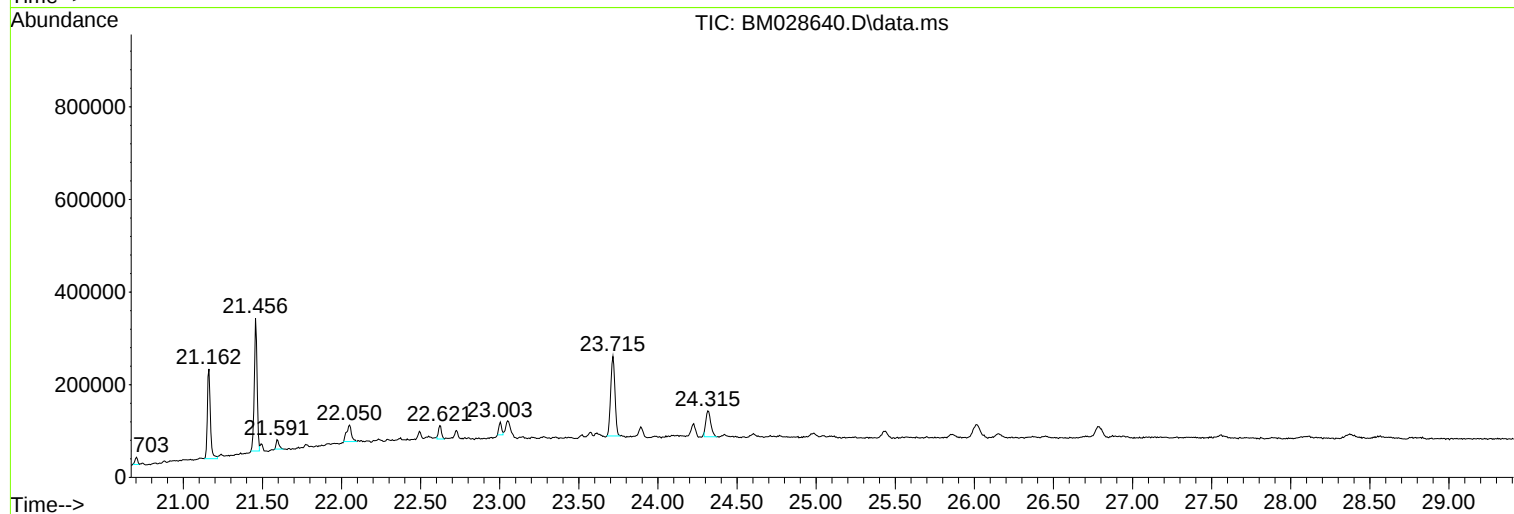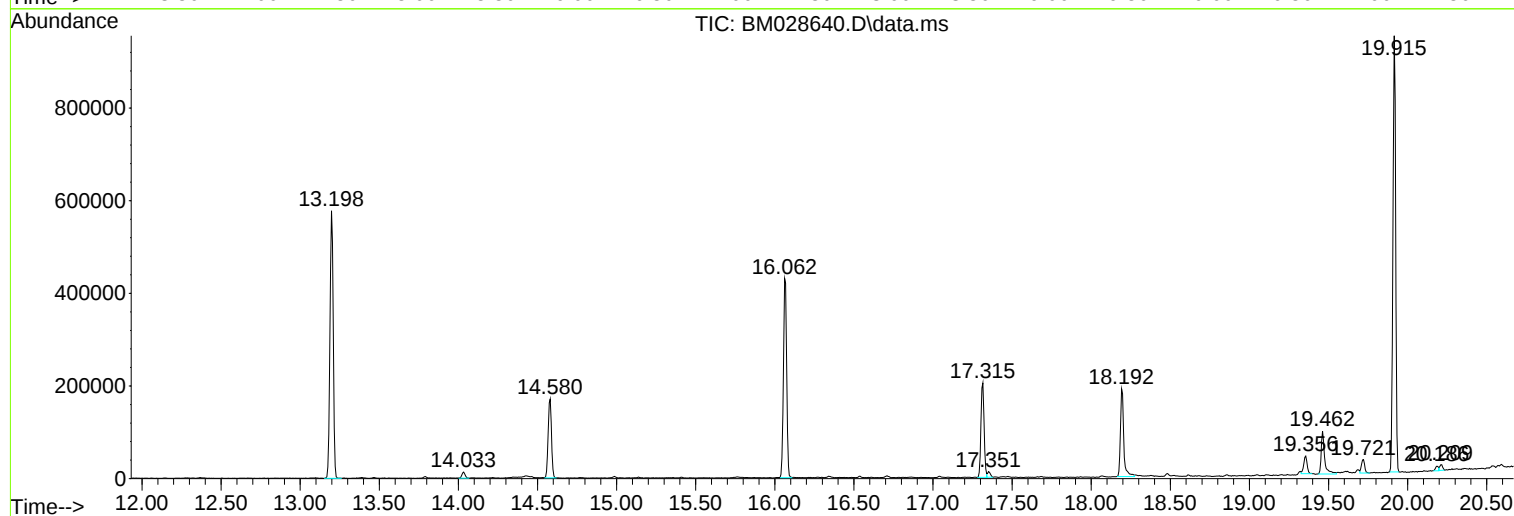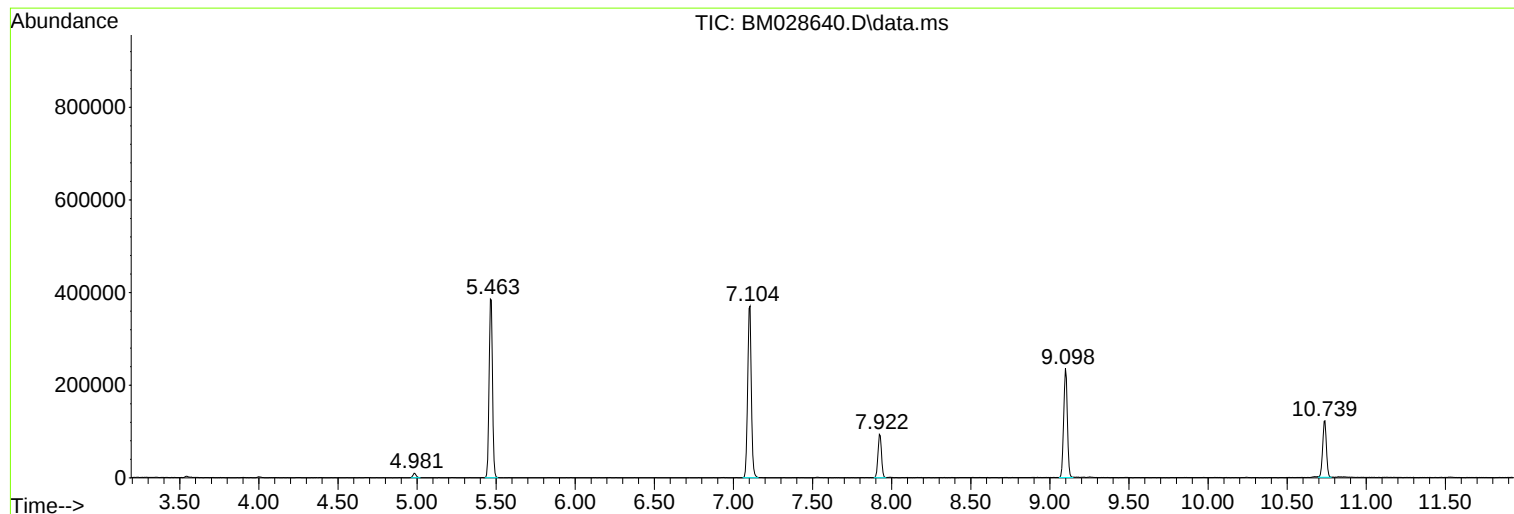

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028640.D
Acq On : 03 Feb 2021 12:42
Operator : CG/JU
Sample : M1292-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-010-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028640.D
Acq On : 03 Feb 2021 12:42
Operator : CG/JU
Sample : M1292-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-010-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------