

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
 Data File : BM028641.D
 Acq On : 03 Feb 2021 13:19
 Operator : CG/JU
 Sample : M1292-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-003-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	302	305	314	rVB	7409	10976	1.07%	0.138%
2	5.463	381	387	395	rBV	402947	588687	57.29%	7.417%
3	7.098	655	665	678	rVB	371502	609968	59.36%	7.685%
4	7.922	797	805	813	rBV	96815	149860	14.58%	1.888%
5	9.098	998	1005	1013	rBV	244391	386570	37.62%	4.870%
6	10.657	1265	1270	1277	rBV5	4265	12930	1.26%	0.163%
7	10.733	1277	1283	1295	rVB	127562	212616	20.69%	2.679%
8	13.198	1696	1702	1709	rVB	572563	803769	78.23%	10.126%
9	14.033	1839	1844	1849	rVB	13445	17068	1.66%	0.215%
10	14.304	1883	1890	1894	rBV	7101	11597	1.13%	0.146%
11	14.427	1901	1911	1916	rBV6	3931	11535	1.12%	0.145%
12	14.574	1931	1936	1944	rBV	180132	264984	25.79%	3.338%
13	16.063	2183	2189	2200	rVB	442235	613727	59.73%	7.732%
14	17.315	2396	2402	2406	rBV	203265	296760	28.88%	3.739%
15	17.351	2406	2408	2413	rVB	27745	32637	3.18%	0.411%
16	18.074	2525	2531	2539	rBV5	6685	13075	1.27%	0.165%
17	18.192	2545	2551	2560	rBV	177069	260052	25.31%	3.276%
18	18.262	2561	2563	2568	rVB	9973	12433	1.21%	0.157%
19	18.374	2577	2582	2586	rBV3	5868	12180	1.19%	0.153%
20	18.486	2597	2601	2605	rBV5	6918	11477	1.12%	0.145%
21	18.727	2638	2642	2646	rBV4	7185	10517	1.02%	0.132%
22	19.356	2744	2749	2755	rVB	88909	129648	12.62%	1.633%
23	19.462	2762	2767	2772	rBV	78172	101771	9.90%	1.282%
24	19.686	2801	2805	2806	rBV	10087	11431	1.11%	0.144%
25	19.715	2806	2810	2818	rVB	74898	104243	10.15%	1.313%
26	19.915	2839	2844	2849	rBV	845752	1027498	100.00%	12.945%
27	20.186	2887	2890	2893	rBV	16610	22136	2.15%	0.279%
28	21.162	3052	3056	3065	rVB	226522	277300	26.99%	3.494%
29	21.456	3101	3106	3110	rBV	301417	420798	40.95%	5.301%
30	22.033	3200	3204	3205	rBV2	50406	66827	6.50%	0.842%
31	22.050	3205	3207	3216	rVB2	108590	140607	13.68%	1.771%
32	23.003	3365	3369	3372	rBV	93608	134854	13.12%	1.699%
33	23.715	3485	3490	3497	rVB2	175109	313539	30.51%	3.950%
34	24.227	3573	3577	3584	rVB	63471	119632	11.64%	1.507%
35	24.321	3588	3593	3601	rVB	93098	199992	19.46%	2.520%
36	26.015	3875	3881	3893	rVB4	88110	262146	25.51%	3.303%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028641.D
Acq On : 03 Feb 2021 13:19
Operator : CG/JU
Sample : M1292-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-003-0002

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	26.791	4007	4013	4025	rVB3	86645	261568	25.46%	3.295%
----	--------	------	------	------	------	-------	--------	--------	--------




Sum of corrected areas: 7937408

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028641.D
Acq On : 03 Feb 2021 13:19
Operator : CG/JU
Sample : M1292-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-003-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

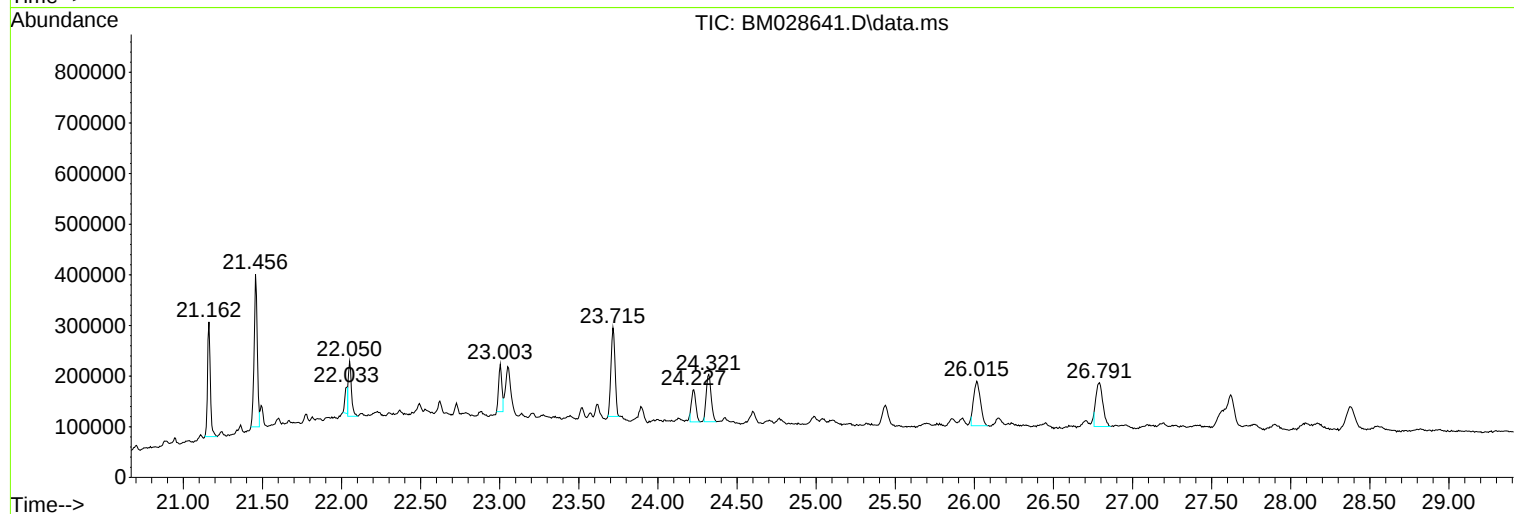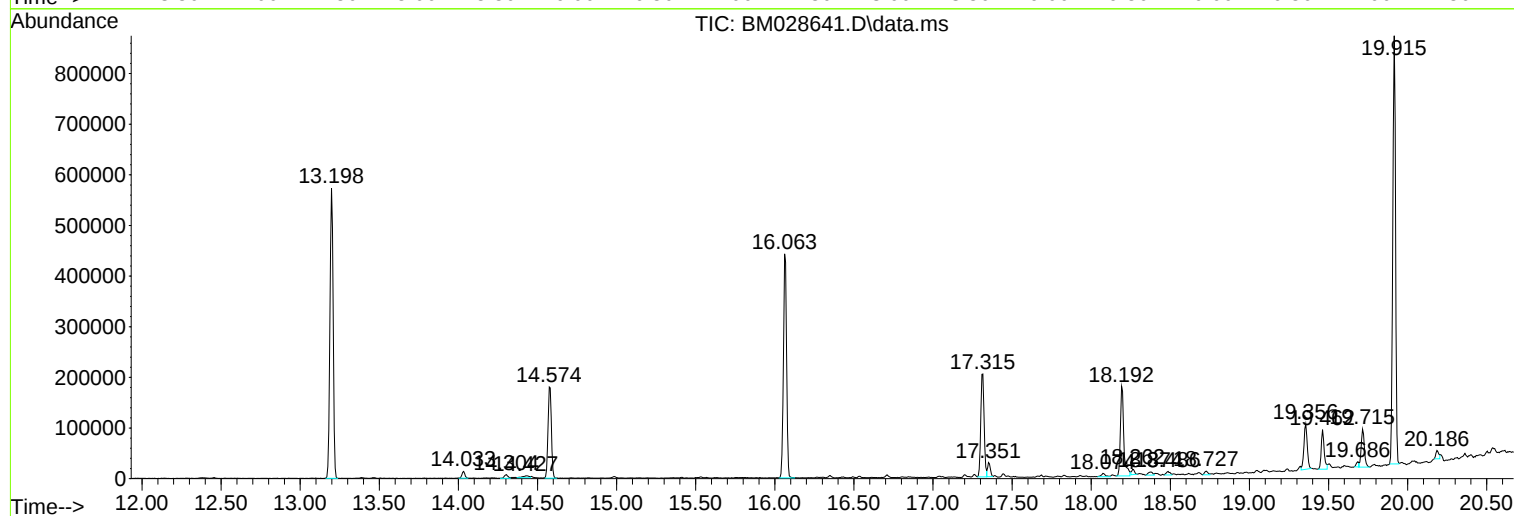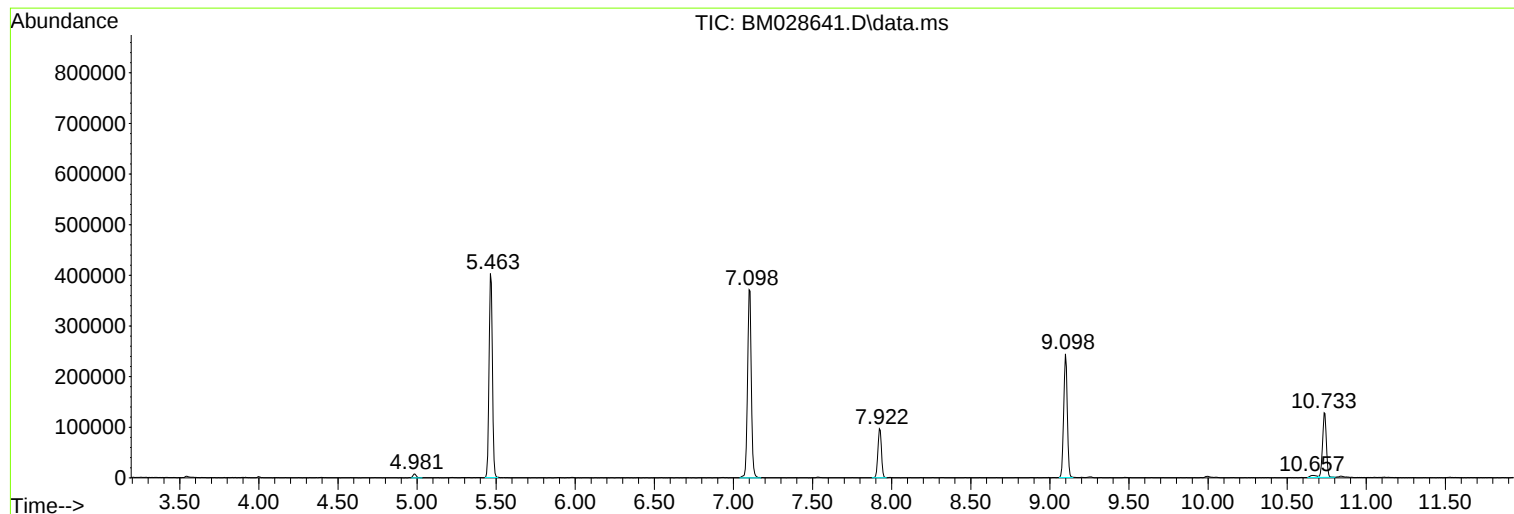

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028641.D
Acq On : 03 Feb 2021 13:19
Operator : CG/JU
Sample : M1292-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-003-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028641.D
Acq On : 03 Feb 2021 13:19
Operator : CG/JU
Sample : M1292-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-003-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------