

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
 Data File : BM028642.D
 Acq On : 03 Feb 2021 13:55
 Operator : CG/JU
 Sample : M1292-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-005-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	381	387	396	rBV	426153	620004	56.34%	10.177%
2	7.098	658	665	678	rBV	398440	639502	58.11%	10.497%
3	7.922	800	805	812	rBV	94370	141587	12.87%	2.324%
4	9.098	996	1005	1017	rBV	253205	405067	36.81%	6.649%
5	10.734	1277	1283	1290	rVB	119271	194843	17.71%	3.198%
6	13.198	1695	1702	1708	rBV	606345	836124	75.98%	13.725%
7	13.463	1742	1747	1753	rBV	22084	31254	2.84%	0.513%
8	14.033	1838	1844	1851	rVB	25656	32838	2.98%	0.539%
9	14.427	1904	1911	1925	rVB5	3867	11795	1.07%	0.194%
10	14.580	1931	1937	1943	rVB	167417	243828	22.16%	4.002%
11	15.686	2120	2125	2132	rBV	9737	12348	1.12%	0.203%
12	16.063	2183	2189	2197	rBV	457942	630148	57.26%	10.344%
13	17.310	2396	2401	2408	rBV	191419	270669	24.60%	4.443%
14	18.192	2546	2551	2561	rBV	98701	134486	12.22%	2.208%
15	19.462	2762	2767	2774	rBV	44241	65523	5.95%	1.076%
16	19.915	2838	2844	2849	rBV	919359	1100455	100.00%	18.064%
17	21.162	3052	3056	3061	rBV	67644	85074	7.73%	1.396%
18	21.456	3101	3106	3115	rBV	254634	317564	28.86%	5.213%
19	23.715	3484	3490	3499	rVB2	172400	318949	28.98%	5.235%




Sum of corrected areas: 6092058

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028642.D
Acq On : 03 Feb 2021 13:55
Operator : CG/JU
Sample : M1292-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

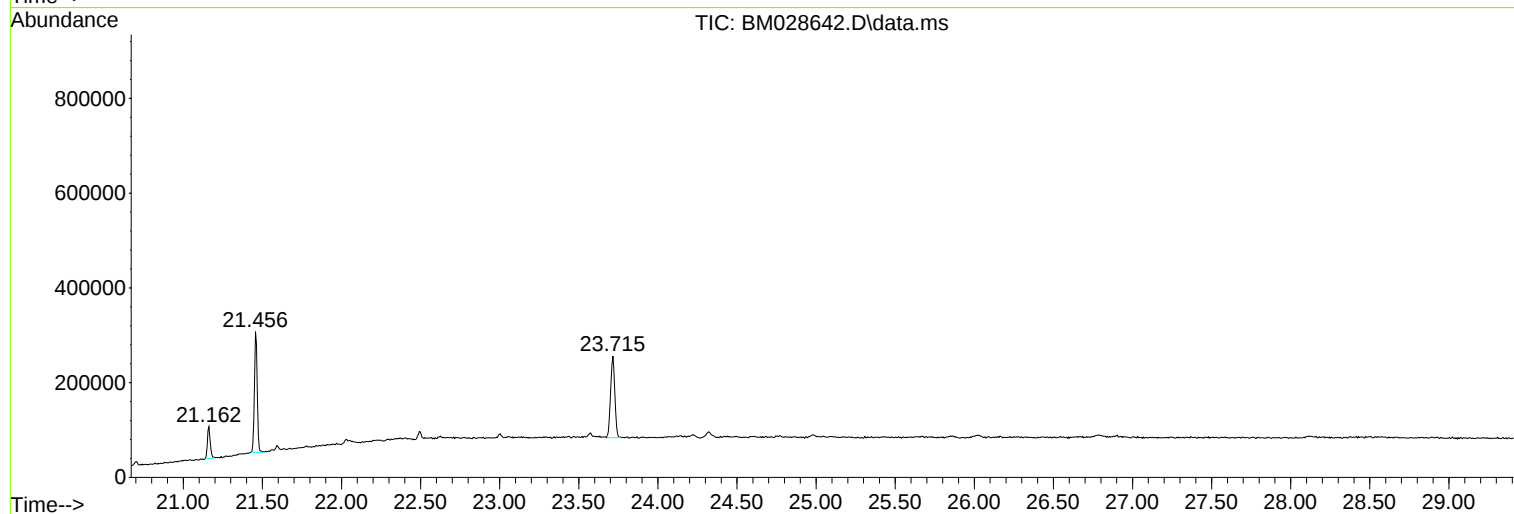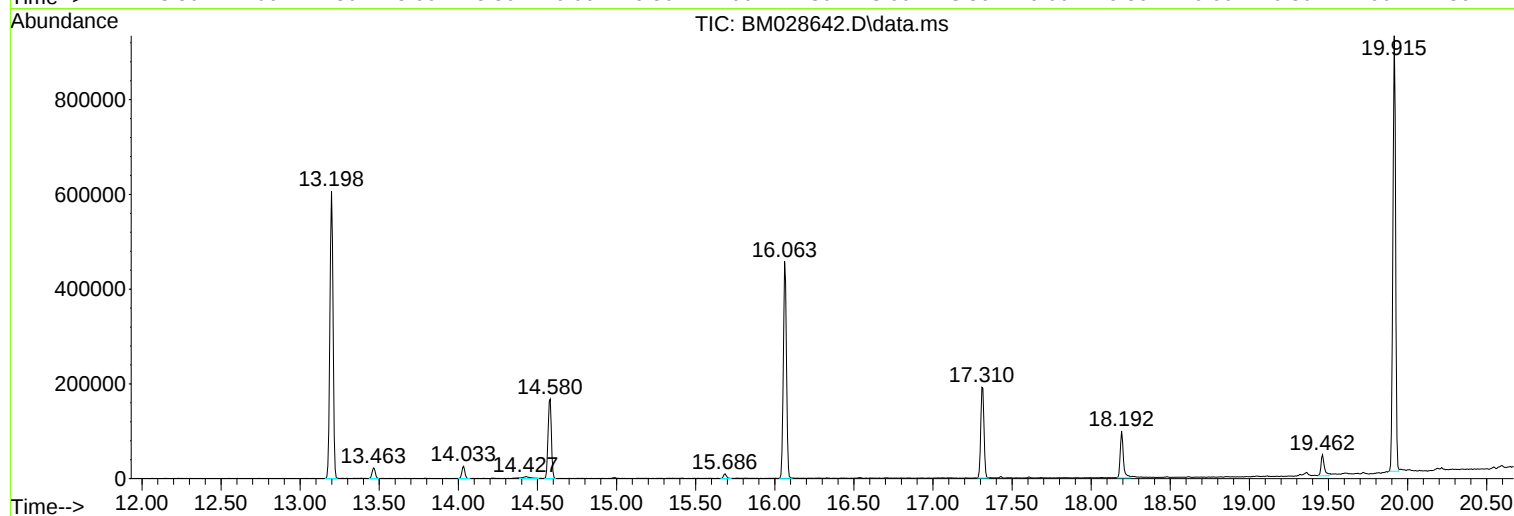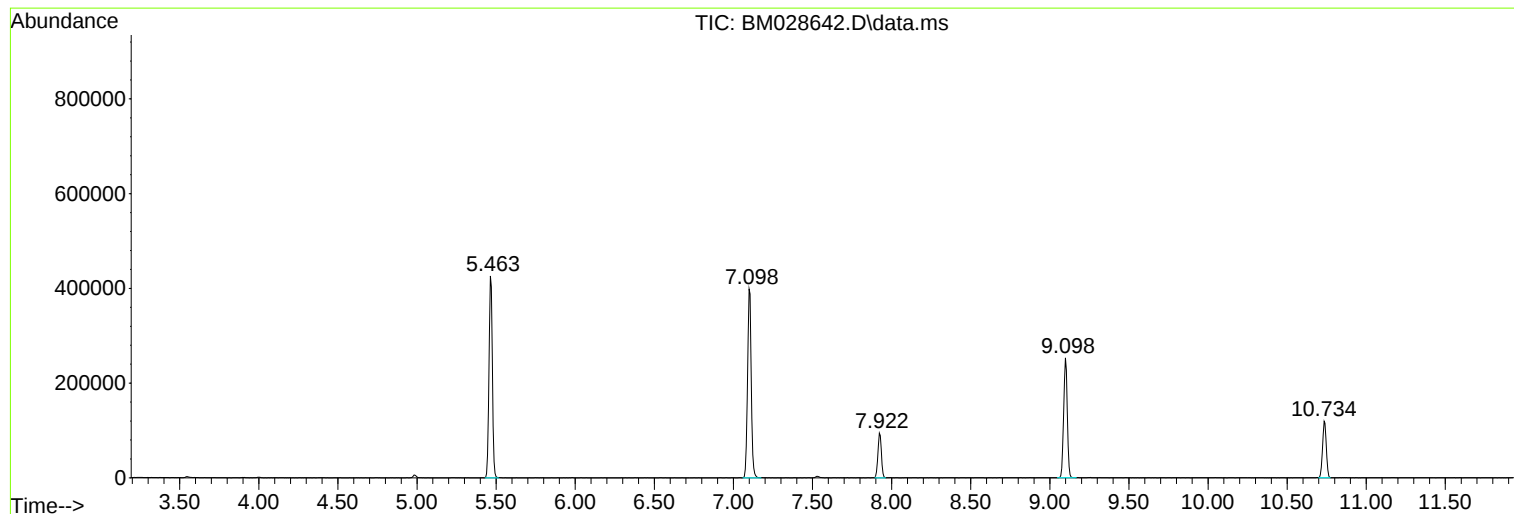

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028642.D
Acq On : 03 Feb 2021 13:55
Operator : CG/JU
Sample : M1292-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028642.D
Acq On : 03 Feb 2021 13:55
Operator : CG/JU
Sample : M1292-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------