

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
 Data File : BM028643.D
 Acq On : 03 Feb 2021 14:32
 Operator : CG/JU
 Sample : M1292-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-005-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	381	387	395	rBV	360333	533241	55.86%	5.643%
2	7.099	659	665	676	rVB	343512	549515	57.57%	5.815%
3	7.922	800	805	812	rVB	92896	143339	15.02%	1.517%
4	9.098	998	1005	1011	rBV	213886	345806	36.23%	3.660%
5	10.692	1265	1276	1278	rBV6	6230	15230	1.60%	0.161%
6	10.734	1278	1283	1289	rVB	119331	195391	20.47%	2.068%
7	10.881	1303	1308	1314	rVB2	7969	13152	1.38%	0.139%
8	11.569	1420	1425	1432	rVB	14965	22722	2.38%	0.240%
9	13.198	1695	1702	1709	rBV	483891	683638	71.62%	7.235%
10	13.463	1742	1747	1753	rVB	21425	30567	3.20%	0.323%
11	14.033	1839	1844	1851	rBV	8336	10913	1.14%	0.115%
12	14.575	1931	1936	1944	rVB2	156993	236042	24.73%	2.498%
13	15.139	2025	2032	2039	rBV2	11551	20244	2.12%	0.214%
14	15.810	2141	2146	2154	rVB	19653	28056	2.94%	0.297%
15	16.063	2183	2189	2195	rBV	371269	510920	53.52%	5.407%
16	16.163	2201	2206	2217	rVB	24711	36058	3.78%	0.382%
17	16.269	2217	2224	2232	rBV5	5820	12009	1.26%	0.127%
18	17.310	2396	2401	2406	rBV	186755	263626	27.62%	2.790%
19	17.921	2501	2505	2510	rVB	11889	16955	1.78%	0.179%
20	18.198	2546	2552	2561	rBV	244327	347616	36.42%	3.679%
21	18.427	2586	2591	2595	rVB6	5936	9995	1.05%	0.106%
22	18.480	2595	2600	2606	rBV	98963	131583	13.78%	1.392%
23	18.692	2631	2636	2642	rBV	200132	267201	27.99%	2.828%
24	18.804	2651	2655	2662	rVB	25113	32715	3.43%	0.346%
25	18.915	2670	2674	2680	rVB5	19471	27912	2.92%	0.295%
26	18.986	2682	2686	2691	rVB5	8258	12283	1.29%	0.130%
27	19.063	2694	2699	2702	rBV	58944	84559	8.86%	0.895%
28	19.104	2702	2706	2714	rVV	114496	174819	18.31%	1.850%
29	19.233	2723	2728	2733	rBV6	9226	15920	1.67%	0.168%
30	19.351	2743	2748	2749	rBV4	46279	61276	6.42%	0.648%
31	19.404	2755	2757	2760	rVB	13226	13397	1.40%	0.142%
32	19.468	2763	2768	2771	rBV	191238	252940	26.50%	2.677%
33	19.498	2771	2773	2781	rVB2	50552	85599	8.97%	0.906%
34	19.592	2786	2789	2792	rVV4	21640	25609	2.68%	0.271%
35	19.621	2792	2794	2797	rVB	11238	10750	1.13%	0.114%
36	19.721	2808	2811	2818	rVB2	15102	26249	2.75%	0.278%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
 Data File : BM028643.D
 Acq On : 03 Feb 2021 14:32
 Operator : CG/JU
 Sample : M1292-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-005-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.815	2825	2827	2834	rVB6	12270	17391	1.82%	0.184%
38	19.915	2839	2844	2857	rVB	800454	954575	100.00%	10.102%
39	20.057	2866	2868	2873	rVB6	9260	10418	1.09%	0.110%
40	20.127	2876	2880	2884	rVB	34328	42641	4.47%	0.451%
41	20.192	2888	2891	2894	rBV4	21596	27981	2.93%	0.296%
42	20.398	2922	2926	2930	rVB	68133	76153	7.98%	0.806%
43	20.468	2935	2938	2941	rVB2	27519	31411	3.29%	0.332%
44	20.633	2963	2966	2973	rVB2	33311	53450	5.60%	0.566%
45	20.704	2975	2978	2984	rVB	28328	35789	3.75%	0.379%
46	20.927	3012	3016	3021	rVB	172259	199045	20.85%	2.106%
47	20.992	3024	3027	3030	rBV2	35361	41032	4.30%	0.434%
48	21.080	3039	3042	3047	rBV	42594	68792	7.21%	0.728%
49	21.162	3052	3056	3059	rBV3	163267	198734	20.82%	2.103%
50	21.262	3070	3073	3077	rVB	80167	90432	9.47%	0.957%
51	21.351	3086	3088	3092	rVB4	27232	29766	3.12%	0.315%
52	21.462	3102	3107	3115	rVB	278159	515133	53.96%	5.451%
53	21.845	3168	3172	3178	rVB	269340	335714	35.17%	3.553%
54	21.915	3180	3184	3189	rVV	254949	307688	32.23%	3.256%
55	22.221	3233	3236	3241	rBV	54659	69249	7.25%	0.733%
56	22.486	3276	3281	3286	rBV3	140408	212913	22.30%	2.253%
57	22.933	3353	3357	3363	rVB	199505	301421	31.58%	3.190%
58	23.715	3485	3490	3499	rVB2	168014	323739	33.91%	3.426%
59	24.315	3587	3592	3602	rVB2	119278	258155	27.04%	2.732%




Sum of corrected areas: 9449469

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028643.D
Acq On : 03 Feb 2021 14:32
Operator : CG/JU
Sample : M1292-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

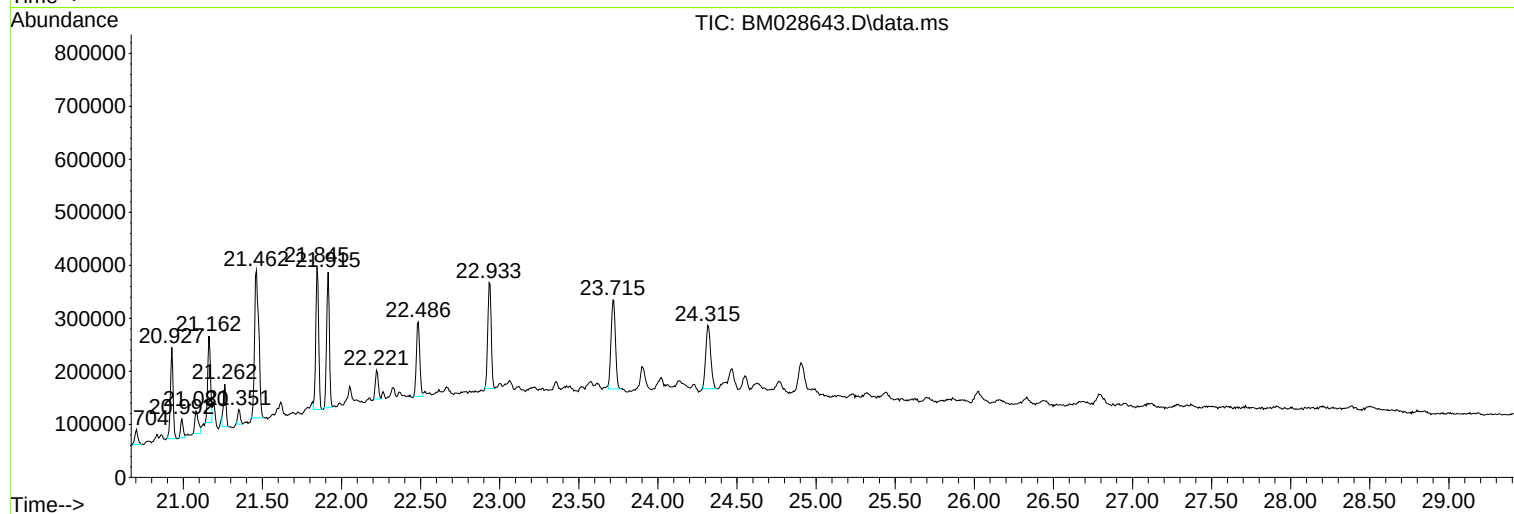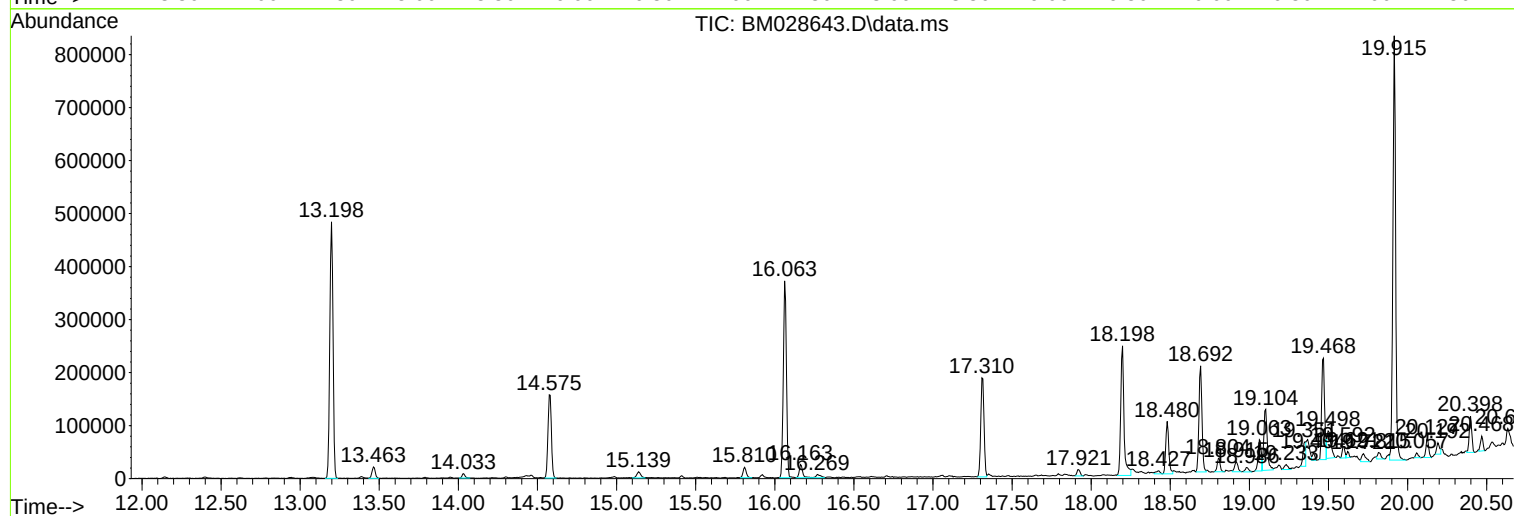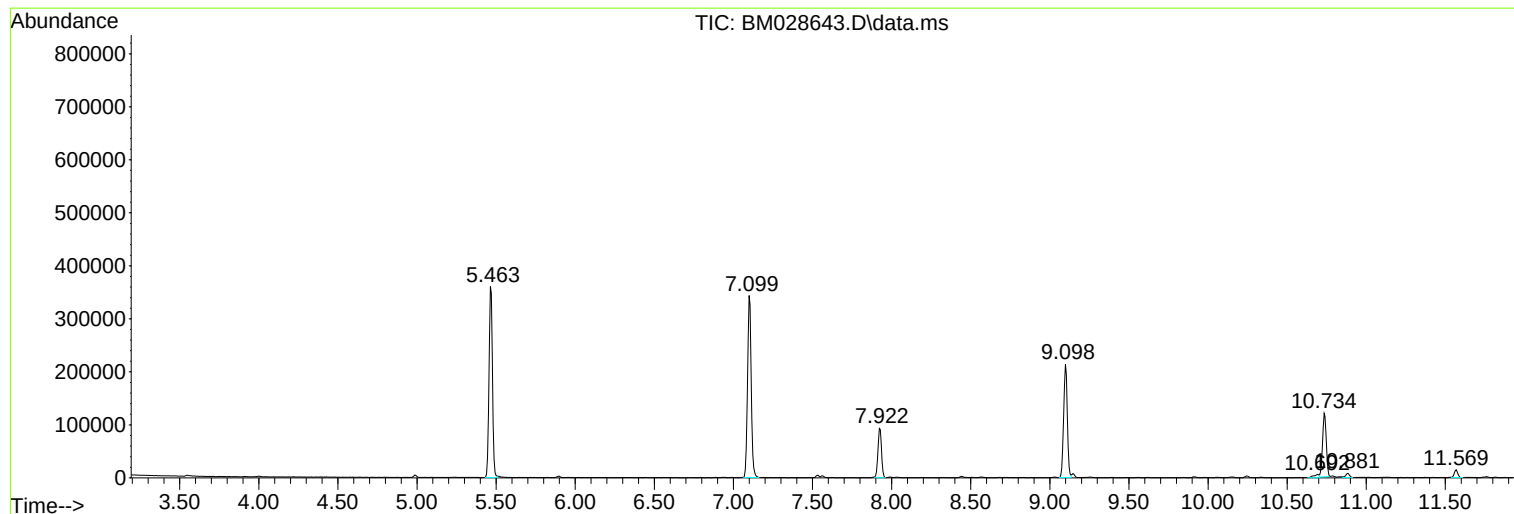

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028643.D
Acq On : 03 Feb 2021 14:32
Operator : CG/JU
Sample : M1292-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028643.D
Acq On : 03 Feb 2021 14:32
Operator : CG/JU
Sample : M1292-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------