


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
 Data File : BM028636.D
 Acq On : 03 Feb 2021 09:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 16:19:07 2021

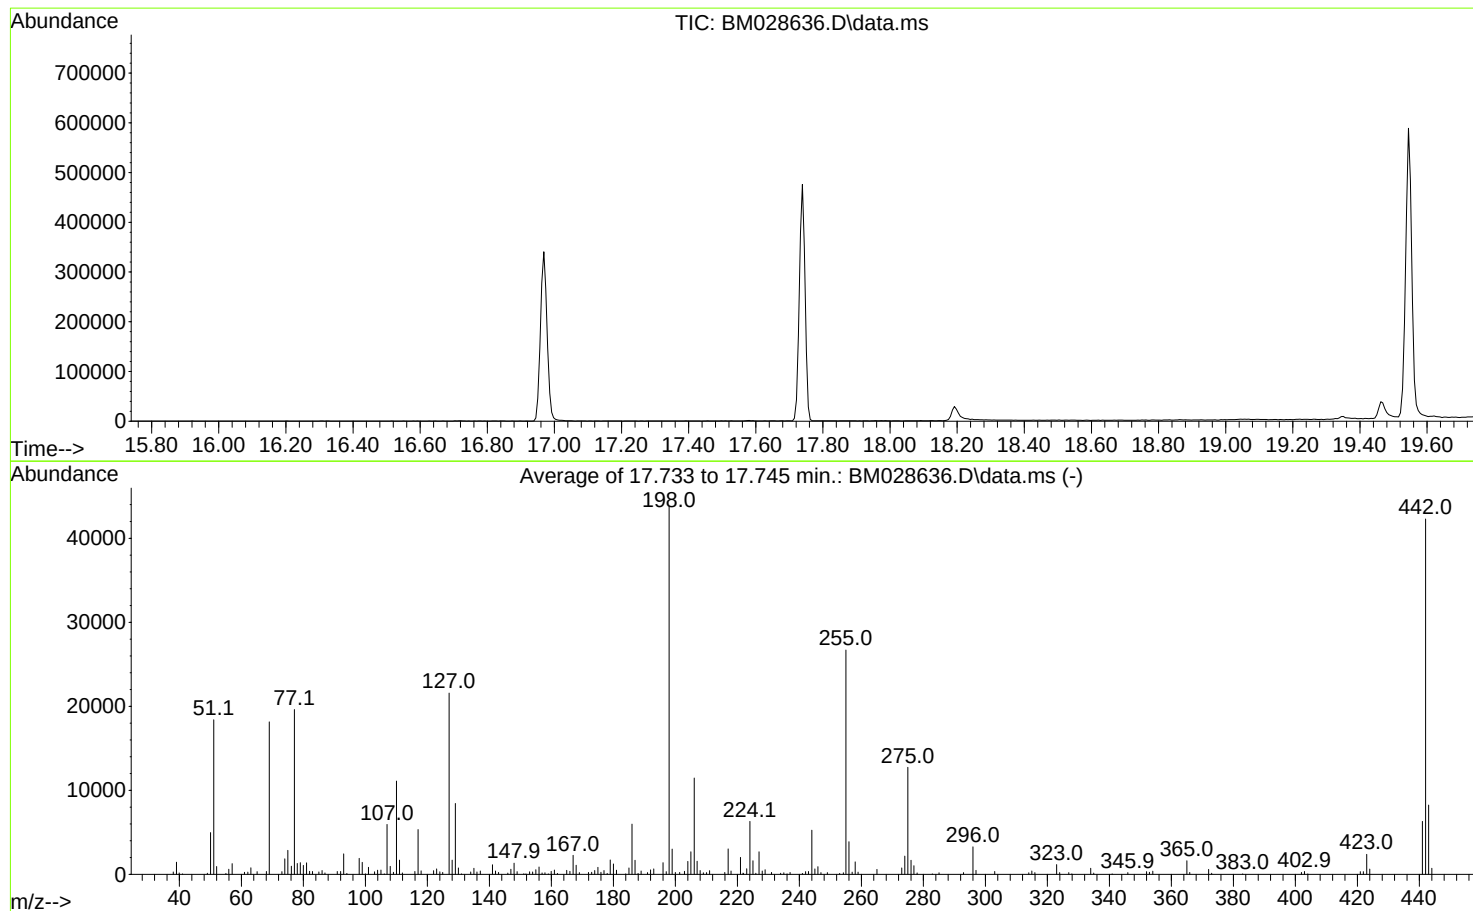

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	18393	PASS
68	69	0.00	2	1.9	341	PASS
69	198	0.00	100	41.4	18140	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	21584	PASS
197	198	0.00	2	0.7	321	PASS
198	198	100	100	100.0	43781	PASS
199	198	5	9	6.9	3013	PASS
275	198	10	60	29.1	12737	PASS
365	198	1	100	3.7	1621	PASS
441	198	0.01	100	14.4	6296	PASS
442	442	50	100	100.0	42291	PASS
443	442	15	24	19.5	8254	PASS

Instrument :
BNA_M
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/3/2021	BNA_M	<u>BM028636.D</u>
Compound Name	Response	Retention Time
DDT	169195	20.762
DDD	4865	20.327
DDE	309	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5174	174369	2.97

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028636.D
Acq On : 03 Feb 2021 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 04 01:24:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

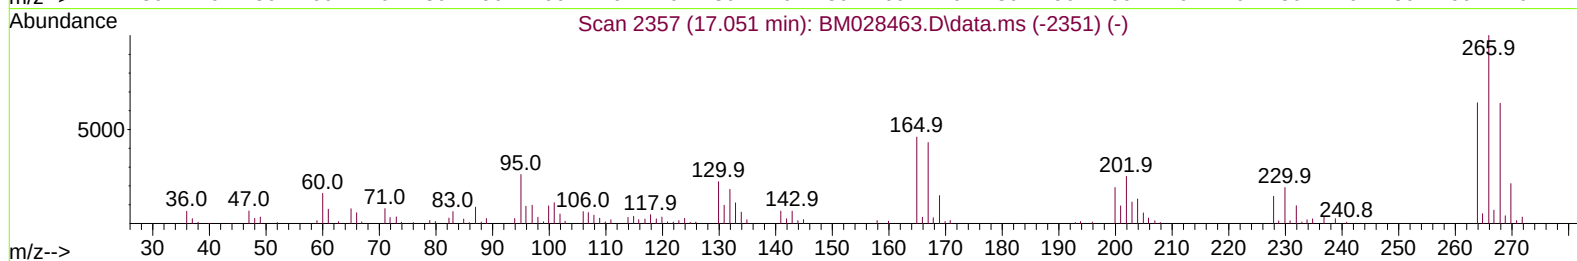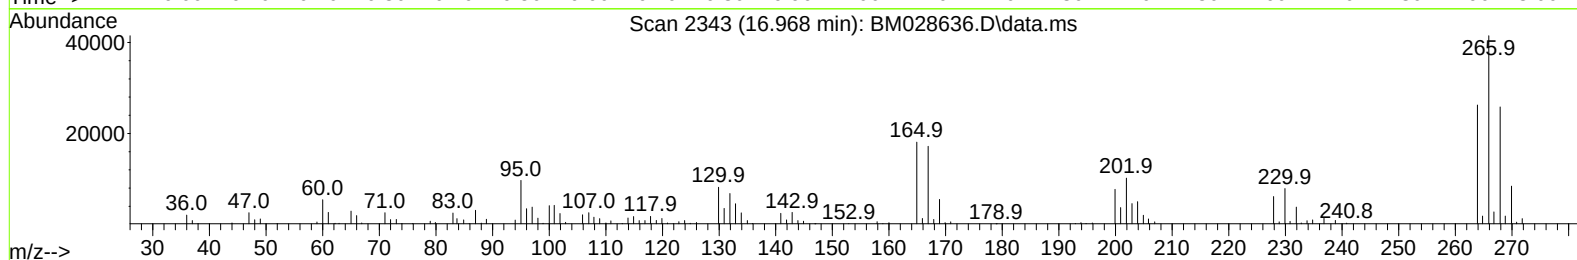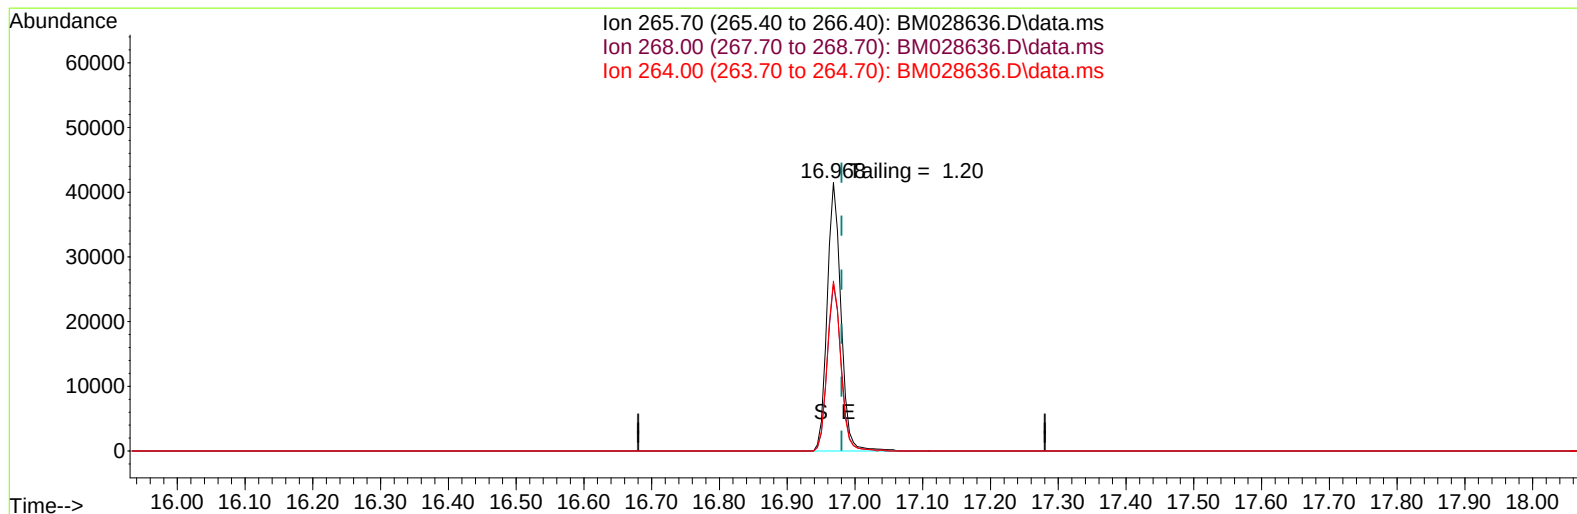

TIC: BM028636.D\data.ms

(70) Pentachlorophenol (C)

16.968min (-0.012) 0.00 ng




response 58352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.26
264.00	63.30	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020321\
Data File : BM028636.D
Acq On : 03 Feb 2021 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 04 01:24:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

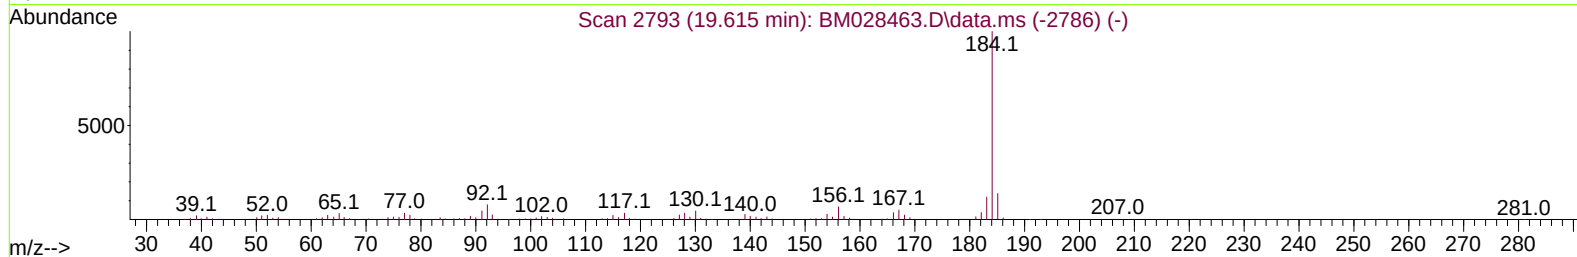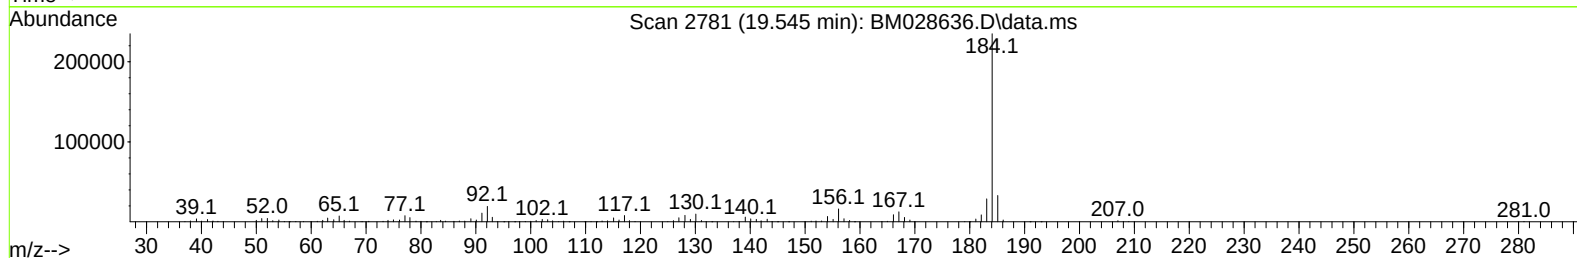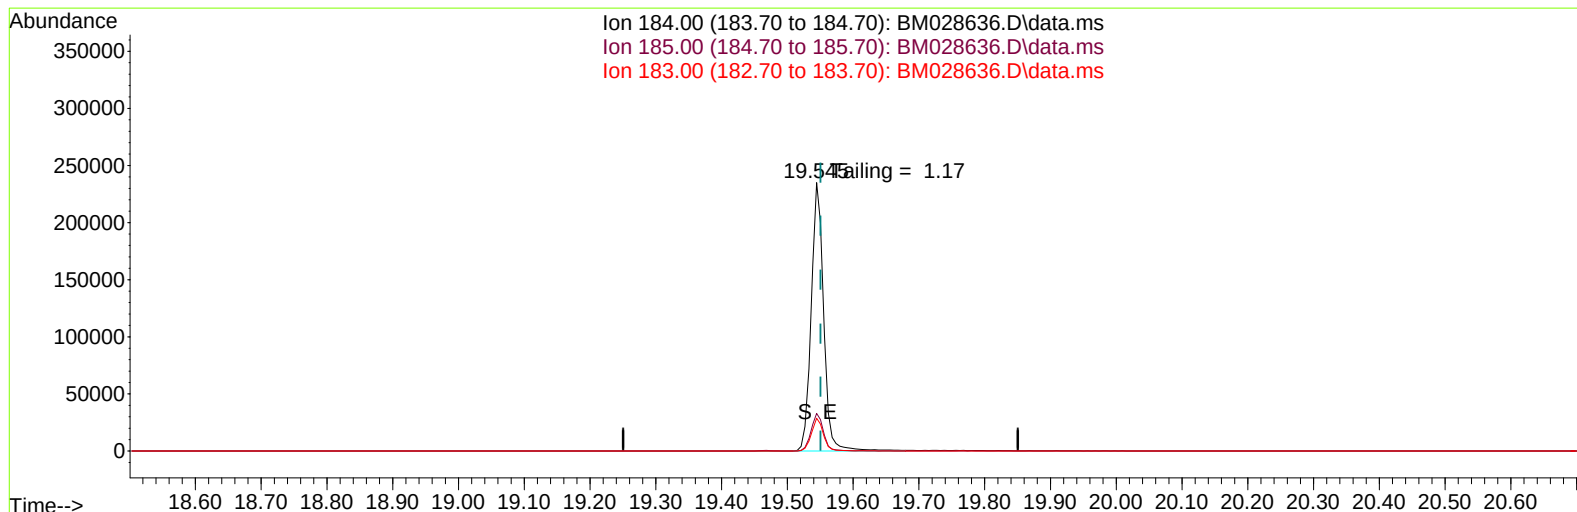

TIC: BM028636.D\data.ms

(77) Benzidine

19.545min (-0.006) 250751.91 ng

response 310136

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.01
183.00	12.10	12.25
0.00	0.00	0.00