




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034009.D
 Acq On : 03 Feb 2022 19:23
 Operator : CG/JU
 Sample : N1365-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGLZ1

Manual IntegrationsAPPROVED

Quant Time: Feb 04 00:08:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :mohammad ahmed 02/04/2022

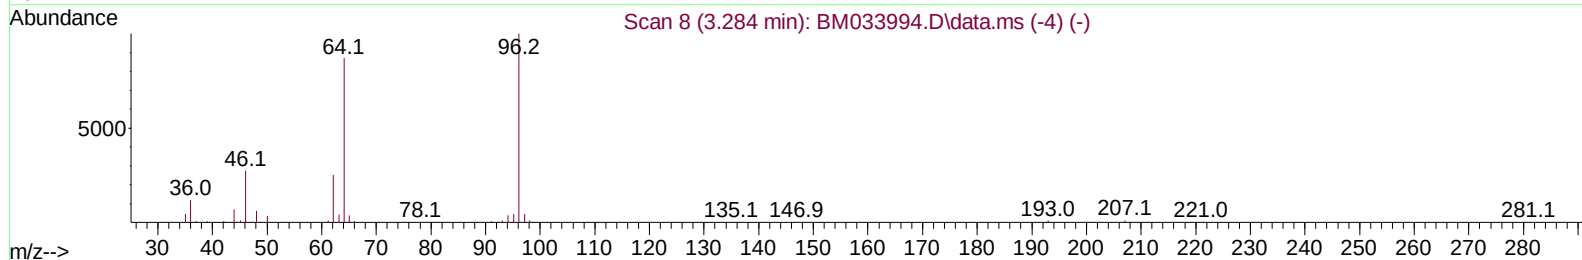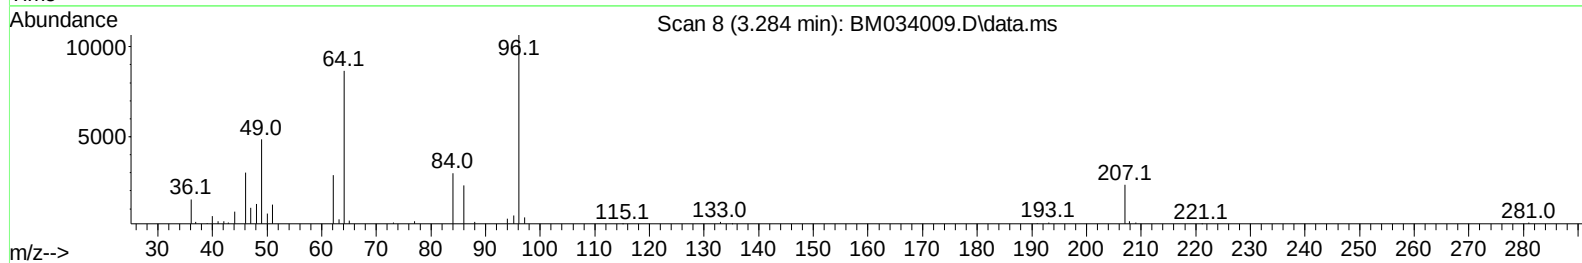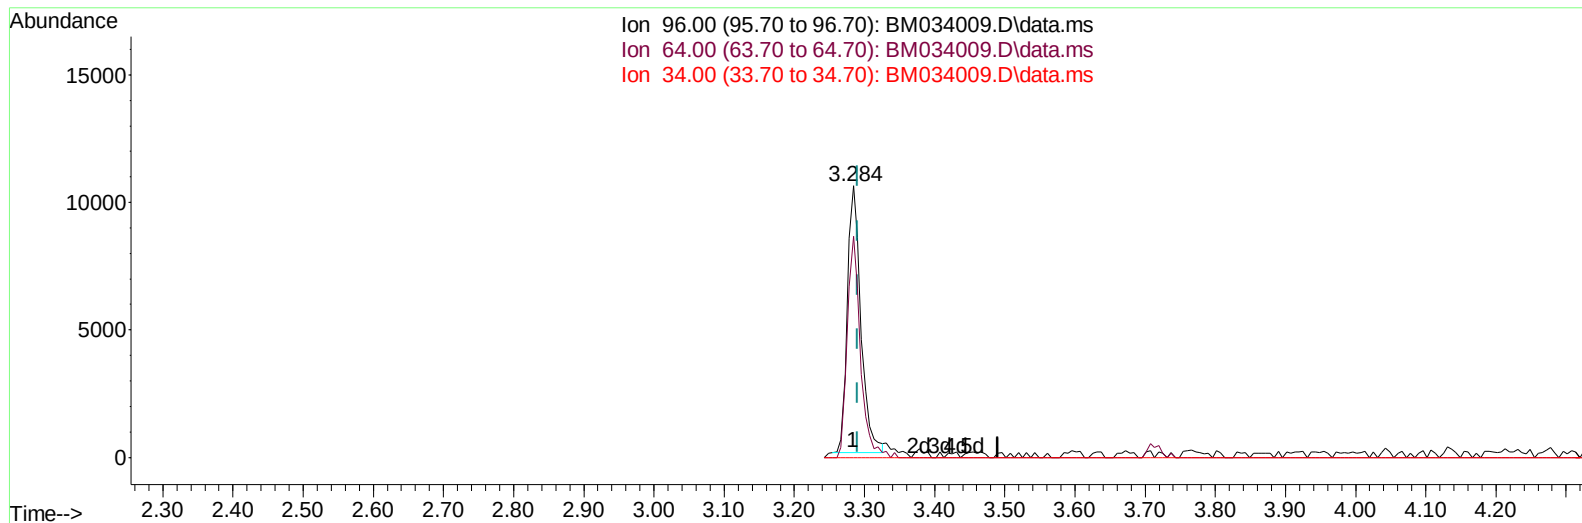

TIC: BM034009.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.284min (-0.006) 5.16 ng/uL

response 14088

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	81.48
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034009.D
 Acq On : 03 Feb 2022 19:23
 Operator : CG/JU
 Sample : N1365-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGLZ1

Manual IntegrationsAPPROVED

Quant Time: Feb 04 00:08:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :mohammad ahmed 02/04/2022

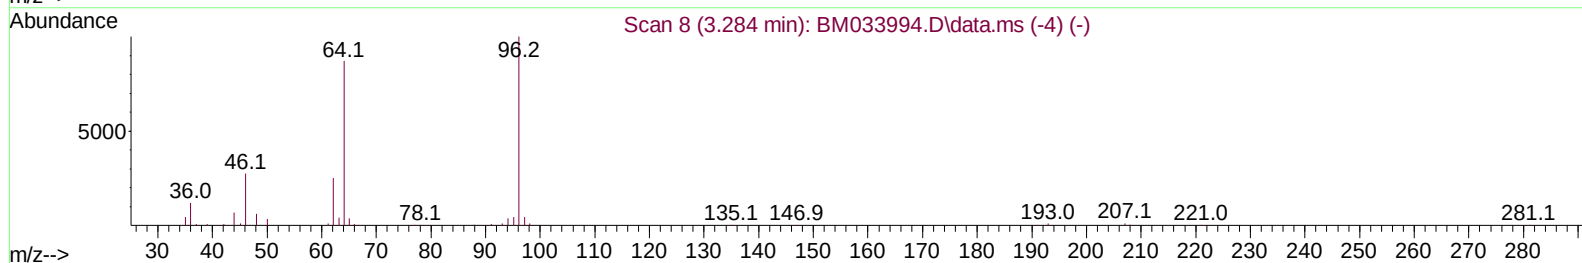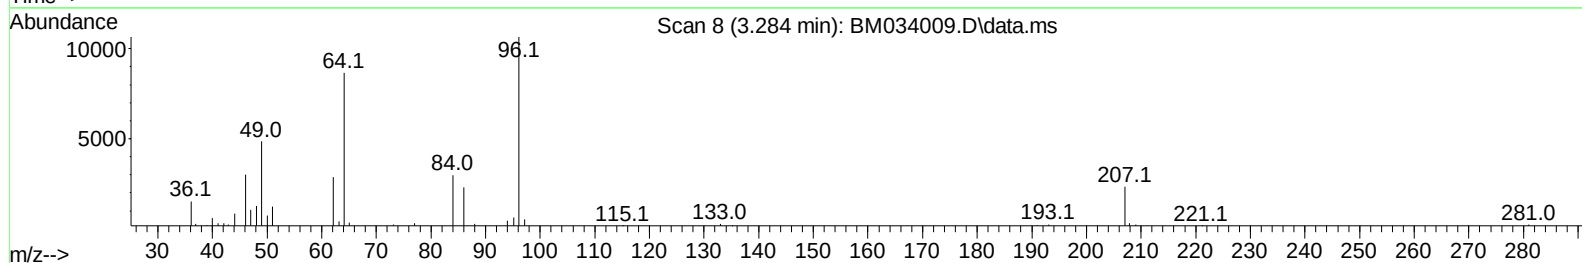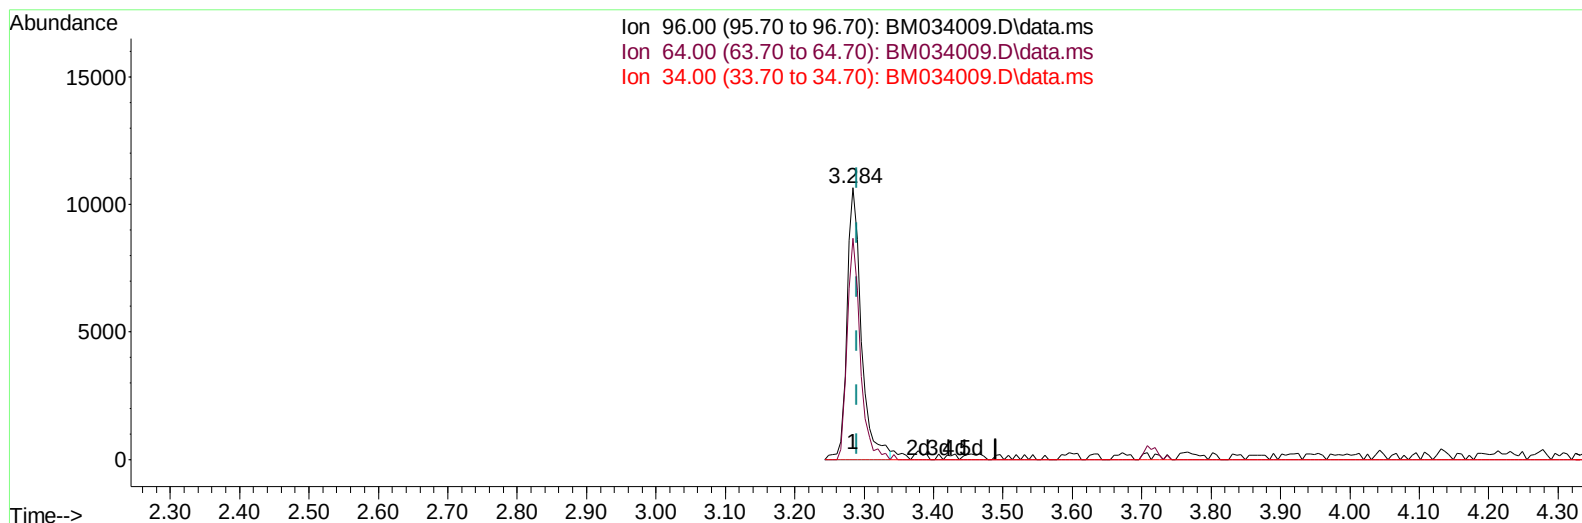

TIC: BM034009.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.284min (-0.006) 5.63 ng/uL m

response 15379

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	81.48
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034009.D
 Acq On : 03 Feb 2022 19:23
 Operator : CG/JU
 Sample : N1365-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGLZ1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :mohammad ahmed 02/04/2022

Quant Time: Feb 04 00:08:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	107679	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.731	136	473853	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.560	164	312804	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.295	188	633295	20.000	ng/ul	-0.01
79) Chrysene-d12	21.459	240	524011	20.000	ng/ul	0.00
88) Perylene-d12	23.847	264	463665	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	15379m	5.633	ng/uL	0.00
4) Pyridine-d5	3.713	84	211046	27.694	ng/ul	0.00
7) Phenol-d5	7.078	99	305443	33.859	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.243	67	190718	34.678	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.449	132	244402	33.816	ng/ul	-0.01
15) 4-Methylphenol-d8	8.631	113	260717	36.473	ng/ul	-0.01
21) Nitrobenzene-d5	9.084	128	130372	34.289	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.807	143	142097	34.608	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.348	165	249411	33.567	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.866	131	368814	35.945	ng/ul	0.00
46) Dimethylphthalate-d6	13.966	166	918399	39.290	ng/ul	-0.01
49) Acenaphthylene-d8	14.254	160	1048765	36.626	ng/ul	0.00
54) 4-Nitrophenol-d4	14.742	143	123715	30.979	ng/ul	-0.01
60) Fluorene-d10	15.548	176	749108	38.381	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.660	200	113646	28.584	ng/ul	-0.01
73) Anthracene-d10	17.395	188	1151142	37.956	ng/ul	0.00
81) Pyrene-d10	19.677	212	1239346	40.061	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.695	264	931584	38.253	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.107	94	13685	1.479	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034009.D
Acq On : 03 Feb 2022 19:23
Operator : CG/JU
Sample : N1365-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGLZ1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :mohammad ahmed 02/04/2022

Quant Time: Feb 04 00:08:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

