

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034006.D
 Acq On : 03 Feb 2022 17:35
 Operator : CG/JU
 Sample : N1365-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGLZ4

Quant Time: Feb 04 00:07:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	111175	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.731	136	476489	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.560	164	316358	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.295	188	641487	20.000	ng/u1	-0.01
79) Chrysene-d12	21.459	240	515194	20.000	ng/u1	0.00
88) Perylene-d12	23.848	264	464283	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	12780	4.534	ng/uL	0.00
4) Pyridine-d5	3.714	84	136577	17.358	ng/u1	0.00
7) Phenol-d5	7.078	99	229120	24.600	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.243	67	145002	25.536	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.449	132	185461	24.854	ng/u1	-0.01
15) 4-Methylphenol-d8	8.631	113	189889	25.729	ng/u1	-0.01
21) Nitrobenzene-d5	9.084	128	95354	24.940	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.807	143	103772	25.134	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.348	165	179184	23.982	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.866	131	265260	25.710	ng/u1	0.00
46) Dimethylphthalate-d6	13.966	166	659880	27.913	ng/u1	-0.01
49) Acenaphthylene-d8	14.254	160	760660	26.266	ng/u1	0.00
54) 4-Nitrophenol-d4	14.748	143	80379	19.901	ng/u1	0.00
60) Fluorene-d10	15.548	176	539642	27.338	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.660	200	77666	19.285	ng/u1	-0.01
73) Anthracene-d10	17.395	188	826129	26.891	ng/u1	0.00
81) Pyrene-d10	19.677	212	897261	29.500	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.695	264	663290	27.200	ng/u1	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.107	94	14964	1.567	ng/u1#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034006.D
Acq On : 03 Feb 2022 17:35
Operator : CG/JU
Sample : N1365-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGLZ4

Quant Time: Feb 04 00:07:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

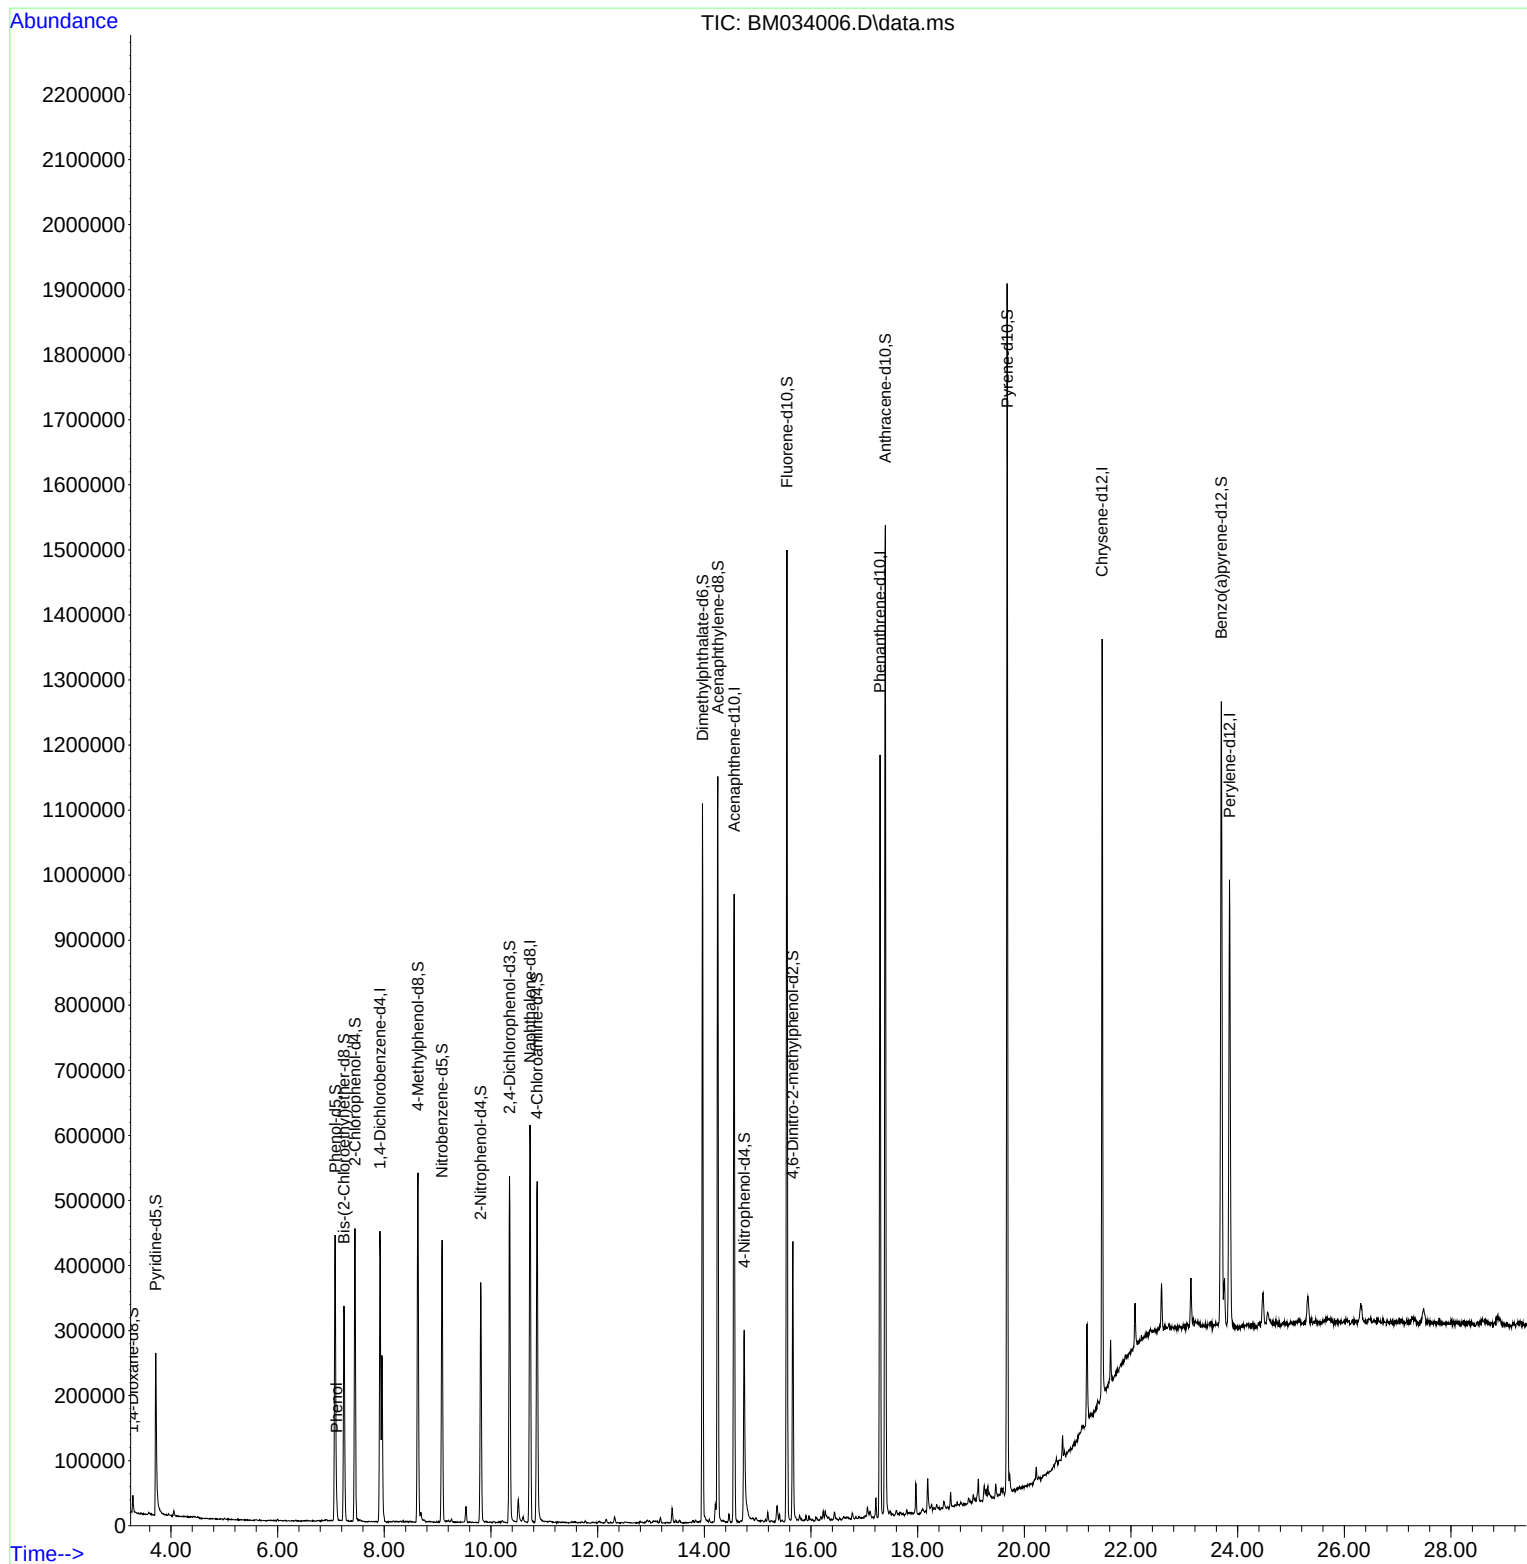

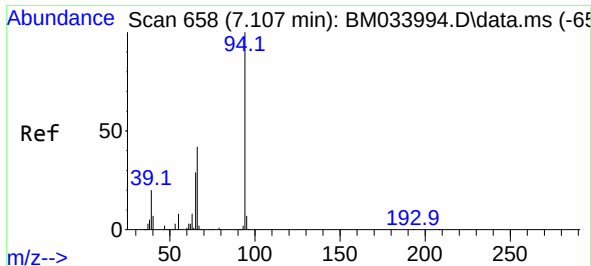

#8
Phenol
Concen: 1.567 ng/ul
RT: 7.107 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM034006.D
Acq: 03 Feb 2022 17:35

Instrument :
BNA_M
ClientSampleId :
BGLZ4

Tgt Ion: 94 Resp: 14964
Ion Ratio Lower Upper
94 100
65 26.3 31.7 47.5#
66 44.0 45.4 68.0#

