

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034007.D
 Acq On : 03 Feb 2022 18:11
 Operator : CG/JU
 Sample : N1365-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGLZ0

Quant Time: Feb 04 00:08:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	101148	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.730	136	433581	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.560	164	283598	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.295	188	562375	20.000	ng/u1	-0.01
79) Chrysene-d12	21.459	240	442170	20.000	ng/u1	0.00
88) Perylene-d12	23.847	264	418067	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	14398	5.614	ng/uL	0.00
4) Pyridine-d5	3.713	84	181514	25.356	ng/u1	0.00
7) Phenol-d5	7.078	99	262632	30.993	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.242	67	169016	32.716	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.448	132	213458	31.441	ng/u1	-0.01
15) 4-Methylphenol-d8	8.631	113	219815	32.736	ng/u1	-0.01
21) Nitrobenzene-d5	9.084	128	110727	31.827	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.807	143	120672	32.119	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.348	165	208202	30.624	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.866	131	298554	31.800	ng/u1	0.00
46) Dimethylphthalate-d6	13.966	166	714797	33.729	ng/u1	-0.01
49) Acenaphthylene-d8	14.254	160	840159	32.362	ng/u1	0.00
54) 4-Nitrophenol-d4	14.748	143	89981	24.852	ng/u1	0.00
60) Fluorene-d10	15.548	176	587486	33.200	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.660	200	82449	23.353	ng/u1	-0.01
73) Anthracene-d10	17.395	188	874434	32.468	ng/u1	0.00
81) Pyrene-d10	19.677	212	912355	34.950	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.694	264	713357	32.487	ng/u1	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.101	94	14538	1.673	ng/u1#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034007.D
Acq On : 03 Feb 2022 18:11
Operator : CG/JU
Sample : N1365-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGLZ0

Quant Time: Feb 04 00:08:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

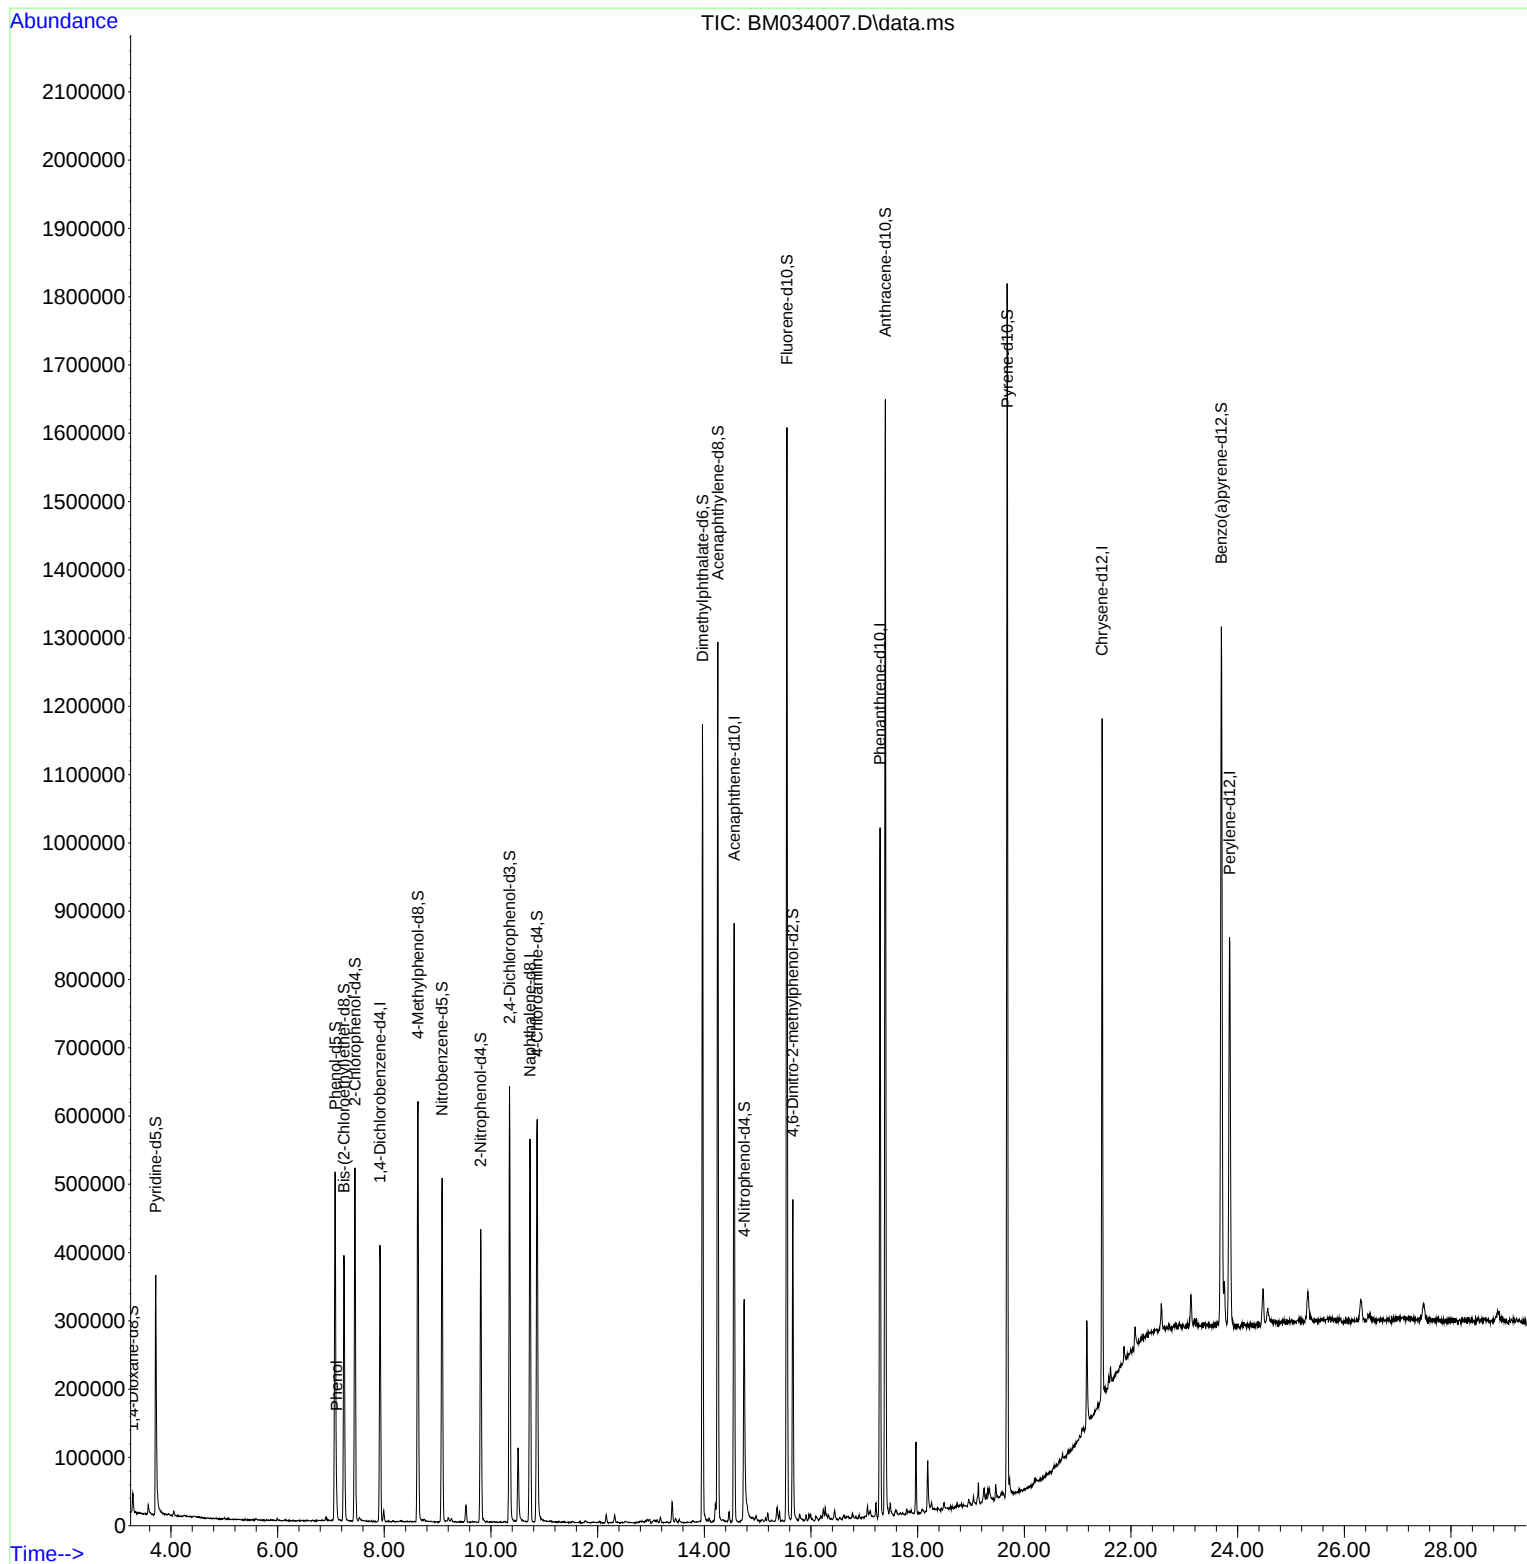

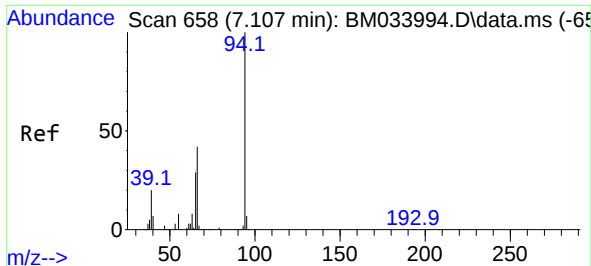

#8
Phenol
Concen: 1.673 ng/ul
RT: 7.101 min Scan# 61
Delta R.T. -0.012 min
Lab File: BM034007.D
Acq: 03 Feb 2022 18:11

Instrument :
BNA_M
ClientSampleId :
BGLZ0

Tgt Ion: 94 Resp: 14538
Ion Ratio Lower Upper
94 100
65 27.6 31.7 47.5#
66 55.8 45.4 68.0

