

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM033995.D
 Acq On : 03 Feb 2022 11:01
 Operator : CG/JU
 Sample : PB142413BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK413

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.284	4	8	16	rVB	32389	42748	1.55%	0.146%
2	3.713	77	81	95	rBV	388553	603011	21.91%	2.058%
3	4.054	135	139	143	rVB	8803	11795	0.43%	0.040%
4	7.078	646	653	664	rBV	505147	785916	28.55%	2.683%
5	7.242	675	681	691	rVB	382398	614194	22.31%	2.097%
6	7.448	709	716	726	rBV	527458	816175	29.65%	2.786%
7	7.919	789	796	804	rBV	397867	649052	23.58%	2.216%
8	8.631	910	917	930	rBV	631895	1001901	36.40%	3.420%
9	9.083	987	994	1004	rBV	504973	814535	29.59%	2.780%
10	9.807	1110	1117	1125	rBV	417631	688754	25.02%	2.351%
11	10.348	1201	1209	1221	rBV	605009	1030090	37.42%	3.516%
12	10.730	1267	1274	1282	rVB	578337	965493	35.08%	3.296%
13	10.866	1290	1297	1310	rBV	614700	1048449	38.09%	3.579%
14	12.324	1539	1545	1551	rVB3	9590	15892	0.58%	0.054%
15	12.501	1571	1575	1578	rBV5	2318	3674	0.13%	0.013%
16	13.966	1818	1824	1837	rBV	1228378	1716971	62.38%	5.861%
17	14.254	1866	1873	1882	rBV	1328987	1856271	67.44%	6.336%
18	14.560	1918	1925	1932	rBV	914771	1316463	47.83%	4.494%
19	14.748	1950	1957	1969	rBV	357765	667536	24.25%	2.279%
20	14.913	1982	1985	1988	rVB5	2172	3425	0.12%	0.012%
21	15.548	2086	2093	2106	rBV	1647371	2320018	84.29%	7.919%
22	15.660	2106	2112	2127	rVV	528314	733023	26.63%	2.502%
23	15.789	2130	2134	2139	rVB3	9637	11960	0.43%	0.041%
24	16.330	2222	2226	2229	rBV4	2604	3002	0.11%	0.010%
25	16.783	2301	2303	2308	rBV5	1903	3231	0.12%	0.011%
26	17.083	2351	2354	2360	rVB3	4537	5949	0.22%	0.020%
27	17.295	2384	2390	2397	rVV	1074496	1528406	55.53%	5.217%
28	17.395	2400	2407	2422	rVV	1894887	2604303	94.62%	8.890%
29	17.965	2500	2504	2506	rBV4	2634	3373	0.12%	0.012%
30	18.442	2584	2585	2590	rBV4	2969	4181	0.15%	0.014%
31	18.624	2614	2616	2620	rBV5	2713	3132	0.11%	0.011%
32	19.248	2718	2722	2726	rVB3	21216	28657	1.04%	0.098%
33	19.318	2730	2734	2739	rVB	20728	27729	1.01%	0.095%
34	19.677	2789	2795	2801	rBV	2100757	2752444	100.00%	9.396%
35	21.459	3093	3098	3106	rBV	1101192	1401218	50.91%	4.783%
36	23.694	3472	3478	3485	rVB2	1075395	2006762	72.91%	6.850%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM033995.D
Acq On : 03 Feb 2022 11:01
Operator : CG/JU
Sample : PB142413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK413

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION

37	23.847	3498	3504	3513	rVB2	603432	1205446	43.80%	4.115%
----	--------	------	------	------	------	--------	---------	--------	--------


Sum of corrected areas: 29295179

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM033995.D
Acq On : 03 Feb 2022 11:01
Operator : CG/JU
Sample : PB142413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK413

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

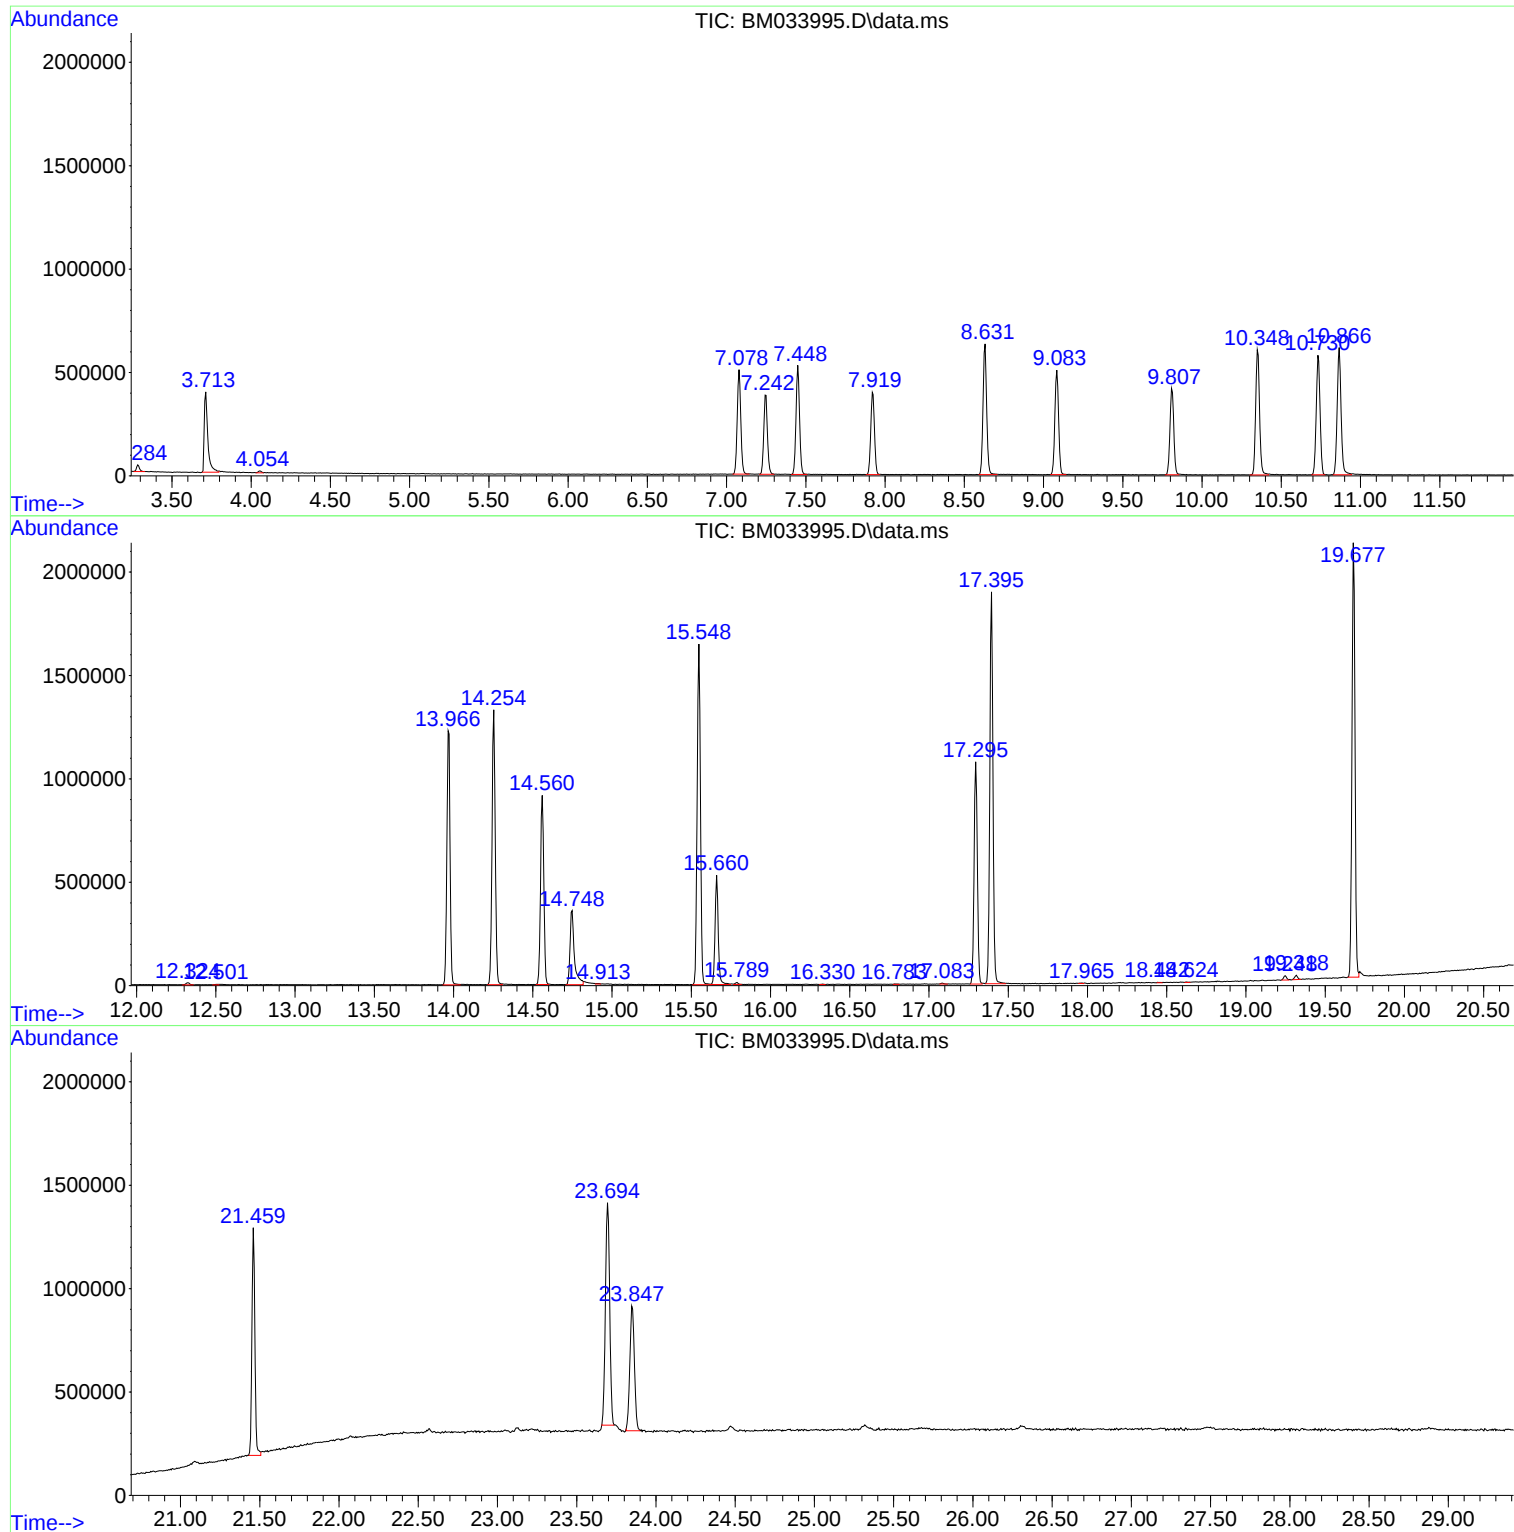

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM033995.D
Acq On : 03 Feb 2022 11:01
Operator : CG/JU
Sample : PB142413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK413

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM033995.D
Acq On : 03 Feb 2022 11:01
Operator : CG/JU
Sample : PB142413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK413

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc