

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM033996.D
 Acq On : 03 Feb 2022 11:37
 Operator : CG/JU
 Sample : PB142431BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK431

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.284	4	8	18	rVB	33921	51079	1.56%	0.156%
2	3.713	77	81	99	rBV	404352	662505	20.29%	2.020%
3	4.055	135	139	144	rVB3	8088	11890	0.36%	0.036%
4	5.072	310	312	319	rVB7	2763	4023	0.12%	0.012%
5	7.078	647	653	662	rBV	549277	844088	25.85%	2.574%
6	7.243	675	681	691	rVB	411514	648972	19.87%	1.979%
7	7.448	709	716	727	rVB	549265	863341	26.44%	2.632%
8	7.919	790	796	807	rVB	404764	632551	19.37%	1.929%
9	8.631	910	917	926	rBV	690520	1085170	33.23%	3.309%
10	9.084	986	994	1002	rBV	548024	891399	27.30%	2.718%
11	9.807	1110	1117	1128	rBV	462735	760470	23.29%	2.319%
12	10.348	1203	1209	1220	rBV	673593	1120388	34.31%	3.416%
13	10.731	1268	1274	1282	rVB	564664	931419	28.52%	2.840%
14	10.866	1288	1297	1308	rBV	695824	1180222	36.14%	3.598%
15	12.319	1540	1544	1556	rVB	11508	19343	0.59%	0.059%
16	13.530	1746	1750	1754	rBV4	2032	3405	0.10%	0.010%
17	13.972	1817	1825	1836	rBV	1409192	1960814	60.05%	5.978%
18	14.254	1866	1873	1884	rBV	1479150	2124583	65.06%	6.478%
19	14.395	1894	1897	1901	rBV4	1839	3340	0.10%	0.010%
20	14.560	1918	1925	1933	rBV	926633	1310479	40.13%	3.996%
21	14.748	1950	1957	1973	rBV	449759	825967	25.29%	2.518%
22	15.548	2086	2093	2101	rBV	1929157	2689475	82.36%	8.200%
23	15.660	2106	2112	2130	rVV	620329	888474	27.21%	2.709%
24	15.783	2130	2133	2138	rVB4	10054	15192	0.47%	0.046%
25	16.219	2200	2207	2209	rBV8	2300	3384	0.10%	0.010%
26	17.083	2350	2354	2358	rBV2	4190	4629	0.14%	0.014%
27	17.295	2384	2390	2399	rBV	1106109	1565434	47.94%	4.773%
28	17.395	2400	2407	2421	rVV	2160980	3000559	91.89%	9.149%
29	17.671	2450	2454	2459	rVB7	2928	4793	0.15%	0.015%
30	18.818	2646	2649	2652	rBV5	4186	6161	0.19%	0.019%
31	19.248	2718	2722	2727	rVB2	22135	30301	0.93%	0.092%
32	19.312	2730	2733	2739	rVB	21840	28403	0.87%	0.087%
33	19.683	2790	2796	2801	rBV	2421280	3265546	100.00%	9.957%
34	21.459	3093	3098	3104	rBV	1151881	1458038	44.65%	4.446%
35	23.694	3471	3478	3485	rBV2	1338981	2581864	79.06%	7.872%
36	23.847	3498	3504	3515	rVB2	653986	1320206	40.43%	4.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM033996.D
Acq On : 03 Feb 2022 11:37
Operator : CG/JU
Sample : PB142431BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK431

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION


Sum of corrected areas: 32797907

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM033996.D
Acq On : 03 Feb 2022 11:37
Operator : CG/JU
Sample : PB142431BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK431

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

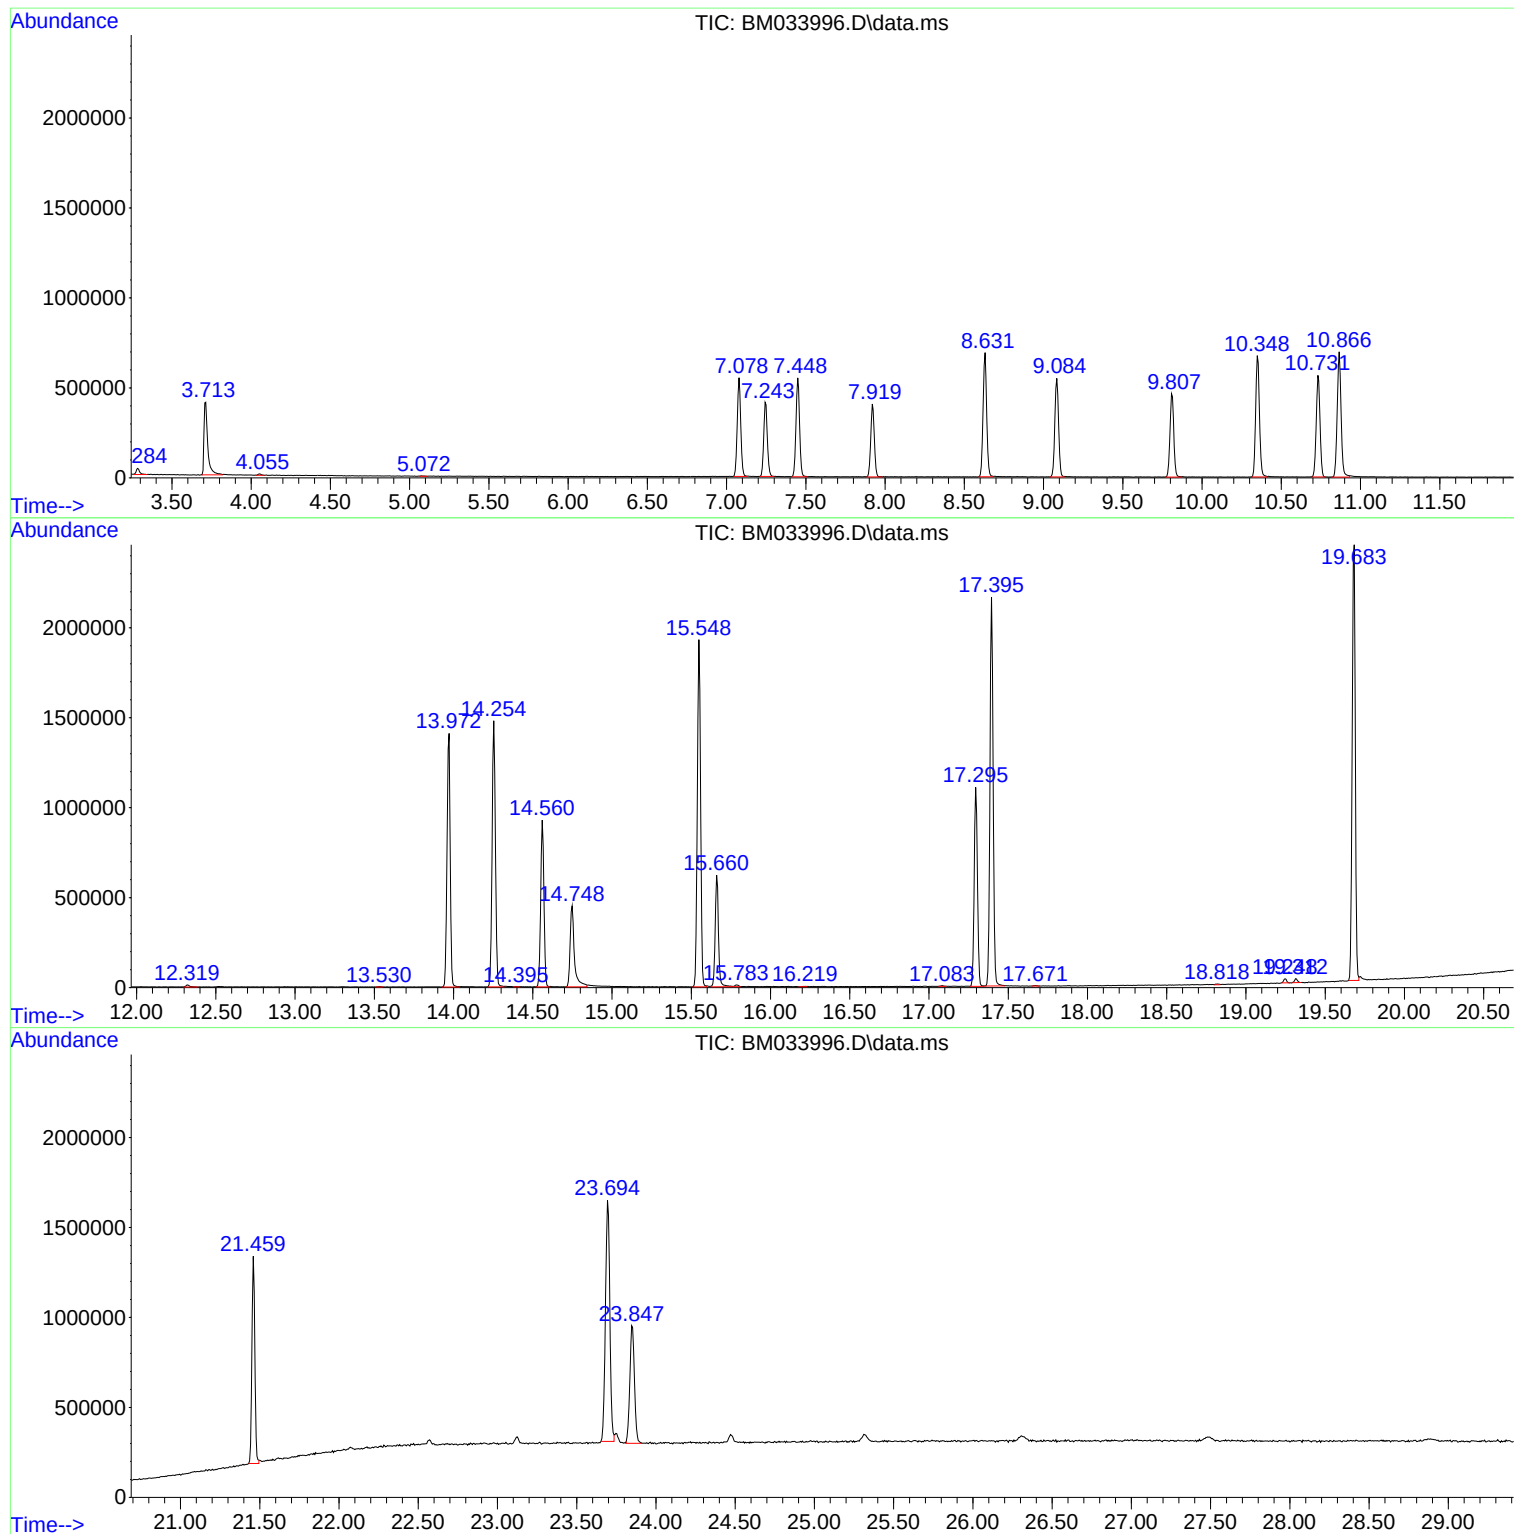

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM033996.D
Acq On : 03 Feb 2022 11:37
Operator : CG/JU
Sample : PB142431BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK431

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM033996.D
Acq On : 03 Feb 2022 11:37
Operator : CG/JU
Sample : PB142431BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK431

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc