

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034003.D
 Acq On : 03 Feb 2022 15:48
 Operator : CG/JU
 Sample : PB142441BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK441

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.284	4	8	15	rVB	34180	47032	1.88%	0.162%
2	3.713	77	81	99	rBV	401520	639618	25.59%	2.197%
3	4.055	135	139	144	rVB	5855	8974	0.36%	0.031%
4	4.943	288	290	294	rBV5	1648	2535	0.10%	0.009%
5	5.072	309	312	318	rVB7	1369	2856	0.11%	0.010%
6	5.913	451	455	460	rVB6	1446	2836	0.11%	0.010%
7	7.078	646	653	662	rBV	515528	807755	32.32%	2.774%
8	7.243	675	681	691	rVB	407408	643608	25.75%	2.210%
9	7.449	709	716	723	rBV	560264	846781	33.88%	2.908%
10	7.919	790	796	805	rBV	435938	675272	27.02%	2.319%
11	8.025	810	814	817	rBV4	1593	2836	0.11%	0.010%
12	8.231	847	849	854	rVB4	1980	2904	0.12%	0.010%
13	8.290	854	859	861	rBV6	1801	2939	0.12%	0.010%
14	8.631	910	917	926	rBV	635880	1037180	41.50%	3.562%
15	9.084	986	994	1002	rBV	526501	854930	34.20%	2.936%
16	9.807	1109	1117	1130	rBV	442353	731575	29.27%	2.512%
17	10.348	1202	1209	1223	rBV	638076	1056265	42.26%	3.627%
18	10.442	1223	1225	1229	rVB3	2658	2824	0.11%	0.010%
19	10.731	1266	1274	1284	rVB	595482	994536	39.79%	3.415%
20	10.866	1289	1297	1309	rBV	620016	1085062	43.41%	3.726%
21	12.319	1540	1544	1550	rBV2	9666	14979	0.60%	0.051%
22	12.525	1576	1579	1584	rVB5	2290	3116	0.12%	0.011%
23	13.966	1818	1824	1836	rBV	1255902	1691332	67.67%	5.808%
24	14.254	1864	1873	1885	rBV	1321175	1906974	76.30%	6.549%
25	14.560	1918	1925	1936	rVV	920289	1327458	53.11%	4.559%
26	14.748	1951	1957	1984	rBV	306069	649141	25.97%	2.229%
27	14.930	1986	1988	1991	rVV4	4581	5471	0.22%	0.019%
28	14.972	1994	1995	2002	rVB7	2283	3063	0.12%	0.011%
29	15.548	2086	2093	2102	rBV	1643351	2320085	92.82%	7.968%
30	15.660	2106	2112	2122	rBV	471008	653315	26.14%	2.244%
31	15.783	2129	2133	2138	rVB3	7766	11671	0.47%	0.040%
32	16.224	2204	2208	2211	rBV4	2470	2555	0.10%	0.009%
33	16.971	2332	2335	2338	rBV5	2193	3461	0.14%	0.012%
34	17.077	2350	2353	2358	rBV4	3745	5035	0.20%	0.017%
35	17.295	2384	2390	2400	rBV	1057604	1476571	59.08%	5.071%
36	17.395	2400	2407	2419	rBV	1676124	2402706	96.13%	8.251%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034003.D
Acq On : 03 Feb 2022 15:48
Operator : CG/JU
Sample : PB142441BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK441

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION

37	19.248	2718	2722	2726	rBV	19420	24882	1.00%	0.085%
38	19.312	2729	2733	2737	rBV2	18301	27011	1.08%	0.093%
39	19.677	2789	2795	2801	rBV	1860766	2499432	100.00%	8.584%
40	21.459	3093	3098	3106	rBV	1075975	1333924	53.37%	4.581%
41	23.695	3471	3478	3485	rBV2	1028878	2037976	81.54%	6.999%
42	23.847	3498	3504	3519	rVB2	607828	1270368	50.83%	4.363%


Sum of corrected areas: 29118844

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034003.D
Acq On : 03 Feb 2022 15:48
Operator : CG/JU
Sample : PB142441BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

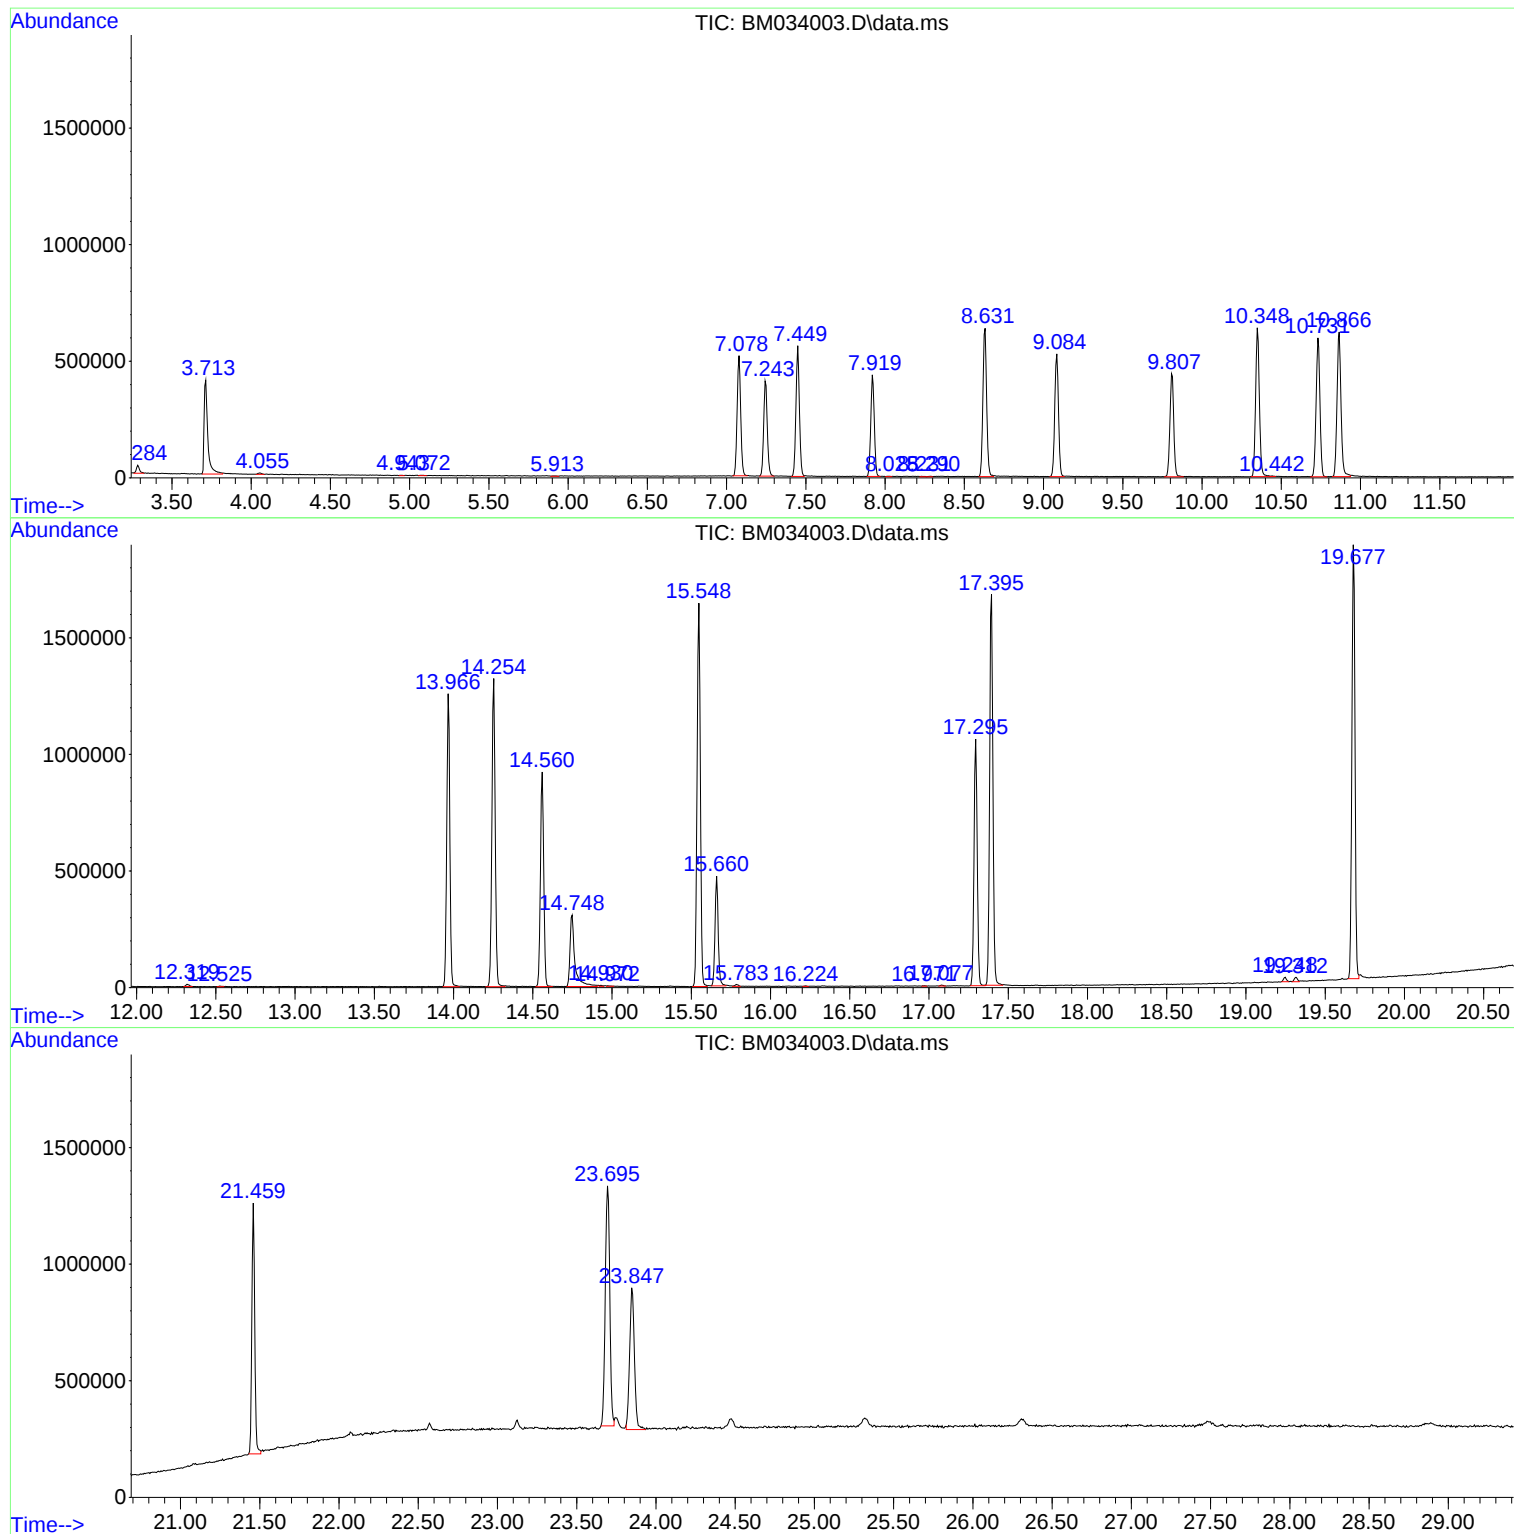

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034003.D
Acq On : 03 Feb 2022 15:48
Operator : CG/JU
Sample : PB142441BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034003.D
Acq On : 03 Feb 2022 15:48
Operator : CG/JU
Sample : PB142441BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc