

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034008.D
 Acq On : 03 Feb 2022 18:47
 Operator : CG/JU
 Sample : N1365-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGLZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.284	4	8	17	rVB	29588	42364	1.84%	0.147%
2	3.572	55	57	63	rBV	8095	10883	0.47%	0.038%
3	3.713	77	81	95	rBV	323366	509637	22.12%	1.764%
4	4.054	136	139	143	rVB2	7405	10516	0.46%	0.036%
5	5.495	378	384	388	rBV2	10079	16127	0.70%	0.056%
6	5.995	464	469	476	rBV8	2772	6176	0.27%	0.021%
7	6.395	532	537	538	rBV4	4331	4425	0.19%	0.015%
8	6.913	618	625	632	rBV9	3755	9574	0.42%	0.033%
9	7.078	646	653	667	rVB	464604	777606	33.75%	2.691%
10	7.242	675	681	690	rVB	354992	558604	24.25%	1.933%
11	7.448	709	716	726	rBV	481291	742090	32.21%	2.568%
12	7.536	726	731	734	rBV5	3874	6830	0.30%	0.024%
13	7.919	790	796	801	rBV	424651	691289	30.01%	2.392%
14	7.954	801	802	807	rVB	52906	56558	2.46%	0.196%
15	8.419	877	881	886	rVB5	3781	4905	0.21%	0.017%
16	8.631	909	917	925	rBV	562826	923988	40.11%	3.197%
17	8.760	933	939	943	rVB5	3947	7252	0.31%	0.025%
18	9.001	976	980	986	rBV5	5716	10599	0.46%	0.037%
19	9.083	986	994	1003	rVB	460519	754099	32.73%	2.609%
20	9.195	1011	1013	1018	rVB5	4839	5654	0.25%	0.020%
21	9.254	1018	1023	1034	rVB5	5595	12032	0.52%	0.042%
22	9.530	1064	1070	1078	rBV	21321	33455	1.45%	0.116%
23	9.807	1110	1117	1130	rBV	391717	638489	27.72%	2.209%
24	10.348	1202	1209	1220	rBV	575409	950662	41.27%	3.290%
25	10.507	1229	1236	1248	rBV	75506	133083	5.78%	0.461%
26	10.730	1267	1274	1280	rBV	608097	1010909	43.88%	3.498%
27	10.783	1280	1283	1289	rVB	49762	72437	3.14%	0.251%
28	10.866	1289	1297	1310	rBV	542528	959006	41.63%	3.319%
29	11.766	1444	1450	1457	rBV9	3444	7583	0.33%	0.026%
30	12.166	1513	1518	1525	rVB3	9043	14304	0.62%	0.049%
31	12.319	1539	1544	1549	rVB2	10587	17939	0.78%	0.062%
32	12.389	1549	1556	1563	rVB2	11295	22317	0.97%	0.077%
33	12.513	1572	1577	1582	rBV6	4806	9846	0.43%	0.034%
34	12.607	1588	1593	1601	rVB	57184	90854	3.94%	0.314%
35	12.930	1645	1648	1652	rVV2	4743	6806	0.30%	0.024%
36	12.971	1652	1655	1659	rVB3	4936	7045	0.31%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034008.D
 Acq On : 03 Feb 2022 18:47
 Operator : CG/JU
 Sample : N1365-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGLZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

37	13.113	1676	1679	1684	rVV5	3141	5654	0.25%	0.020%
38	13.177	1686	1690	1697	rVB7	7631	12158	0.53%	0.042%
39	13.395	1722	1727	1735	rVV2	30018	45307	1.97%	0.157%
40	13.460	1735	1738	1746	rVV7	6556	10939	0.47%	0.038%
41	13.530	1746	1750	1754	rVB5	3180	4589	0.20%	0.016%
42	13.630	1761	1767	1768	rBV5	3434	5407	0.23%	0.019%
43	13.713	1776	1781	1784	rBV7	2442	4077	0.18%	0.014%
44	13.883	1805	1810	1817	rBV2	10935	21627	0.94%	0.075%
45	13.965	1818	1824	1830	rBV	1093565	1481954	64.33%	5.128%
46	14.054	1836	1839	1842	rVB4	4095	5492	0.24%	0.019%
47	14.101	1842	1847	1853	rBV7	8722	18407	0.80%	0.064%
48	14.207	1860	1865	1867	rBV2	22992	31638	1.37%	0.109%
49	14.254	1867	1873	1881	rVB	1170575	1701213	73.85%	5.887%
50	14.460	1904	1908	1913	rBV2	13153	17440	0.76%	0.060%
51	14.560	1918	1925	1932	rVV	935829	1363464	59.18%	4.718%
52	14.624	1932	1936	1942	rVB4	9100	15216	0.66%	0.053%
53	14.742	1949	1956	1979	rBV	304671	596466	25.89%	2.064%
54	14.901	1981	1983	1986	rVV4	4139	5480	0.24%	0.019%
55	14.960	1989	1993	1999	rVB6	9068	15848	0.69%	0.055%
56	15.107	2011	2018	2022	rBV	18449	34502	1.50%	0.119%
57	15.189	2028	2032	2038	rVB3	13460	20739	0.90%	0.072%
58	15.336	2052	2057	2066	rBV3	69181	134909	5.86%	0.467%
59	15.407	2066	2069	2074	rVB	14538	18943	0.82%	0.066%
60	15.548	2085	2093	2100	rBV	1470008	2096920	91.02%	7.256%
61	15.659	2105	2112	2122	rBV	436463	607838	26.38%	2.103%
62	15.783	2130	2133	2136	rBV3	5299	6101	0.26%	0.021%
63	15.812	2136	2138	2142	rVB5	6006	7600	0.33%	0.026%
64	15.907	2149	2154	2158	rVB7	7245	11338	0.49%	0.039%
65	15.959	2160	2163	2165	rBV4	5988	6612	0.29%	0.023%
66	15.995	2165	2169	2172	rVB5	8058	10923	0.47%	0.038%
67	16.095	2183	2186	2189	rBV5	7030	10153	0.44%	0.035%
68	16.189	2199	2202	2205	rBV4	5568	6204	0.27%	0.021%
69	16.230	2205	2209	2212	rBV4	10482	14331	0.62%	0.050%
70	16.265	2212	2215	2218	rBV3	13001	15634	0.68%	0.054%
71	16.324	2223	2225	2230	rVB6	5653	7702	0.33%	0.027%
72	16.383	2231	2235	2240	rBV5	3584	4635	0.20%	0.016%
73	16.442	2240	2245	2251	rBV5	14269	22868	0.99%	0.079%
74	16.536	2258	2261	2268	rVB9	2584	4697	0.20%	0.016%
75	16.601	2268	2272	2273	rBV4	5279	6461	0.28%	0.022%
76	16.771	2296	2301	2309	rBV10	8593	16808	0.73%	0.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
 Data File : BM034008.D
 Acq On : 03 Feb 2022 18:47
 Operator : CG/JU
 Sample : N1365-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGLZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

77	16.842	2309	2313	2319	rBV9	4906	8228	0.36%	0.028%
78	16.901	2319	2323	2327	rVB6	3239	5675	0.25%	0.020%
79	17.059	2345	2350	2353	rBV2	20351	28260	1.23%	0.098%
80	17.112	2357	2359	2363	rVB5	10590	10178	0.44%	0.035%
81	17.218	2373	2377	2383	rVB3	20092	26394	1.15%	0.091%
82	17.295	2383	2390	2396	rBV	1109902	1562647	67.83%	5.407%
83	17.336	2396	2397	2399	rVV2	9915	6672	0.29%	0.023%
84	17.395	2400	2407	2418	rVV	1550046	2200760	95.53%	7.616%
85	17.483	2418	2422	2429	rVB9	15874	26291	1.14%	0.091%
86	17.801	2472	2476	2480	rBV6	6285	8954	0.39%	0.031%
87	17.971	2496	2505	2509	rVB2	87943	128085	5.56%	0.443%
88	18.095	2524	2526	2531	rVB5	5447	5345	0.23%	0.018%
89	18.189	2537	2542	2550	rBV2	88611	153870	6.68%	0.532%
90	18.489	2591	2593	2597	rVB4	7852	9537	0.41%	0.033%
91	19.136	2701	2703	2710	rVB7	18284	19604	0.85%	0.068%
92	19.247	2718	2722	2726	rBV2	20415	30383	1.32%	0.105%
93	19.318	2731	2734	2737	rVV2	12900	14866	0.65%	0.051%
94	19.465	2755	2759	2769	rBV4	27330	48090	2.09%	0.166%
95	19.677	2789	2795	2801	rBV	1723878	2303758	100.00%	7.972%
96	20.653	2958	2961	2965	rBV3	44587	48436	2.10%	0.168%
97	21.171	3045	3049	3057	rBV2	168724	256887	11.15%	0.889%
98	21.459	3093	3098	3104	rBV	1091178	1375698	59.72%	4.760%
99	23.694	3471	3478	3484	rBV2	939082	1793389	77.85%	6.206%
100	23.847	3498	3504	3513	rVB2	609277	1262074	54.78%	4.367%




Sum of corrected areas: 28898318

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034008.D
Acq On : 03 Feb 2022 18:47
Operator : CG/JU
Sample : N1365-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGLZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

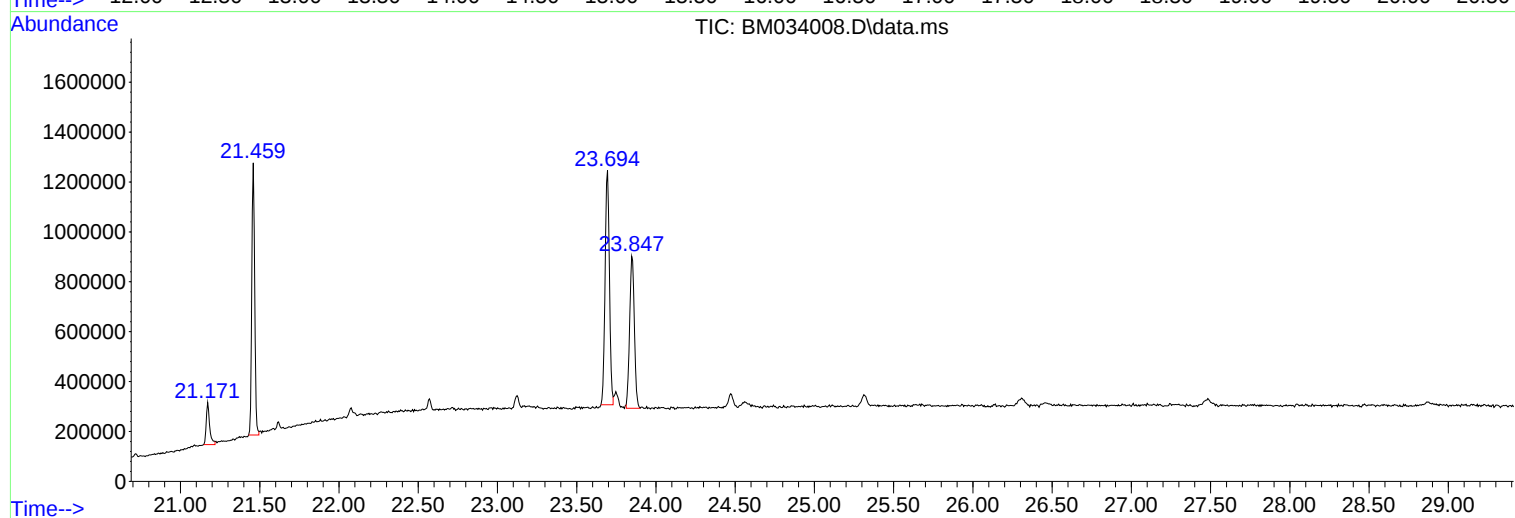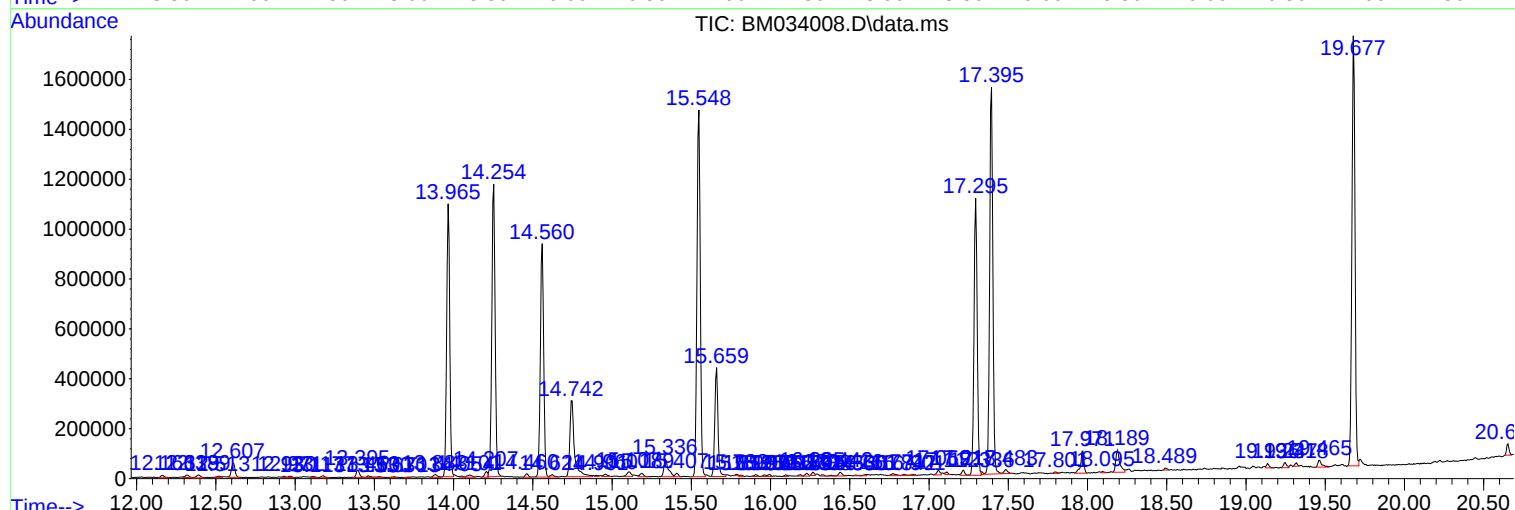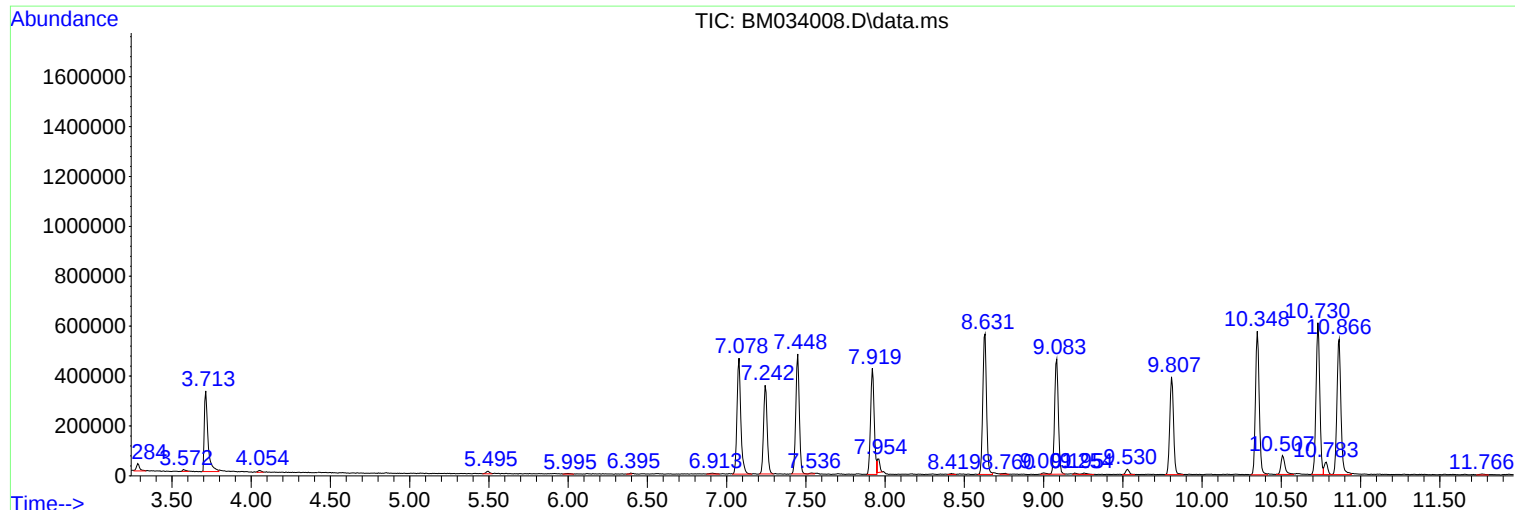

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034008.D
Acq On : 03 Feb 2022 18:47
Operator : CG/JU
Sample : N1365-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGLZ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.507	2.63 ng/ul	133083	Naphthalene-d8	10.730

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83

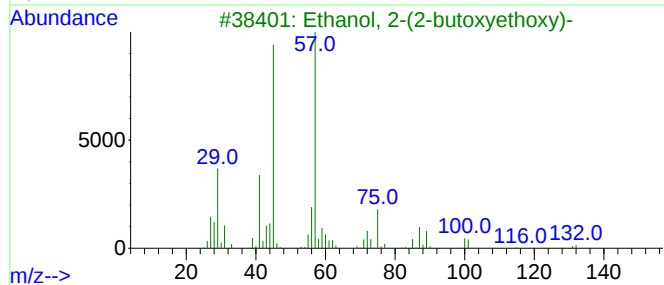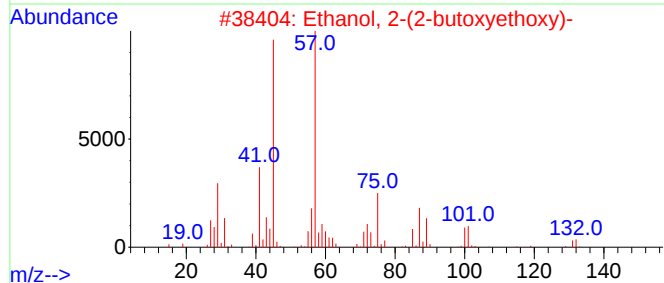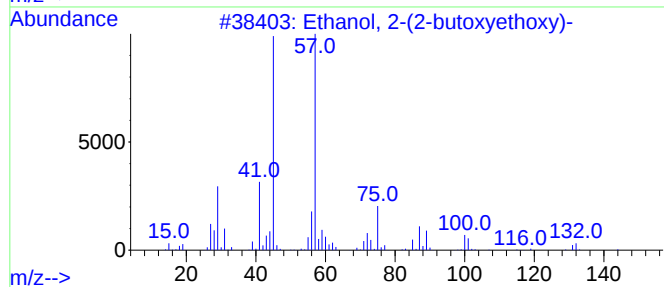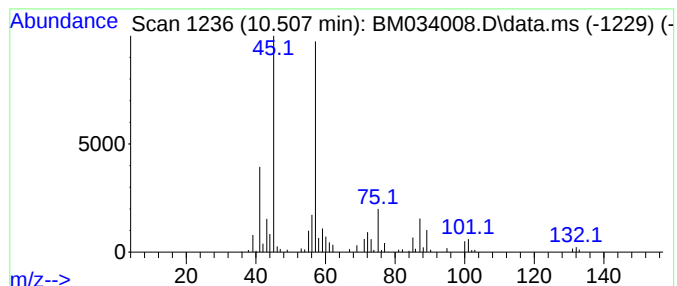

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034008.D
Acq On : 03 Feb 2022 18:47
Operator : CG/JU
Sample : N1365-07
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
BGLZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.171	3.73 ng/ul	256887	Chrysene-d12		21.459	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Hexacosene		364	C26H52	018835-33-1	95
2	Heptadecyl trifluoroacetate		352	C19H35F3O2	1010351-87-0	95
3	Heptadecyl heptafluorobutyrate		452	C21H35F7O2	959085-66-6	95
4	1-Octadecene		252	C18H36	000112-88-9	94
5	Pentafluoropropionic acid, hexad...		388	C19H33F5O2	006222-07-7	94

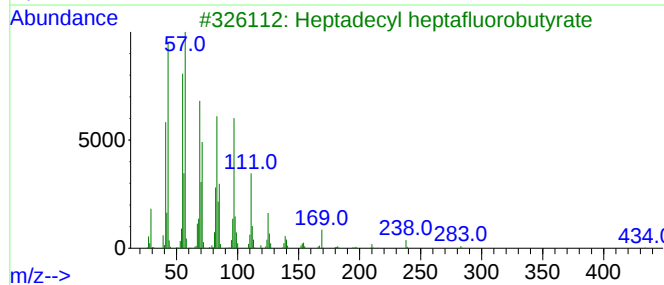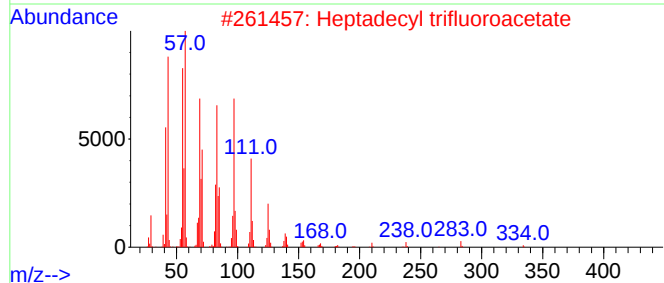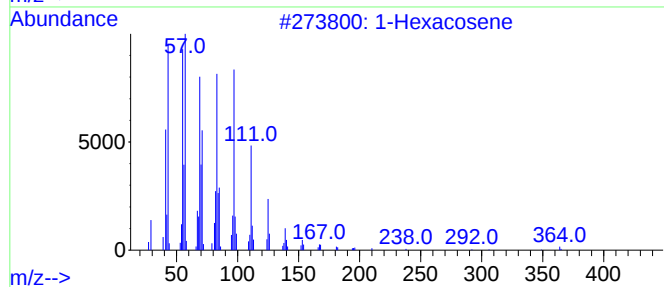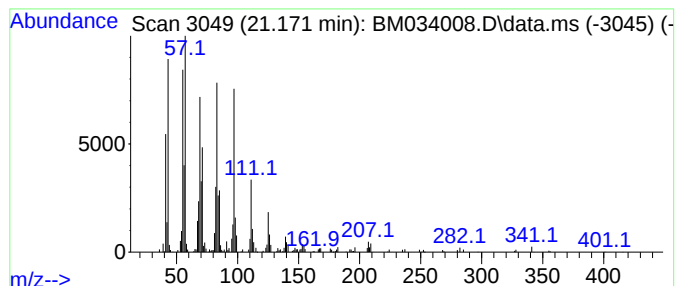

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020322\
Data File : BM034008.D
Acq On : 03 Feb 2022 18:47
Operator : CG/JU
Sample : N1365-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGLZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.507	2.6	ng/u1	133083	2	10.730	1010910	20.0
(DEL) Alkane: S...	21.171	3.7	ng/u1	256887	5	21.459	1375700	20.0