
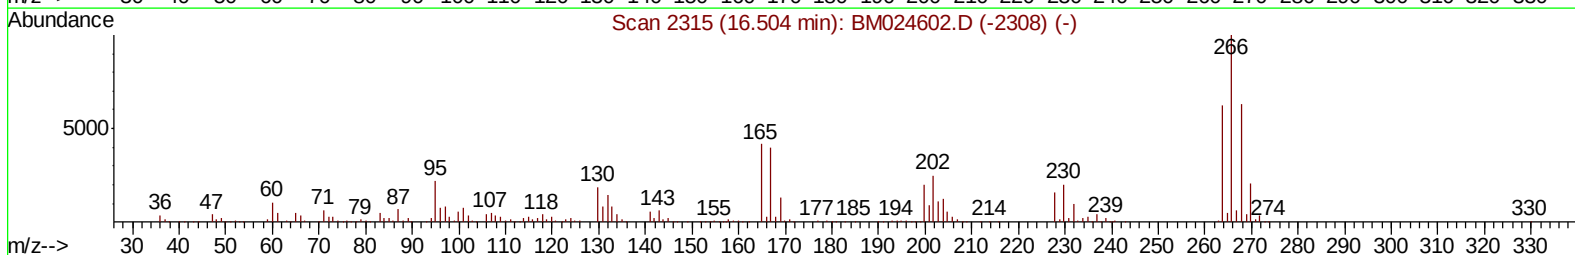
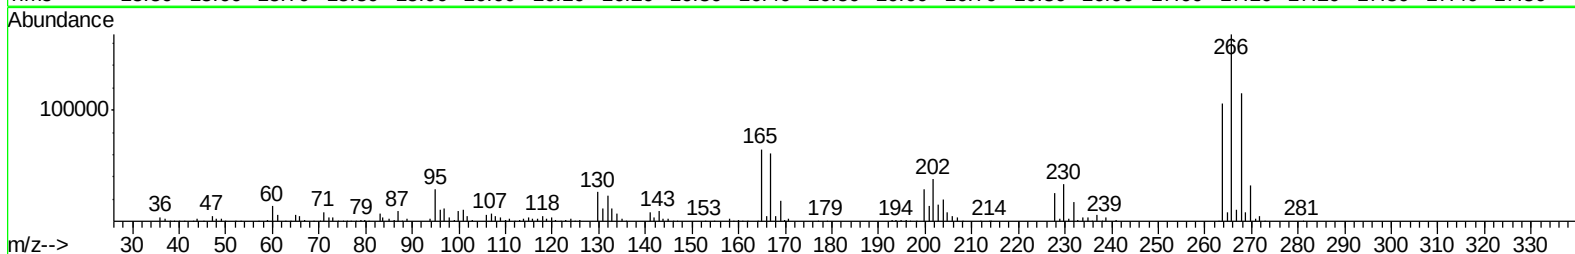


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020420\  
 Data File : BM024708.D  
 Acq On : 04 Feb 2020 16:06  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 04:14:47 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jan 23 14:57:07 2020  
 Response via : Initial Calibration

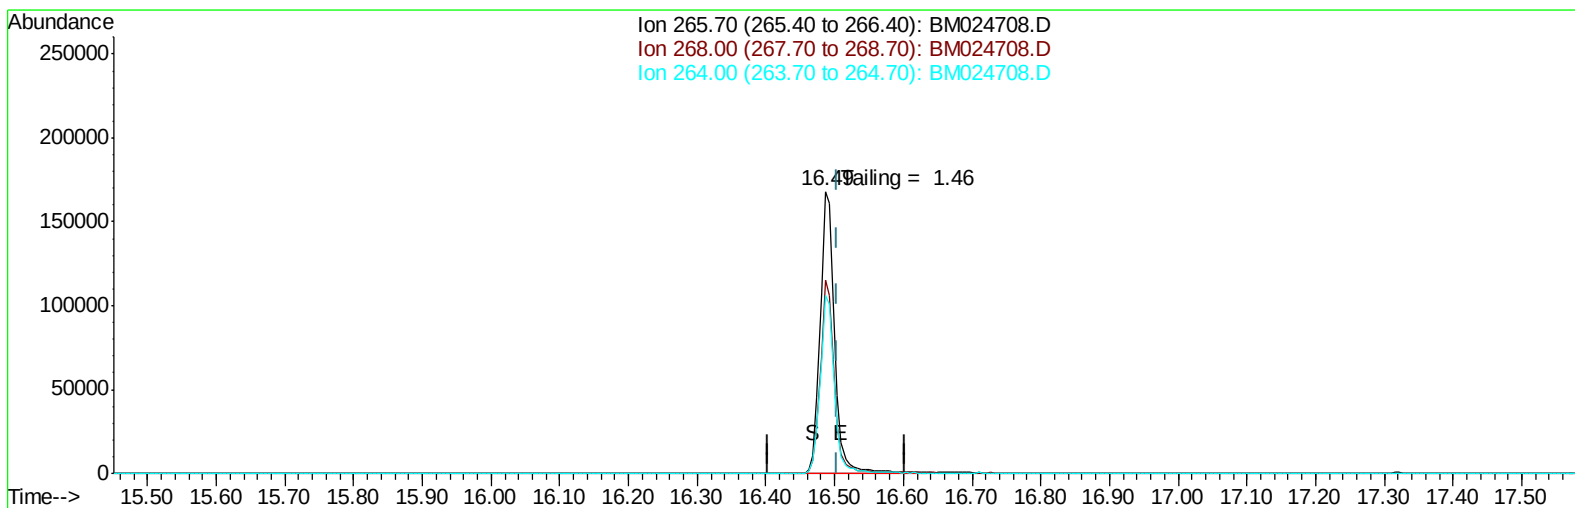

TIC: BM024708.D

(70) Pentachlorophenol (C)




16.486min (-0.018) 0.00ng

response 245827

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.00 | 68.79 |
| 264.00 | 62.40 | 63.04 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020420\  
 Data File : BM024708.D  
 Acq On : 04 Feb 2020 16:06  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 04:14:47 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM012320.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jan 23 14:57:07 2020  
 Response via : Initial Calibration

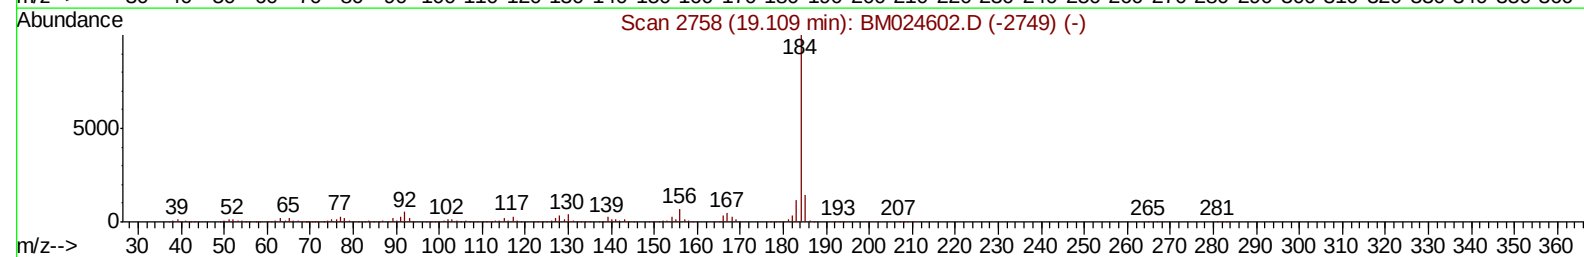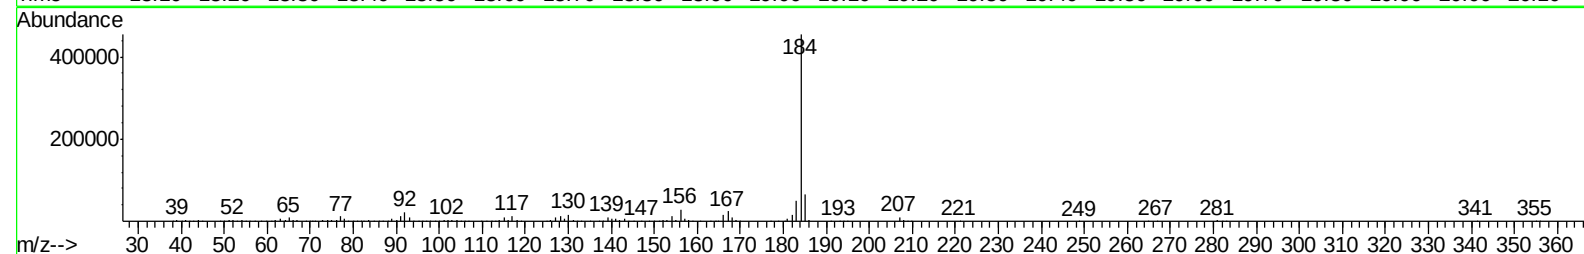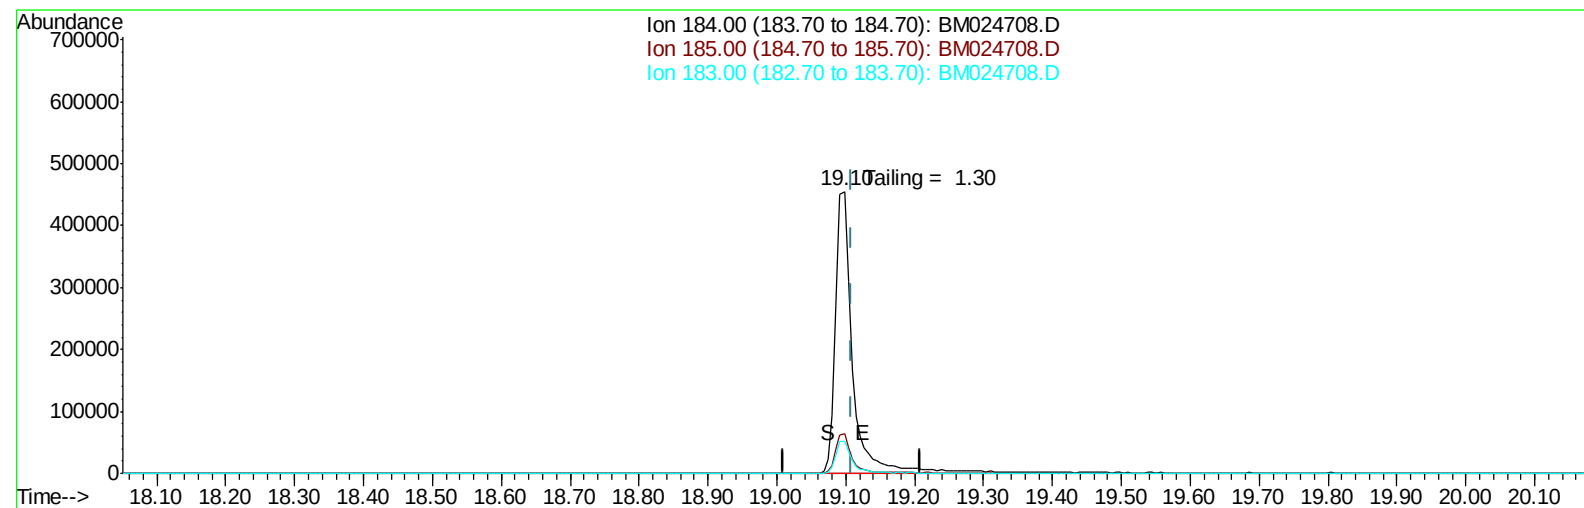

TIC: BM024708.D

(77) Benzidine

19.098min (-0.012) 36276.71ng

response 742611

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.10 | 14.16 |
| 183.00 | 12.00 | 11.38 |
| 0.00   | 0.00  | 0.00  |