


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020420\
 Data File : BM024708.D
 Acq On : 04 Feb 2020 16:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM012320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 23 14:57:07 2020

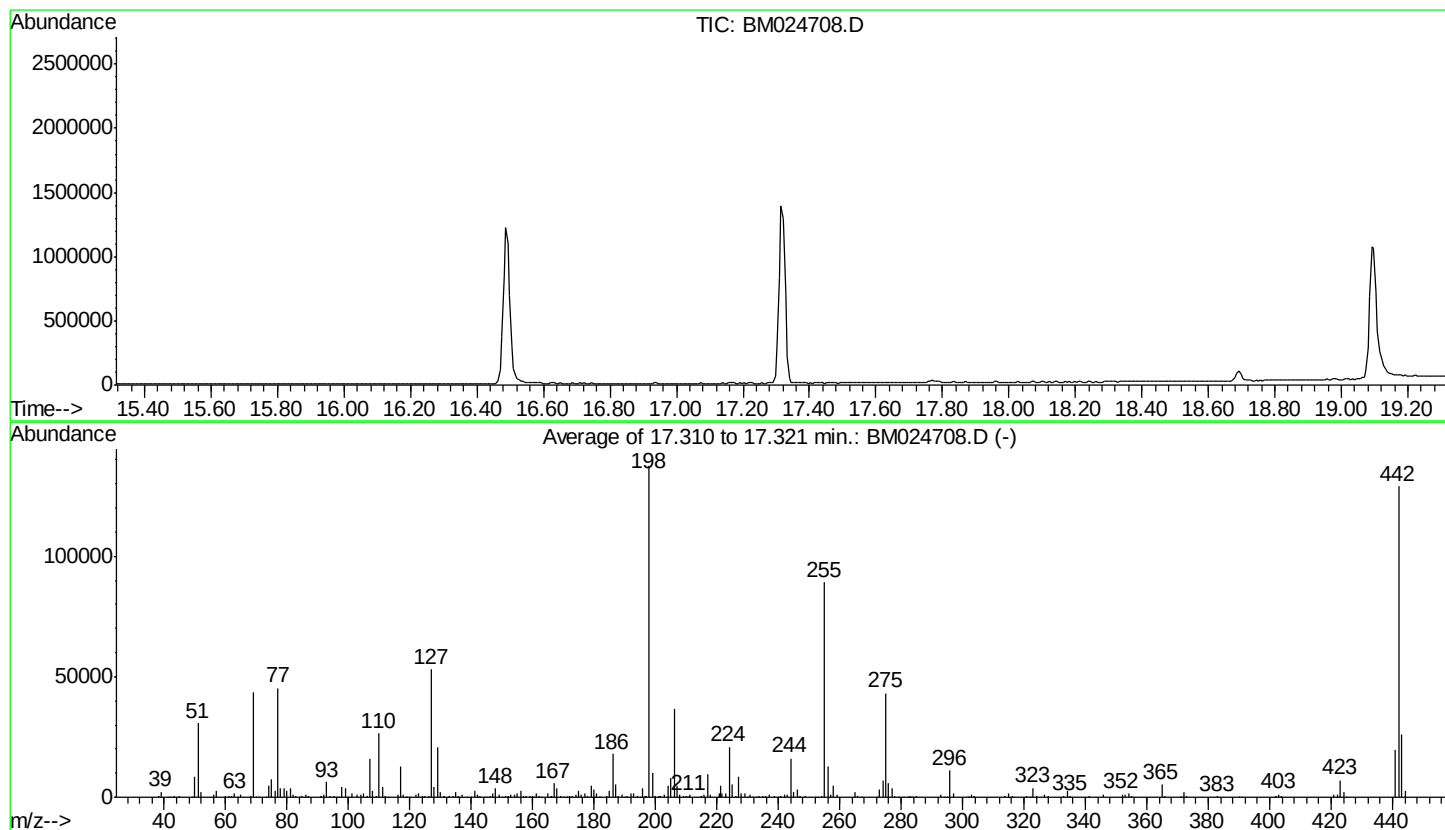

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	30805	PASS
68	69	0.00	2	1.4	614	PASS
69	198	0.00	100	31.6	43445	PASS
70	69	0.00	2	0.6	274	PASS
127	198	10	80	38.6	53093	PASS
197	198	0.00	2	0.4	548	PASS
198	198	100	100	100.0	137578	PASS
199	198	5	9	7.2	9888	PASS
275	198	10	60	31.3	43024	PASS
365	198	1	100	3.7	5132	PASS
441	198	0.01	100	14.3	19625	PASS
442	198	50	100	93.8	128984	PASS
443	442	15	24	20.2	26071	PASS