
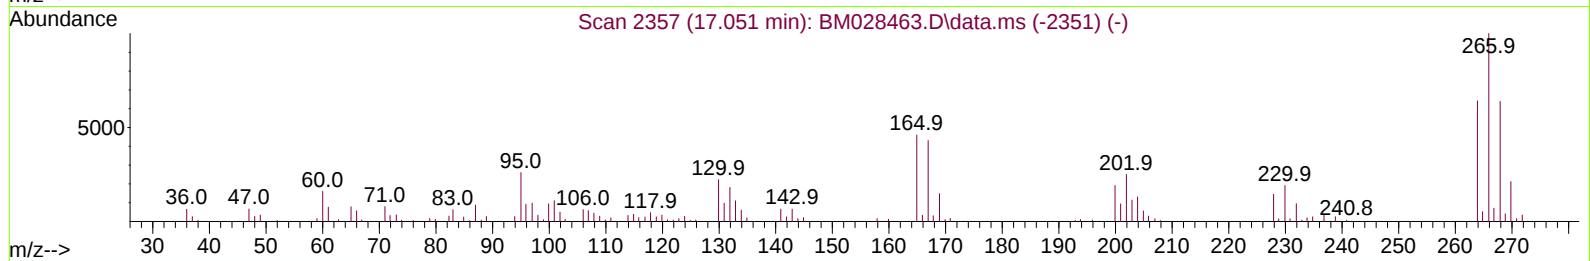
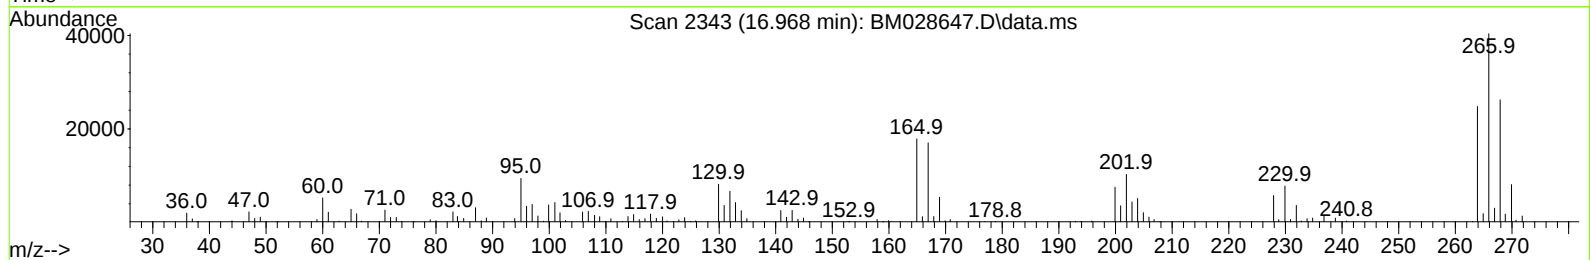


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM020421\  
Data File : BM028647.D  
Acq On : 04 Feb 2021 09:55  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 01:41:42 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 29 16:19:07 2021  
Response via : Initial Calibration

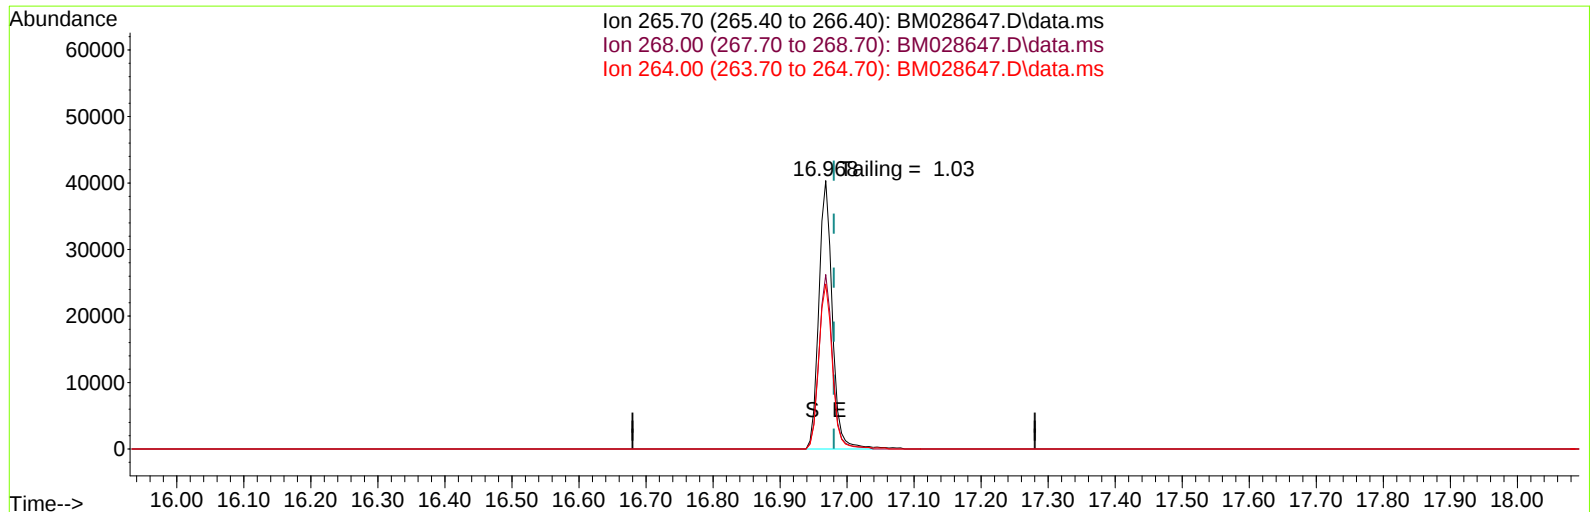

TIC: BM028647.D\data.ms

**(70) Pentachlorophenol (C)**




16.968min (-0.012) 0.00 ng

response 56598

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.40  | 64.98  |
| 264.00 | 63.30  | 61.45  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM020421\  
Data File : BM028647.D  
Acq On : 04 Feb 2021 09:55  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 01:41:42 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM012021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 29 16:19:07 2021  
Response via : Initial Calibration

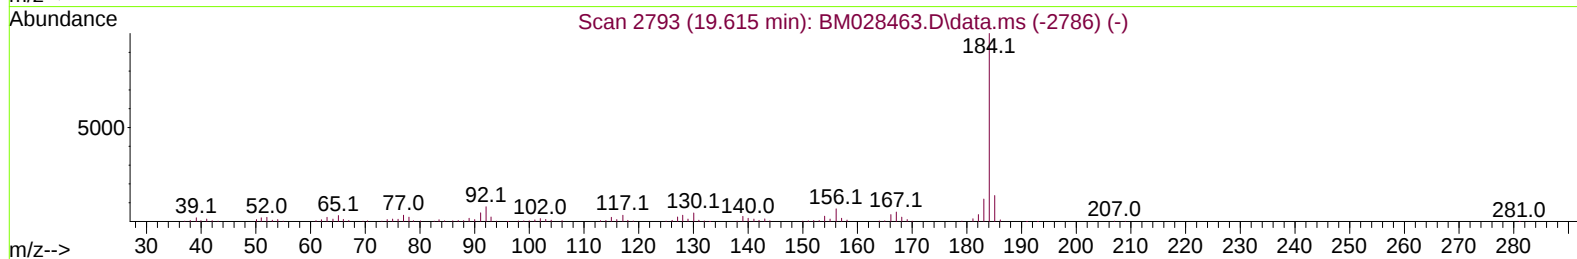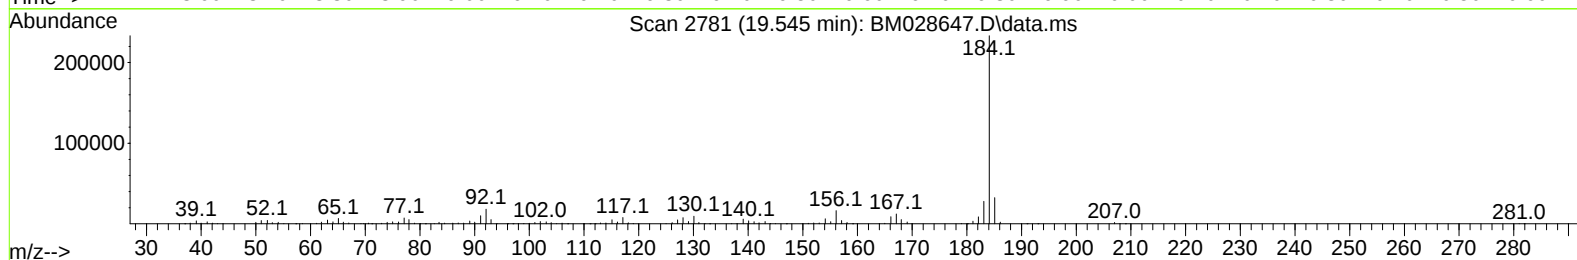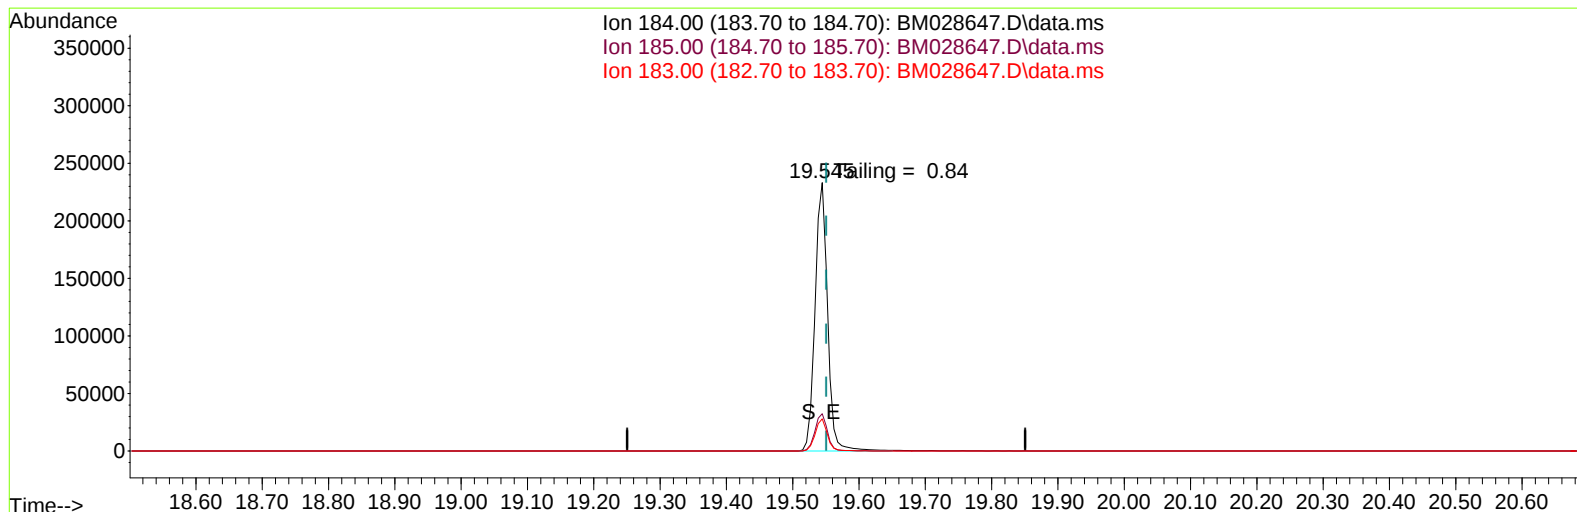

TIC: BM028647.D\data.ms

**(77) Benzidine**

19.545min (-0.006) 0.00 ng

response 306089

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 13.93  |
| 183.00 | 12.10  | 11.99  |
| 0.00   | 0.00   | 0.00   |