

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
 Data File : BM028651.D
 Acq On : 04 Feb 2021 13:14
 Operator : CG/JU
 Sample : M1291-16
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-004-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	300	305	313	rBV	9463	13746	1.32%	0.133%
2	5.463	381	387	399	rBV	437716	625540	60.00%	6.052%
3	7.099	658	665	677	rBV	406151	647557	62.11%	6.265%
4	7.922	799	805	812	rVB	110263	166675	15.99%	1.613%
5	9.098	997	1005	1014	rBV	254260	412712	39.58%	3.993%
6	10.734	1276	1283	1291	rBV	137849	227492	21.82%	2.201%
7	13.198	1695	1702	1710	rBV	599010	856256	82.13%	8.284%
8	14.033	1839	1844	1850	rVB	16419	22562	2.16%	0.218%
9	14.298	1884	1889	1895	rBV	24358	38142	3.66%	0.369%
10	14.427	1903	1911	1927	rVV4	7223	23362	2.24%	0.226%
11	14.575	1931	1936	1944	rVB2	184380	272234	26.11%	2.634%
12	14.980	1998	2005	2011	rBV3	7071	13229	1.27%	0.128%
13	15.757	2132	2137	2146	rBV	5202	12072	1.16%	0.117%
14	16.063	2183	2189	2208	rVB	434566	626240	60.06%	6.059%
15	16.710	2293	2299	2304	rBV5	10735	17147	1.64%	0.166%
16	17.310	2396	2401	2405	rBV	207335	288752	27.69%	2.794%
17	17.351	2405	2408	2414	rVB	54698	71606	6.87%	0.693%
18	17.445	2419	2424	2427	rBV	11166	15694	1.51%	0.152%
19	18.068	2525	2530	2537	rBV9	5231	13235	1.27%	0.128%
20	18.192	2544	2551	2564	rBV2	210854	326818	31.35%	3.162%
21	18.480	2595	2600	2603	rBV	19294	28095	2.69%	0.272%
22	18.521	2603	2607	2612	rVB4	19237	29189	2.80%	0.282%
23	18.727	2638	2642	2648	rVB3	11261	16912	1.62%	0.164%
24	18.915	2660	2674	2678	rBV	58406	198079	19.00%	1.916%
25	19.233	2724	2728	2732	rBV2	11280	16847	1.62%	0.163%
26	19.321	2738	2743	2744	rBV2	23559	33650	3.23%	0.326%
27	19.357	2744	2749	2757	rVB	170292	258906	24.83%	2.505%
28	19.462	2762	2767	2772	rBV	123635	171689	16.47%	1.661%
29	19.504	2772	2774	2779	rVB	16774	19648	1.88%	0.190%
30	19.680	2801	2804	2806	rBV	12046	15778	1.51%	0.153%
31	19.715	2806	2810	2816	rVB	159008	206631	19.82%	1.999%
32	19.786	2818	2822	2825	rBV3	8592	12899	1.24%	0.125%
33	19.915	2838	2844	2849	rBV	852392	1042622	100.00%	10.087%
34	20.180	2885	2889	2891	rBV5	10326	15519	1.49%	0.150%
35	20.274	2897	2905	2913	rBV	92247	237728	22.80%	2.300%
36	20.698	2975	2977	2982	rVB2	14446	15902	1.53%	0.154%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028651.D
Acq On : 04 Feb 2021 13:14
Operator : CG/JU
Sample : M1291-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-0002

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.156	3051	3055	3058	rBV2	161756	248439	23.83%	2.404%
38	21.233	3065	3068	3077	rVB2	34774	52410	5.03%	0.507%
39	21.456	3099	3106	3110	rBV2	287749	467278	44.82%	4.521%
40	21.492	3110	3112	3121	rVB	82982	102785	9.86%	0.994%
41	21.956	3186	3191	3197	rVB	106365	190180	18.24%	1.840%
42	22.051	3200	3207	3216	rVB	189276	430892	41.33%	4.169%
43	22.203	3229	3233	3243	rVB5	87106	174532	16.74%	1.689%
44	22.786	3328	3332	3341	rVB	91111	186668	17.90%	1.806%
45	23.033	3370	3374	3387	rVB	97885	284548	27.29%	2.753%
46	23.515	3452	3456	3462	rVB	61920	98004	9.40%	0.948%
47	23.609	3469	3472	3478	rVB	54209	83773	8.03%	0.811%
48	23.709	3484	3489	3507	rVB2	193904	510138	48.93%	4.936%
49	24.556	3627	3633	3651	rVB4	153173	495043	47.48%	4.790%




Sum of corrected areas: 10335855

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028651.D
Acq On : 04 Feb 2021 13:14
Operator : CG/JU
Sample : M1291-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

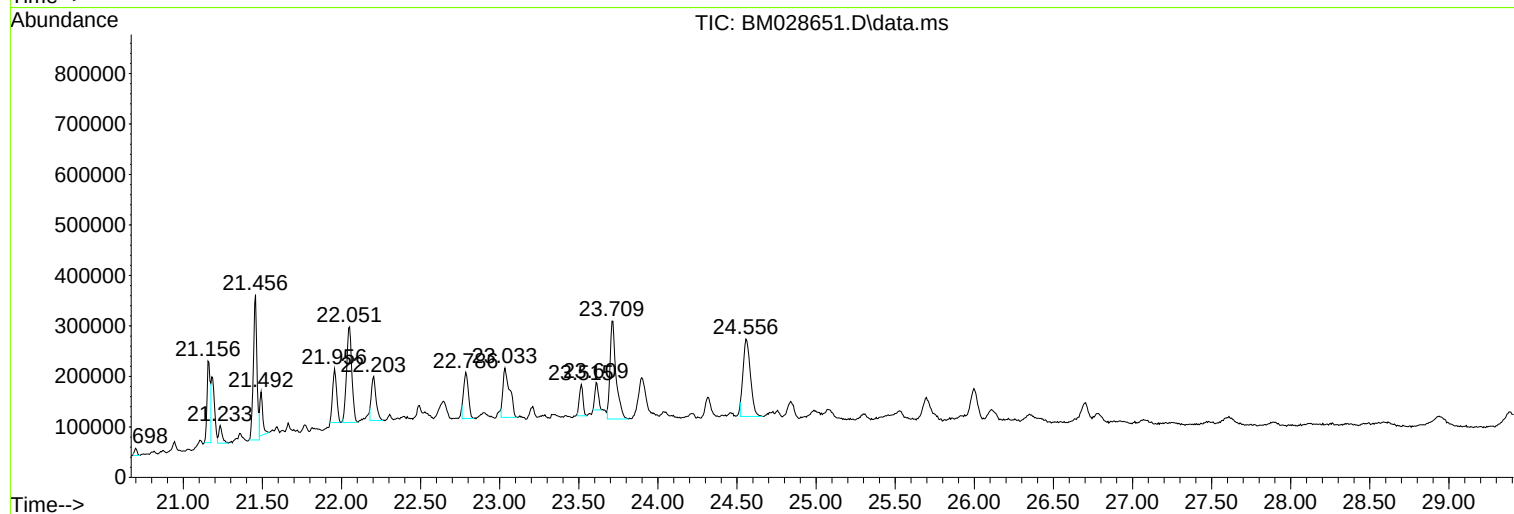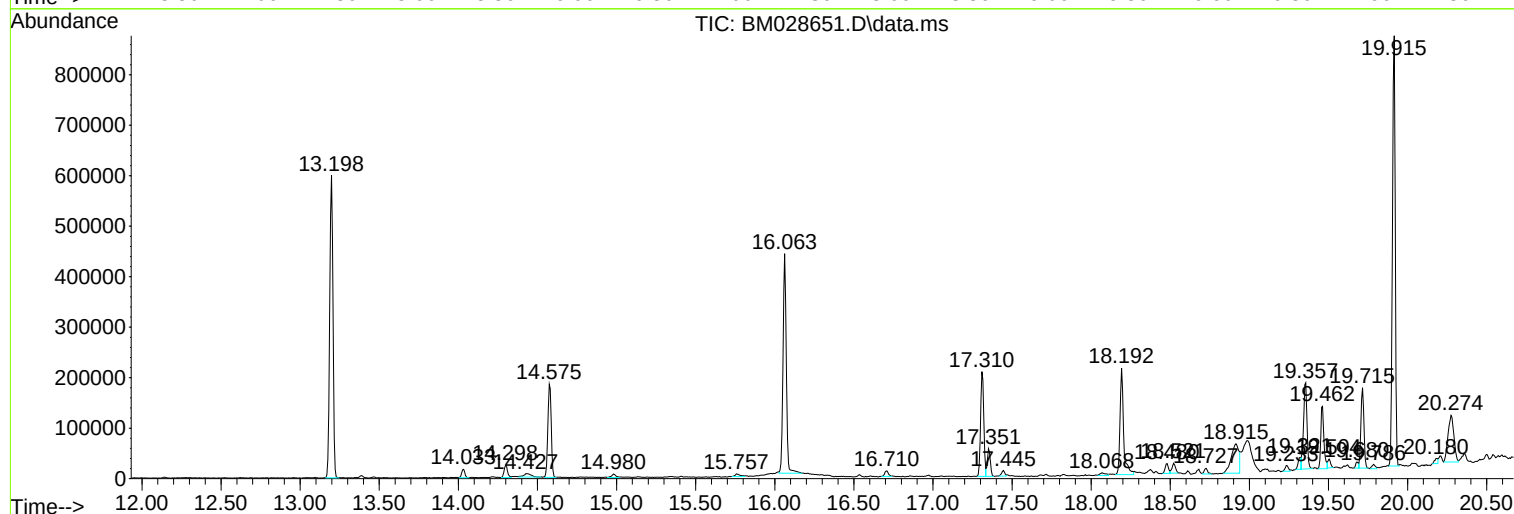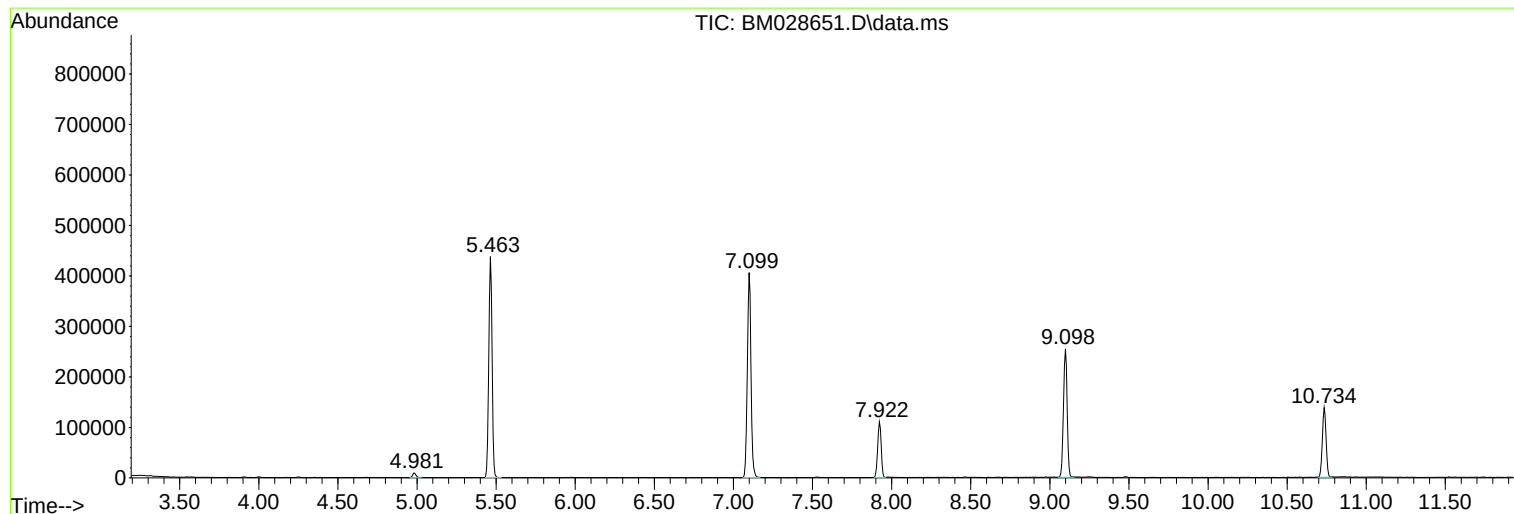

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028651.D
Acq On : 04 Feb 2021 13:14
Operator : CG/JU
Sample : M1291-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028651.D
Acq On : 04 Feb 2021 13:14
Operator : CG/JU
Sample : M1291-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------