

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
 Data File : BM028652.D
 Acq On : 04 Feb 2021 13:50
 Operator : CG/JU
 Sample : M1291-18
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-004-0510

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	299	306	311	rBV	9101	13473	1.42%	0.223%
2	5.463	381	387	401	rVB	423474	616809	64.85%	10.225%
3	7.098	658	665	678	rVB	406103	636952	66.97%	10.559%
4	7.922	799	805	813	rVB	109563	167672	17.63%	2.780%
5	9.098	997	1005	1014	rBV	252762	403310	42.40%	6.686%
6	10.733	1276	1283	1292	rVB	140210	230199	24.20%	3.816%
7	13.198	1695	1702	1710	rBV	590458	835365	87.83%	13.848%
8	14.033	1839	1844	1850	rVB	13775	18594	1.95%	0.308%
9	14.421	1902	1910	1914	rBV3	5562	13008	1.37%	0.216%
10	14.574	1930	1936	1942	rVB	189879	273563	28.76%	4.535%
11	16.062	2183	2189	2199	rBV	416032	569115	59.84%	9.435%
12	17.309	2395	2401	2407	rBV	208340	282982	29.75%	4.691%
13	18.192	2545	2551	2563	rBV	110308	162579	17.09%	2.695%
14	19.345	2744	2747	2753	rVB2	7153	12489	1.31%	0.207%
15	19.456	2762	2766	2772	rBV	56063	81774	8.60%	1.356%
16	19.915	2838	2844	2849	rBV	775334	951130	100.00%	15.768%
17	21.156	3051	3055	3063	rBV	105249	139704	14.69%	2.316%
18	21.456	3101	3106	3112	rVB	256493	312018	32.80%	5.173%
19	23.709	3484	3489	3497	rVB2	168237	311452	32.75%	5.163%




Sum of corrected areas: 6032188

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028652.D
Acq On : 04 Feb 2021 13:50
Operator : CG/JU
Sample : M1291-18
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

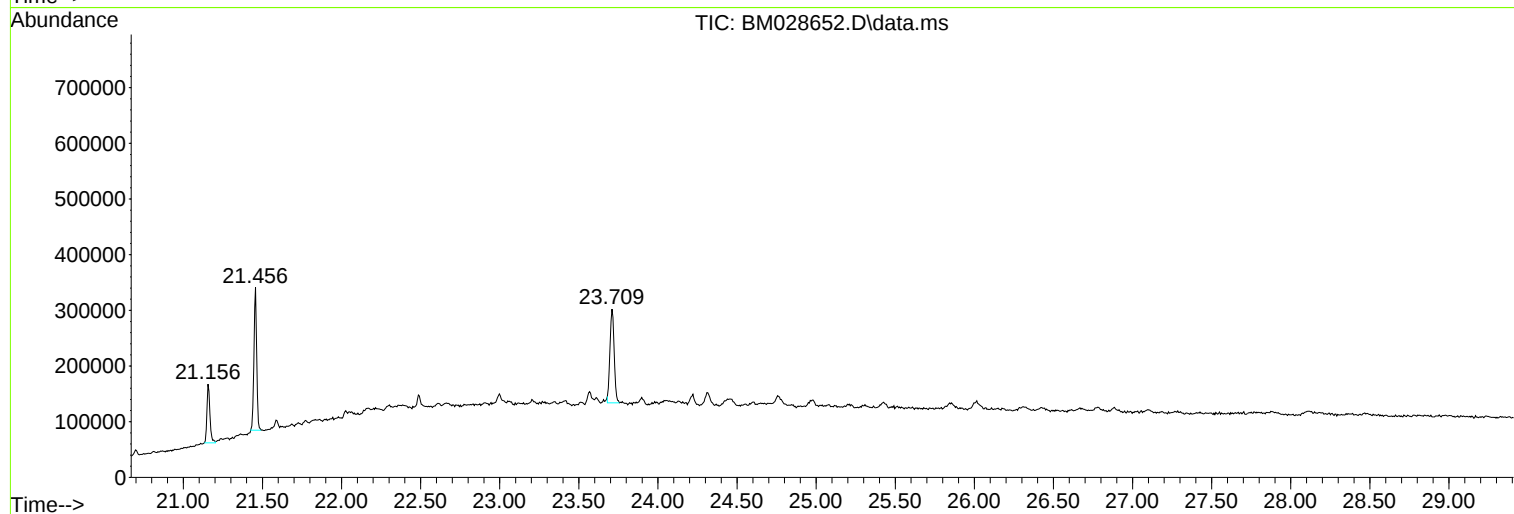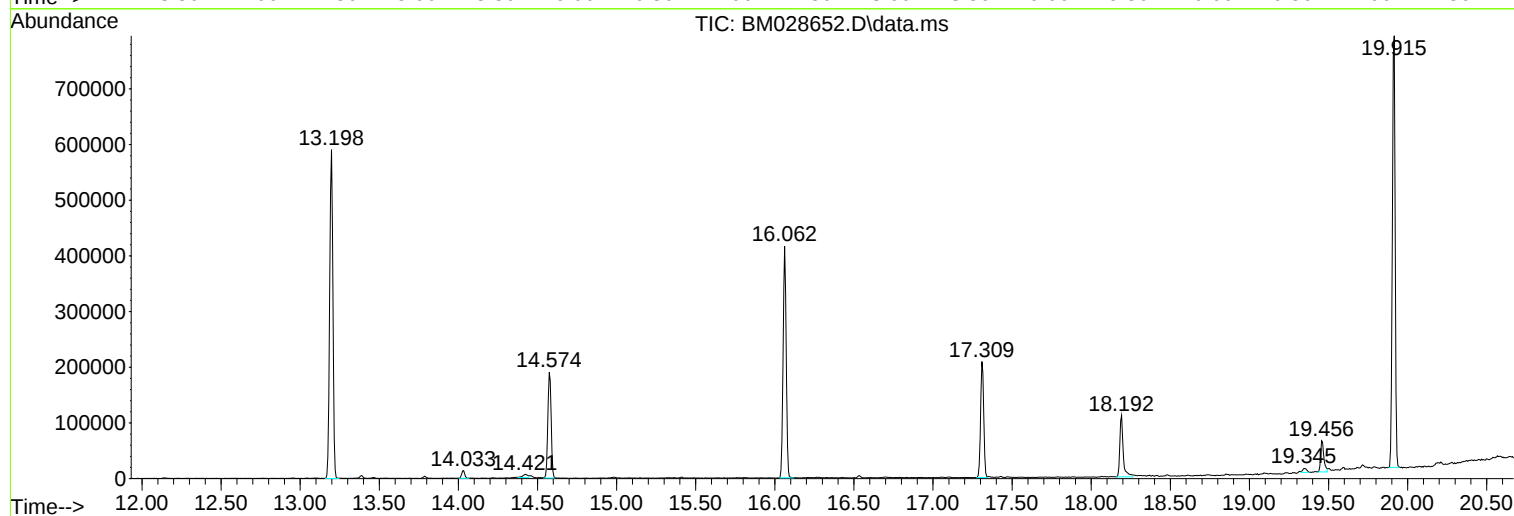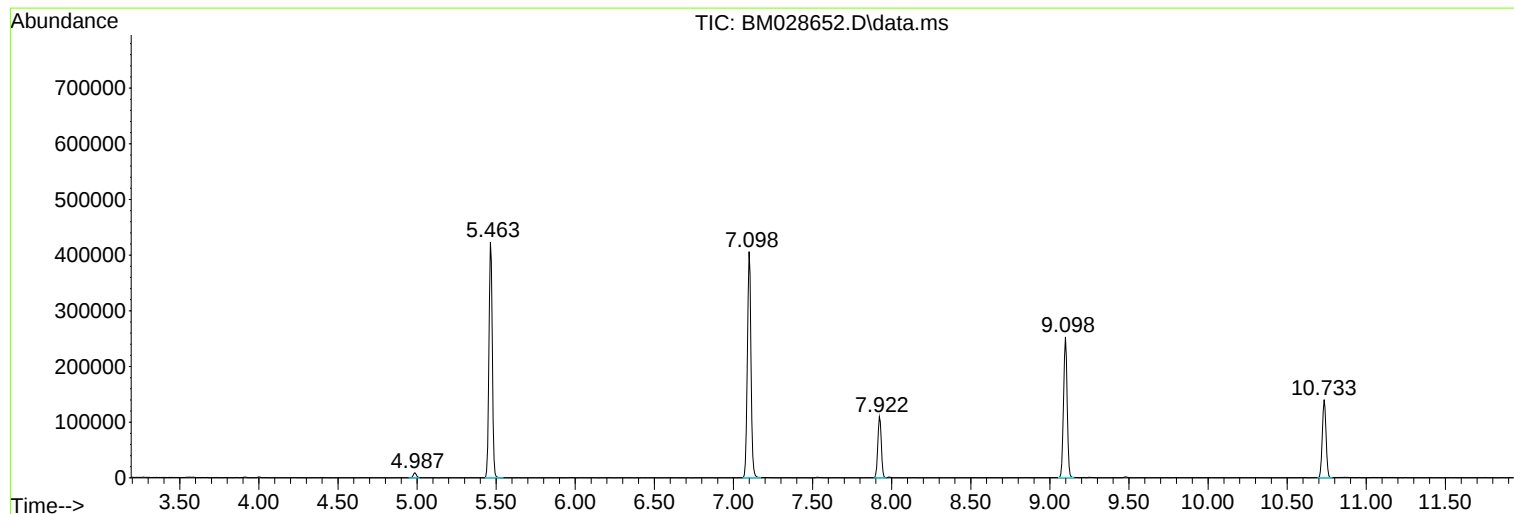

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028652.D
Acq On : 04 Feb 2021 13:50
Operator : CG/JU
Sample : M1291-18
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028652.D
Acq On : 04 Feb 2021 13:50
Operator : CG/JU
Sample : M1291-18
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------