

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
 Data File : BM028653.D
 Acq On : 04 Feb 2021 14:27
 Operator : CG/JU
 Sample : M1291-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-004-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	381	387	397	rBV	425384	609901	63.09%	9.973%
2	7.098	658	665	674	rBV	397062	620671	64.20%	10.149%
3	7.922	799	805	812	rBV	113739	173564	17.95%	2.838%
4	9.098	998	1005	1017	rBV	249363	398666	41.24%	6.519%
5	10.733	1277	1283	1292	rVB	141906	230417	23.84%	3.768%
6	13.198	1695	1702	1713	rBV	586493	824032	85.24%	13.475%
7	14.033	1838	1844	1849	rBV	11793	15935	1.65%	0.261%
8	14.421	1905	1910	1922	rVB5	6208	18684	1.93%	0.306%
9	14.574	1930	1936	1943	rVB2	186243	276727	28.63%	4.525%
10	16.062	2183	2189	2199	rVB	410361	572884	59.26%	9.368%
11	17.309	2395	2401	2407	rBV	213159	292029	30.21%	4.775%
12	18.192	2545	2551	2561	rBV	118049	166904	17.27%	2.729%
13	19.462	2762	2767	2778	rBV	106961	156457	16.18%	2.558%
14	19.915	2838	2844	2849	rBV	774815	966715	100.00%	15.808%
15	20.703	2974	2978	2982	rBV2	14817	17704	1.83%	0.289%
16	21.156	3051	3055	3061	rBV	75731	97309	10.07%	1.591%
17	21.456	3101	3106	3111	rBV	246508	318332	32.93%	5.205%
18	21.586	3126	3128	3132	rVB	25764	27348	2.83%	0.447%
19	23.709	3483	3489	3497	rVB2	179761	331115	34.25%	5.414%




Sum of corrected areas: 6115394

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028653.D
Acq On : 04 Feb 2021 14:27
Operator : CG/JU
Sample : M1291-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

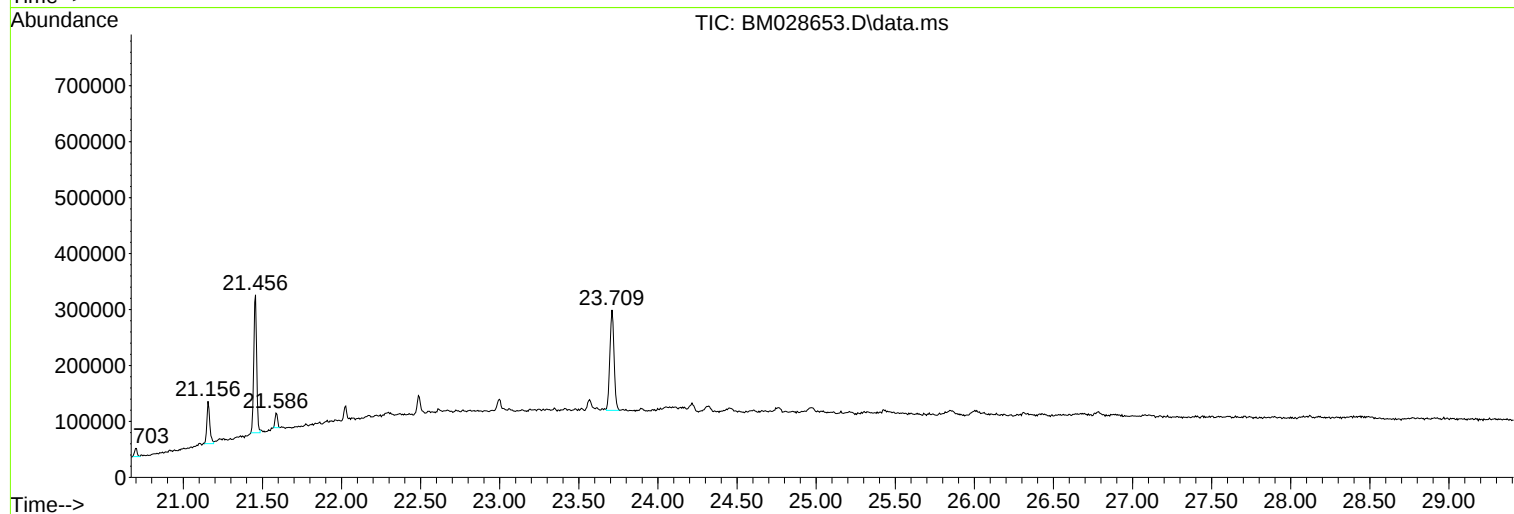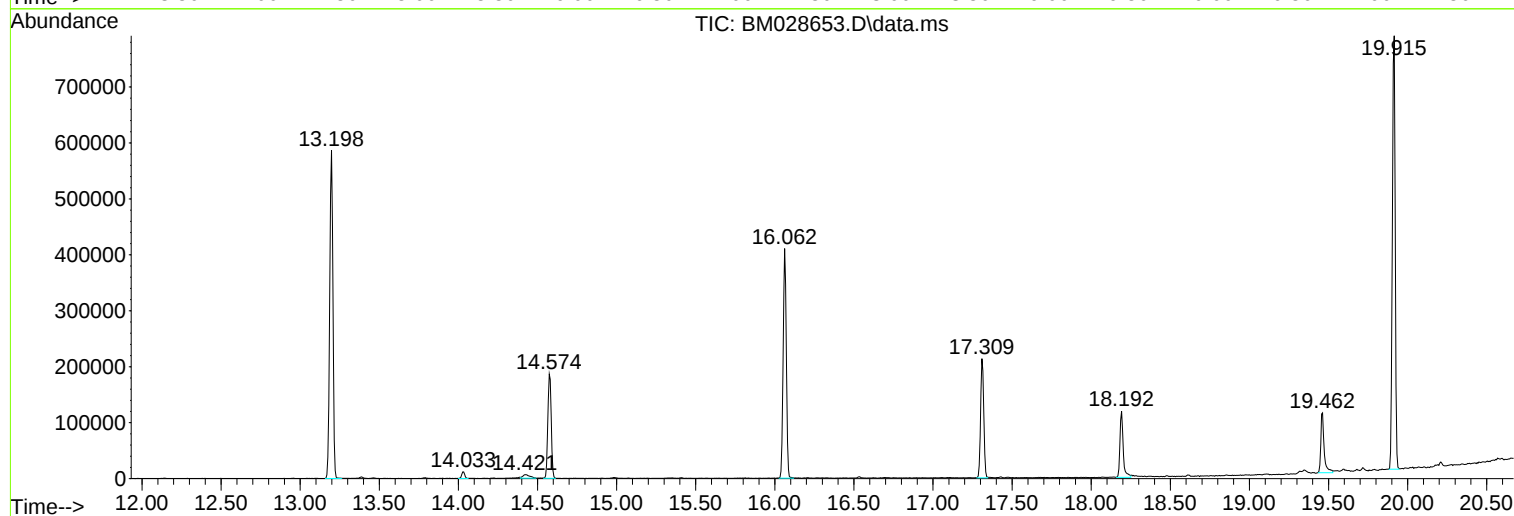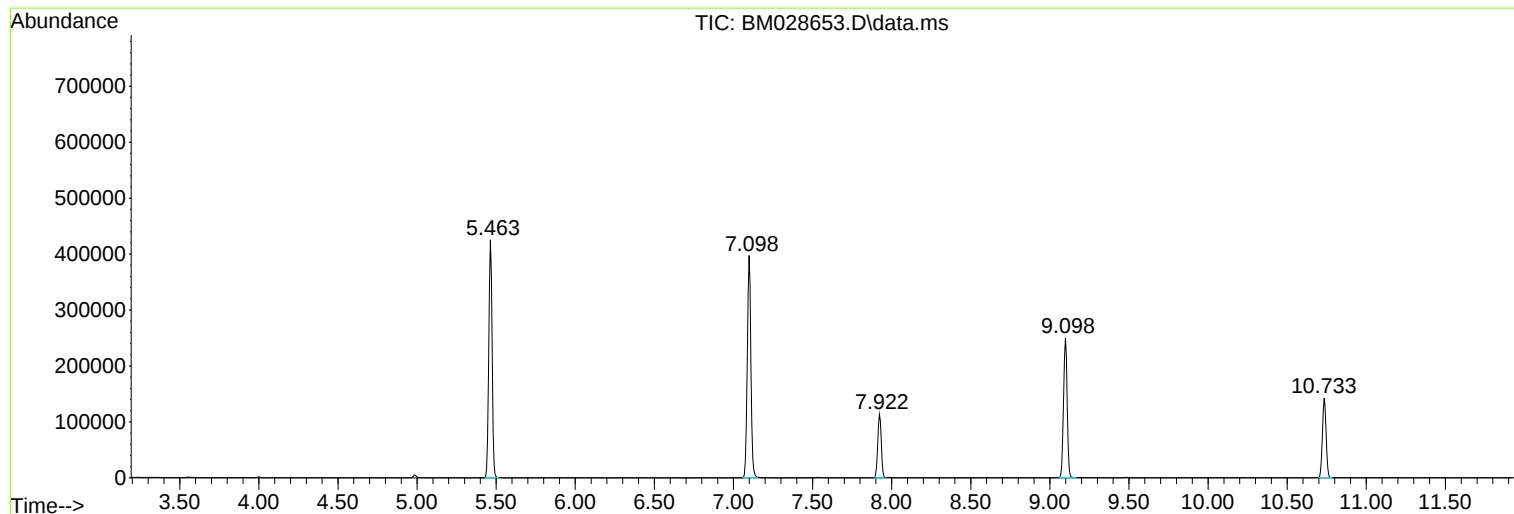

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028653.D
Acq On : 04 Feb 2021 14:27
Operator : CG/JU
Sample : M1291-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028653.D
Acq On : 04 Feb 2021 14:27
Operator : CG/JU
Sample : M1291-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-004-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------