

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
 Data File : BM028654.D
 Acq On : 04 Feb 2021 15:03
 Operator : CG/JU
 Sample : M1291-21
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-005-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	381	387	398	rVB	306820	447203	59.01%	7.040%
2	7.098	657	665	679	rBV	291766	457765	60.40%	7.206%
3	7.922	798	805	812	rBV	109491	167509	22.10%	2.637%
4	9.098	998	1005	1013	rBV	184527	292426	38.58%	4.603%
5	10.733	1277	1283	1290	rVB	133271	221929	29.28%	3.494%
6	13.198	1695	1702	1711	rVB	420365	599809	79.14%	9.442%
7	14.033	1839	1844	1849	rVB	14462	19945	2.63%	0.314%
8	14.298	1883	1889	1896	rBV	42392	65791	8.68%	1.036%
9	14.427	1903	1911	1926	rVB6	7547	25781	3.40%	0.406%
10	14.574	1930	1936	1945	rVB	180162	268370	35.41%	4.225%
11	16.063	2181	2189	2196	rBV	307694	425708	56.17%	6.702%
12	17.310	2395	2401	2406	rBV	207898	290376	38.31%	4.571%
13	17.351	2406	2408	2416	rVB	28221	35612	4.70%	0.561%
14	17.445	2420	2424	2430	rBV	23498	33739	4.45%	0.531%
15	18.192	2545	2551	2556	rBV	124887	170613	22.51%	2.686%
16	18.374	2577	2582	2586	rBV3	9343	16591	2.19%	0.261%
17	18.486	2596	2601	2604	rBV4	4577	7951	1.05%	0.125%
18	18.680	2627	2634	2638	rBV2	8201	14665	1.93%	0.231%
19	18.727	2638	2642	2645	rBV4	9766	12314	1.62%	0.194%
20	19.098	2700	2705	2710	rBV5	7733	18354	2.42%	0.289%
21	19.233	2725	2728	2733	rBV2	8723	11764	1.55%	0.185%
22	19.356	2743	2749	2756	rVB	151246	206704	27.27%	3.254%
23	19.462	2762	2767	2771	rBV	70542	99602	13.14%	1.568%
24	19.504	2771	2774	2779	rVB	22796	33446	4.41%	0.527%
25	19.686	2801	2805	2806	rBV	12544	16101	2.12%	0.253%
26	19.715	2806	2810	2819	rVB	159998	209152	27.60%	3.293%
27	19.915	2838	2844	2849	rBV	608886	757906	100.00%	11.931%
28	21.156	3052	3055	3059	rBV2	65824	83920	11.07%	1.321%
29	21.456	3100	3106	3110	rBV2	309447	487550	64.33%	7.675%
30	21.492	3110	3112	3117	rVB	88268	97090	12.81%	1.528%
31	23.033	3370	3374	3380	rBV	102659	230616	30.43%	3.630%
32	23.515	3453	3456	3462	rVB	69906	113100	14.92%	1.780%
33	23.615	3469	3473	3480	rVB	85396	142096	18.75%	2.237%
34	23.715	3485	3490	3496	rVB	155428	270821	35.73%	4.263%

Sum of corrected areas: 6352319

Instrument :

BNA_M

ClientSampleId :




OU421-005-0002

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028654.D
Acq On : 04 Feb 2021 15:03
Operator : CG/JU
Sample : M1291-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

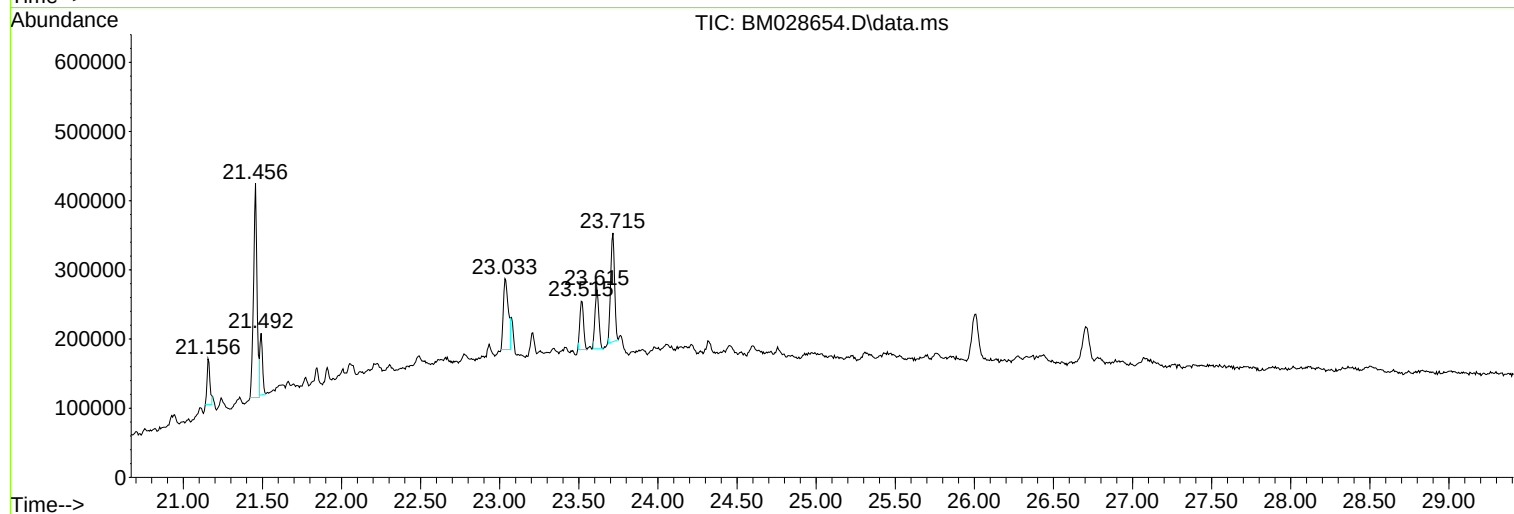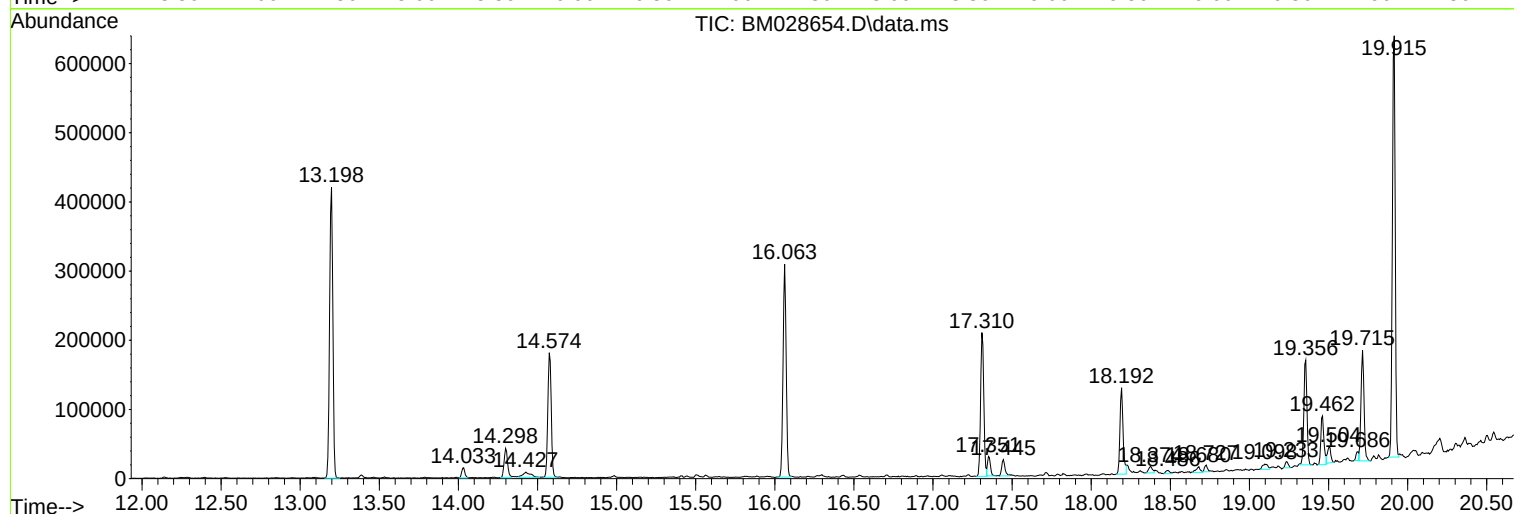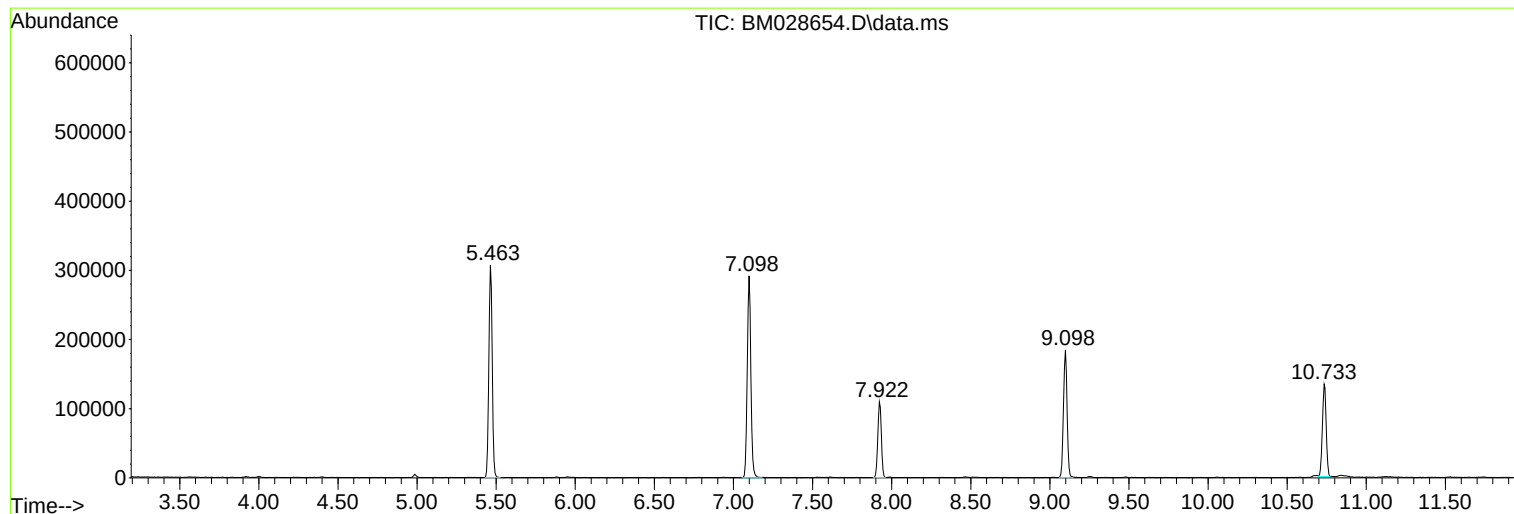

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028654.D
Acq On : 04 Feb 2021 15:03
Operator : CG/JU
Sample : M1291-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028654.D
Acq On : 04 Feb 2021 15:03
Operator : CG/JU
Sample : M1291-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-005-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
