

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
 Data File : BM028658.D
 Acq On : 04 Feb 2021 17:30
 Operator : CG/JU
 Sample : M1291-01 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU421-007-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	381	388	395	rVB	65325	98048	19.51%	1.938%
2	7.104	660	666	676	rBV	62288	99656	19.83%	1.970%
3	7.928	800	806	812	rVB	125658	191906	38.19%	3.793%
4	9.104	998	1006	1011	rBV	50009	81200	16.16%	1.605%
5	10.739	1277	1284	1290	rBV	155986	251180	49.99%	4.965%
6	13.198	1696	1702	1708	rVB	120082	165023	32.84%	3.262%
7	13.392	1731	1735	1739	rBV	4348	5766	1.15%	0.114%
8	14.039	1840	1845	1852	rVB3	10996	17407	3.46%	0.344%
9	14.304	1884	1890	1896	rBV	43432	67292	13.39%	1.330%
10	14.445	1909	1914	1915	rBV3	4312	6894	1.37%	0.136%
11	14.463	1915	1917	1924	rVB2	8165	9314	1.85%	0.184%
12	14.580	1931	1937	1945	rVB	205197	295310	58.77%	5.837%
13	14.986	1998	2006	2013	rBV7	4305	9895	1.97%	0.196%
14	15.180	2035	2039	2045	rVB5	3058	5524	1.10%	0.109%
15	15.410	2074	2078	2081	rBV2	6359	8193	1.63%	0.162%
16	15.451	2081	2085	2092	rVB	6831	10574	2.10%	0.209%
17	15.569	2101	2105	2110	rVB2	6318	8797	1.75%	0.174%
18	15.833	2146	2150	2154	rVB6	3933	6842	1.36%	0.135%
19	16.069	2185	2190	2195	rVB	63300	88248	17.56%	1.744%
20	16.204	2207	2213	2217	rBV2	5130	10677	2.12%	0.211%
21	16.269	2221	2224	2226	rBV2	7165	8955	1.78%	0.177%
22	16.351	2235	2238	2244	rVB6	5185	8212	1.63%	0.162%
23	16.716	2297	2300	2306	rVB7	5187	7758	1.54%	0.153%
24	16.980	2342	2345	2350	rBV6	3562	5811	1.16%	0.115%
25	17.057	2355	2358	2362	rVB2	7521	9104	1.81%	0.180%
26	17.316	2397	2402	2407	rBV	226628	317310	63.15%	6.272%
27	17.357	2407	2409	2416	rVB	29168	35613	7.09%	0.704%
28	17.451	2420	2425	2430	rBV	36031	56731	11.29%	1.121%
29	17.792	2481	2483	2487	rVB3	7482	7587	1.51%	0.150%
30	18.198	2546	2552	2565	rBV2	288109	502450	100.00%	9.932%
31	18.386	2579	2584	2587	rBV4	14225	26419	5.26%	0.522%
32	18.486	2596	2601	2615	rBV	170204	275550	54.84%	5.447%
33	18.692	2632	2636	2652	rVB	278829	462316	92.01%	9.139%
34	18.810	2653	2656	2661	rVB	31680	40597	8.08%	0.802%
35	19.074	2696	2701	2703	rBV	58734	92296	18.37%	1.824%
36	19.104	2703	2706	2719	rVB	120156	190093	37.83%	3.758%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028658.D
Acq On : 04 Feb 2021 17:30
Operator : CG/JU
Sample : M1291-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-007-0002

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.362	2745	2750	2756	rBV	96502	163087	32.46%	3.224%
38	19.468	2763	2768	2772	rBV	215296	297448	59.20%	5.880%
39	19.509	2772	2775	2779	rVB	58251	79395	15.80%	1.569%
40	19.721	2807	2811	2820	rBV	83087	130252	25.92%	2.575%
41	19.915	2840	2844	2851	rBV	170110	201364	40.08%	3.980%
42	21.462	3102	3107	3111	rBV2	307971	429785	85.54%	8.496%
43	23.727	3488	3492	3497	rVB	167034	273047	54.34%	5.397%




Sum of corrected areas: 5058926

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028658.D
Acq On : 04 Feb 2021 17:30
Operator : CG/JU
Sample : M1291-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-007-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

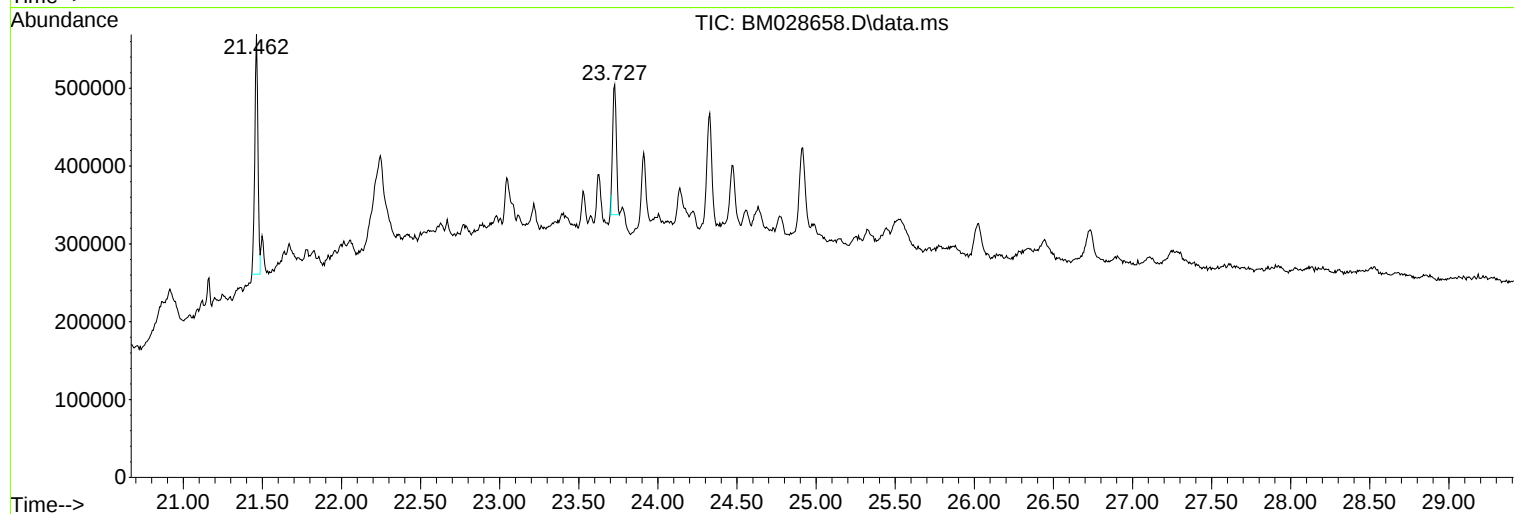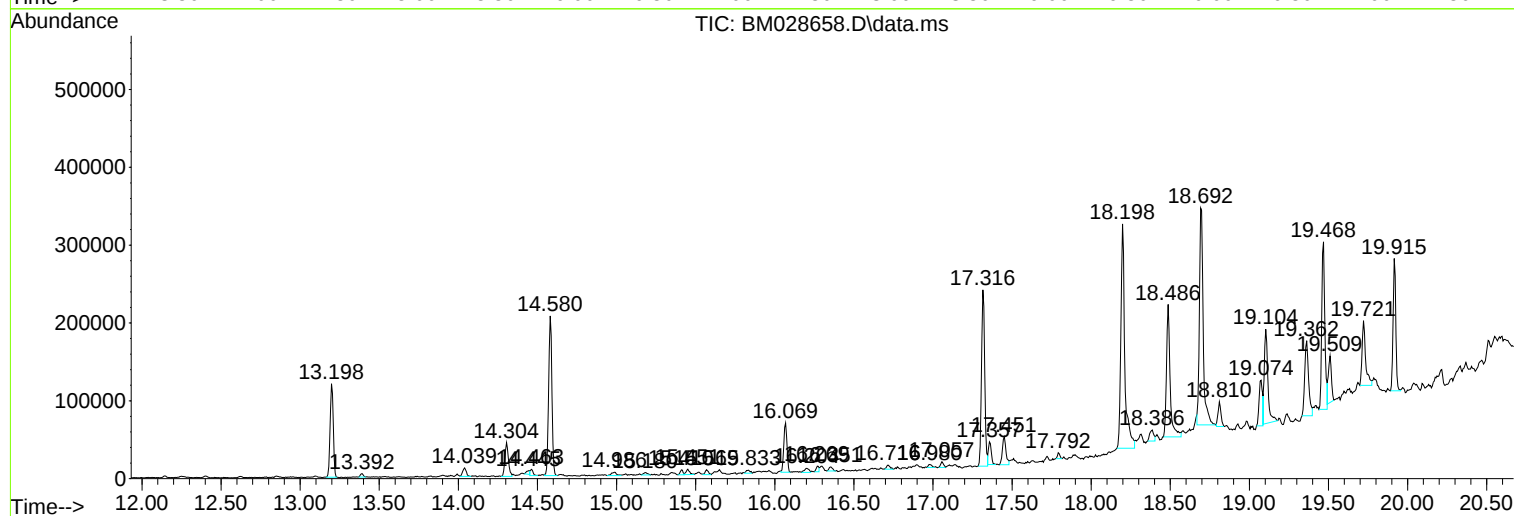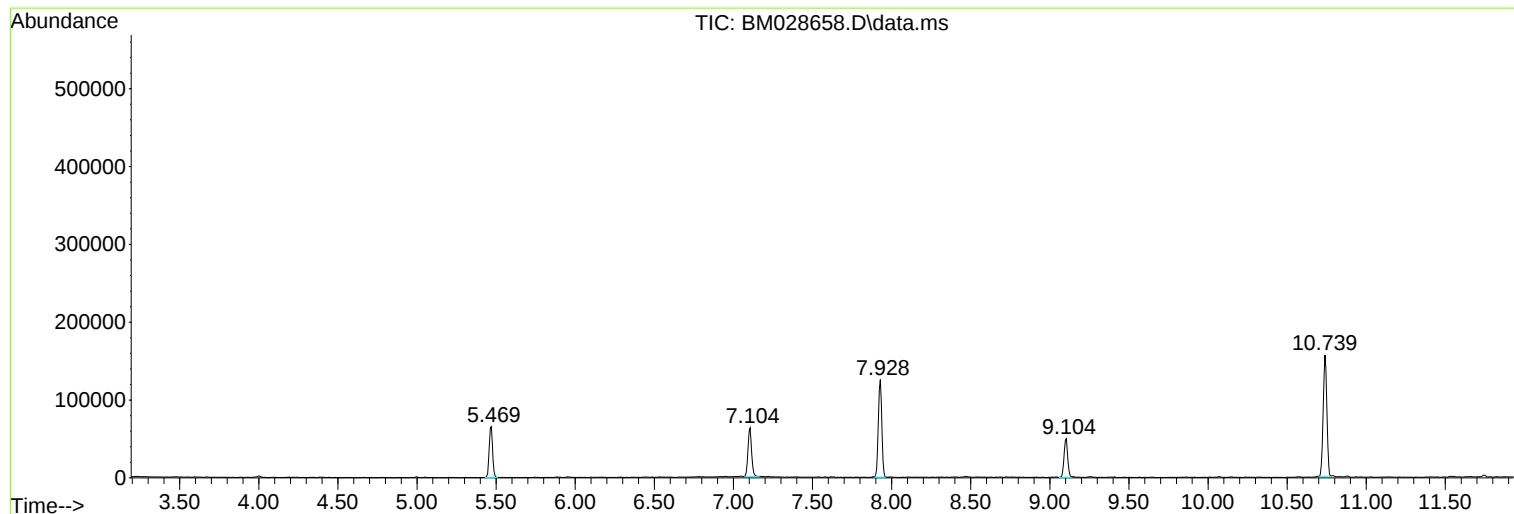

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028658.D
Acq On : 04 Feb 2021 17:30
Operator : CG/JU
Sample : M1291-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-007-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028658.D
Acq On : 04 Feb 2021 17:30
Operator : CG/JU
Sample : M1291-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU421-007-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------