
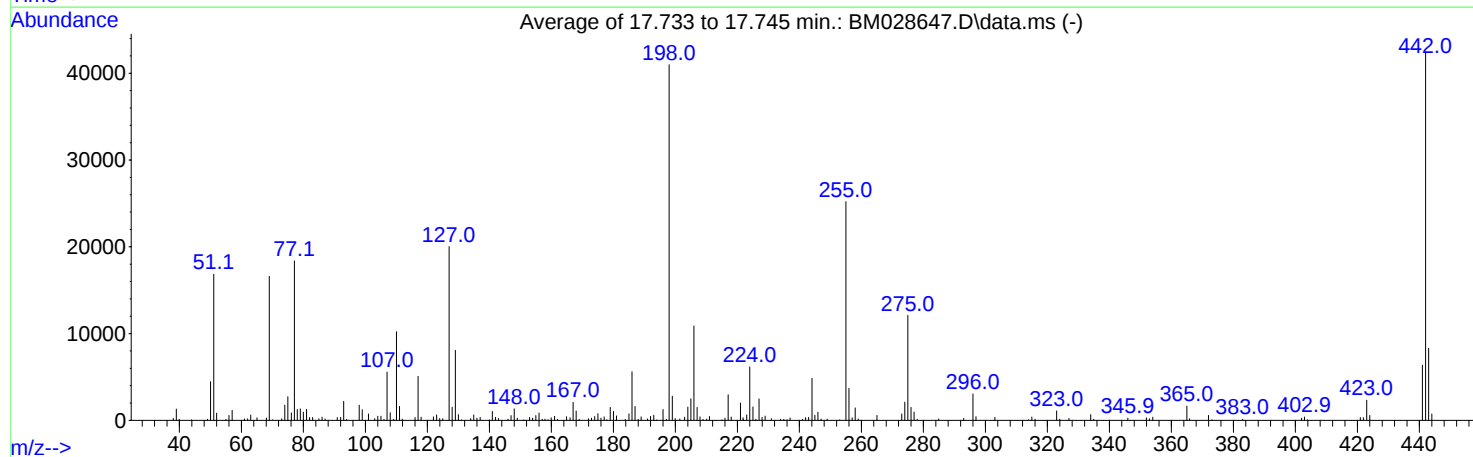


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
 Data File : BM028647.D
 Acq On : 04 Feb 2021 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 16:19:07 2021

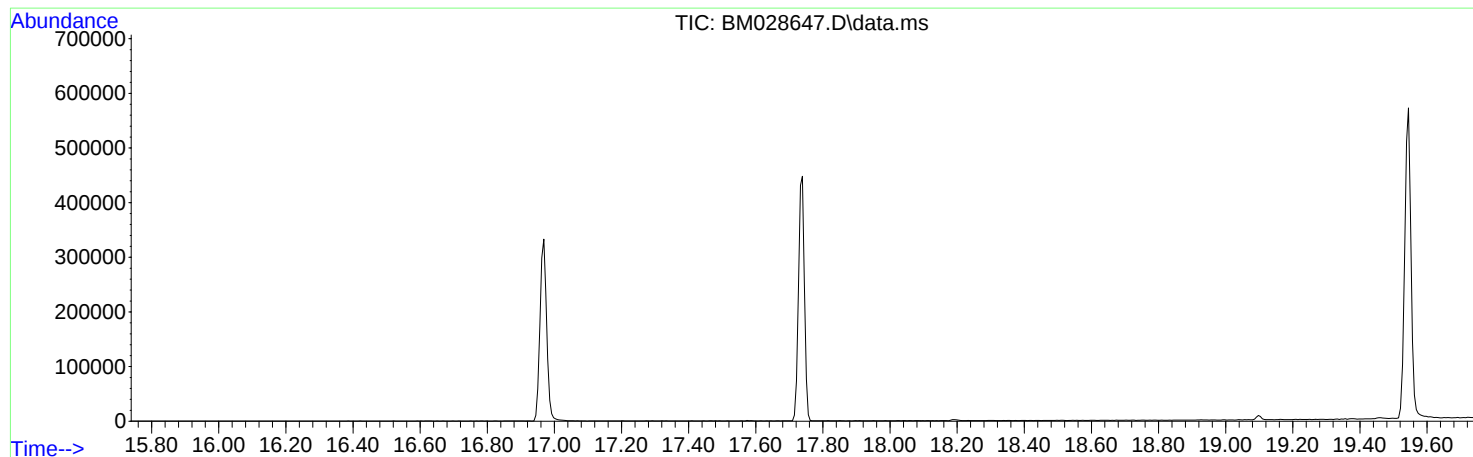

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	16832	PASS
68	69	0.00	2	1.7	279	PASS
69	198	0.00	100	40.5	16595	PASS
70	69	0.00	2	0.3	52	PASS
127	198	10	80	48.8	20018	PASS
197	198	0.00	2	0.3	119	PASS
198	198	100	100	100.0	40984	PASS
199	198	5	9	6.8	2786	PASS
275	198	10	60	29.5	12090	PASS
365	198	1	100	4.0	1642	PASS
441	198	0.01	100	15.5	6357	PASS
442	442	50	100	100.0	42392	PASS
443	442	15	24	19.6	8300	PASS

DDT Breakdown




Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
2/4/2021	BNA_M	<u>BM028647.D</u>
Compound Name	Response	Retention Time
DDT	149891	20.756
DDD	3288	20.327
DDE	224	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3512	153403	2.29

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020421\
Data File : BM028647.D
Acq On : 04 Feb 2021 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 05 01:41:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 16:19:07 2021
Response via : Initial Calibration

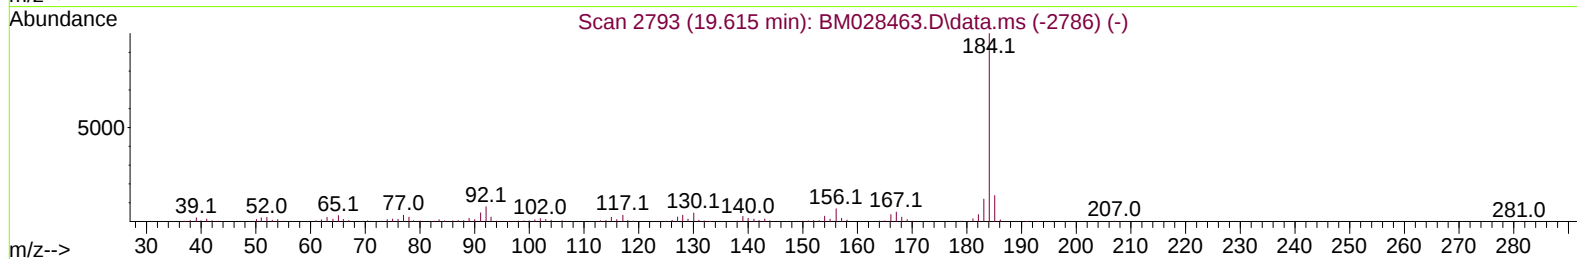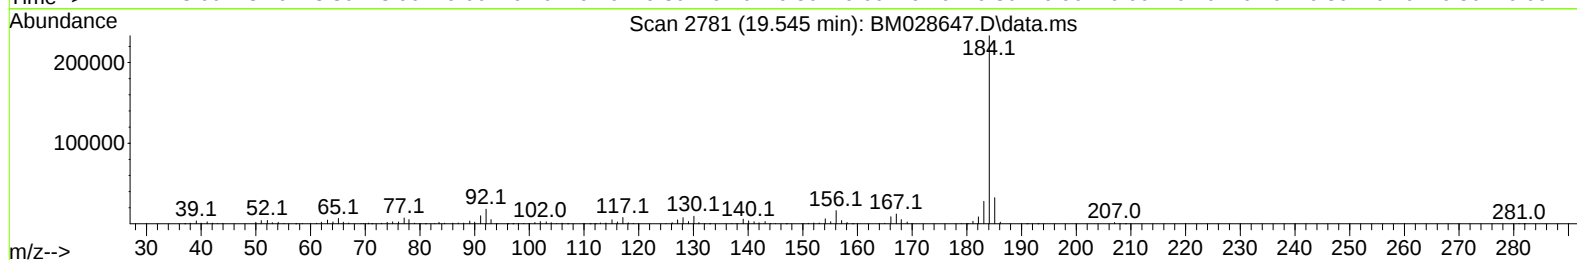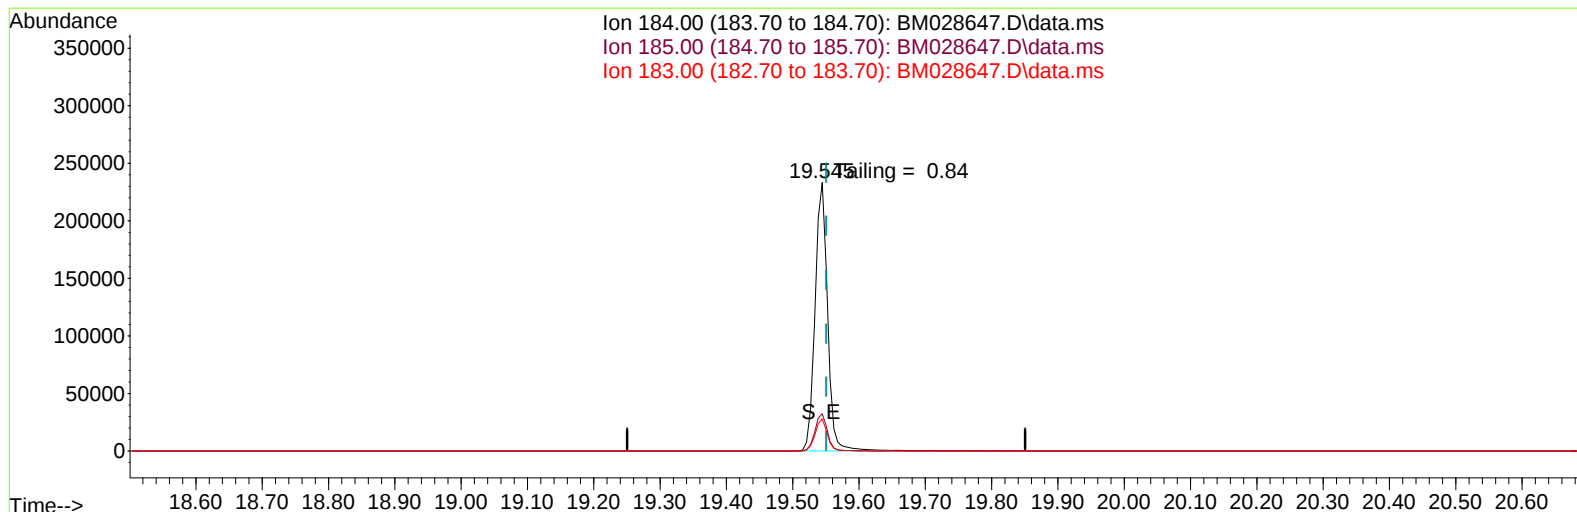

TIC: BM028647.D\data.ms

(77) Benzidine

19.545min (-0.006) 0.00 ng

response 306089

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.93
183.00	12.10	11.99
0.00	0.00	0.00