

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020422\
 Data File : BM034022.D
 Acq On : 04 Feb 2022 17:30
 Operator : CG/JU
 Sample : PB1423358BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB1423358BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.466	372	379	391	rBV	2137461	2984130	52.95%	11.284%
2	7.078	645	653	662	rBV	1911398	3015117	53.50%	11.402%
3	7.913	788	795	807	rVB	393443	605808	10.75%	2.291%
4	9.078	985	993	1003	rBV	1226599	1988307	35.28%	7.519%
5	10.725	1266	1273	1283	rBV	490427	803494	14.26%	3.038%
6	13.183	1684	1691	1701	rBV	2986495	4181680	74.20%	15.813%
7	14.554	1918	1924	1936	rBV	679950	974056	17.28%	3.683%
8	16.036	2169	2176	2189	rBV	2129989	2939302	52.16%	11.115%
9	17.289	2383	2389	2400	rVB	781909	1079258	19.15%	4.081%
10	19.906	2828	2834	2839	rBV	4665245	5635595	100.00%	21.311%
11	21.453	3092	3097	3103	rBV	914977	1141335	20.25%	4.316%
12	23.836	3496	3502	3512	rVB2	550760	1096614	19.46%	4.147%




Sum of corrected areas: 26444696

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020422\
Data File : BM034022.D
Acq On : 04 Feb 2022 17:30
Operator : CG/JU
Sample : PB1423358BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB1423358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

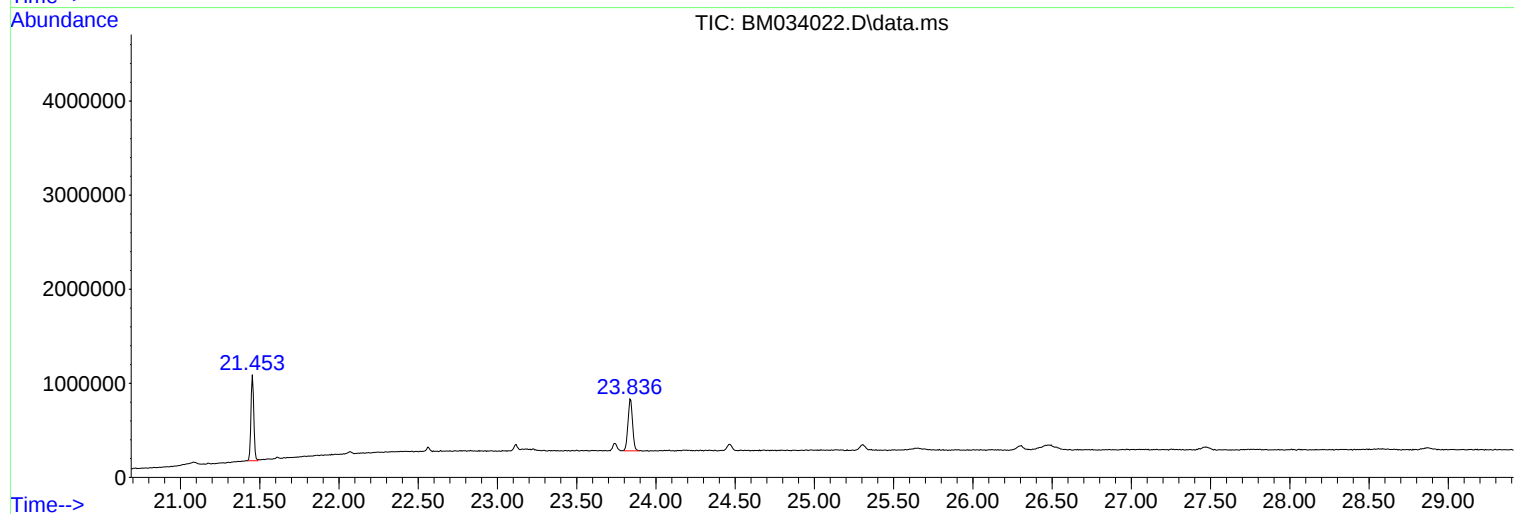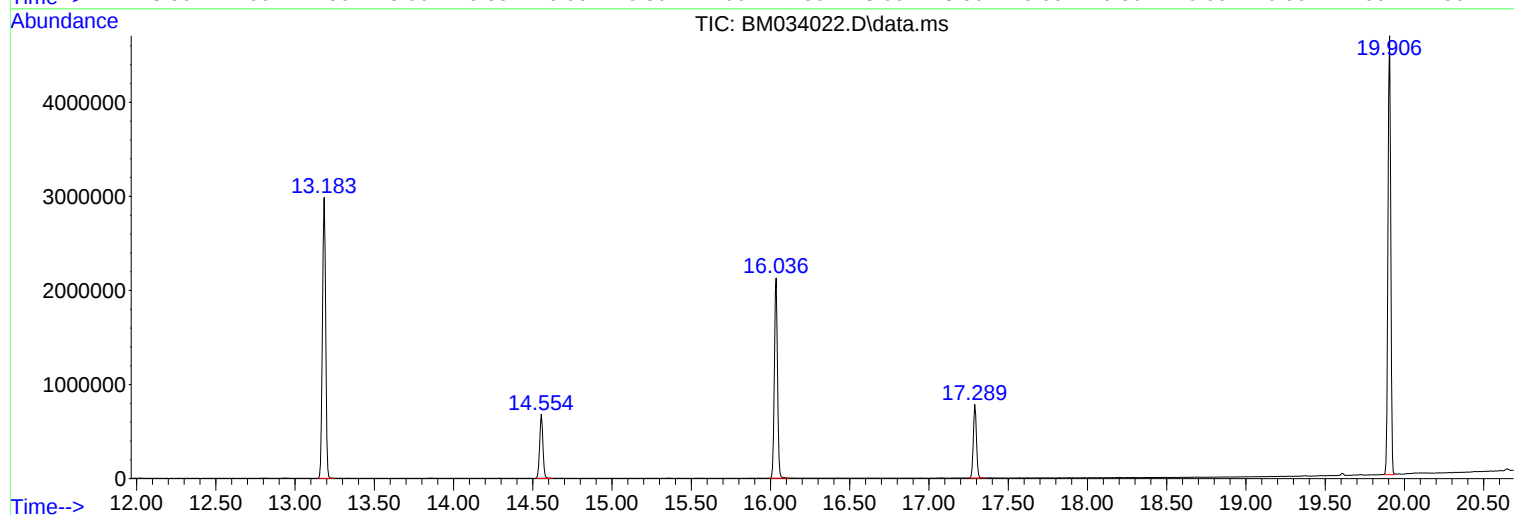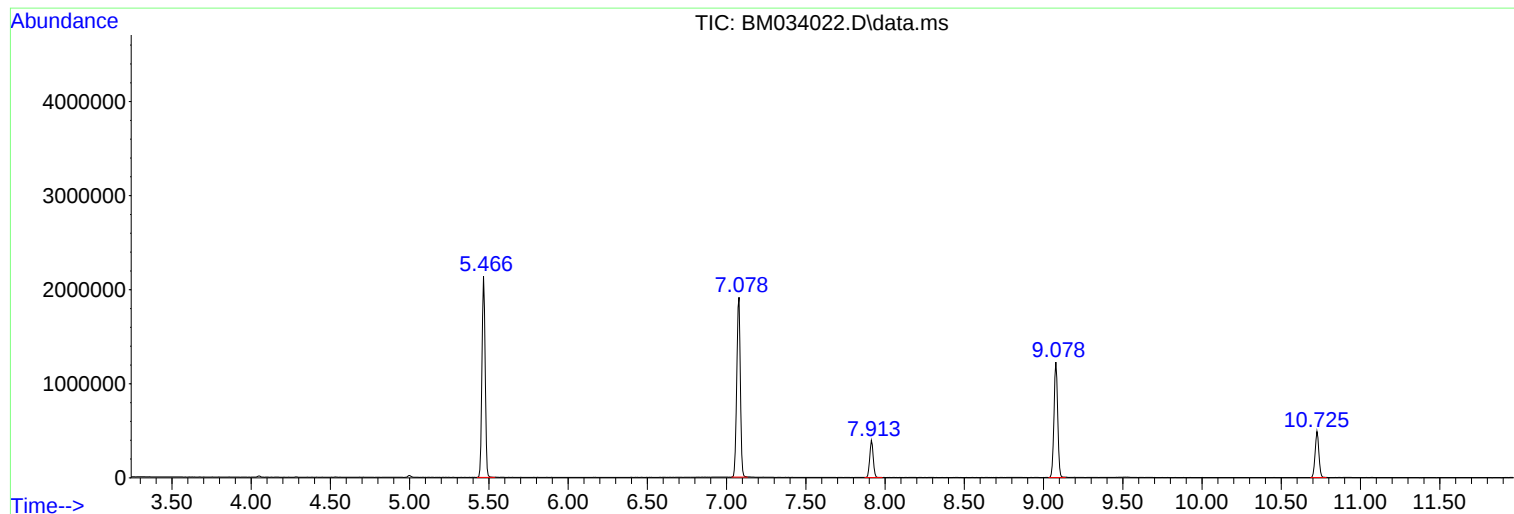

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020422\
Data File : BM034022.D
Acq On : 04 Feb 2022 17:30
Operator : CG/JU
Sample : PB1423358BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB1423358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020422\
Data File : BM034022.D
Acq On : 04 Feb 2022 17:30
Operator : CG/JU
Sample : PB1423358BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB1423358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------